

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
 Data File : PL042217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 22:42
 Operator : AJ\SJ
 Sample : J5925-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 05:46:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	94950181	51369305	15.377	17.339
28)	SA Decachlor...	8.204	9.228	105.5E6	41444858	15.394	16.249
Target Compounds							
6)	B beta-BHC	4.402f	0.000	11108116	0	3.010	N.D. #
8)	B Heptachlo...	0.000	5.993	0	2267394	N.D.	0.631 #
13)	MA Dieldrin	5.739	0.000	2321447	0	0.298	N.D. #
23)	Chlordane-1	4.378	5.148	4030507	-505945	13.505	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
Data File : PL042217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 22:42
Operator : AJ\SJ
Sample : J5925-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 05:46:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

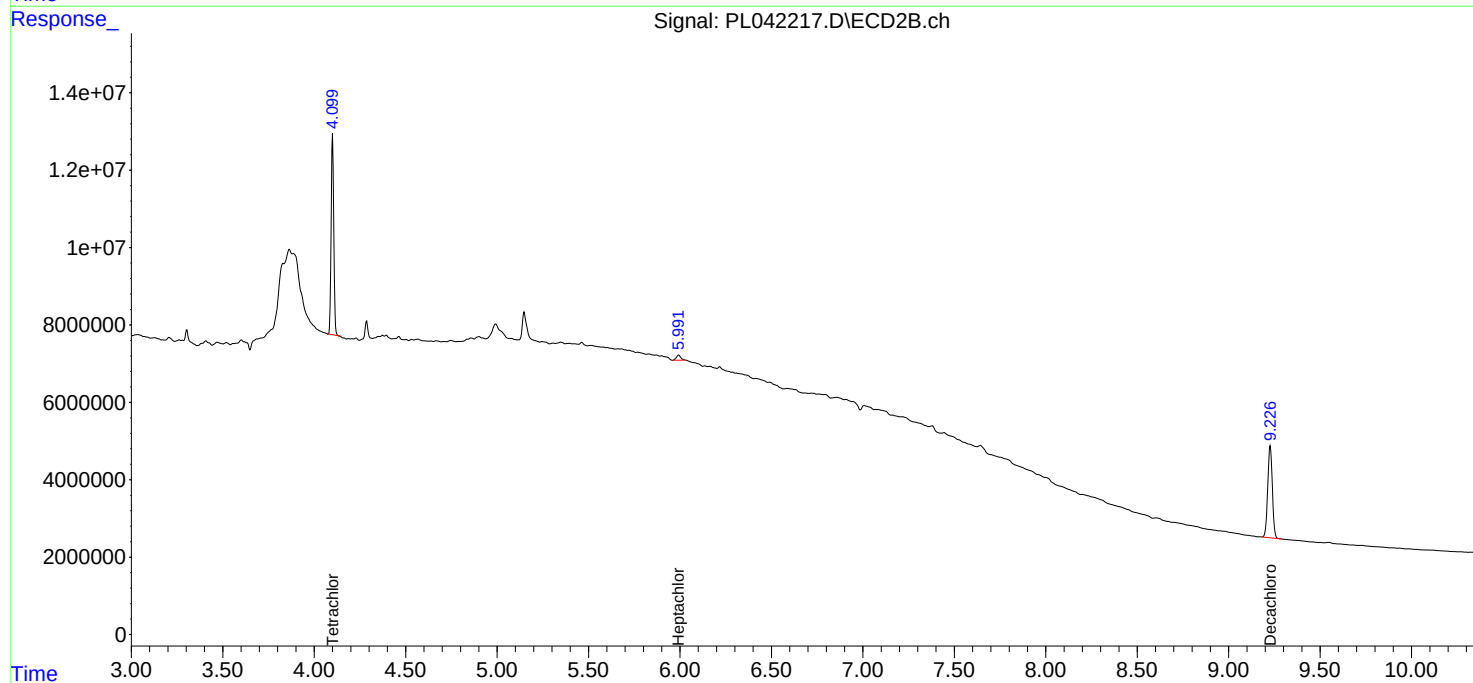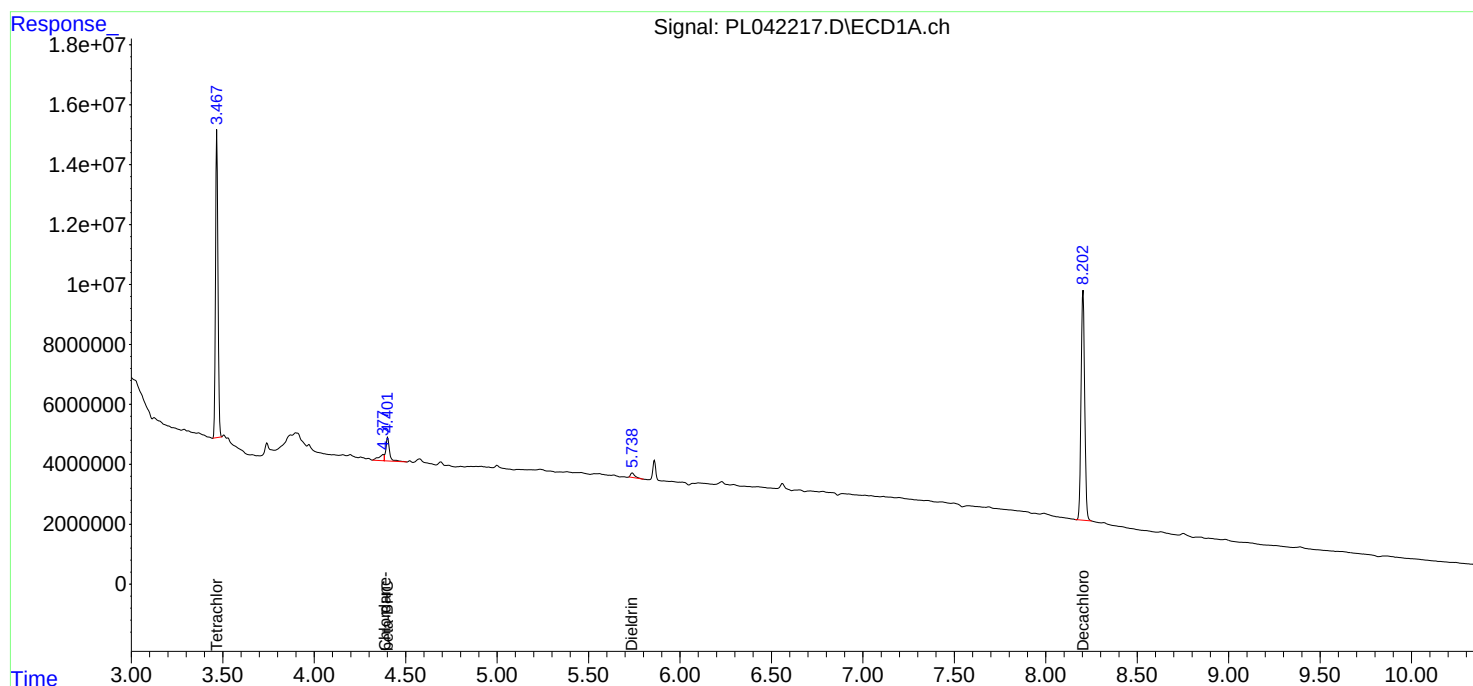


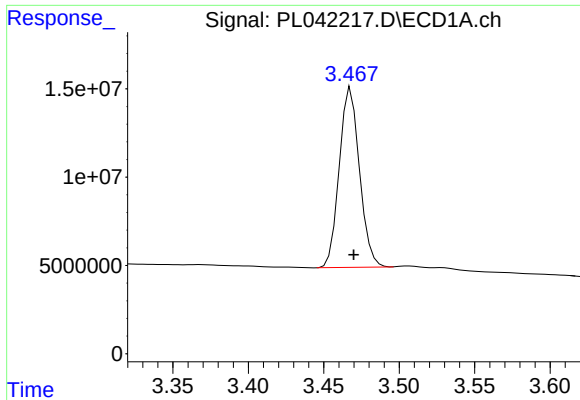

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 94950181
Conc: 15.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

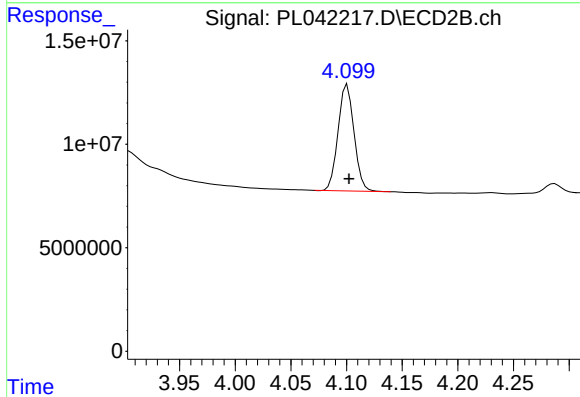


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.001 min
Response: 51369305
Conc: 17.34 ng/ml

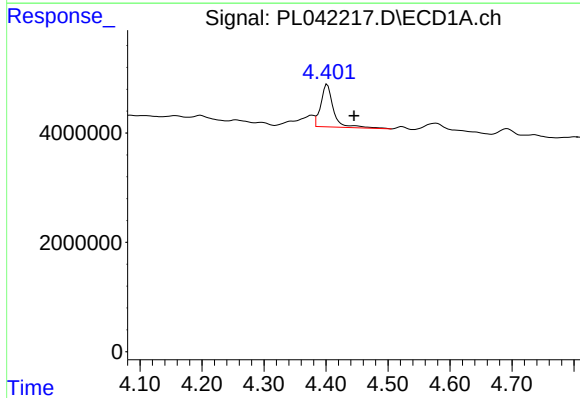


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 11108116
Conc: 3.01 ng/ml

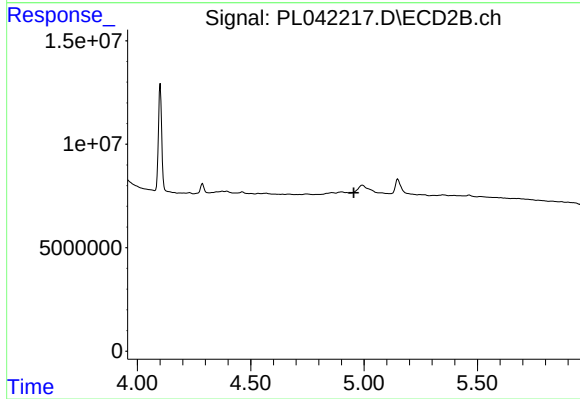

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

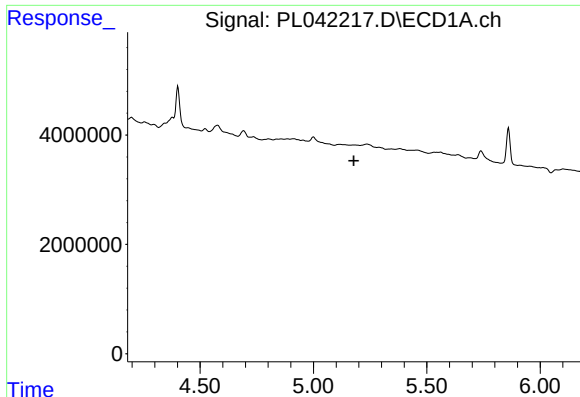

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

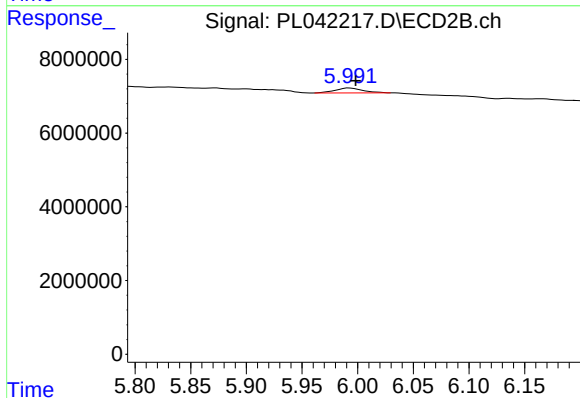


#8 Heptachlor epoxide

R.T.: 5.993 min
Delta R.T.: -0.006 min
Response: 2267394
Conc: 0.63 ng/ml

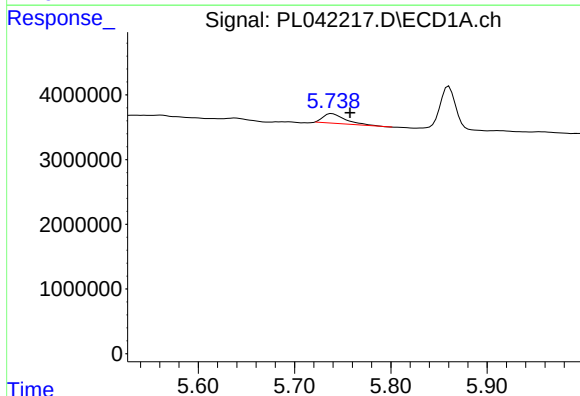


#13 Dieldrin

R.T.: 5.739 min
Delta R.T.: -0.019 min
Response: 2321447
Conc: 0.30 ng/ml

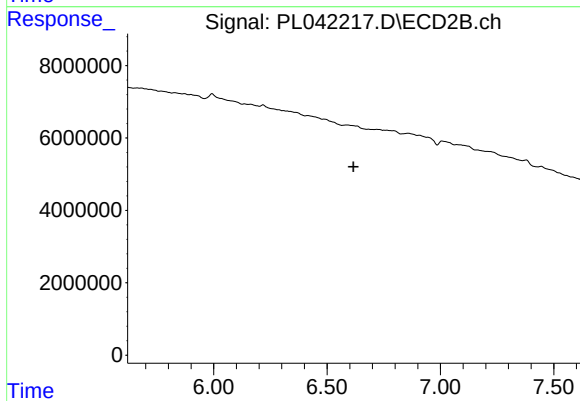

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

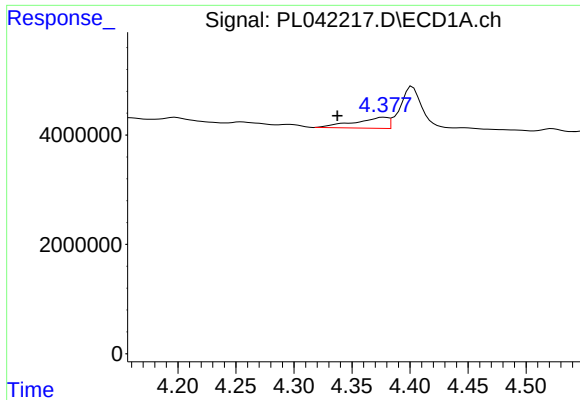

#23 Chlordane-1


R.T.: 4.378 min
Delta R.T.: 0.040 min
Response: 4030507
Conc: 13.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

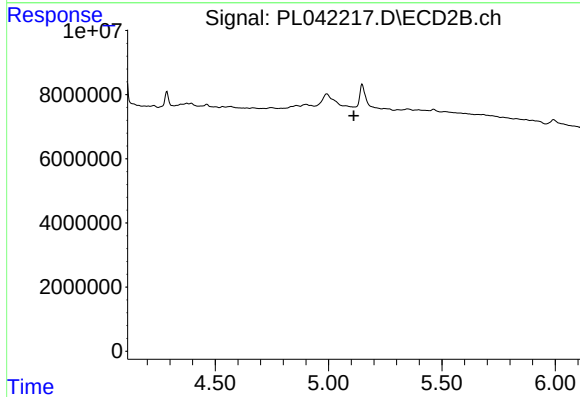


#23 Chlordane-1

R.T.: 5.148 min
Delta R.T.: 0.037 min
Response: -505945
Conc: N.D.

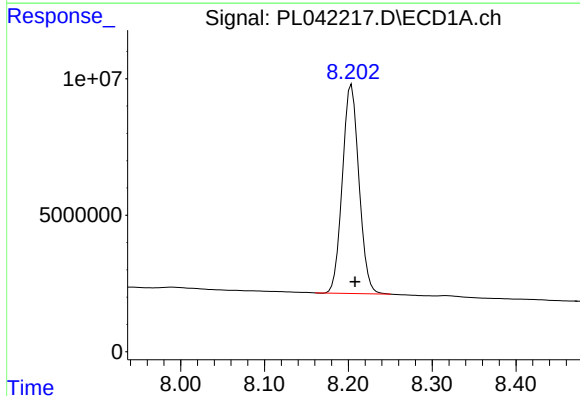

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.004 min
Response: 105457620
Conc: 15.39 ng/ml

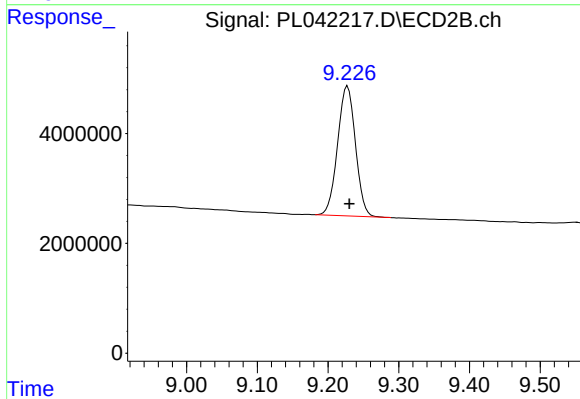

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.003 min
Response: 41444858
Conc: 16.25 ng/ml