

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
 Data File : PL042221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 23:38
 Operator : AJ\SJ
 Sample : J5925-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 05:47:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 09 12:38:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	103.8E6	45817077	16.803	15.465
28)	SA Decachlor...	8.204	9.227	105.7E6	41701948	15.424	16.350
Target Compounds							
2)	A alpha-BHC	3.914	0.000	4667734	0	0.492	N.D. #
3)	MA gamma-BHC...	0.000	4.827f	0	1484656	N.D.	0.360 #
6)	B beta-BHC	4.403f	0.000	12678994	0	3.436	N.D. #
7)	B delta-BHC	0.000	5.149f	0	18351	N.D.	0.005 #
8)	B Heptachlo...	0.000	5.993	0	4351310	N.D.	1.211 #
13)	MA Dieldrin	5.763	0.000	2557299	0	0.329	N.D. #
14)	MA Endrin	6.064f	0.000	1894474	0	0.266	N.D. #
15)	B Endosulfa...	6.228f	0.000	1410551	0	0.207	N.D. #
19)	B Endosulfa...	6.653	7.383	6165525	3818757	0.967	1.404 #
20)	A Methoxychlor	0.000	7.645f	0	4295833	N.D.	3.126 #
23)	Chlordane-1	4.364	5.149	6771941	18351	22.691	0.127 #
27)	Chlordane-5	6.228	0.000	1410551	0	5.385	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111618\
Data File : PL042221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 23:38
Operator : AJ\SJ
Sample : J5925-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 05:47:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110918.M
Quant Title : GC Extractables
QLast Update : Fri Nov 09 12:38:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

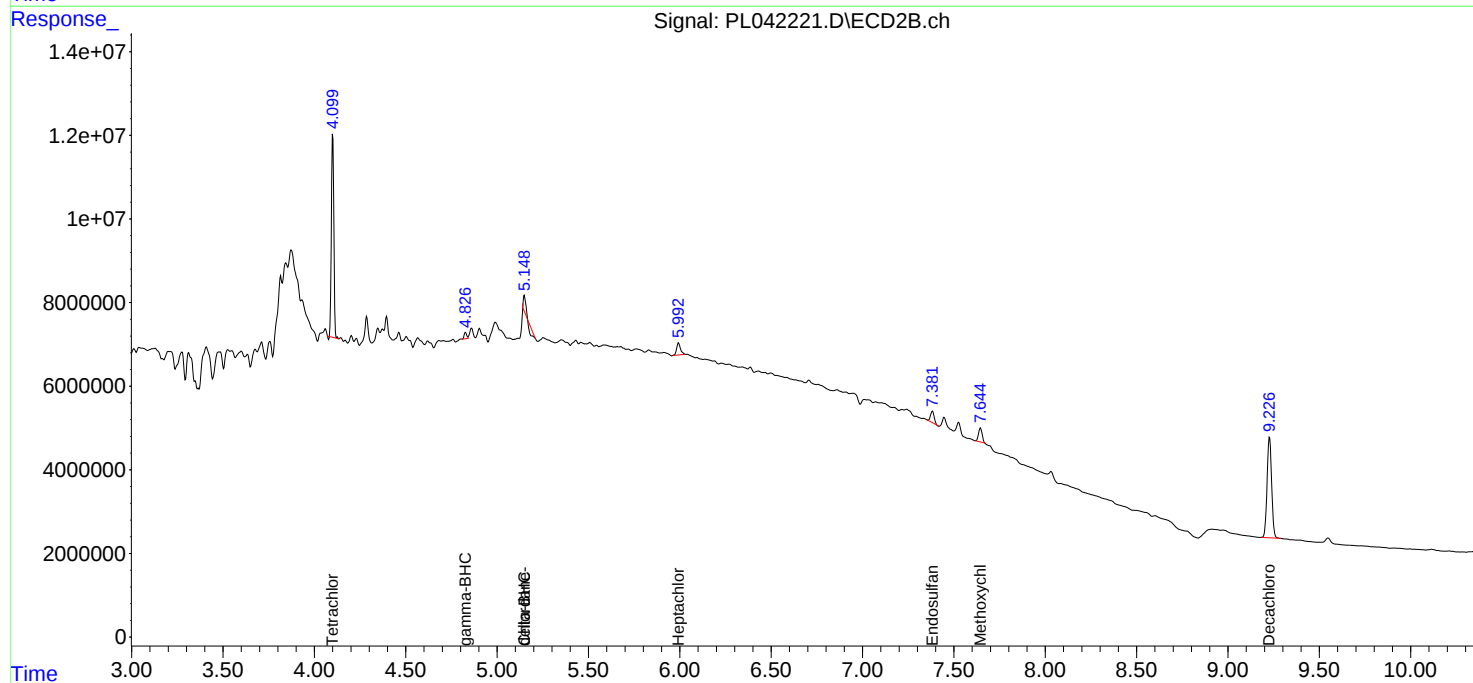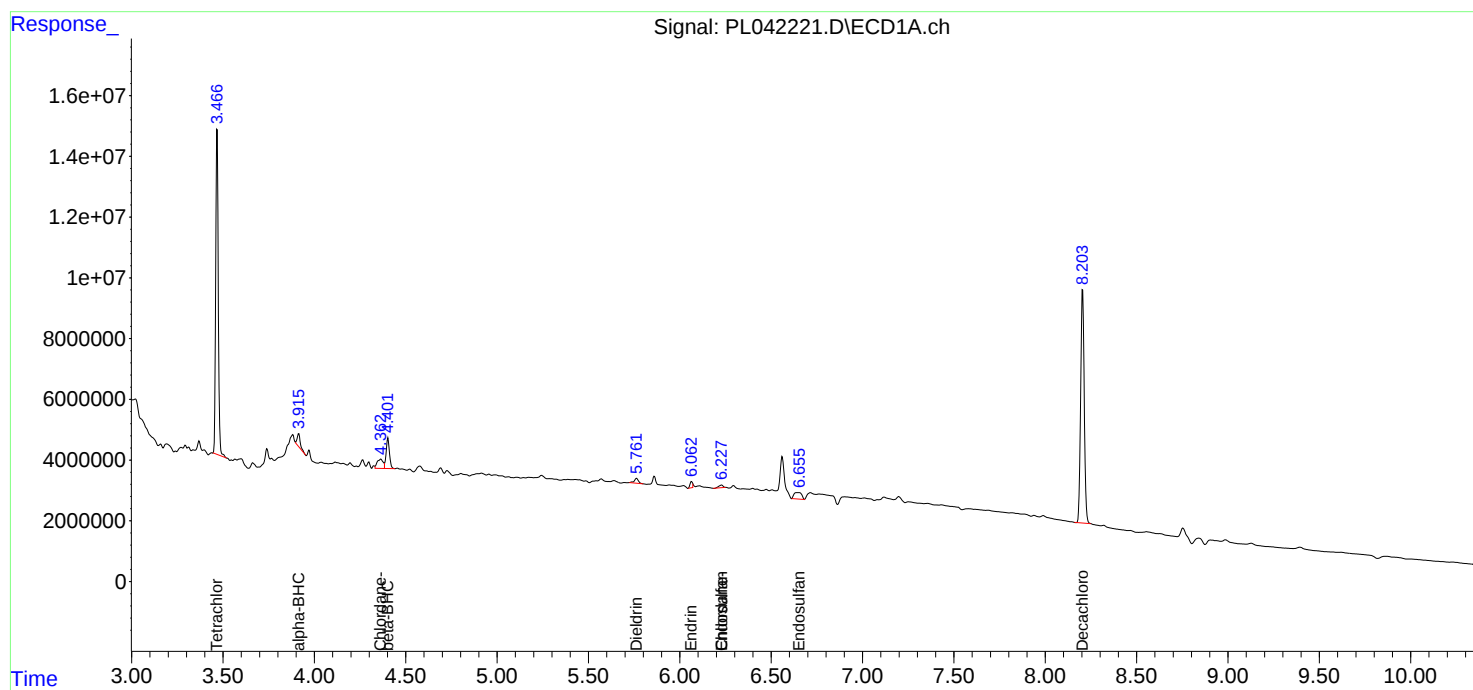


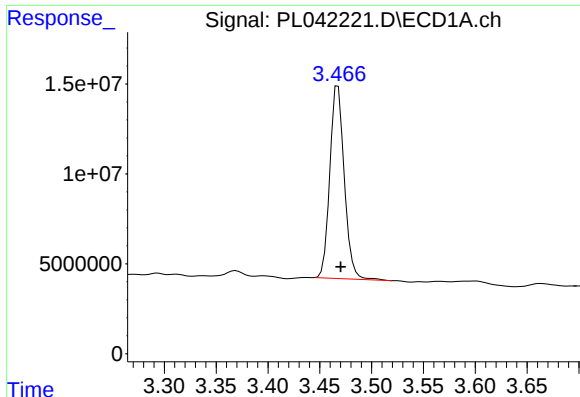

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: -0.002 min
Response: 103756809
Conc: 16.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

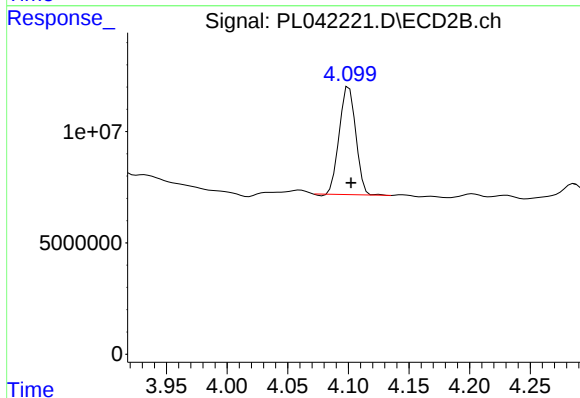


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.001 min
Response: 45817077
Conc: 15.46 ng/ml

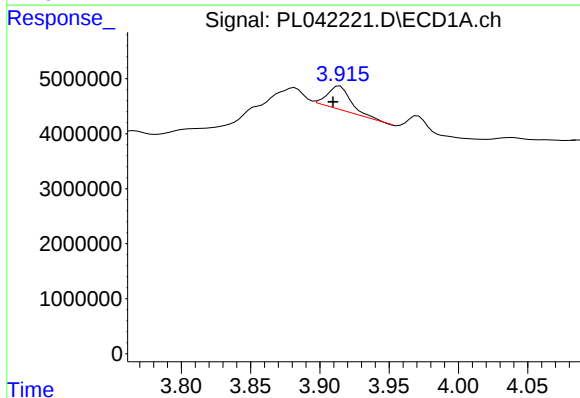


#2 alpha-BHC

R.T.: 3.914 min
Delta R.T.: 0.005 min
Response: 4667734
Conc: 0.49 ng/ml

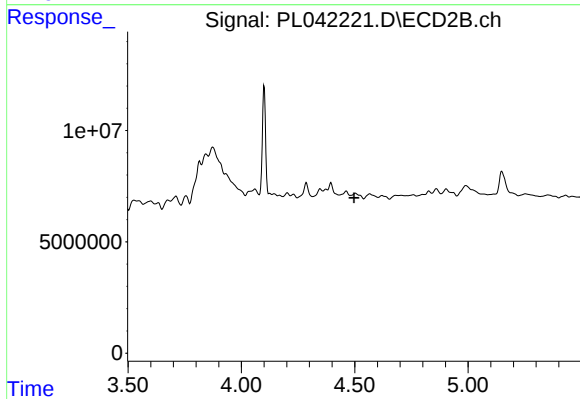

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.498 min
Response: 0
Conc: N.D.

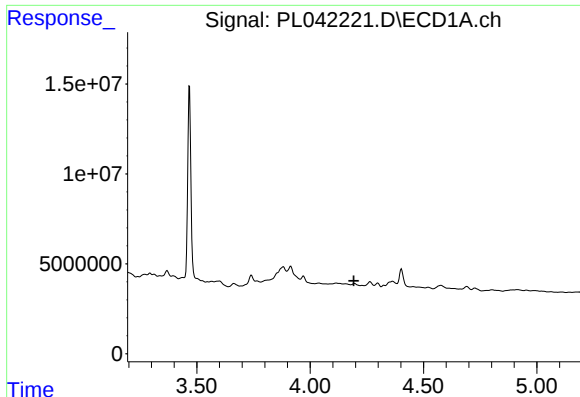

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

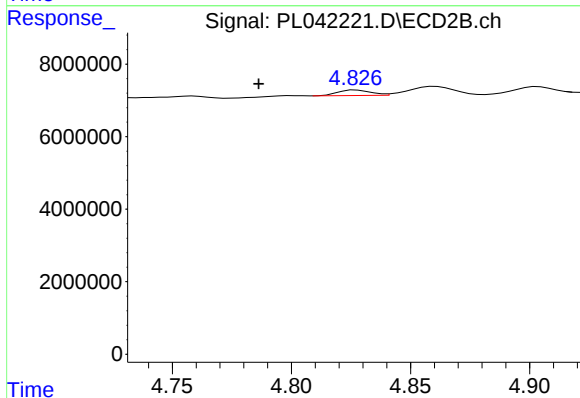


#3 gamma-BHC (Lindane)

R.T.: 4.827 min
Delta R.T.: 0.041 min
Response: 1484656
Conc: 0.36 ng/ml

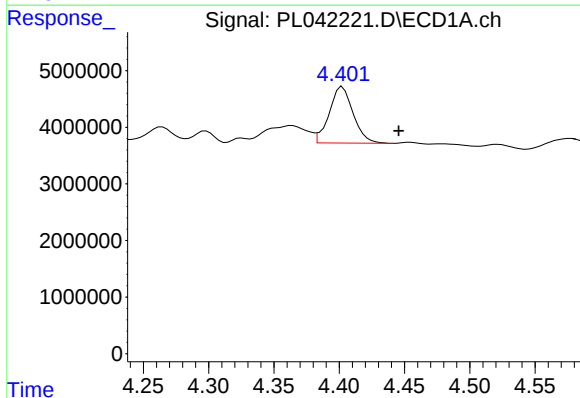


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: -0.043 min
Response: 12678994
Conc: 3.44 ng/ml

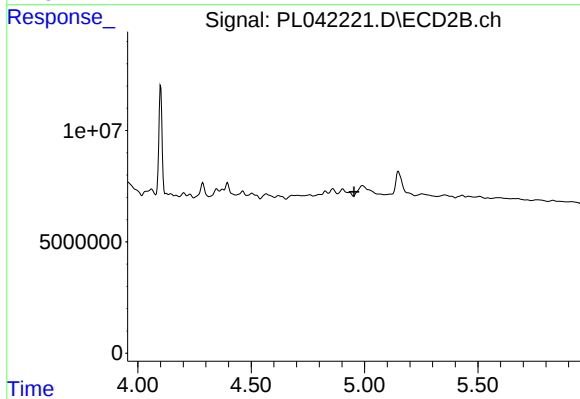

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

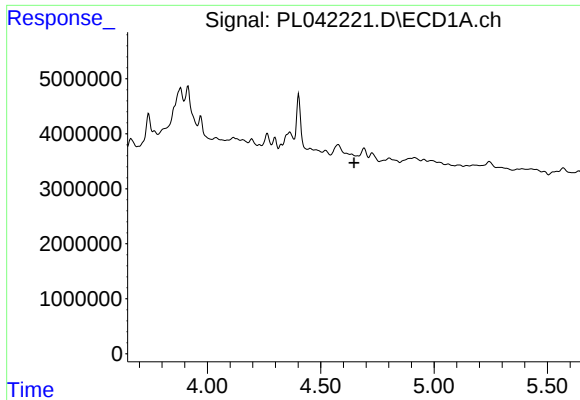

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

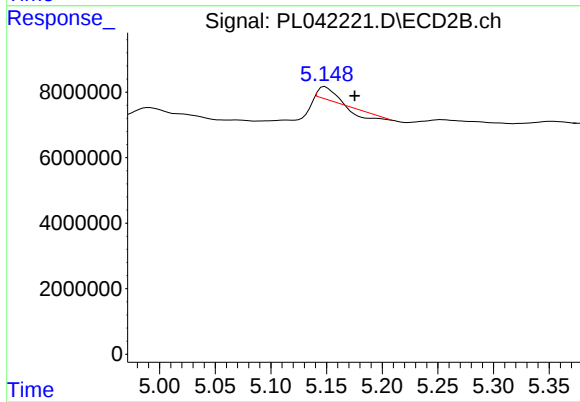


#7 delta-BHC

R.T.: 5.149 min
Delta R.T.: -0.027 min
Response: 18351
Conc: 0.00 ng/ml

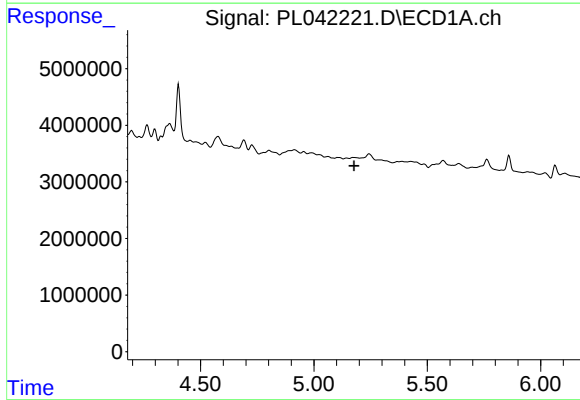


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

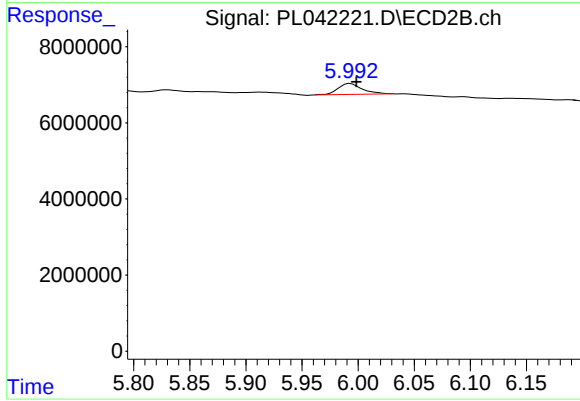

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.005 min
Response: 4351310
Conc: 1.21 ng/ml

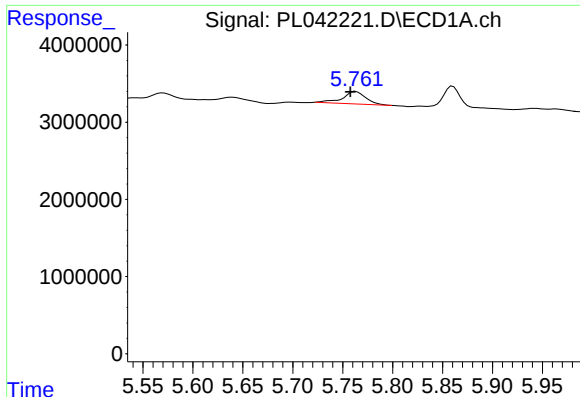

#13 Dieldrin


R.T.: 5.763 min
Delta R.T.: 0.005 min
Response: 2557299
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

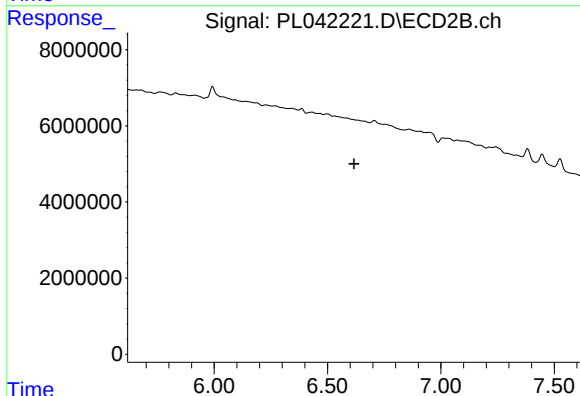


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

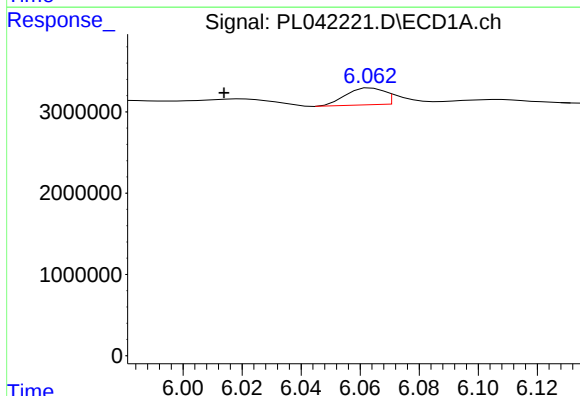


#14 Endrin

R.T.: 6.064 min
Delta R.T.: 0.050 min
Response: 1894474
Conc: 0.27 ng/ml

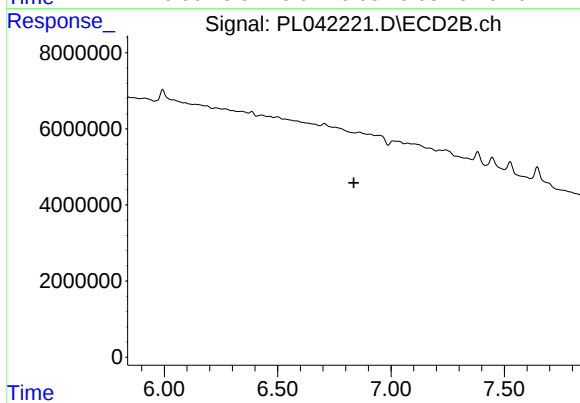

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

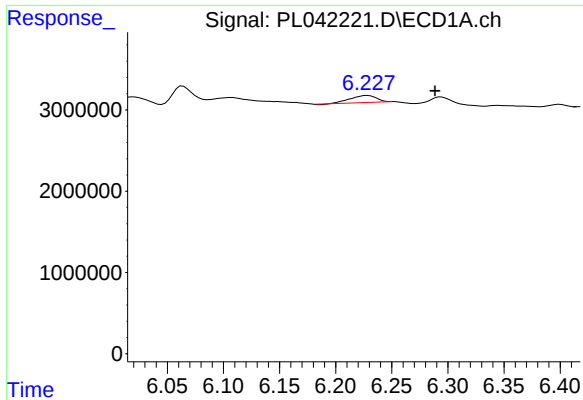

#15 Endosulfan II


R.T.: 6.228 min
Delta R.T.: -0.060 min
Response: 1410551
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

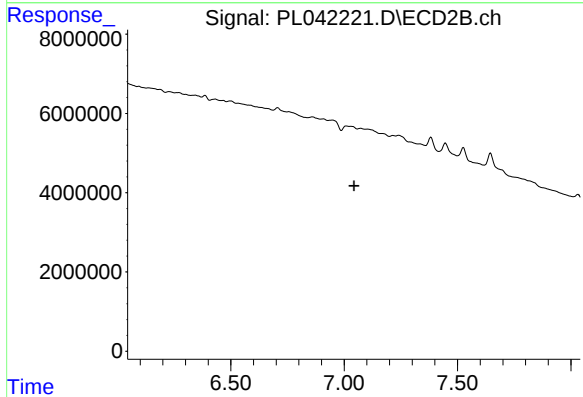


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

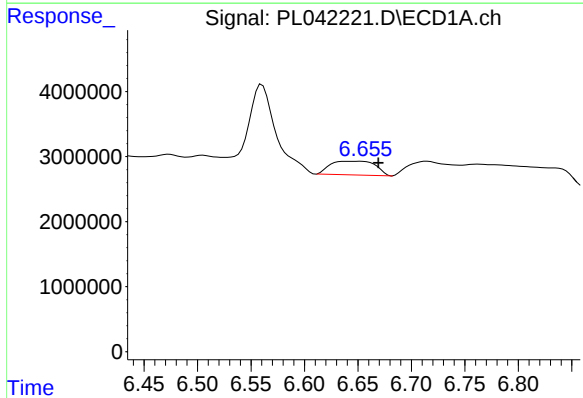


#19 Endosulfan Sulfate

R.T.: 6.653 min
Delta R.T.: -0.016 min
Response: 6165525
Conc: 0.97 ng/ml

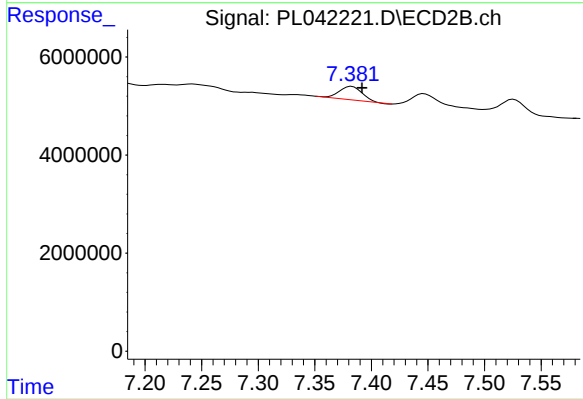

#19 Endosulfan Sulfate


R.T.: 7.383 min
Delta R.T.: -0.009 min
Response: 3818757
Conc: 1.40 ng/ml

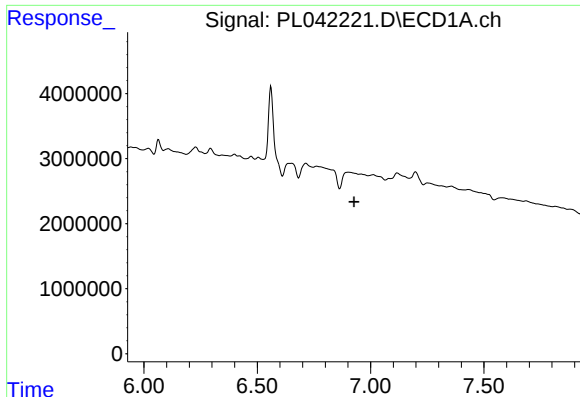

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

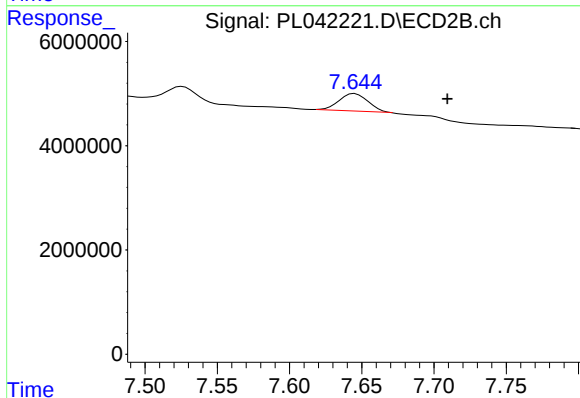


#20 Methoxychlor

R.T.: 7.645 min
Delta R.T.: -0.064 min
Response: 4295833
Conc: 3.13 ng/ml

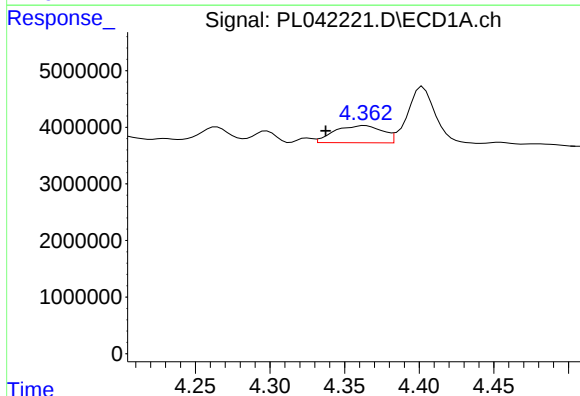


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.026 min
Response: 6771941
Conc: 22.69 ng/ml

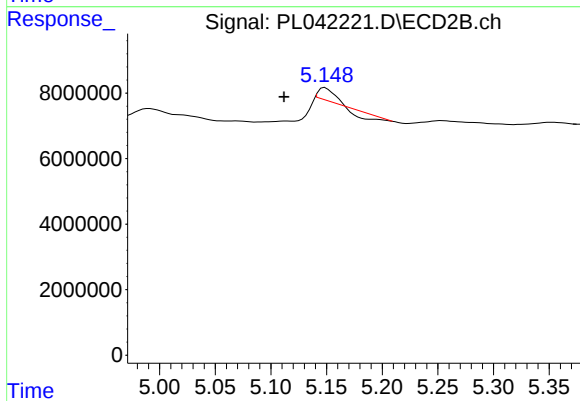

#23 Chlordane-1


R.T.: 5.149 min
Delta R.T.: 0.037 min
Response: 18351
Conc: 0.13 ng/ml

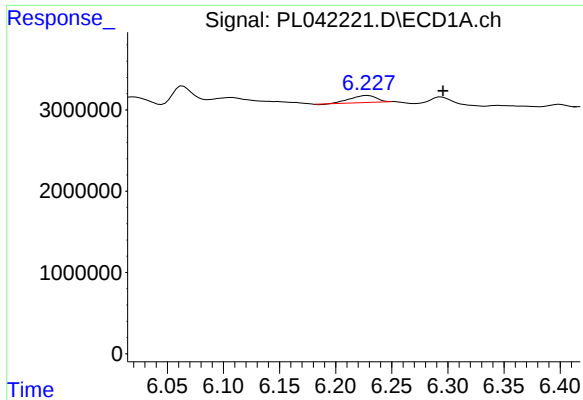

#27 Chlordane-5


R.T.: 6.228 min
Delta R.T.: -0.067 min
Response: 1410551
Conc: 5.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

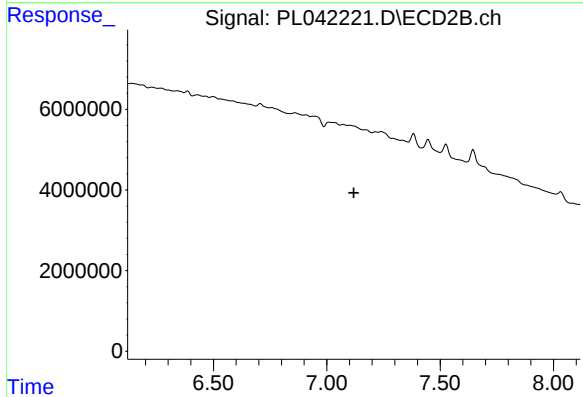


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

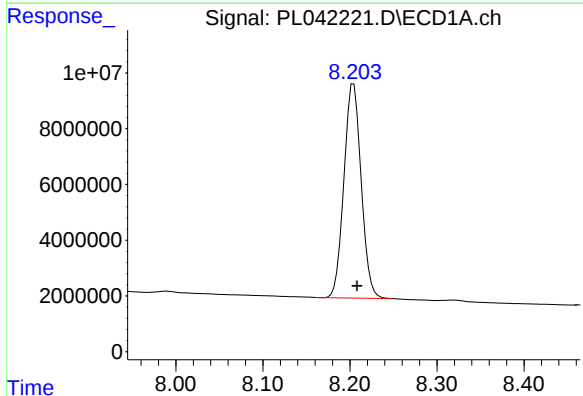

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.004 min
Response: 105660009
Conc: 15.42 ng/ml

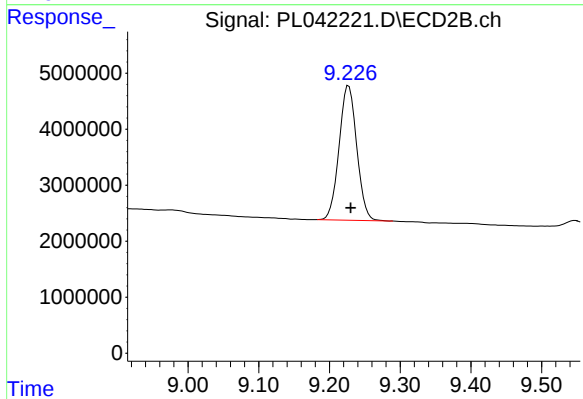

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: -0.003 min
Response: 41701948
Conc: 16.35 ng/ml