

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
 Data File : PL079138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 13:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 14:07:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 14:06:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.567	159.1E6	232.4E6	74.484	73.469
28)	SA Decachlor...	8.771	7.635	119.1E6	148.0E6	73.751	72.705
Target Compounds							
23)	Chlordane-1	4.469	3.532	65078687	73728352	747.920	726.776
24)	Chlordane-2	5.002	4.098	71968593	74308024	729.374	721.763
25)	Chlordane-3	5.712	4.718	293.1E6	232.7E6	761.205	738.867
26)	Chlordane-4	5.790	4.777	355.6E6	248.9E6	750.971	733.136
27)	Chlordane-5	6.646	5.439	57412700	63527893	759.432	737.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
Data File : PL079138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 13:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 14:07:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 14:06:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

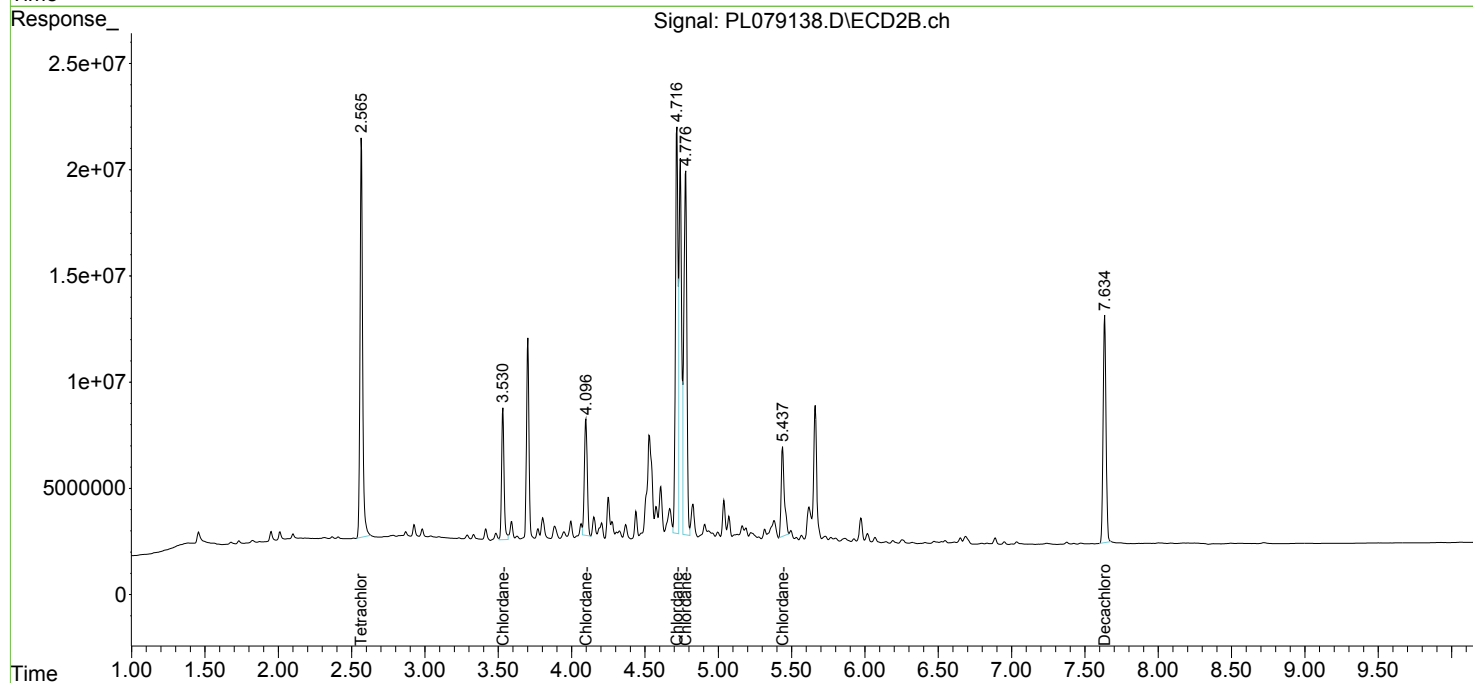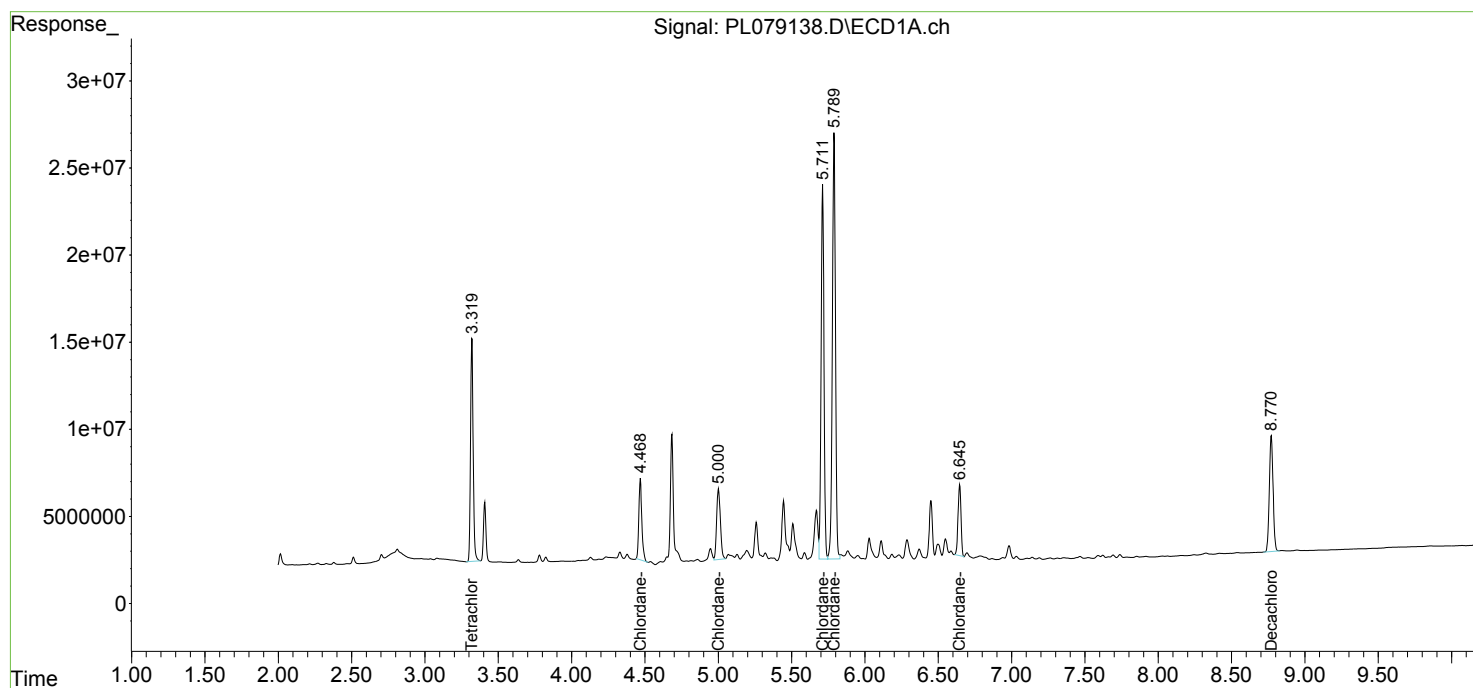


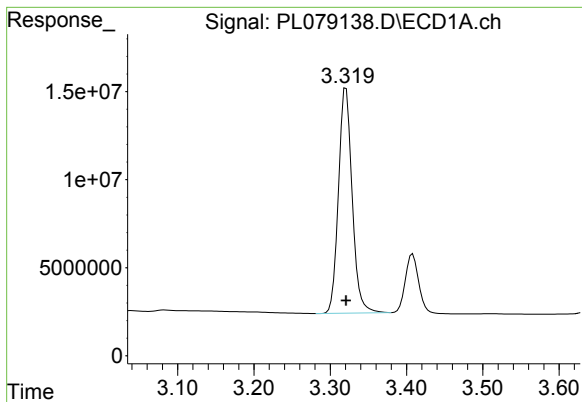

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 159087690
Conc: 74.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

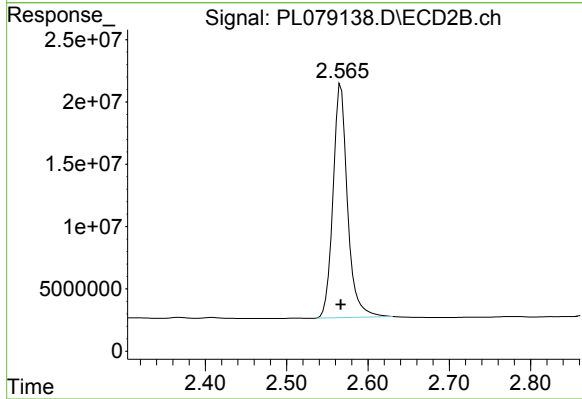


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: 0.000 min
Response: 232411856
Conc: 73.47 ng/ml

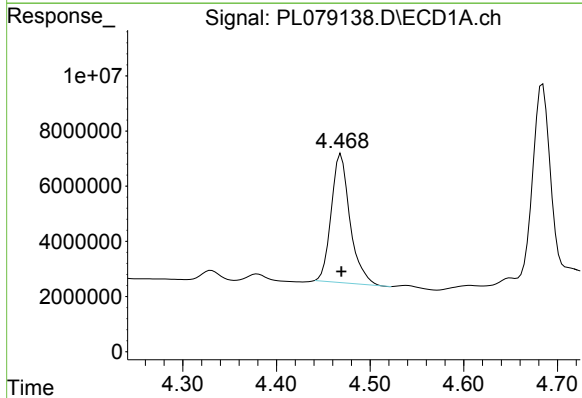


#23 Chlordane-1

R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 65078687
Conc: 747.92 ng/ml

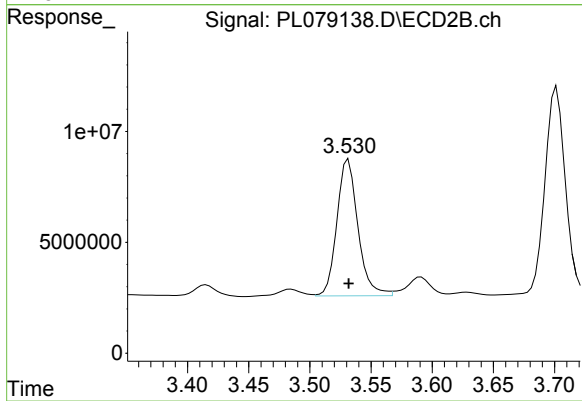

#23 Chlordane-1


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 73728352
Conc: 726.78 ng/ml

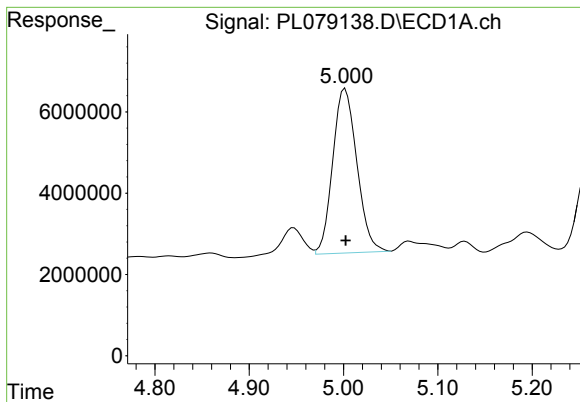

#24 Chlordane-2


R.T.: 5.002 min
Delta R.T.: 0.000 min
Response: 71968593
Conc: 729.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

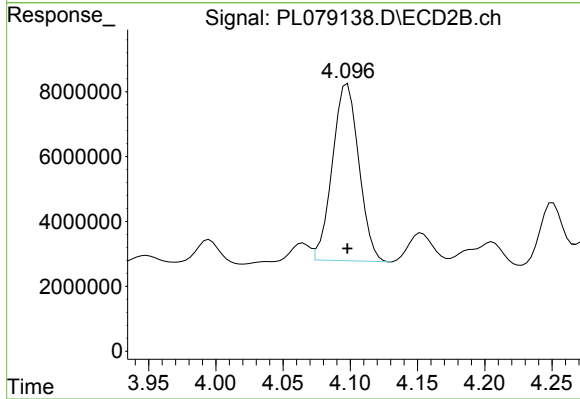


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 74308024
Conc: 721.76 ng/ml

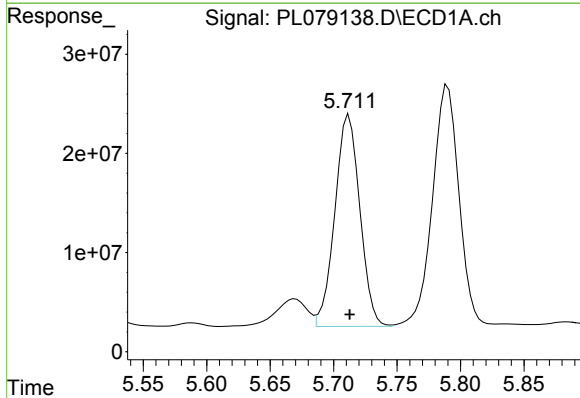


#25 Chlordane-3

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 293050576
Conc: 761.21 ng/ml

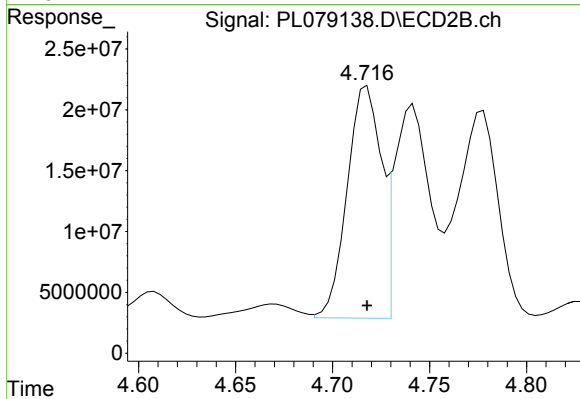

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 232735488
Conc: 738.87 ng/ml

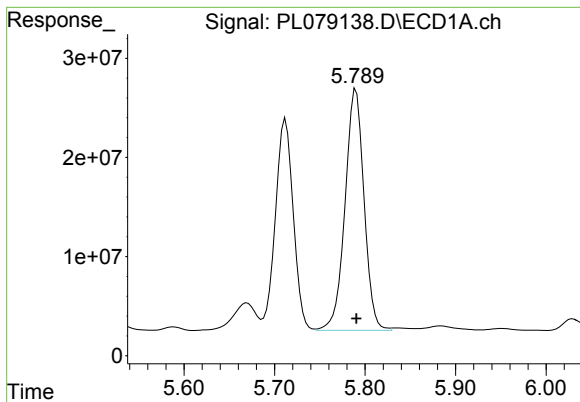

#26 Chlordane-4


R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 355622965
Conc: 750.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

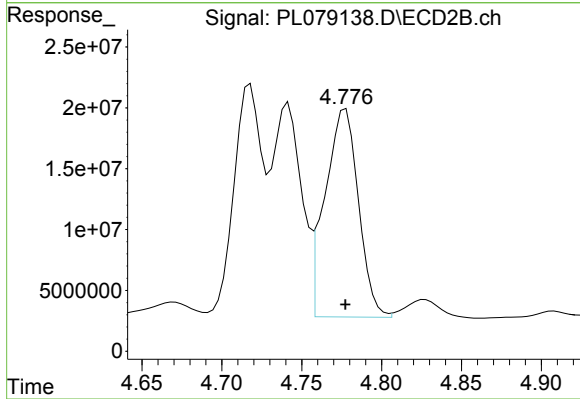


#26 Chlordane-4

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 248885290
Conc: 733.14 ng/ml

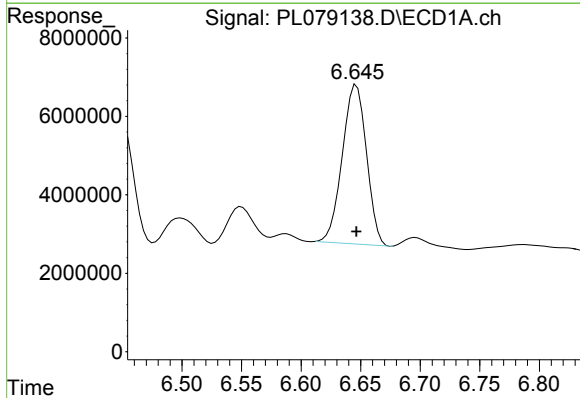


#27 Chlordane-5

R.T.: 6.646 min
Delta R.T.: 0.000 min
Response: 57412700
Conc: 759.43 ng/ml

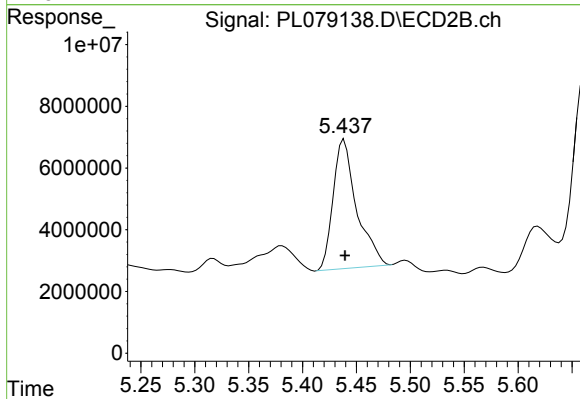

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 63527893
Conc: 737.68 ng/ml

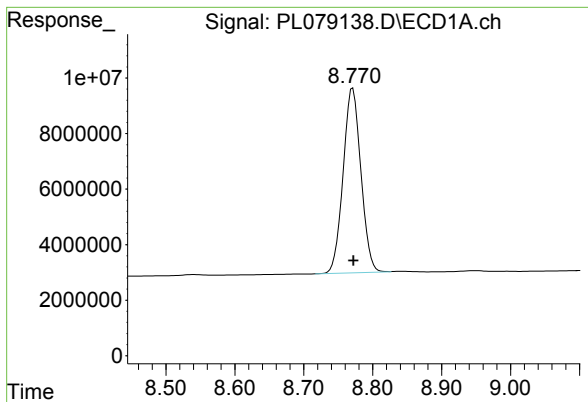

#28 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.001 min
Response: 119075506
Conc: 73.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

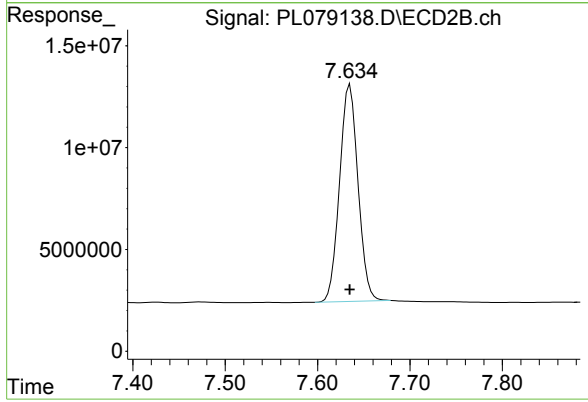

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 148049538
Conc: 72.71 ng/ml