

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
 Data File : PL079148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 15:39
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL111622CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 16:18:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:29:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.567	105.2E6	155.3E6	49.213	48.827
28)	SA Decachlor...	8.770	7.635	81163162	103.0E6	49.878	49.275
Target Compounds							
23)	Chlordane-1	4.469	3.531	43878598	49863222	500.771	482.619
24)	Chlordane-2	5.002	4.097	49255588	51286077	483.915	482.947
25)	Chlordane-3	5.713	4.717	193.2E6	155.8E6	501.650	488.900
26)	Chlordane-4	5.790	4.777	235.4E6	167.5E6	497.534	488.007
27)	Chlordane-5	6.646	5.439	38569535	43105631	519.838	505.525



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
Data File : PL079148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 15:39
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL111622CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 16:18:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:29:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

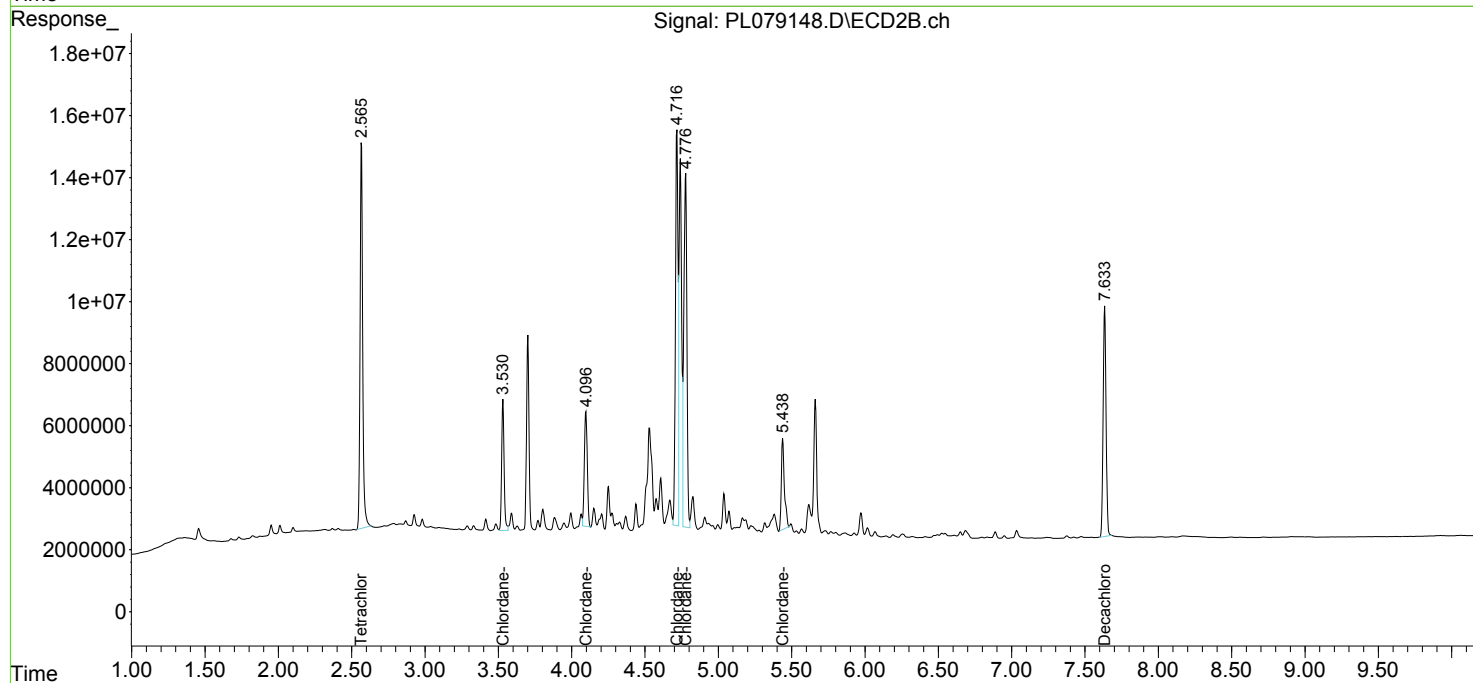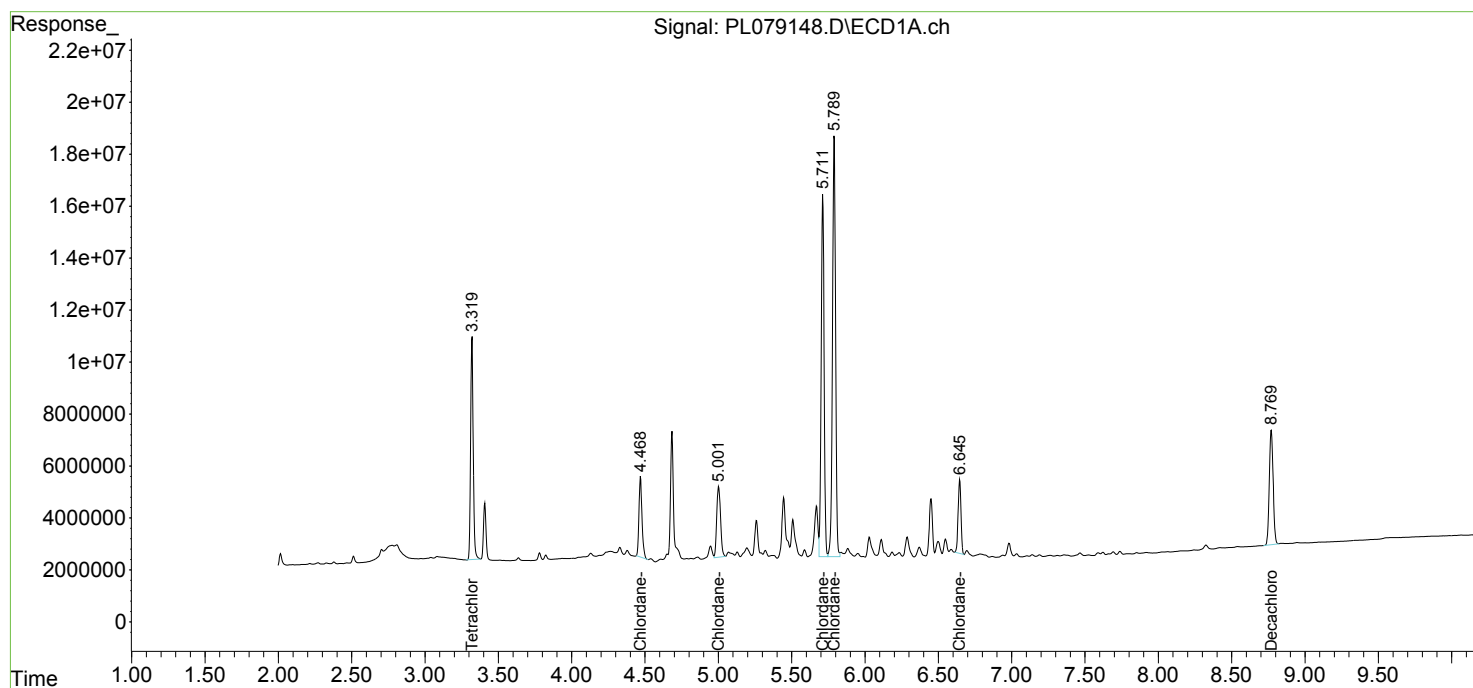


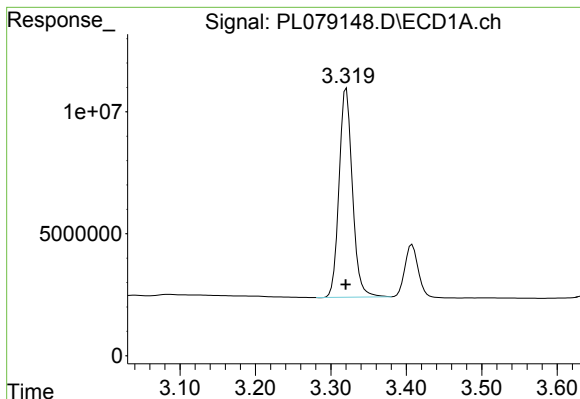

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 105237654
Conc: 49.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111622CHLOR

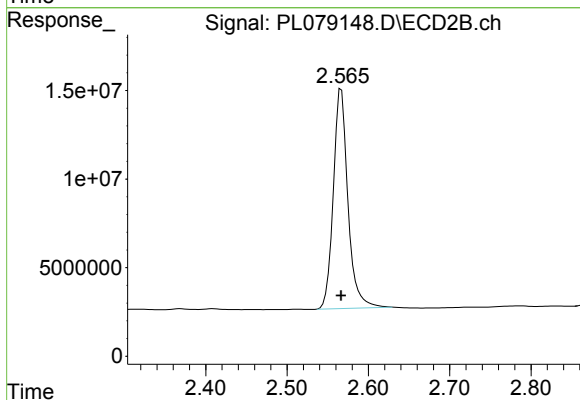


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: 0.000 min
Response: 155323486
Conc: 48.83 ng/ml

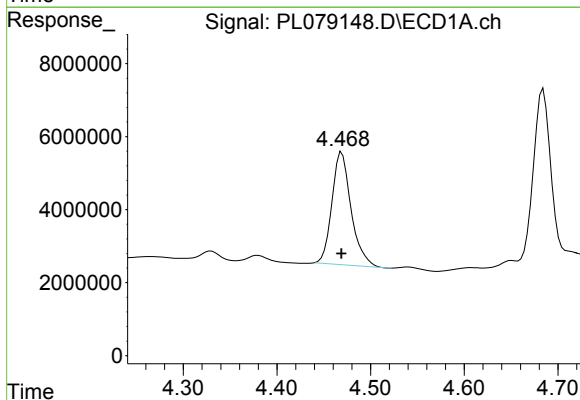


#23 Chlordane-1

R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 43878598
Conc: 500.77 ng/ml

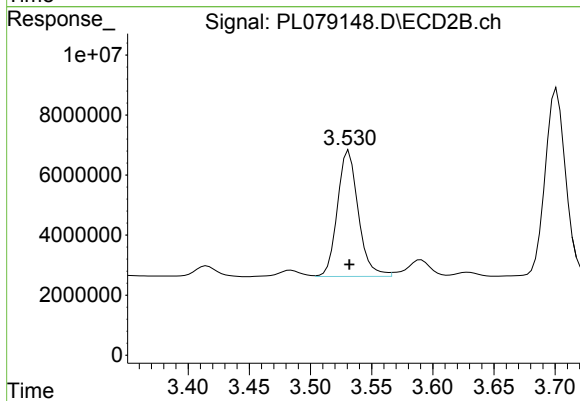

#23 Chlordane-1


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 49863222
Conc: 482.62 ng/ml

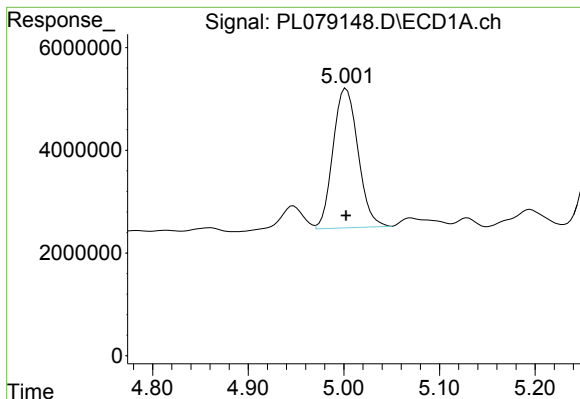

#24 Chlordane-2


R.T.: 5.002 min
Delta R.T.: 0.000 min
Response: 49255588
Conc: 483.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111622CHLOR

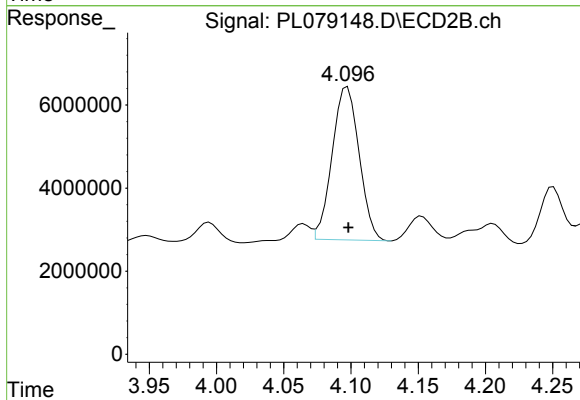


#24 Chlordane-2

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 51286077
Conc: 482.95 ng/ml

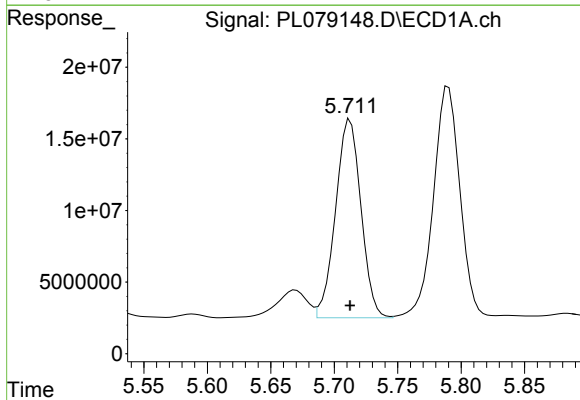


#25 Chlordane-3

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 193236392
Conc: 501.65 ng/ml

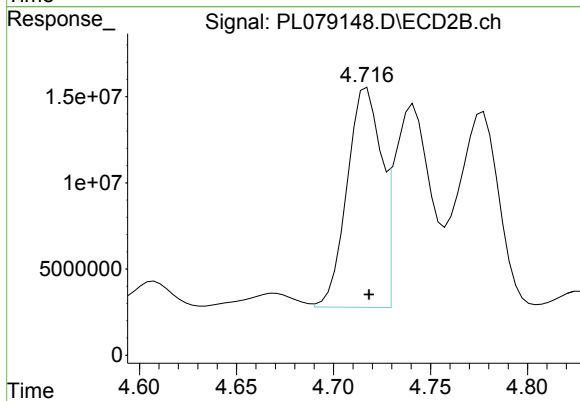

#25 Chlordane-3


R.T.: 4.717 min
Delta R.T.: -0.001 min
Response: 155770953
Conc: 488.90 ng/ml

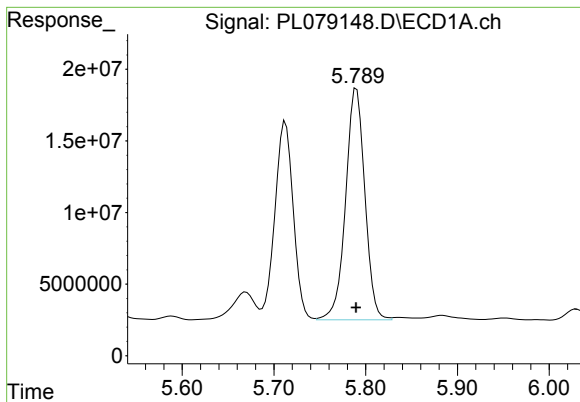

#26 Chlordane-4


R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 235414516
Conc: 497.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111622CHLOR

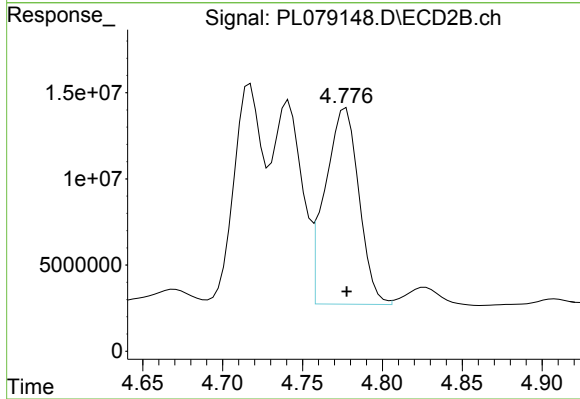


#26 Chlordane-4

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 167465989
Conc: 488.01 ng/ml

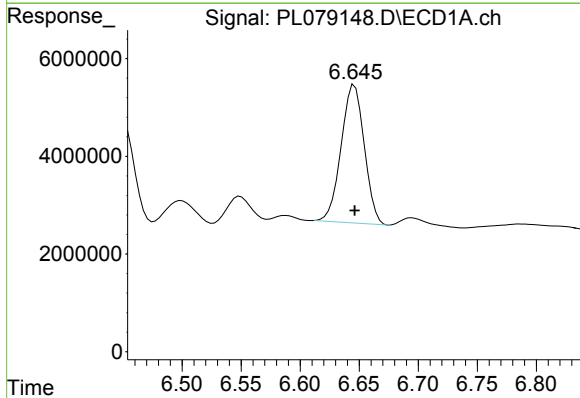


#27 Chlordane-5

R.T.: 6.646 min
Delta R.T.: 0.000 min
Response: 38569535
Conc: 519.84 ng/ml

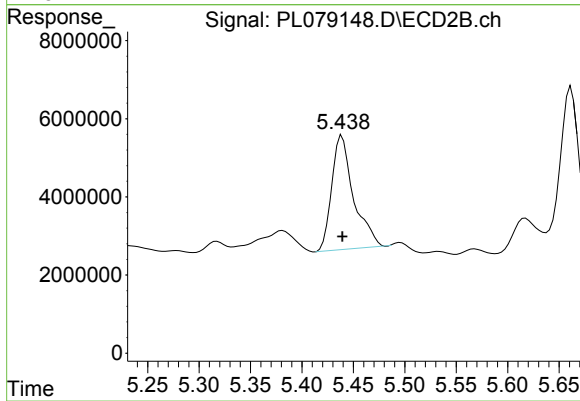

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 43105631
Conc: 505.53 ng/ml

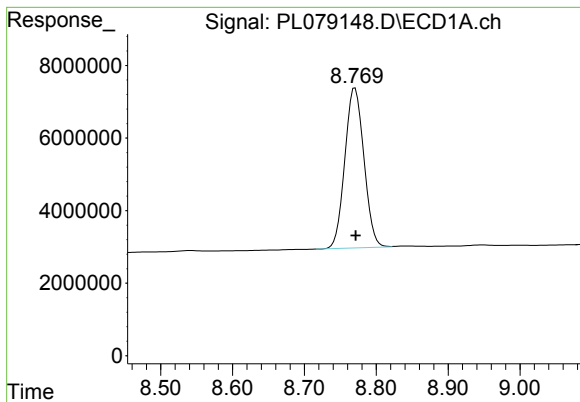

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: 0.000 min
Response: 81163162
Conc: 49.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111622CHLOR

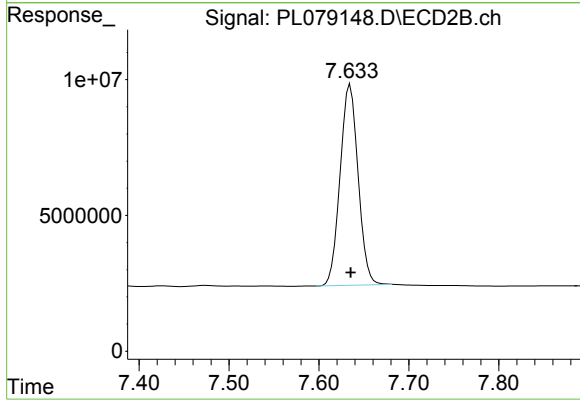

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 102987093
Conc: 49.27 ng/ml