

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
 Data File : PL079154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 17:32
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:39:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.567	104.8E6	150.5E6	50.314	59.077
28)	SA Decachlor...	8.772	7.636	79542751	99086274	47.552	47.765
Target Compounds							
23)	Chlordane-1	4.470	3.532	43501290	48679924	496.465	471.166
24)	Chlordane-2	5.003	4.098	48746264	49910146	478.911	469.991
25)	Chlordane-3	5.712	4.718	190.8E6	151.5E6	495.309	475.510
26)	Chlordane-4	5.790	4.778	232.3E6	162.6E6	490.883	473.873
27)	Chlordane-5	6.645	5.440	37894996	41945818	510.746	491.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
Data File : PL079154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 17:32
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:39:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

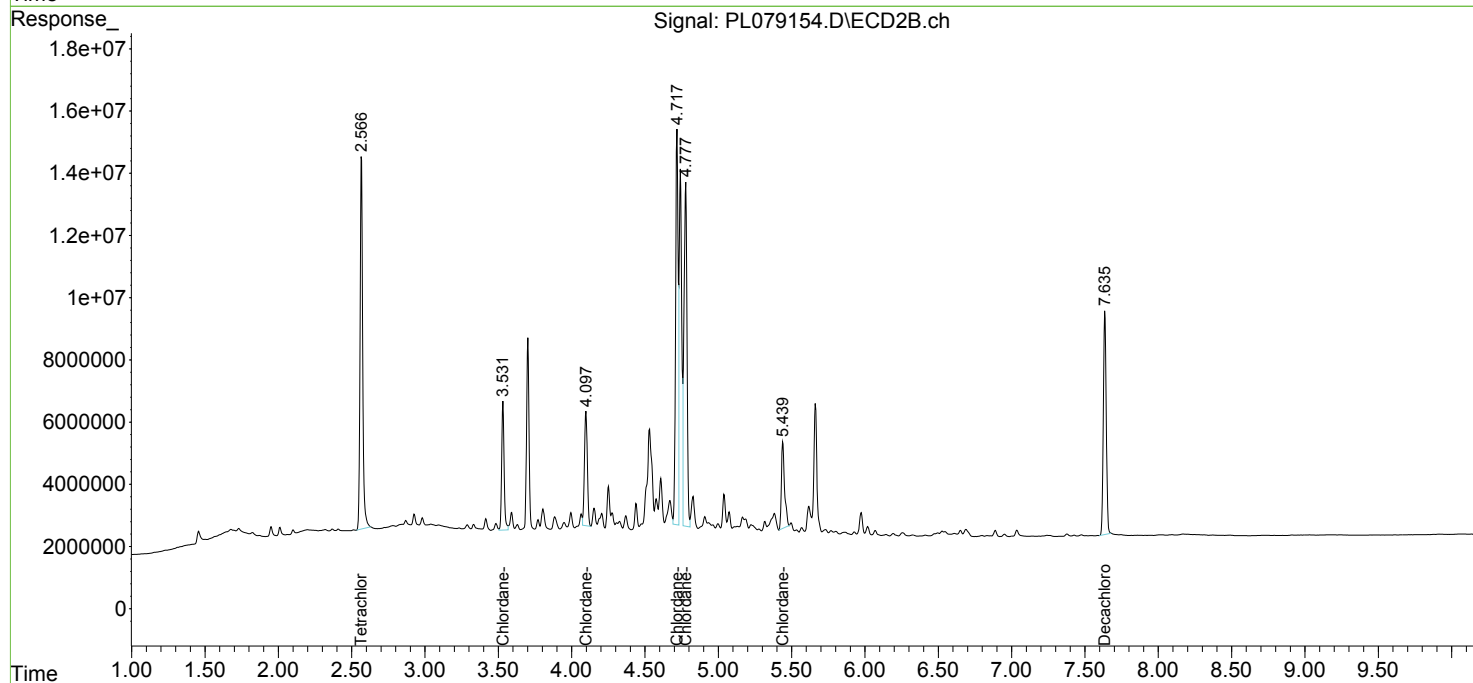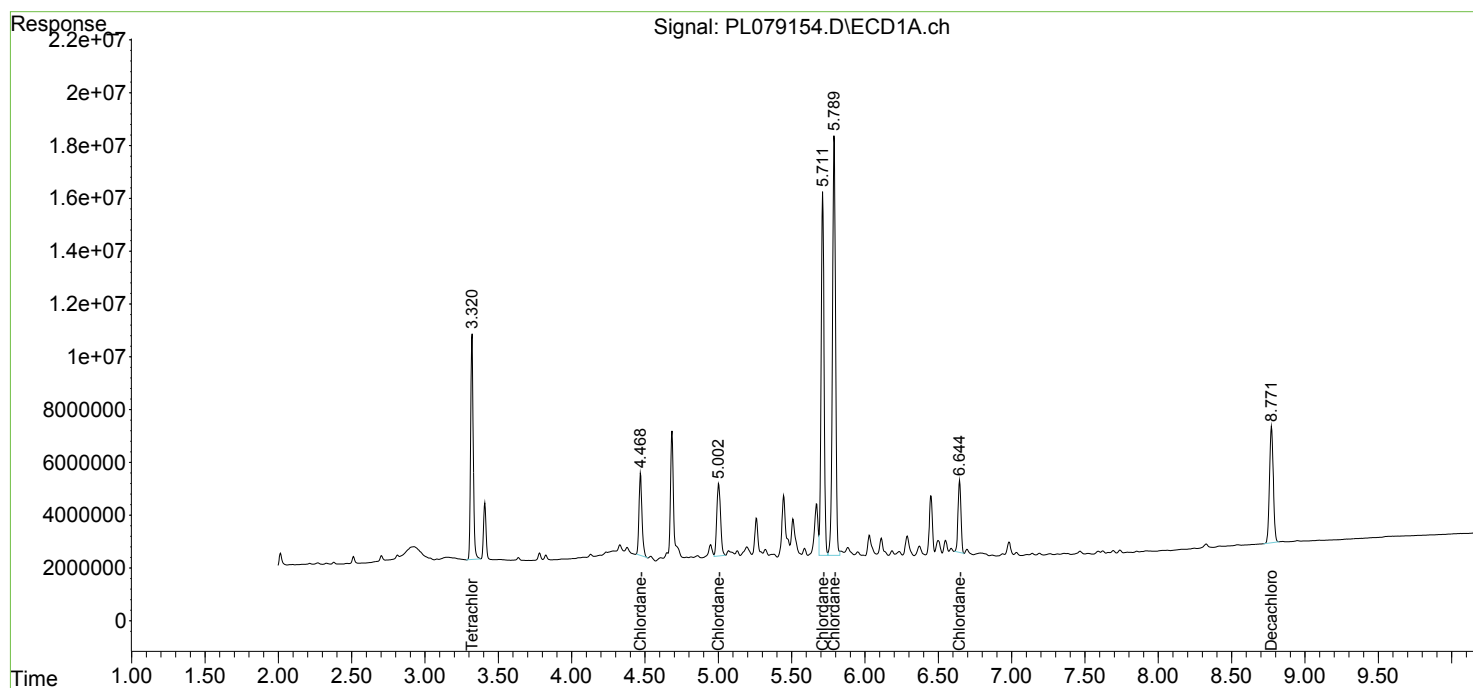


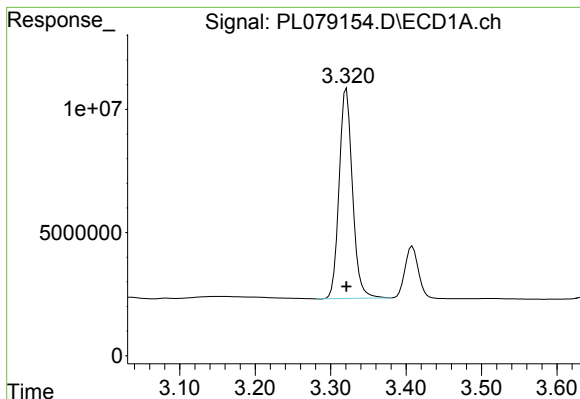

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 104774192
Conc: 50.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

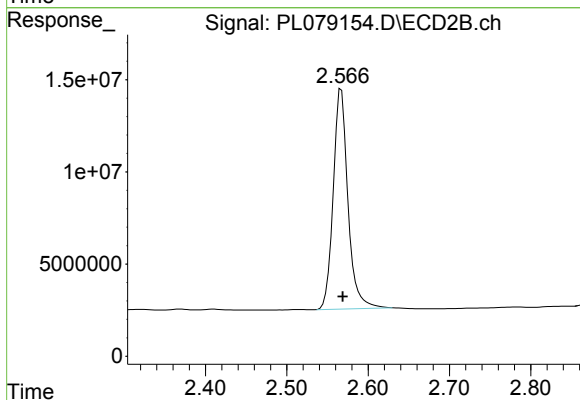


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.002 min
Response: 150461848
Conc: 59.08 ng/ml

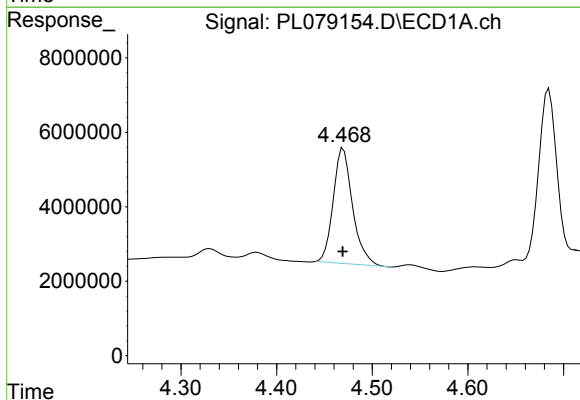


#23 Chlordane-1

R.T.: 4.470 min
Delta R.T.: 0.000 min
Response: 43501290
Conc: 496.46 ng/ml

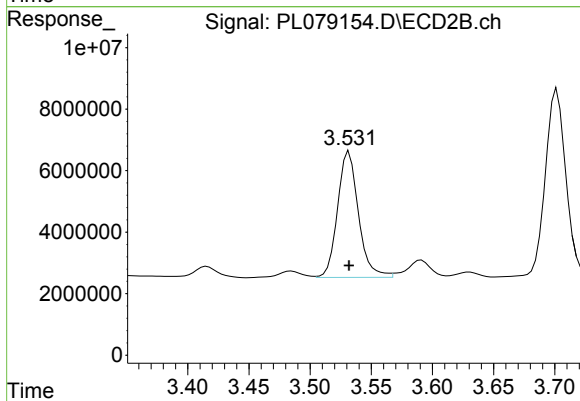

#23 Chlordane-1


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 48679924
Conc: 471.17 ng/ml

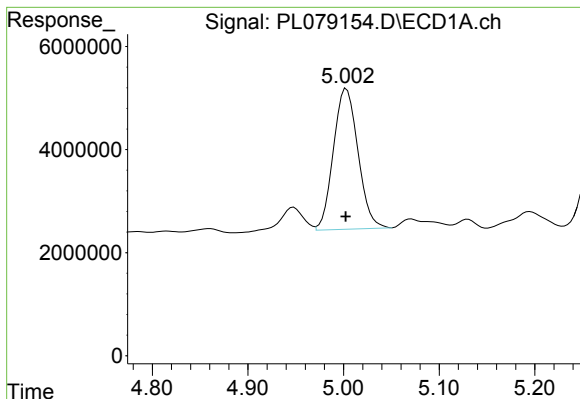

#24 Chlordane-2


R.T.: 5.003 min
Delta R.T.: 0.000 min
Response: 48746264
Conc: 478.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

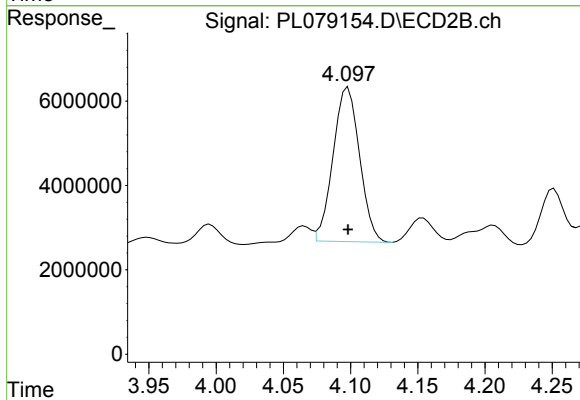


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 49910146
Conc: 469.99 ng/ml

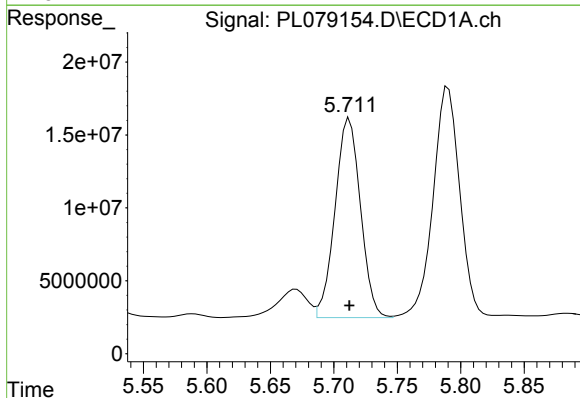


#25 Chlordane-3

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 190793943
Conc: 495.31 ng/ml

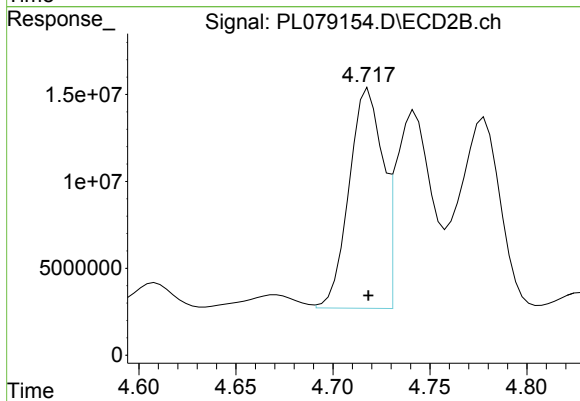

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 151504866
Conc: 475.51 ng/ml

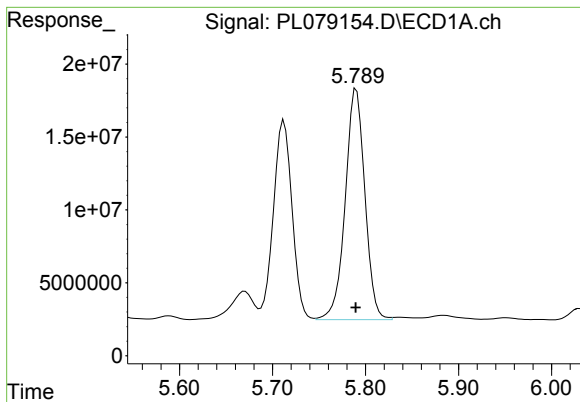

#26 Chlordane-4


R.T.: 5.790 min
Delta R.T.: 0.000 min
Response: 232267511
Conc: 490.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

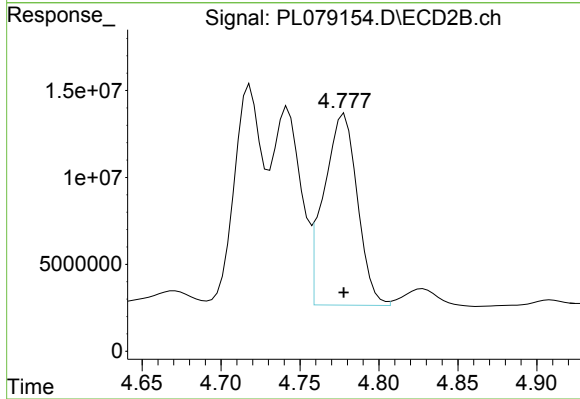


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 162615717
Conc: 473.87 ng/ml

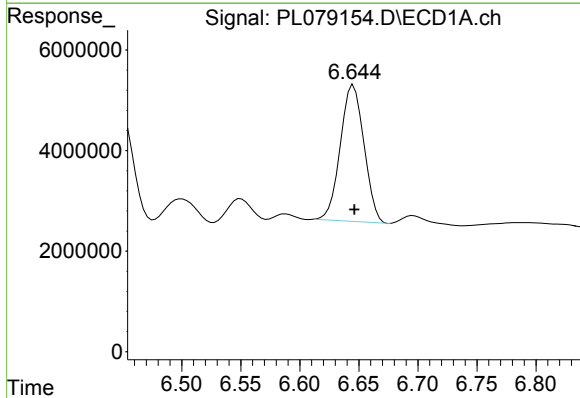


#27 Chlordane-5

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 37894996
Conc: 510.75 ng/ml

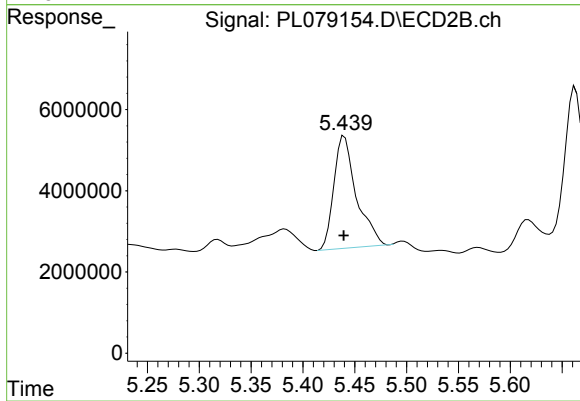

#27 Chlordane-5


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 41945818
Conc: 491.92 ng/ml

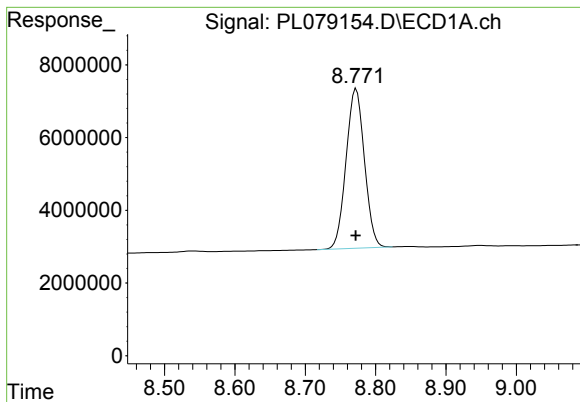

#28 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: 0.000 min
Response: 79542751
Conc: 47.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

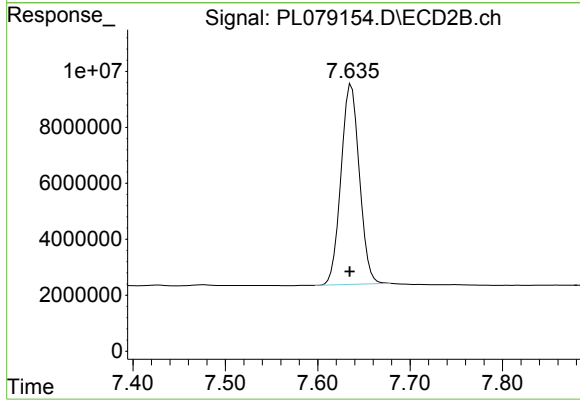

#28 Decachlorobiphenyl

R.T.: 7.636 min
Delta R.T.: 0.002 min
Response: 99086274
Conc: 47.76 ng/ml