

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
 Data File : PL079172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 22:09
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:43:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.566	103.4E6	148.6E6	49.659	58.340
28)	SA Decachlor...	8.771	7.635	81996606	100.3E6	49.019	48.360
Target Compounds							
23)	Chlordane-1	4.468	3.531	43462107	47480607	496.017	459.558
24)	Chlordane-2	5.001	4.098	47757661	48939388	469.198	460.849
25)	Chlordane-3	5.711	4.718	187.3E6	149.3E6	486.341	468.742
26)	Chlordane-4	5.789	4.778	228.9E6	160.9E6	483.815	468.927
27)	Chlordane-5	6.646	5.439	37299311	41063273	502.718	481.573



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111622\
Data File : PL079172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 22:09
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:43:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

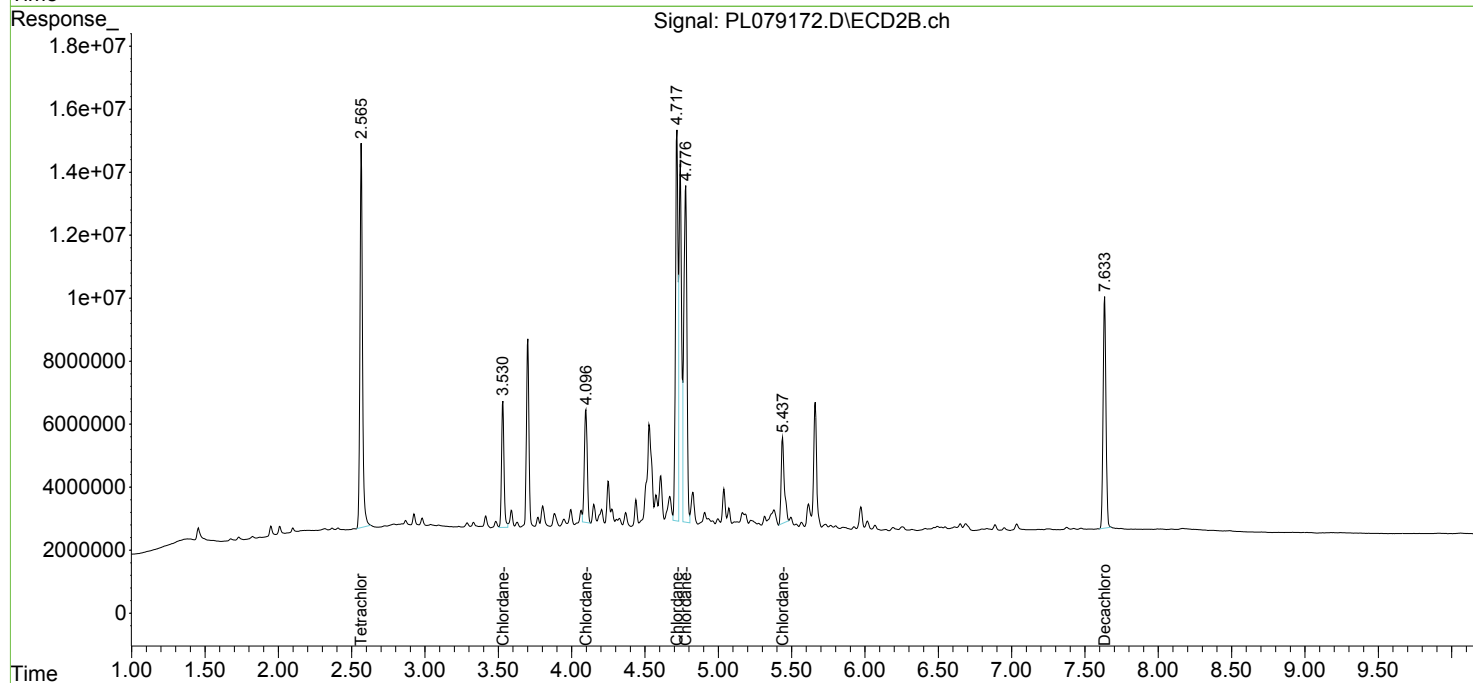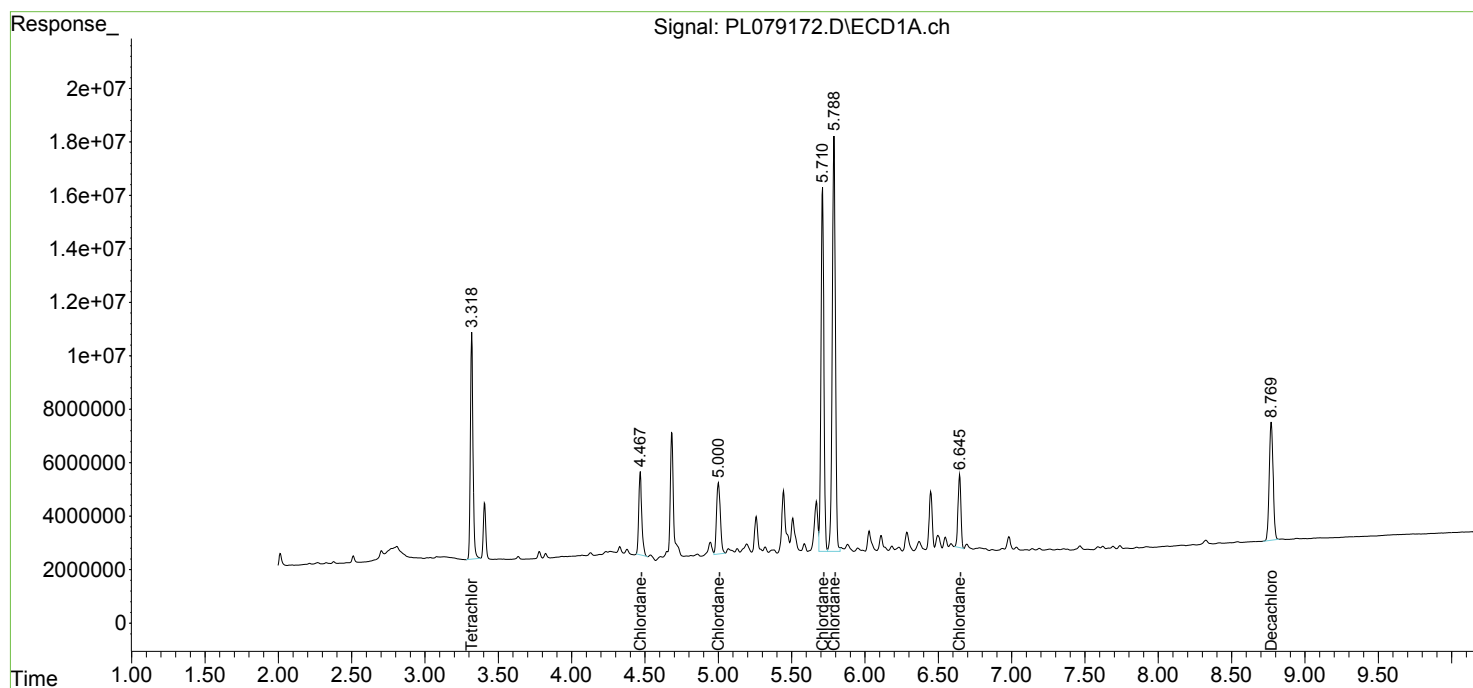


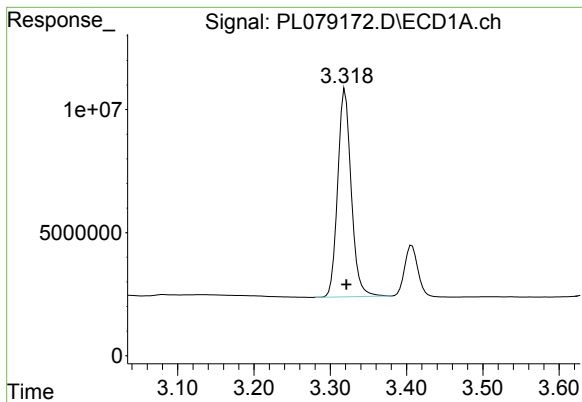

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 103410487
Conc: 49.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

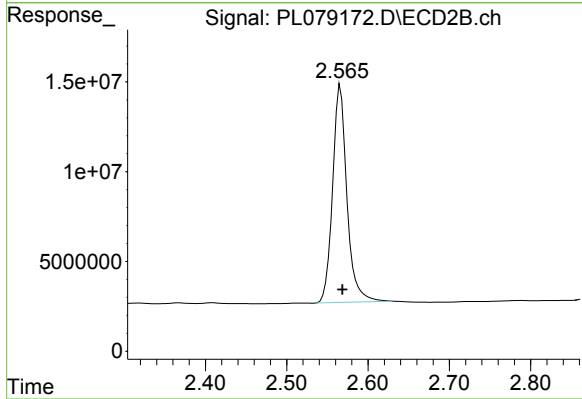


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.002 min
Response: 148583789
Conc: 58.34 ng/ml

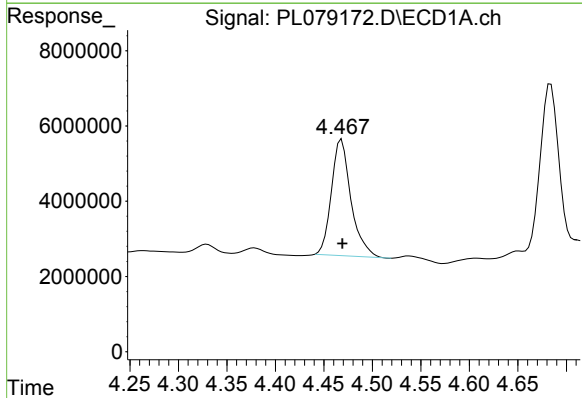


#23 Chlordane-1

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 43462107
Conc: 496.02 ng/ml

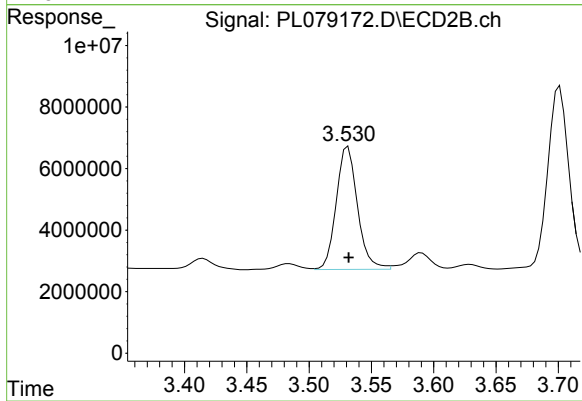

#23 Chlordane-1


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 47480607
Conc: 459.56 ng/ml

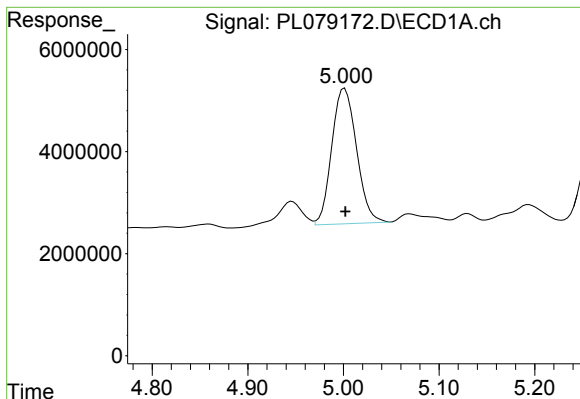

#24 Chlordane-2


R.T.: 5.001 min
Delta R.T.: -0.001 min
Response: 47757661
Conc: 469.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

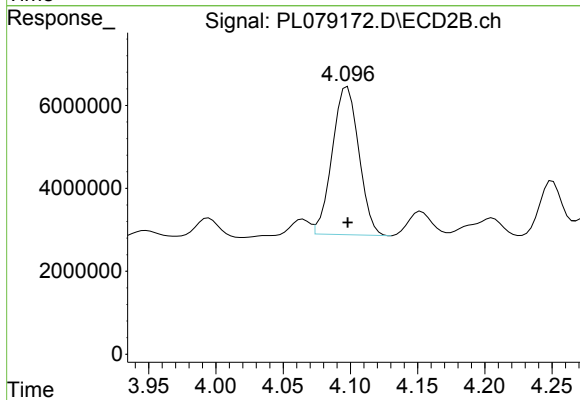


#24 Chlordane-2

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 48939388
Conc: 460.85 ng/ml

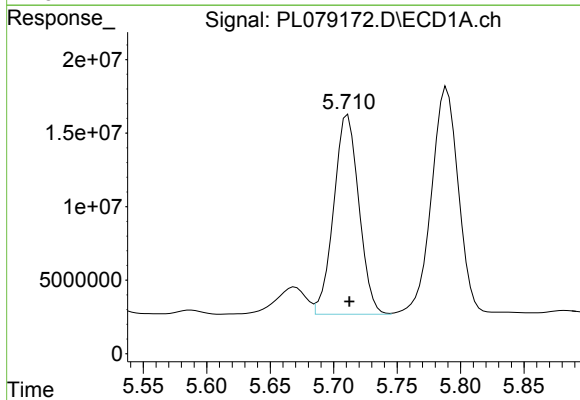


#25 Chlordane-3

R.T.: 5.711 min
Delta R.T.: -0.001 min
Response: 187339526
Conc: 486.34 ng/ml

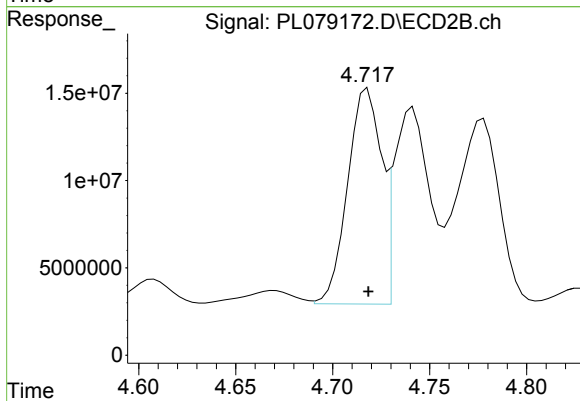

#25 Chlordane-3


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 149348507
Conc: 468.74 ng/ml

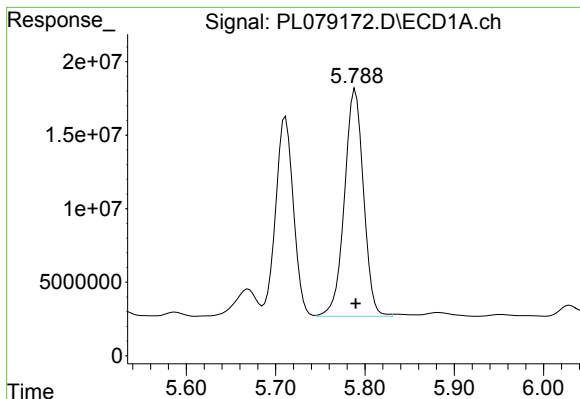

#26 Chlordane-4


R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 228923071
Conc: 483.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

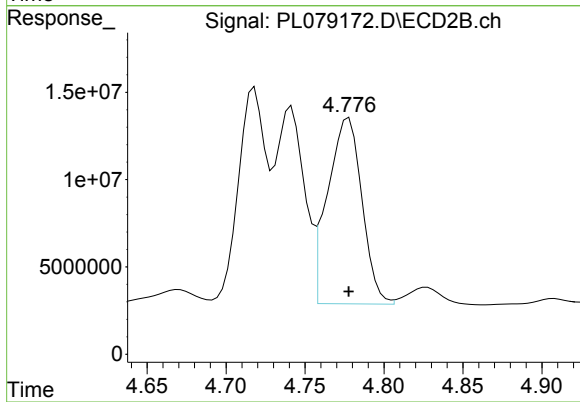


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 160918309
Conc: 468.93 ng/ml

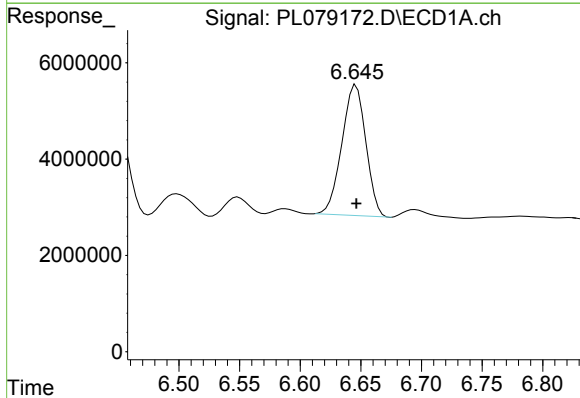


#27 Chlordane-5

R.T.: 6.646 min
Delta R.T.: 0.000 min
Response: 37299311
Conc: 502.72 ng/ml

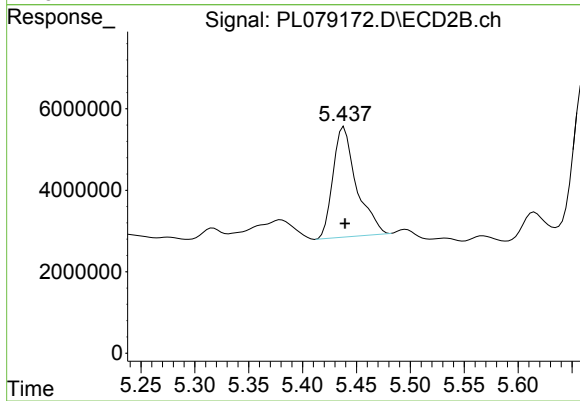

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 41063273
Conc: 481.57 ng/ml

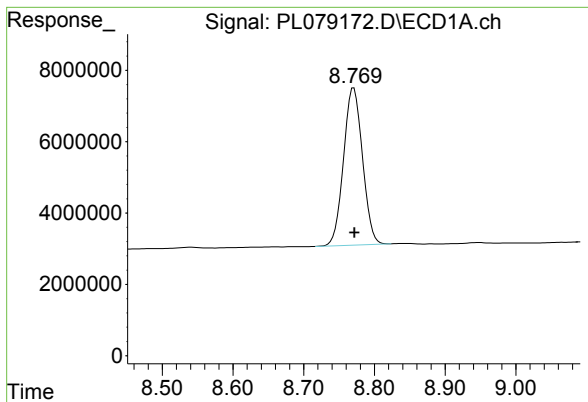

#28 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 81996606
Conc: 49.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

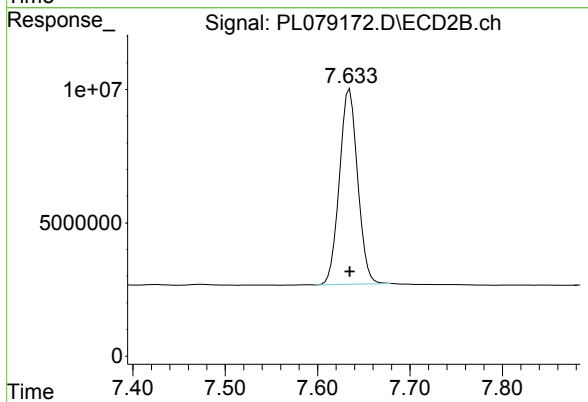

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 100322123
Conc: 48.36 ng/ml