

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111623\
 Data File : PL086690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2023 13:51
 Operator : AR\AJ
 Sample : PB157196BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB157196BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/17/2023
 Supervised By :Ankita Jodhani 11/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 19:48:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.363	2.617	53055233	16240333	16.340	16.494
28) SA Decachlor...	8.866	7.771	55268085	23411640	18.881m	19.387

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111623\
Data File : PL086690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2023 13:51
Operator : AR\AJ
Sample : PB157196BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB157196BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/17/2023
Supervised By : Ankita Jodhani 11/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 19:48:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

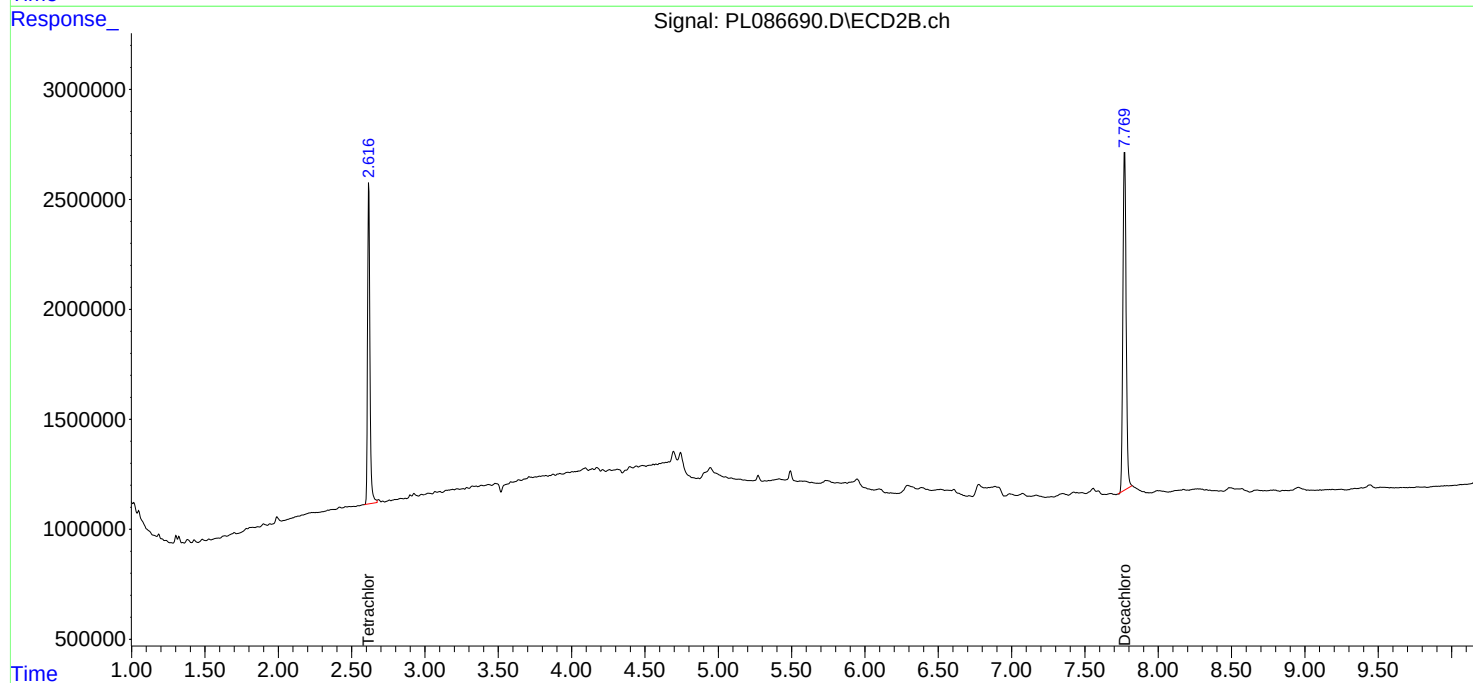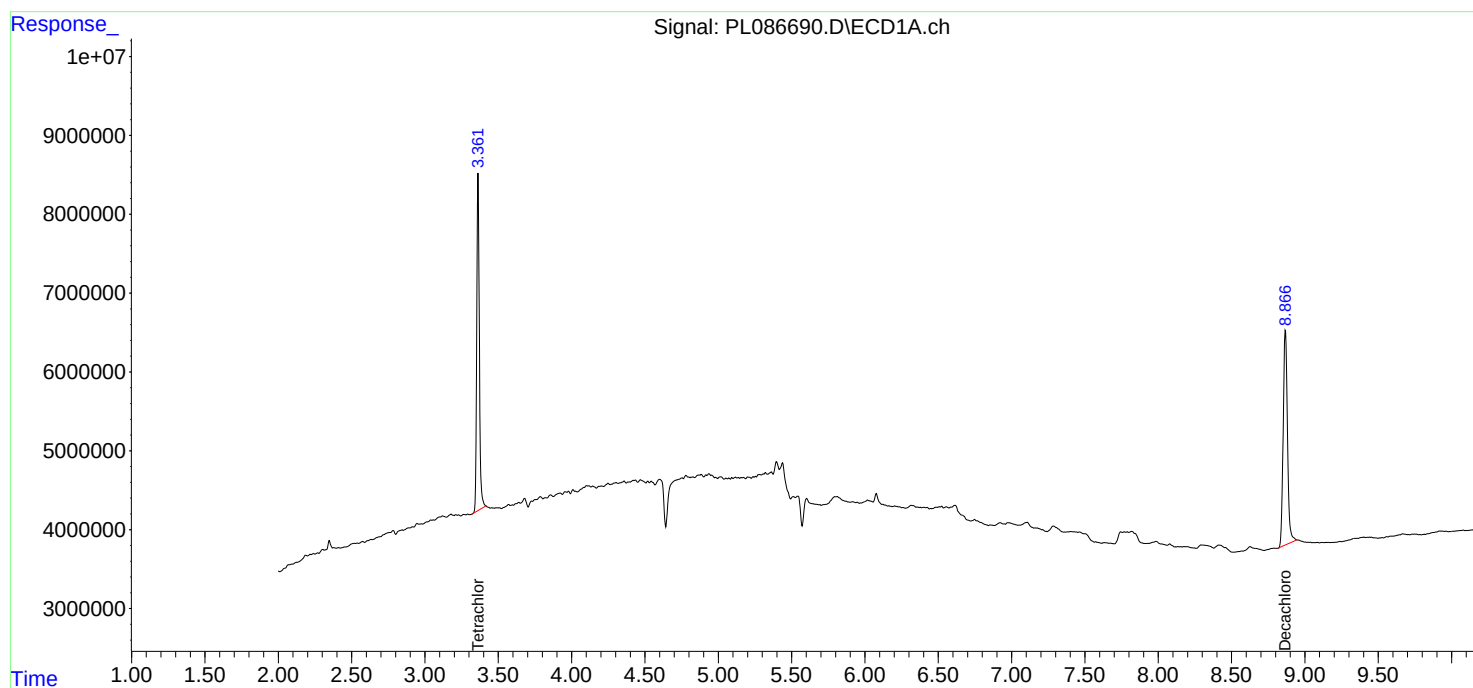

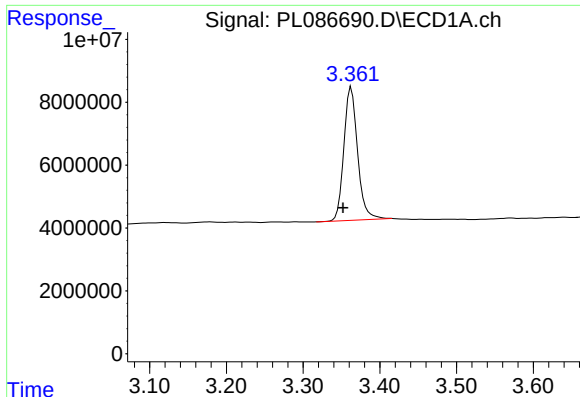


#1 Tetrachloro-m-xylene

R.T.: 3.363 min
Delta R.T.: 0.011 min
Response: 53055233
Conc: 16.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB157196BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/17/2023
Supervised By :Ankita Jodhani 11/17/2023

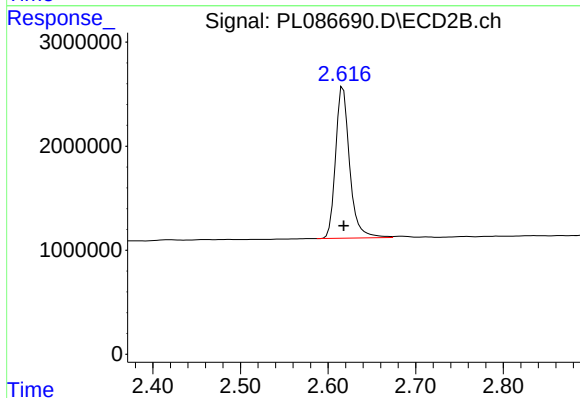


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 16240333
Conc: 16.49 ng/ml

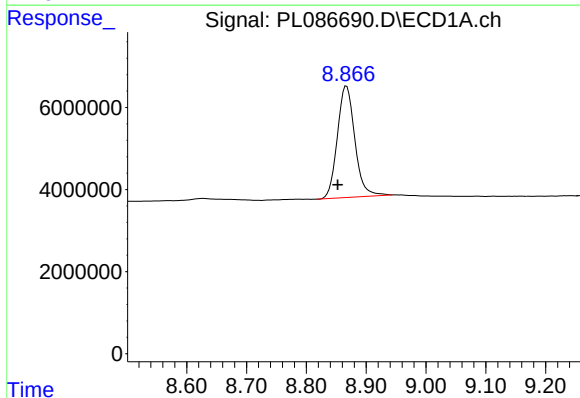

#28 Decachlorobiphenyl

R.T.: 8.866 min
Delta R.T.: 0.013 min
Response: 55268085
Conc: 18.88 ng/ml m

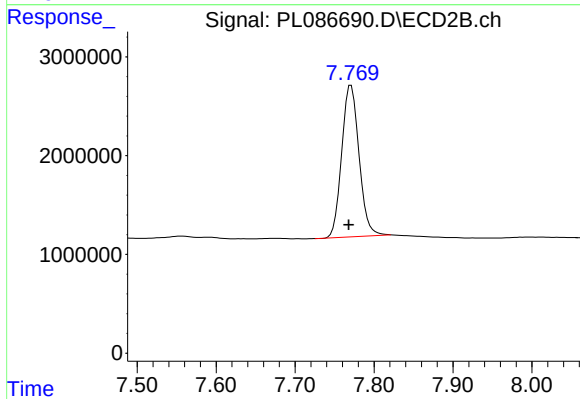

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: 0.003 min
Response: 23411640
Conc: 19.39 ng/ml