

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111623\
 Data File : PL086711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2023 18:54
 Operator : AR\AJ
 Sample : 05432-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/17/2023
 Supervised By :Ankita Jodhani 11/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 20:07:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 13:04:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.618	59108207	18215687	18.204	18.500
2) SA Decachlor...	8.850	7.766	54537662	22004708	18.632	18.222
Target Compounds						
16) A 4,4'-DDD	6.530	5.628	2231418	580903	0.838m	0.682

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111623\
Data File : PL086711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2023 18:54
Operator : AR\AJ
Sample : 05432-05
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/17/2023
Supervised By : Ankita Jodhani 11/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 20:07:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110823.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 13:04:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

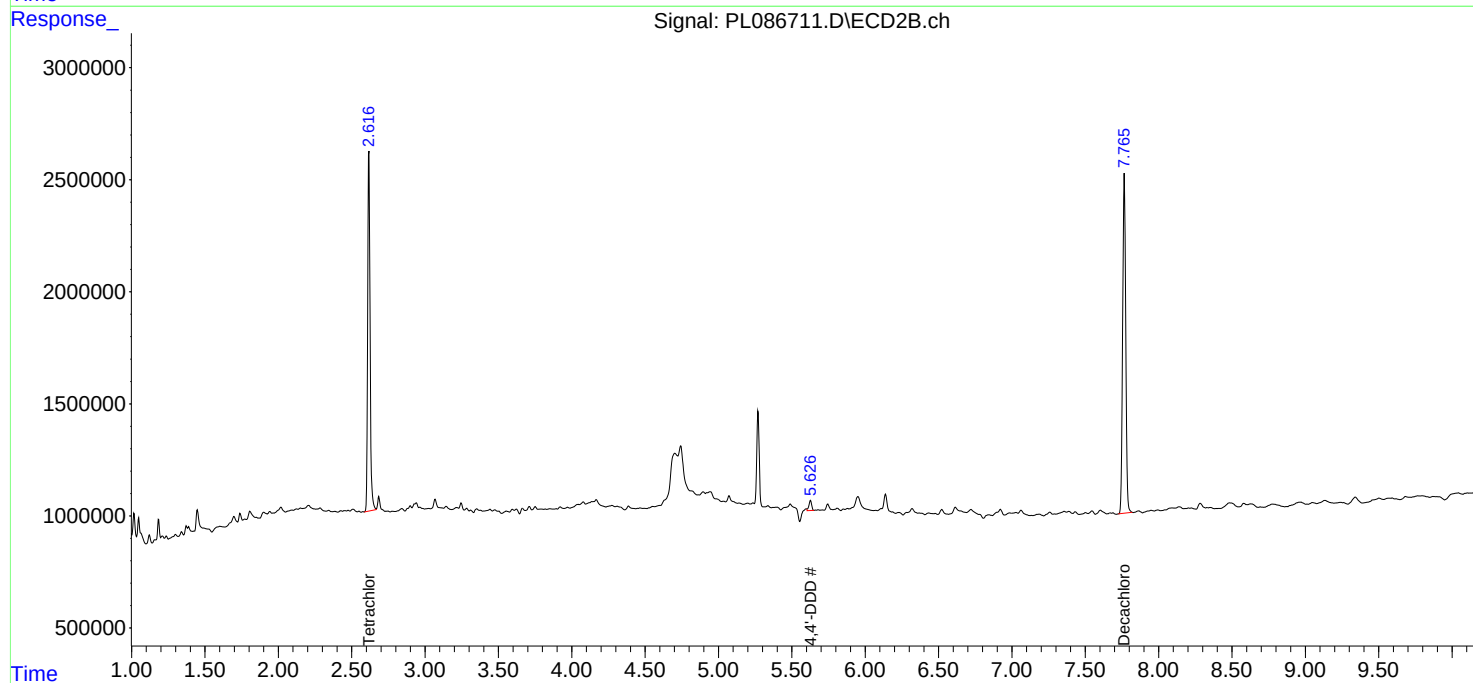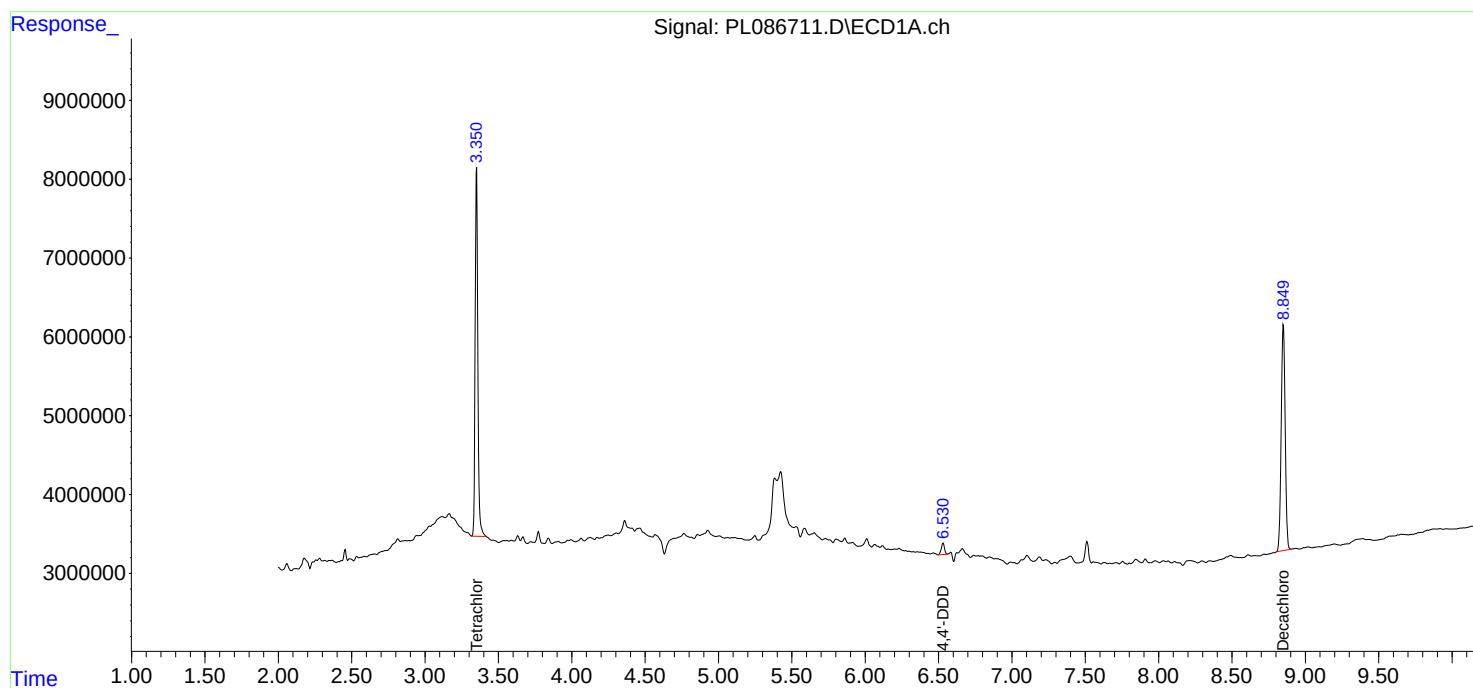

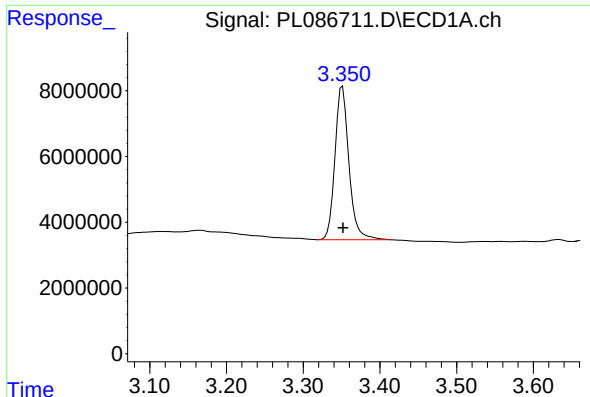


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 59108207
Conc: 18.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/17/2023
Supervised By :Ankita Jodhani 11/17/2023

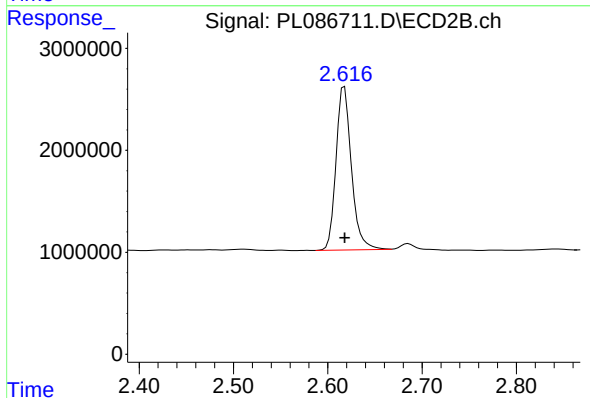


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: 0.000 min
Response: 18215687
Conc: 18.50 ng/ml

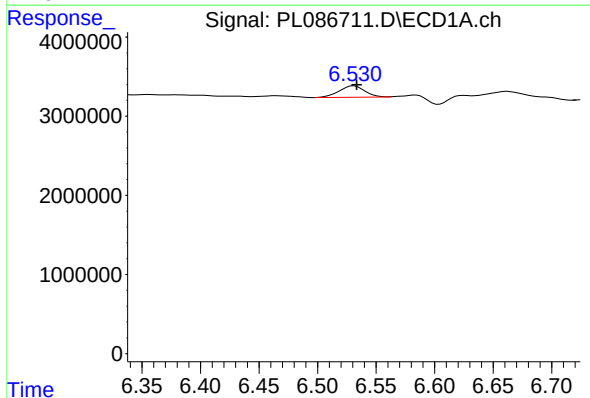


#16 4,4'-DDD

R.T.: 6.530 min
Delta R.T.: -0.004 min
Response: 2231418
Conc: 0.84 ng/ml m

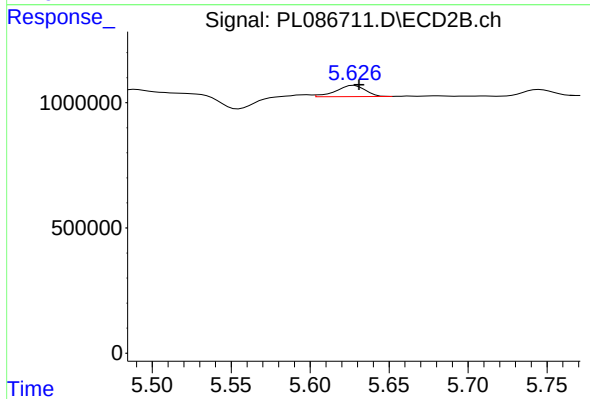

#16 4,4'-DDD

R.T.: 5.628 min
Delta R.T.: -0.003 min
Response: 580903
Conc: 0.68 ng/ml

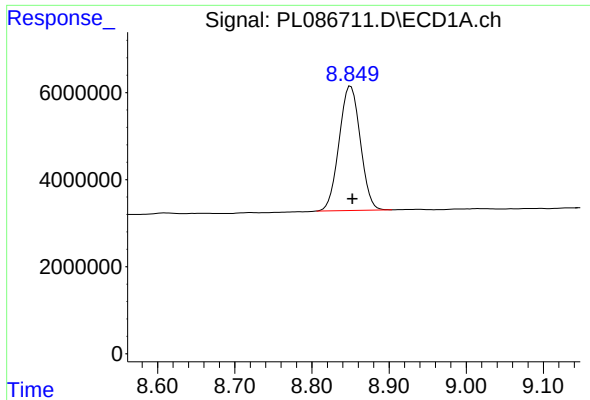


#28 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: -0.002 min
Response: 54537662
Conc: 18.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/17/2023
Supervised By :Ankita Jodhani 11/17/2023

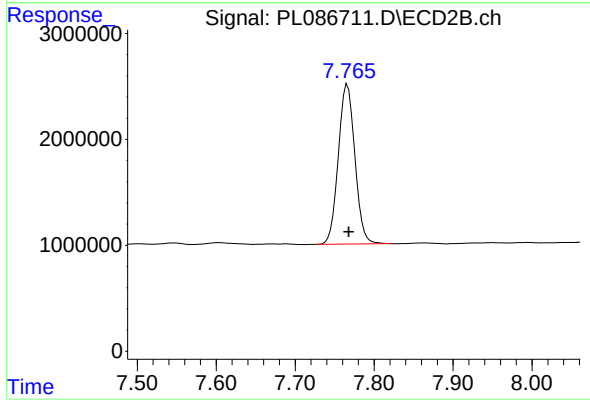

#28 Decachlorobiphenyl

R.T.: 7.766 min
Delta R.T.: -0.002 min
Response: 22004708
Conc: 18.22 ng/ml