

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 10:03
 Operator : AJ\SJ
 Sample : PSTDICC100
 Misc : FOR MIREX
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC100

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:15:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:14:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	568.4E6	273.1E6	103.220	100.527
28)	SA Decachlor...	8.203	9.228	569.6E6	223.3E6	95.371	94.544
Target Compounds							
22)	Mirex	7.337	8.322	523.7E6	177.1E6	97.092	100.229



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 10:03
Operator : AJ\SJ
Sample : PSTDICC100
Misc : FOR MIREX
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC100

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:15:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:14:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

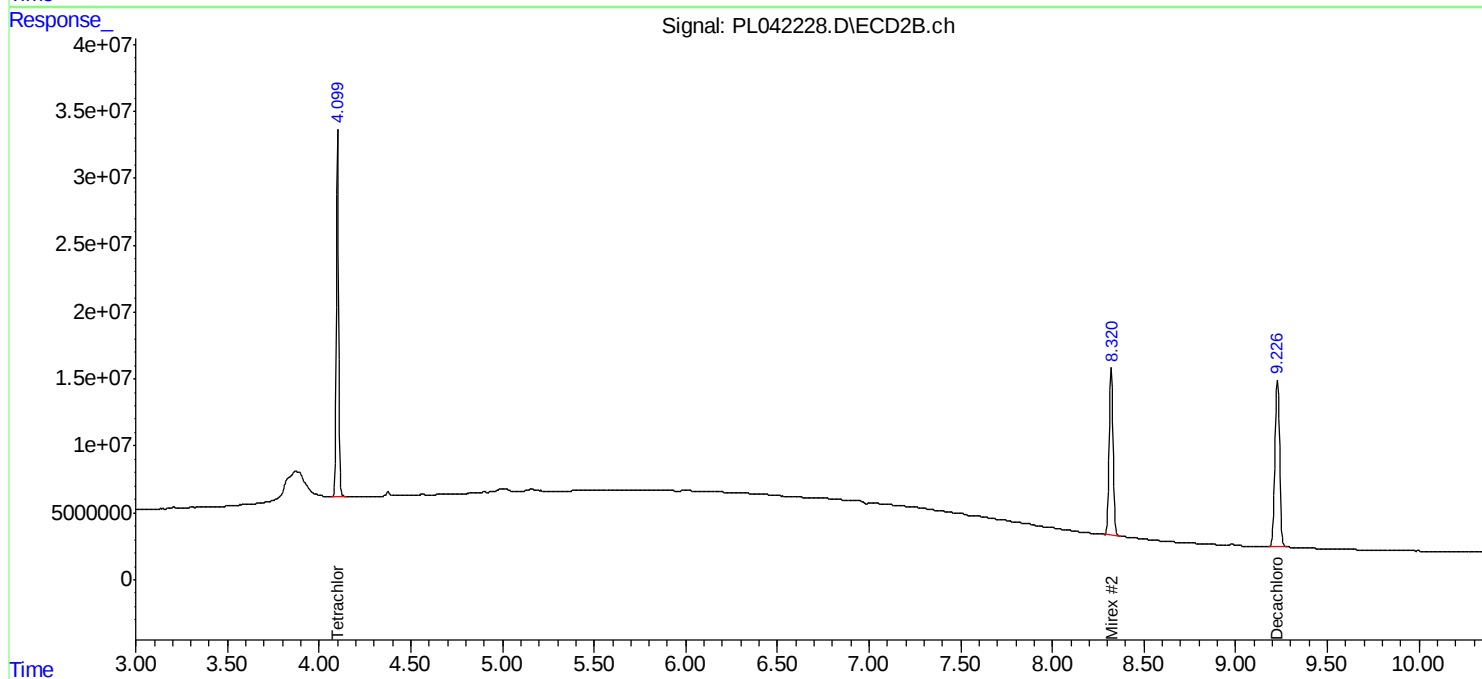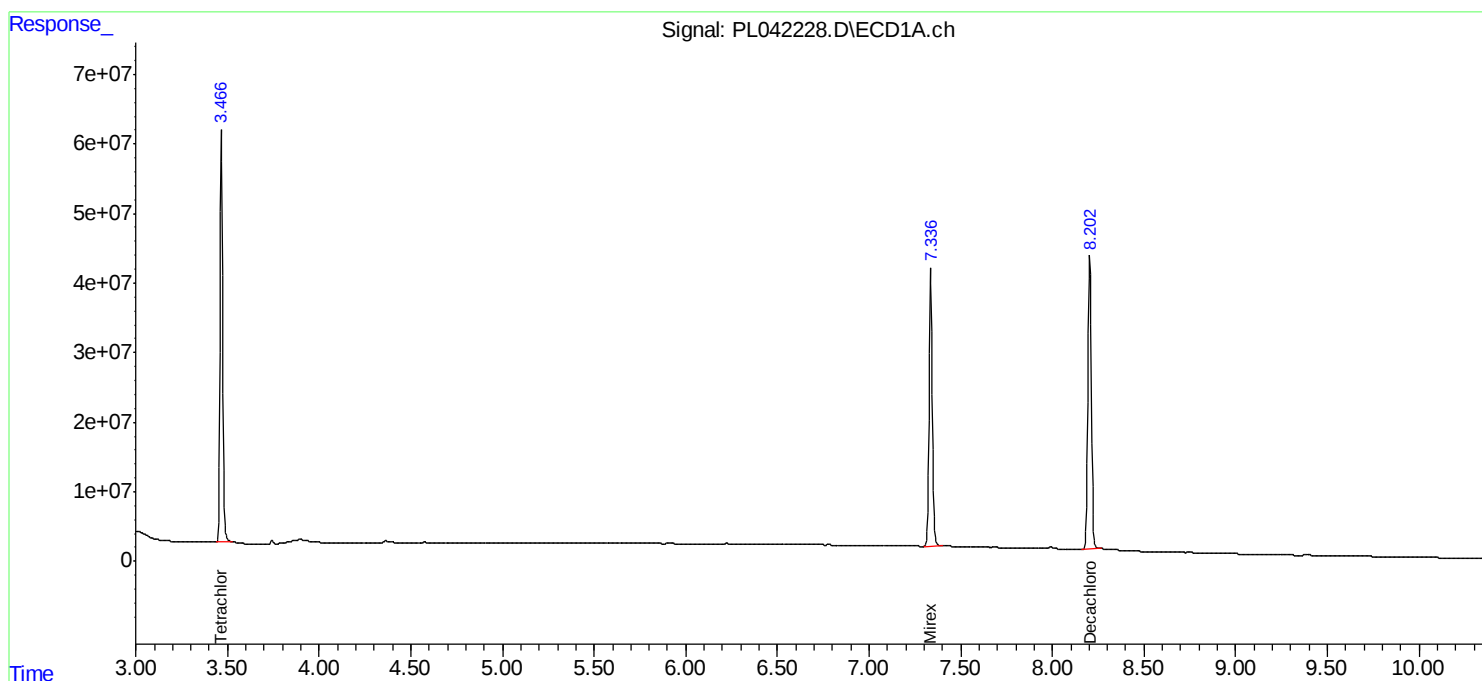


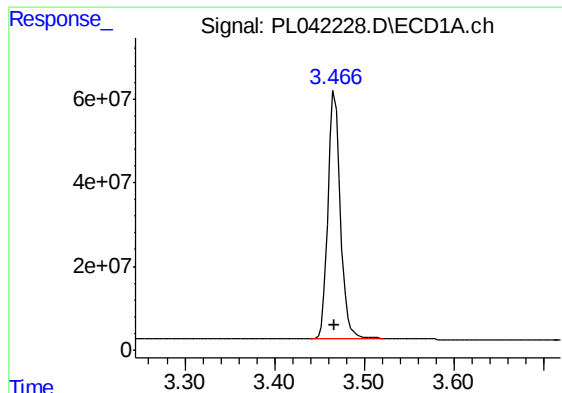

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 568399264
Conc: 103.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100

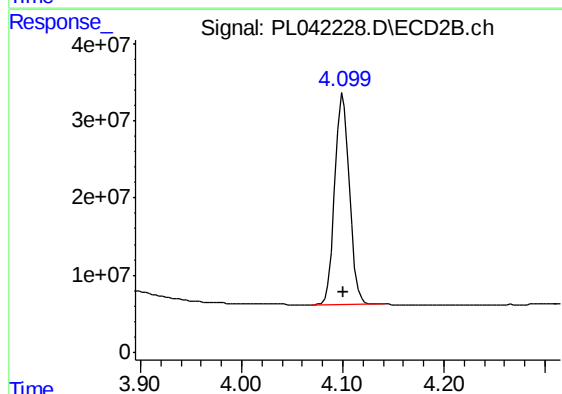


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 273087929
Conc: 100.53 ng/ml

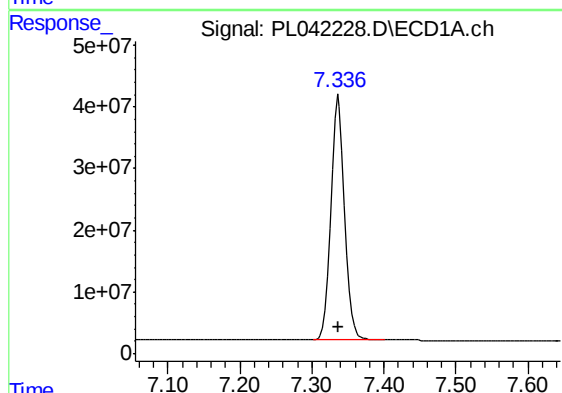


#22 Mirex

R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 523666645
Conc: 97.09 ng/ml

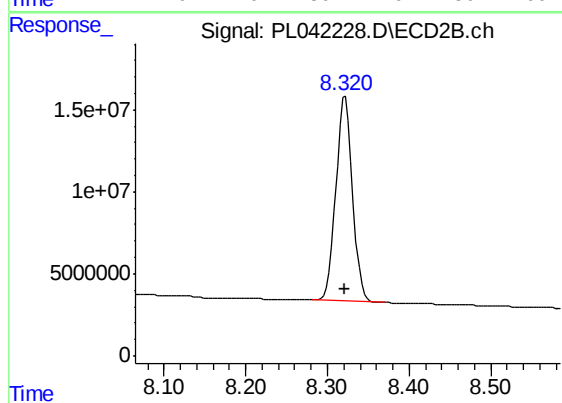

#22 Mirex


R.T.: 8.322 min
Delta R.T.: 0.000 min
Response: 177108033
Conc: 100.23 ng/ml

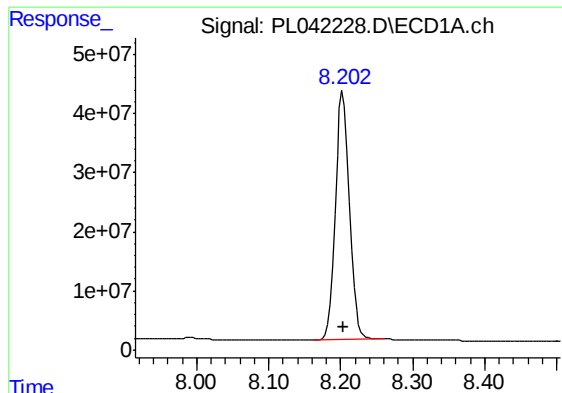

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 569550063
Conc: 95.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100

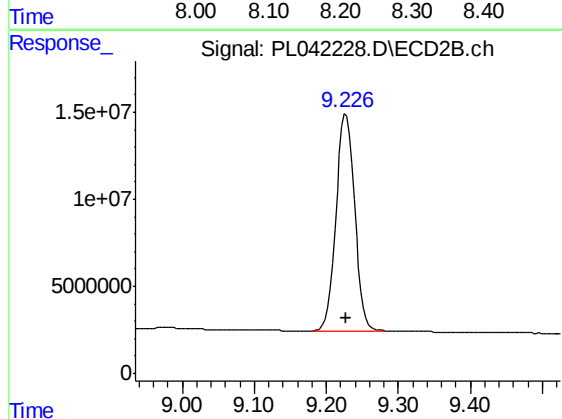

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 223309935
Conc: 94.54 ng/ml