

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 10:17
 Operator : AJ\SJ
 Sample : PSTDICC075
 Misc : FOR MIREX
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC075

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:15:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:14:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	423.2E6	205.2E6	76.851	75.531
28)	SA Decachlor...	8.204	9.229	428.1E6	168.4E6	71.683	71.293
Target Compounds							
22)	Mirex	7.339	8.322	398.1E6	134.5E6	73.811	76.091



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 10:17
Operator : AJ\SJ
Sample : PSTDICC075
Misc : FOR MIREX
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC075

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:15:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:14:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

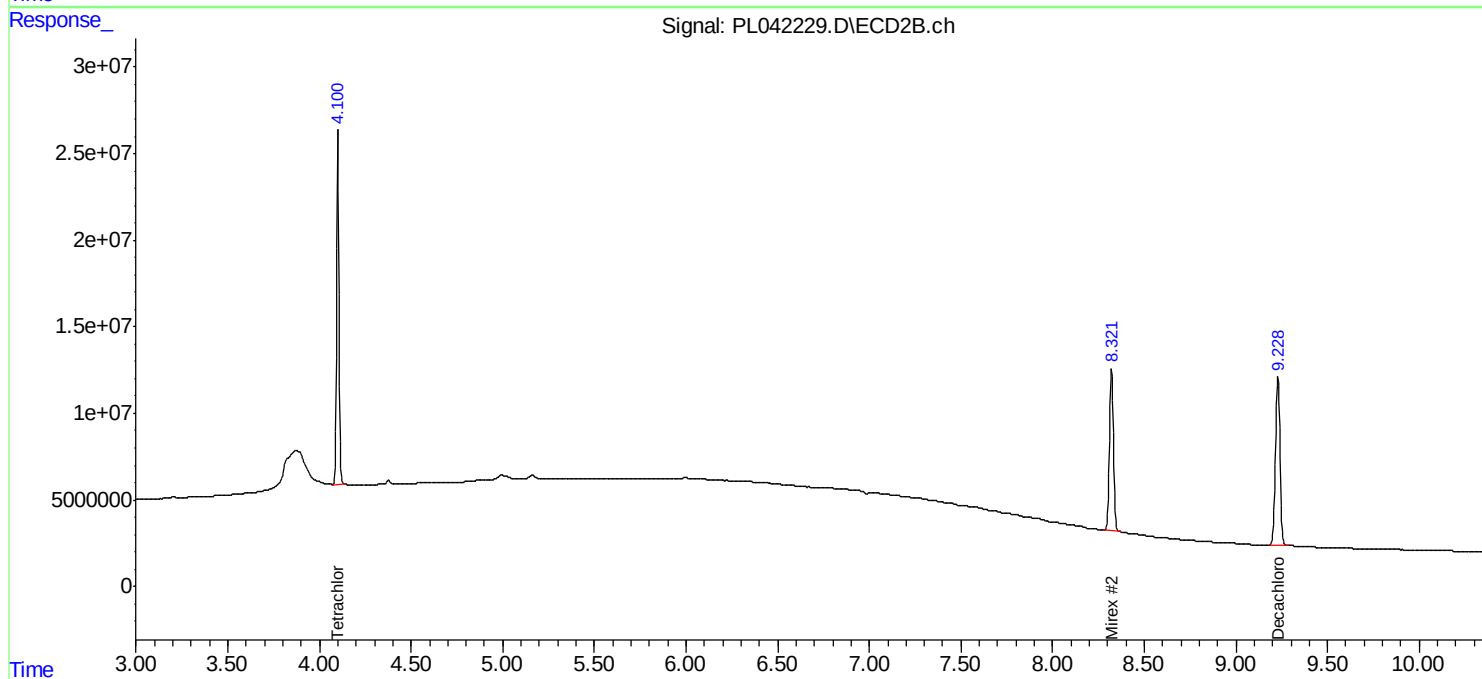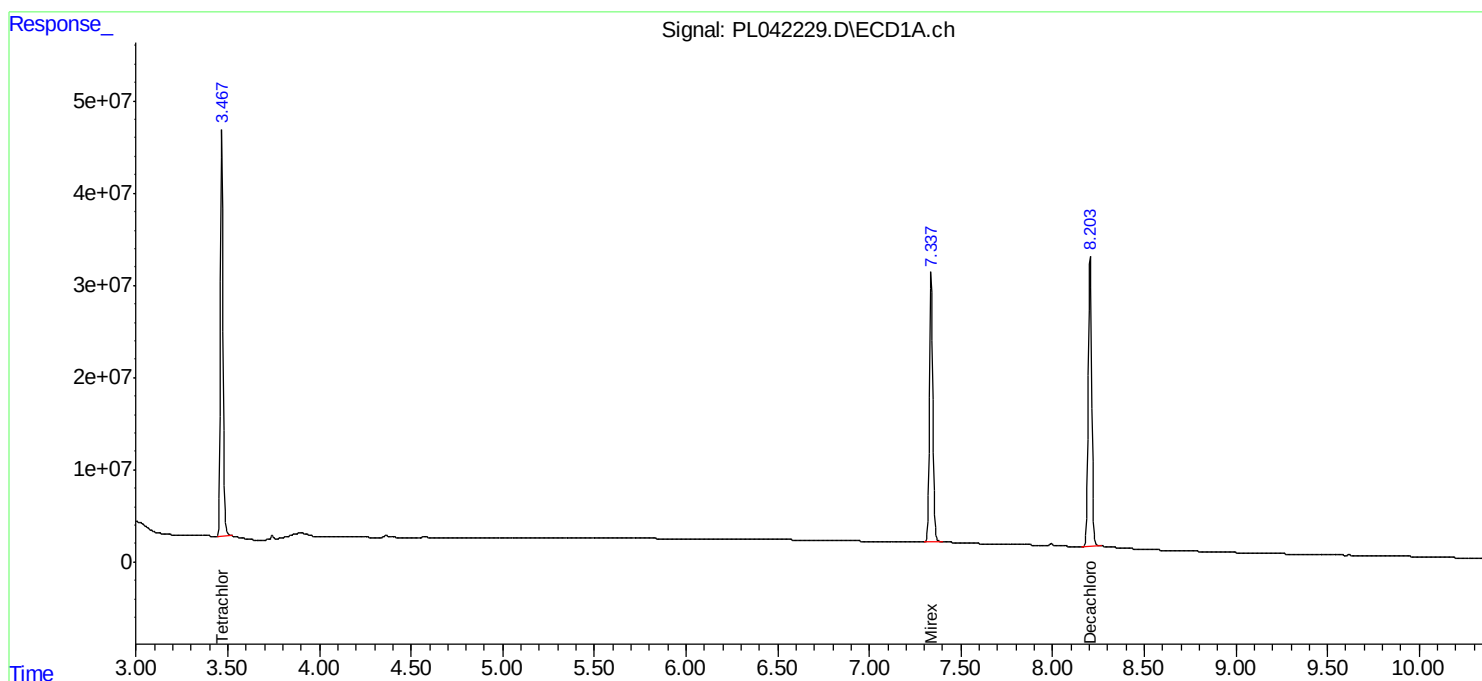


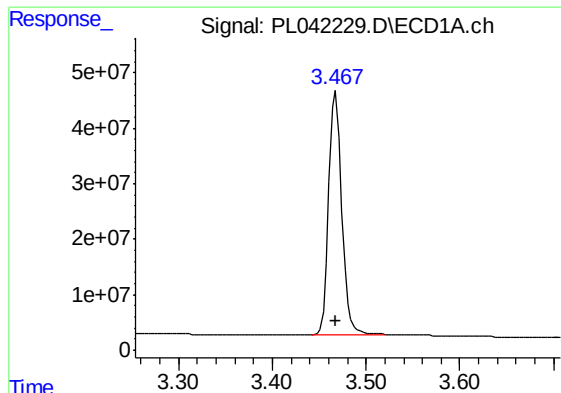

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 423191279
Conc: 76.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075

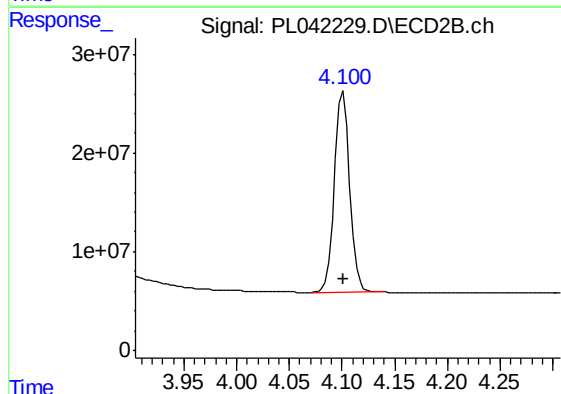


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 205184523
Conc: 75.53 ng/ml

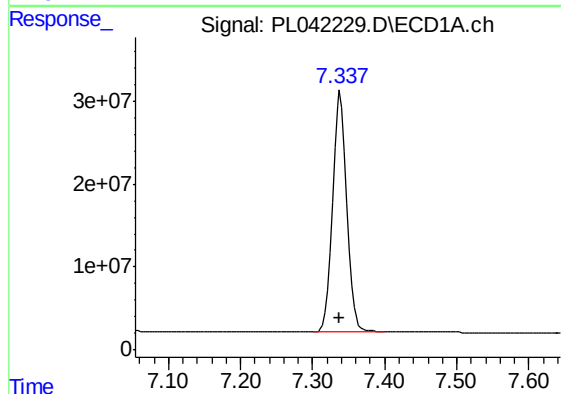


#22 Mirex

R.T.: 7.339 min
Delta R.T.: 0.002 min
Response: 398098604
Conc: 73.81 ng/ml

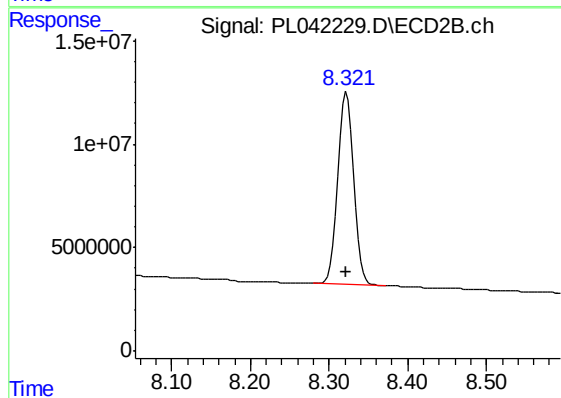

#22 Mirex


R.T.: 8.322 min
Delta R.T.: 0.000 min
Response: 134454959
Conc: 76.09 ng/ml

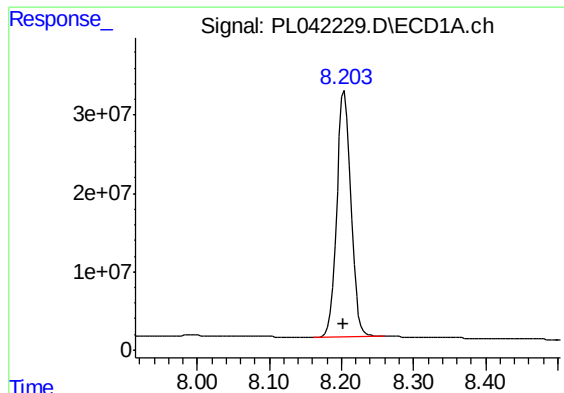

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 428089570
Conc: 71.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDIC075

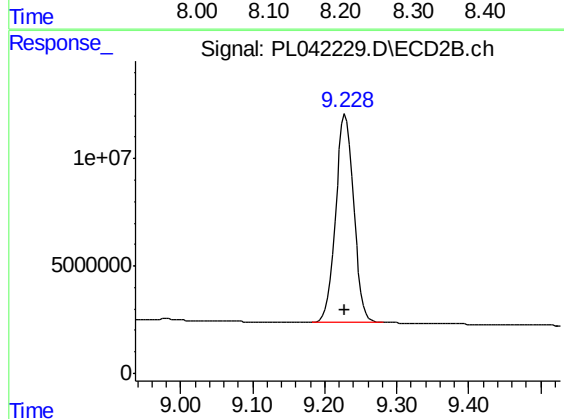

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 168391168
Conc: 71.29 ng/ml