

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 10:31
 Operator : AJ\SJ
 Sample : PSTDCC050
 Misc : FOR MIREX
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:15:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:14:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	275.3E6	135.8E6	50.000	50.000
28)	SA Decachlor...	8.204	9.228	298.6E6	118.1E6	50.000	50.000
Target Compounds							
22)	Mirex	7.337	8.321	269.7E6	88351945	50.000	50.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 10:31
Operator : AJ\SJ
Sample : PSTDCC050
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:15:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:14:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

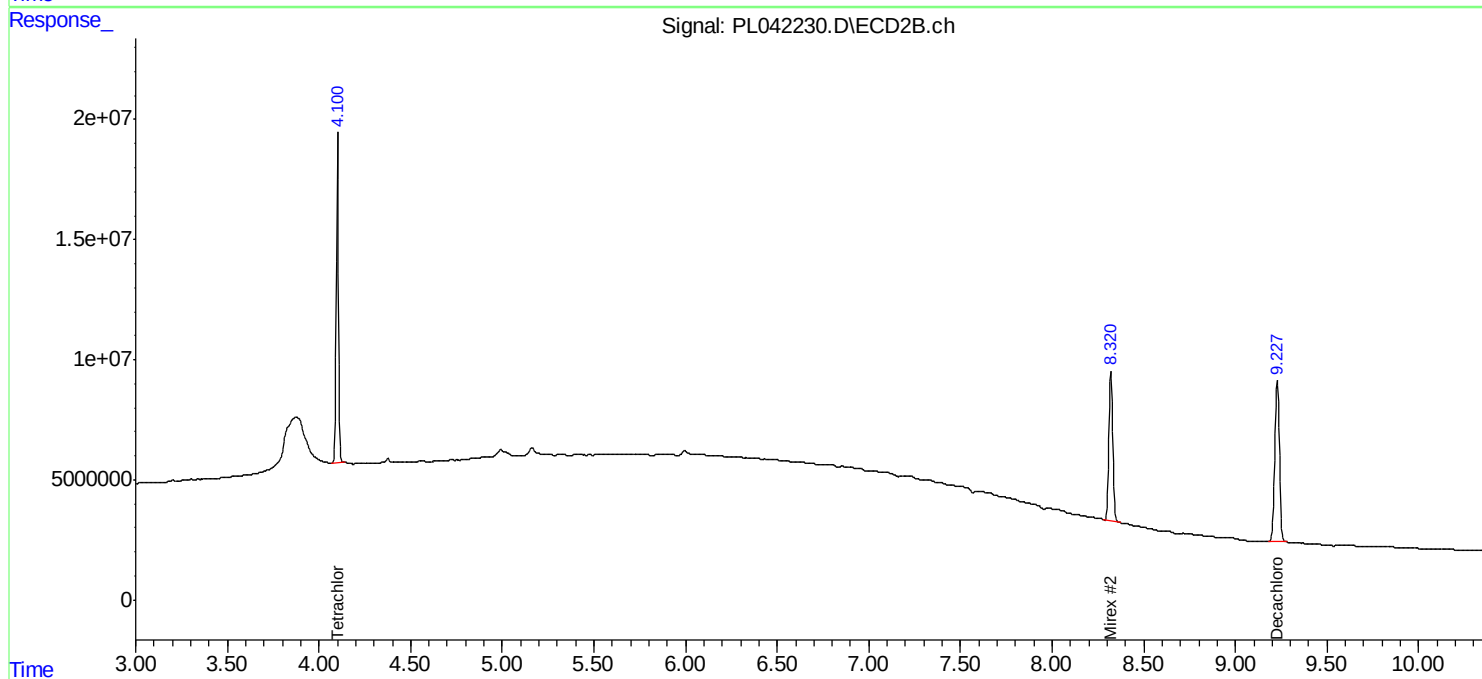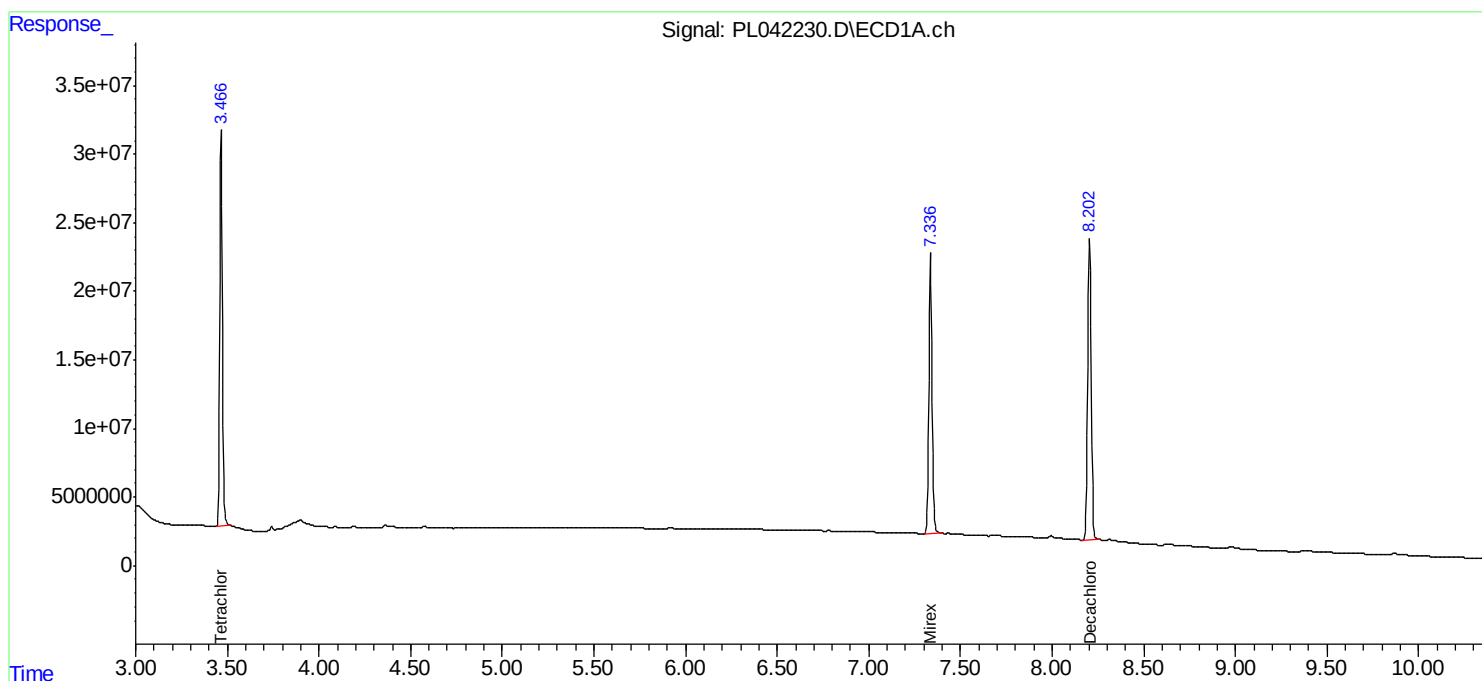


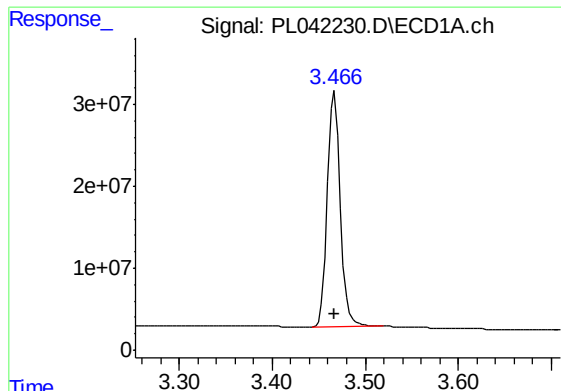

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 275333021
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCC050

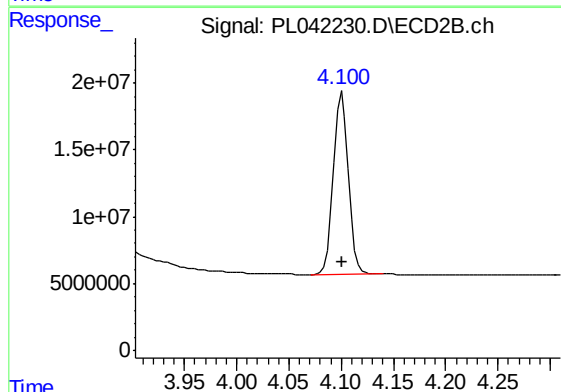


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 135828102
Conc: 50.00 ng/ml

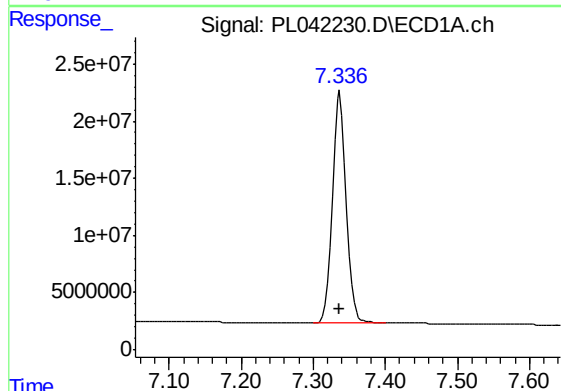


#22 Mirex

R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 269674247
Conc: 50.00 ng/ml

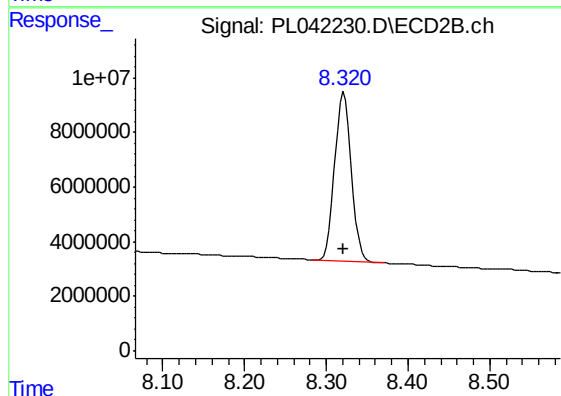

#22 Mirex


R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 88351945
Conc: 50.00 ng/ml

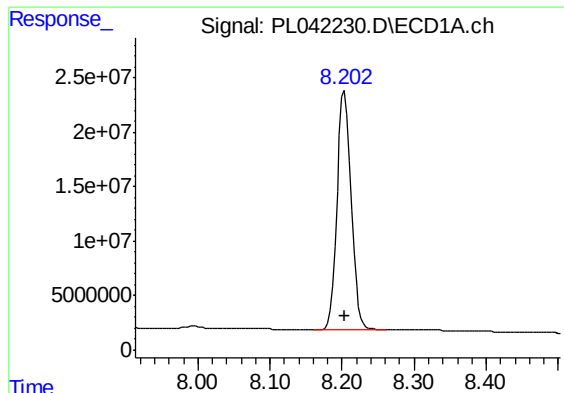

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 298598146
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCC050

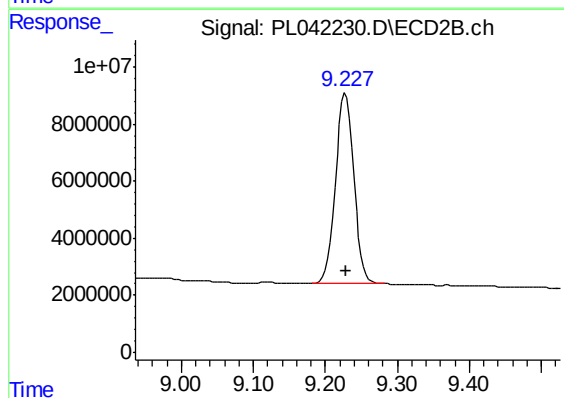

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 118098160
Conc: 50.00 ng/ml