

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 10:59
 Operator : AJ\SJ
 Sample : PSTDICC005
 Misc : FOR MIREX
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC005

Manual Integrations
 APPROVED

Sohil
 11/16/2018 4:01:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:15:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:14:41 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	27512096	14460708	4.996	5.323
28)	SA Decachlor...	8.203	9.229	37165253	13381903	6.223m	5.666
Target Compounds							
22)	Mirex	7.337	8.321	34247362	10516786	6.350m	5.952

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 10:59
Operator : AJ\SJ
Sample : PSTDICC005
Misc : FOR MIREX
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PSTDICC005


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:15:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:14:41 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

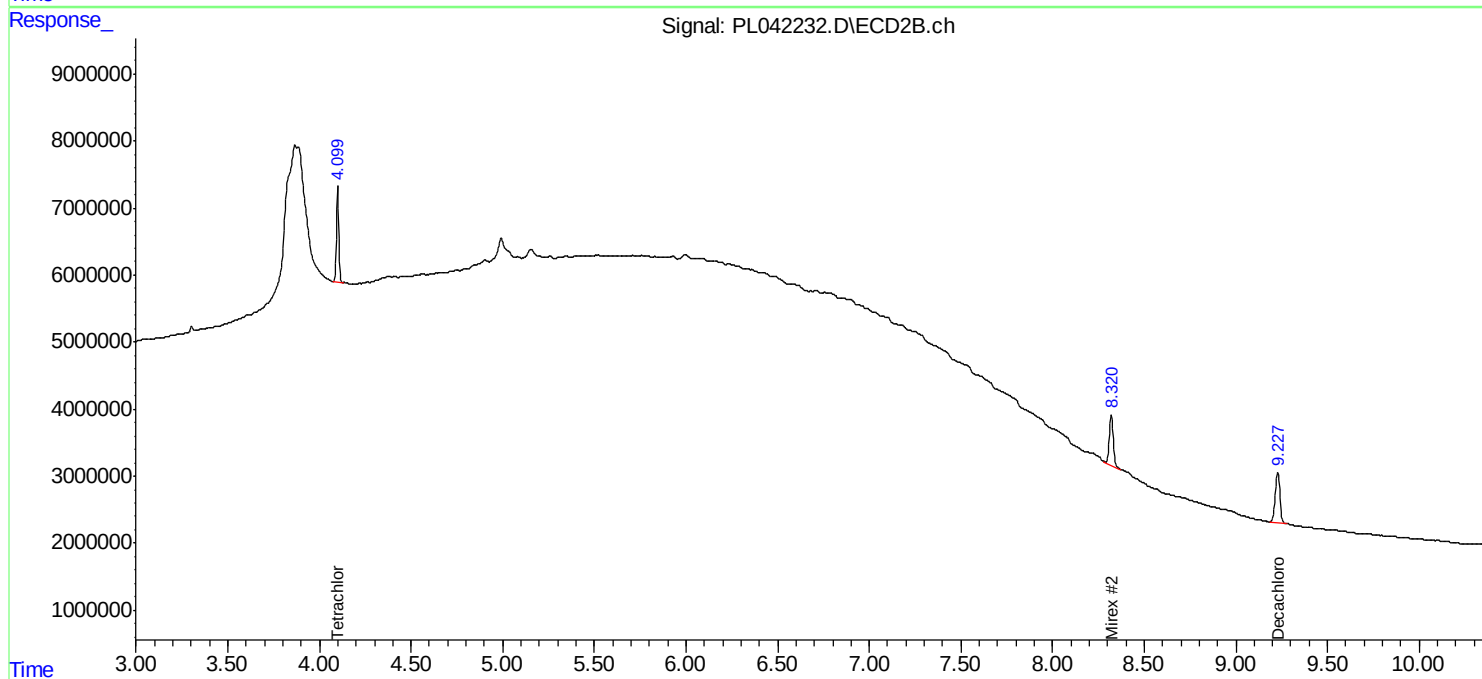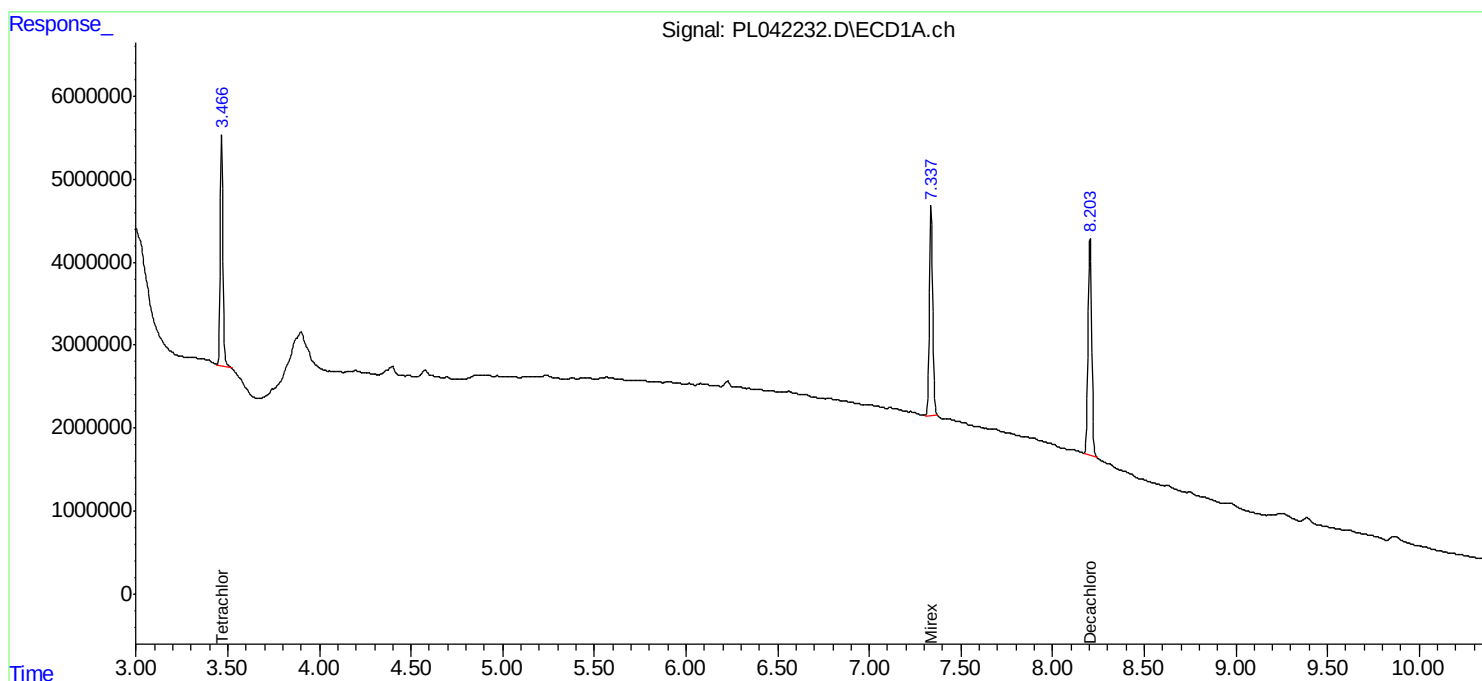

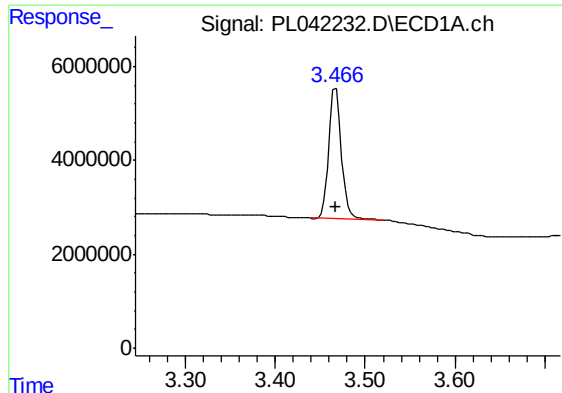


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 27512096
Conc: 5.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDIC005


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:34 PM

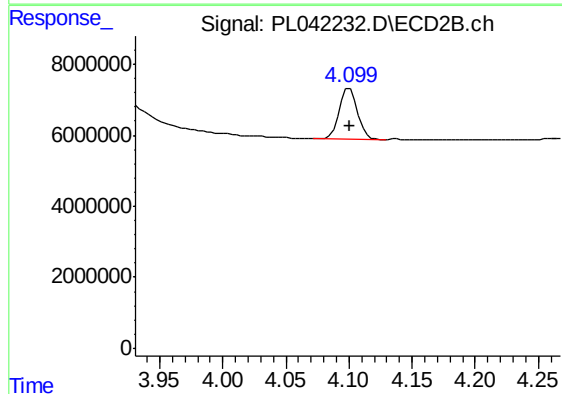


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 14460708
Conc: 5.32 ng/ml

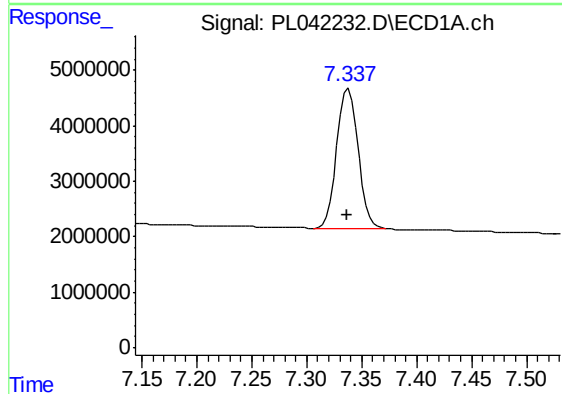


#22 Mirex

R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 34247362
Conc: 6.35 ng/ml m

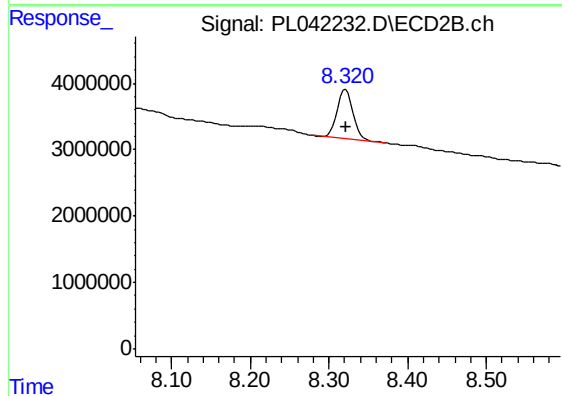

#22 Mirex

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 10516786
Conc: 5.95 ng/ml

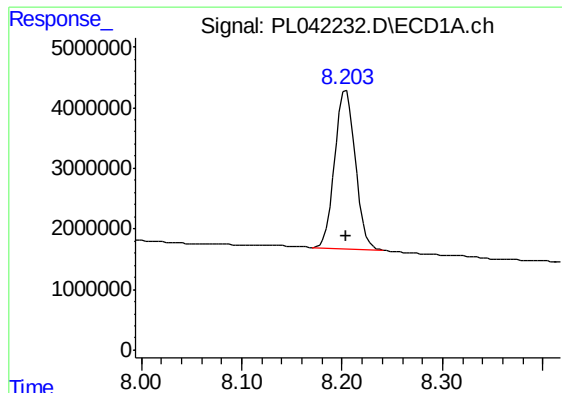


#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 37165253
Conc: 6.22 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDIC005

Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:34 PM

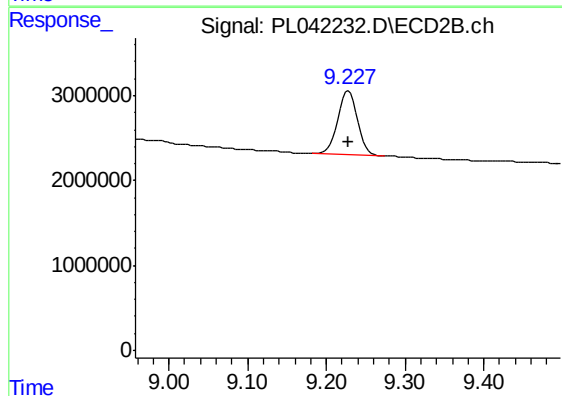

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 13381903
Conc: 5.67 ng/ml