

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 11:13
 Operator : AJ\SJ
 Sample : PSTDICV050
 Misc : FOR MIREX
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL111718

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 11:24:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	282.4E6	140.6E6	50.871	50.845
28)	SA Decachlor...	8.204	9.228	298.5E6	117.4E6	48.244	49.310
Target Compounds							
22)	Mirex	7.338	8.322	276.8E6	94695197	48.551	50.798



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 11:13
Operator : AJ\SJ
Sample : PSTDICV050
Misc : FOR MIREX
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL111718

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 11:24:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

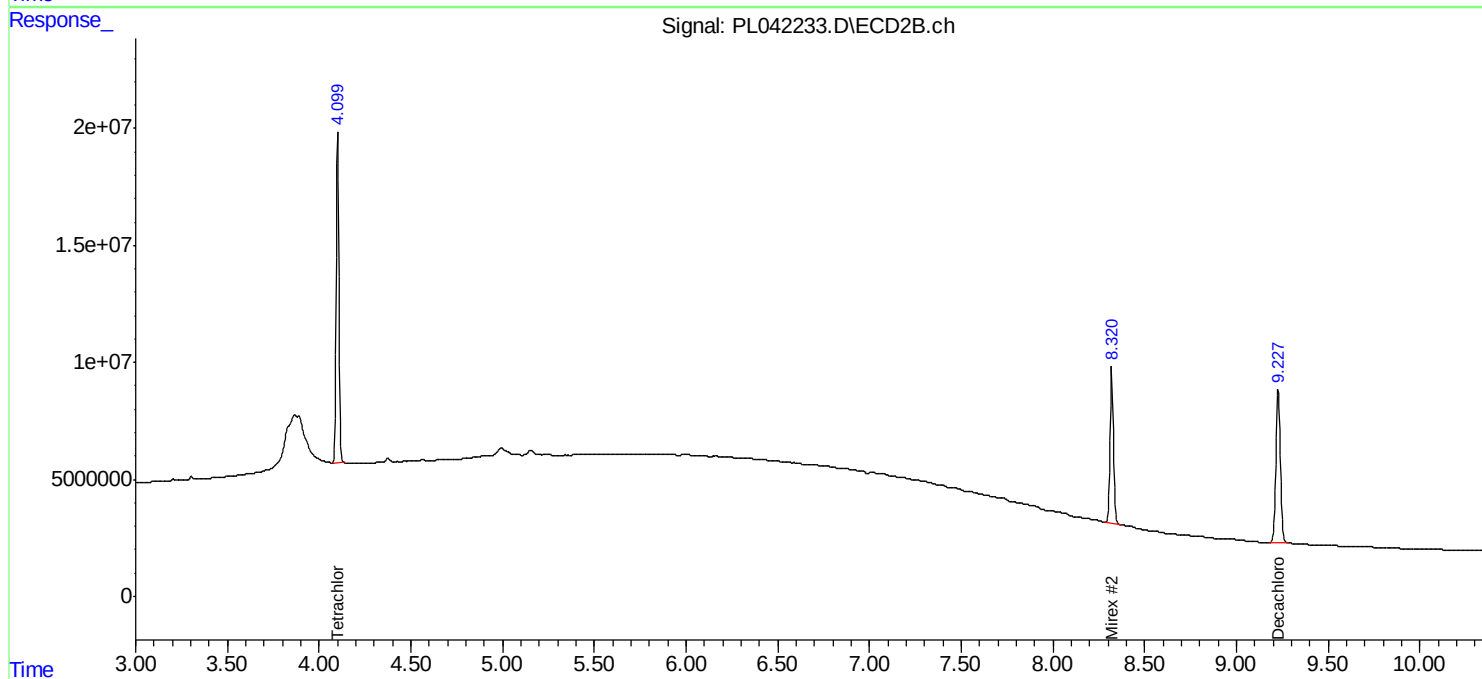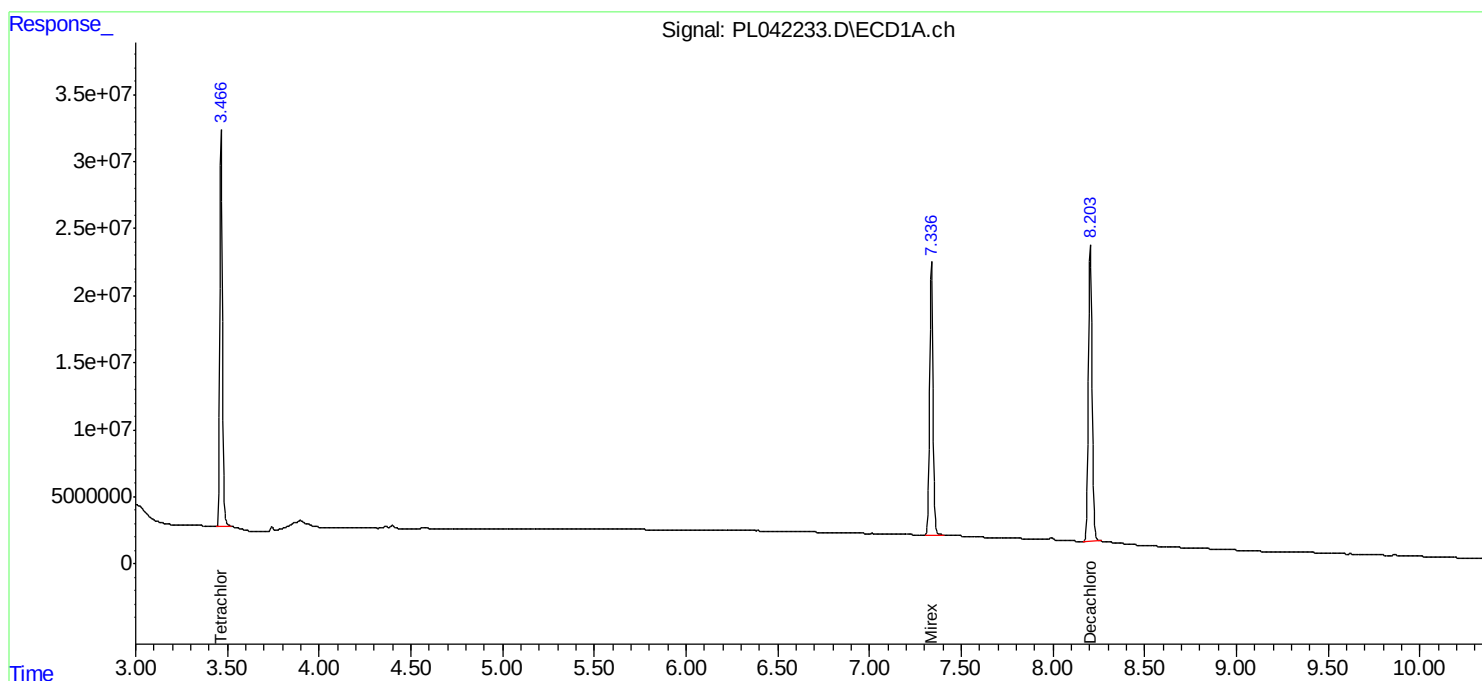


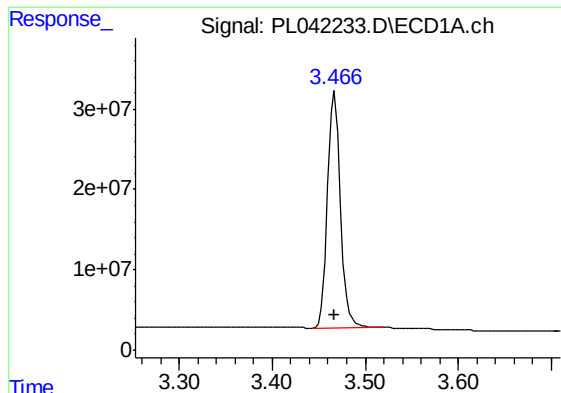

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 282354767
Conc: 50.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111718

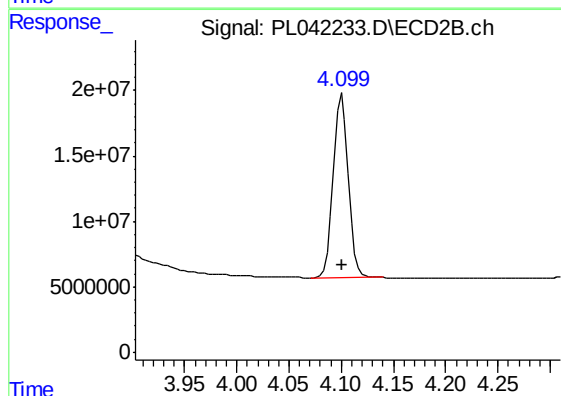


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 140554196
Conc: 50.85 ng/ml

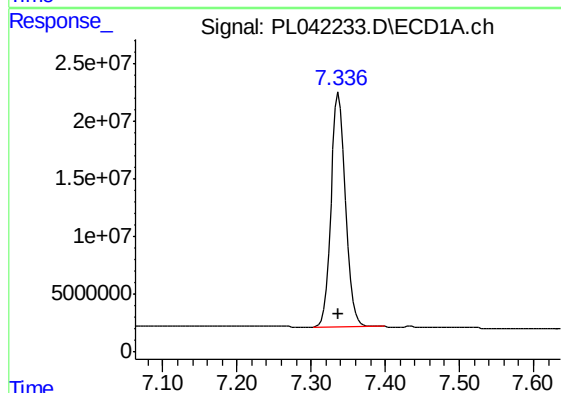


#22 Mirex

R.T.: 7.338 min
Delta R.T.: 0.000 min
Response: 276762251
Conc: 48.55 ng/ml

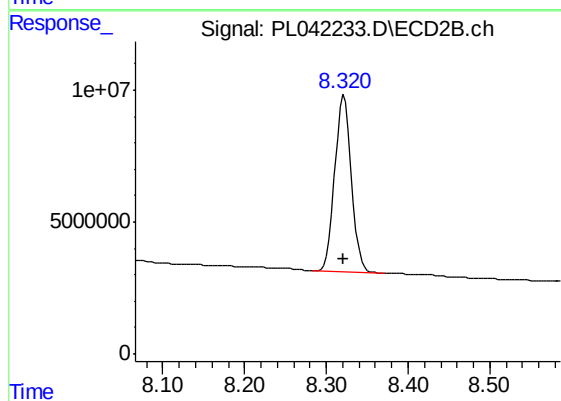

#22 Mirex


R.T.: 8.322 min
Delta R.T.: 0.000 min
Response: 94695197
Conc: 50.80 ng/ml

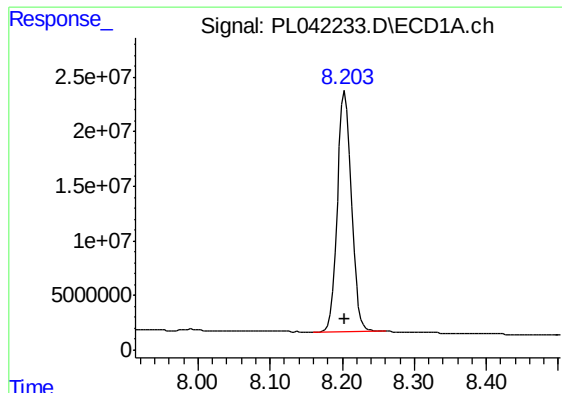

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 298549006
Conc: 48.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL111718

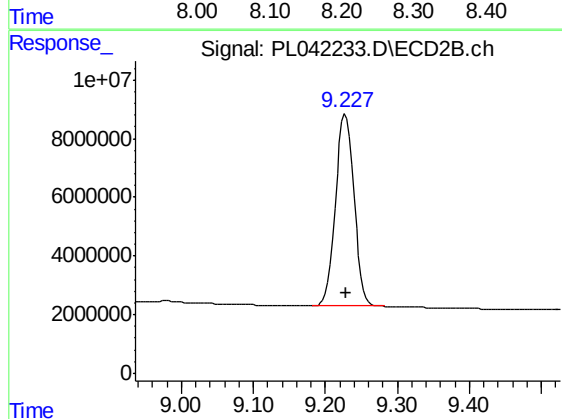

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 117379390
Conc: 49.31 ng/ml