

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 11:56
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc : FOR MIREX
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 12:10:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	276.9E6	137.7E6	49.880	49.809
28)	SA Decachlor...	8.205	9.229	297.3E6	116.9E6	48.034	49.089
Target Compounds							
22)	Mirex	7.339	8.323	273.5E6	91685521	47.972	49.183



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 11:56
Operator : AJ\SJ
Sample : PSTDCCC050
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 12:10:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

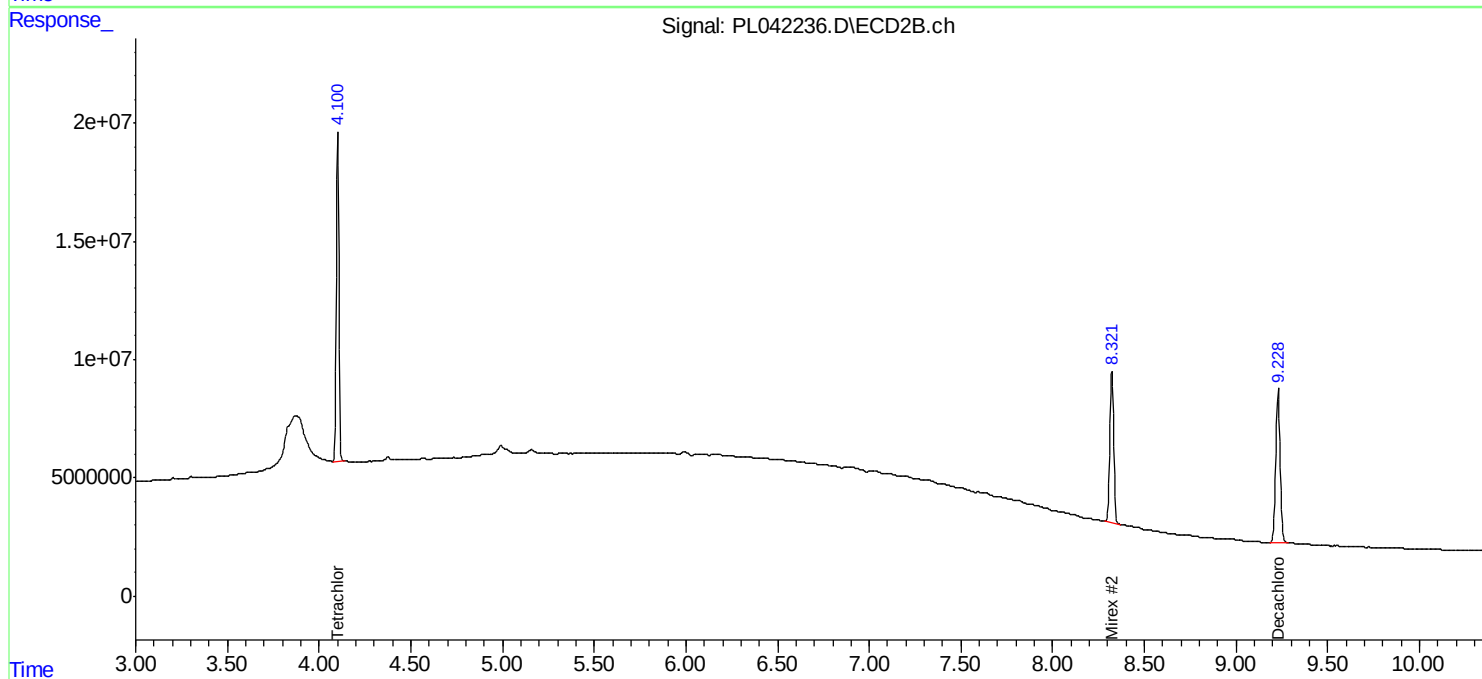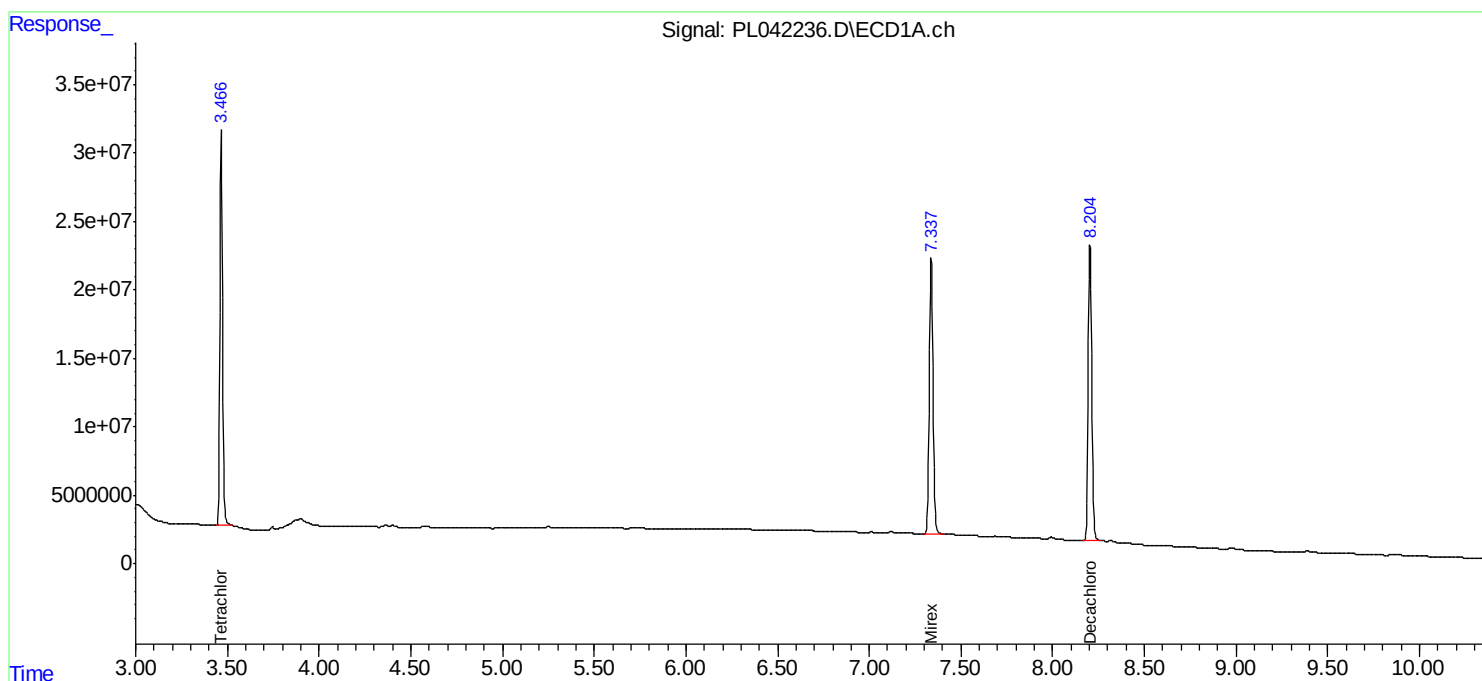


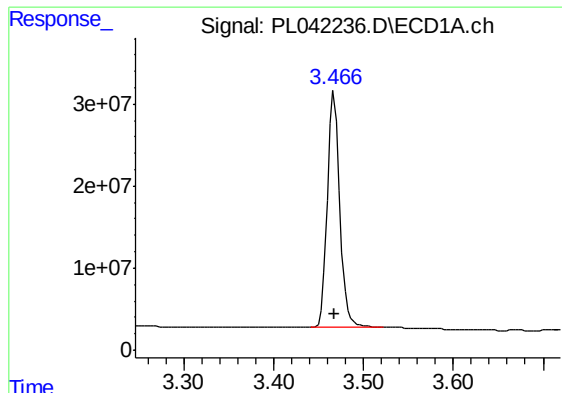

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 276857389
Conc: 49.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

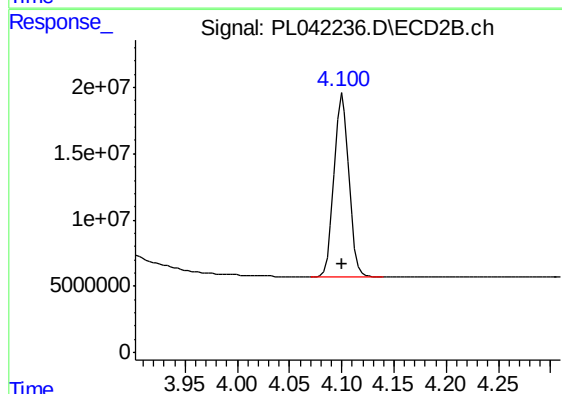


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 137688988
Conc: 49.81 ng/ml

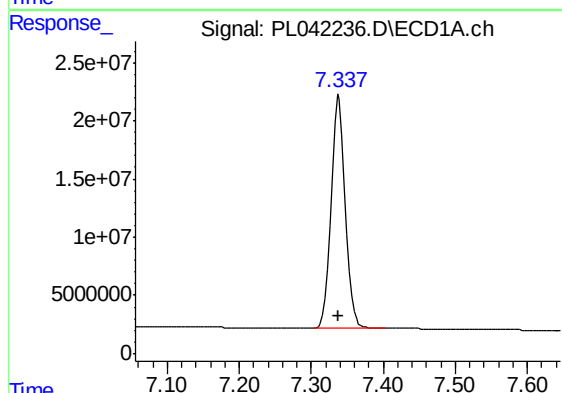


#22 Mirex

R.T.: 7.339 min
Delta R.T.: 0.002 min
Response: 273460666
Conc: 47.97 ng/ml

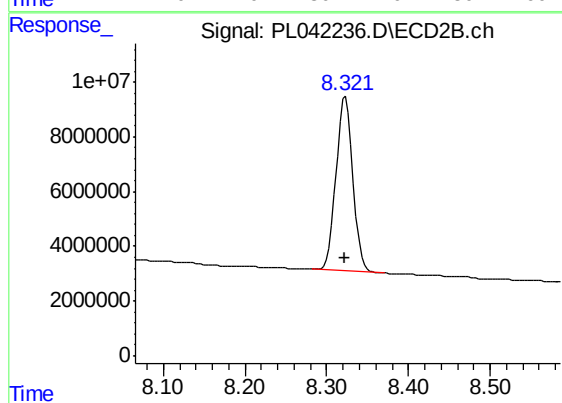

#22 Mirex


R.T.: 8.323 min
Delta R.T.: 0.001 min
Response: 91685521
Conc: 49.18 ng/ml

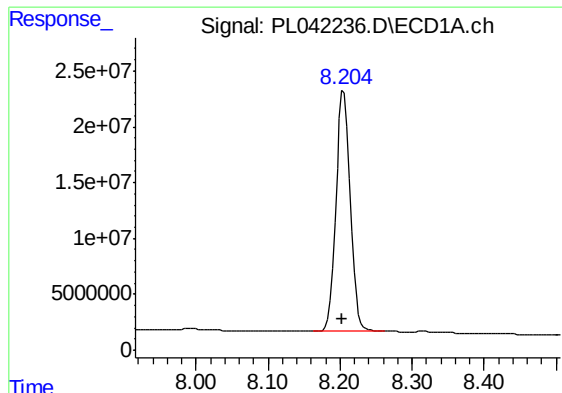

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.002 min
Response: 297250945
Conc: 48.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

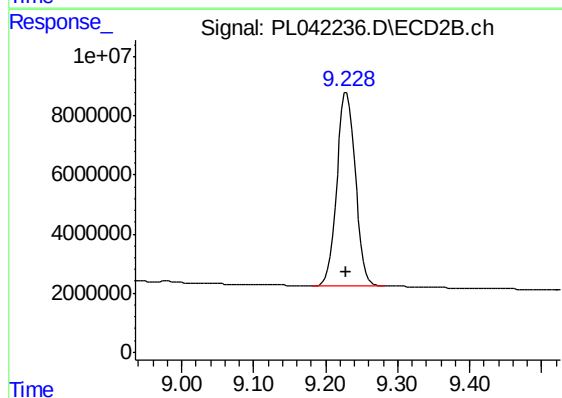

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 116853102
Conc: 49.09 ng/ml