

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 13:54
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-01
 Misc : FOR MIREX
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-01

Manual Integrations
 APPROVED

Sohil
 11/16/2018 4:01:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 14:18:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.101	94382111	48081737	17.004	17.393
28)	SA Decachlor...	8.206	9.230	112.5E6	43754654	18.175	18.381
Target Compounds							
22)	Mirex	7.341	8.321	6627618	2185635	1.163	1.172m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 13:54
Operator : AJ\SJ
Sample : MIREX-MDL-W-01
Misc : FOR MIREX
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-01


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 14:18:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

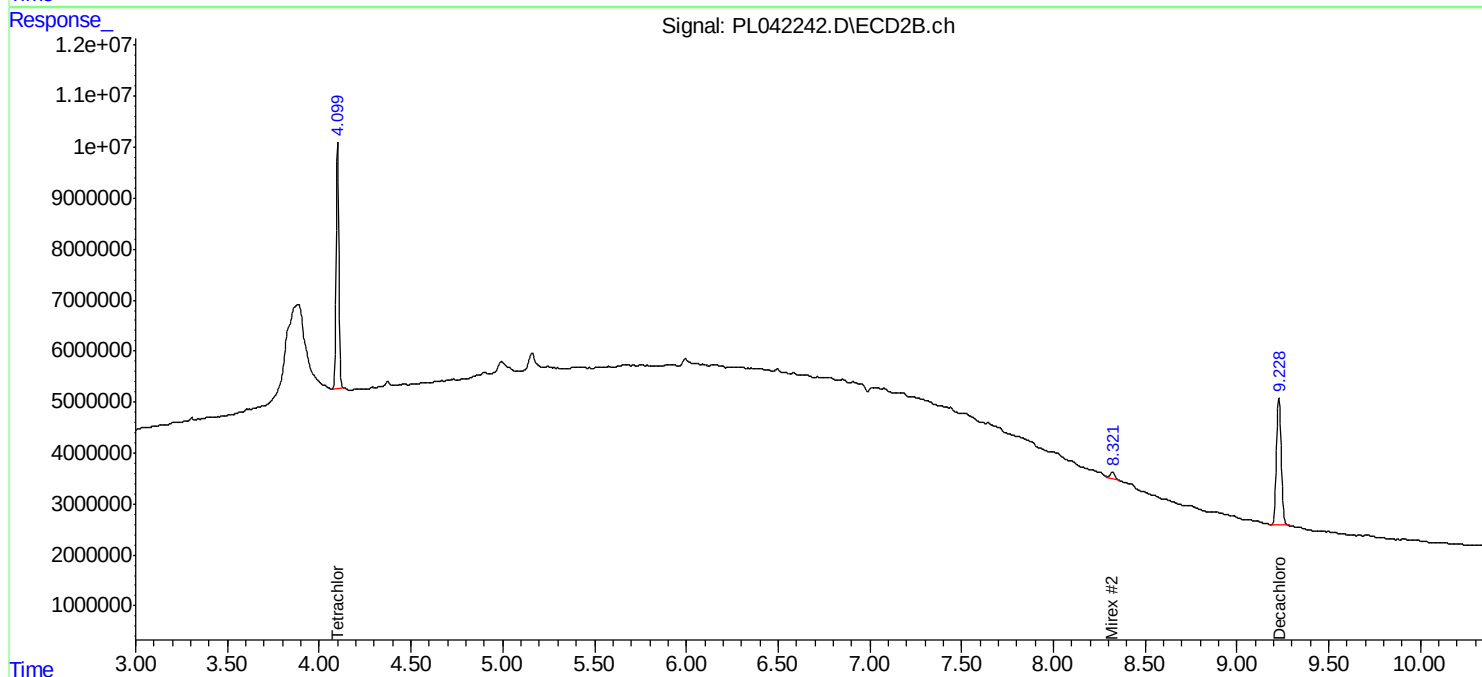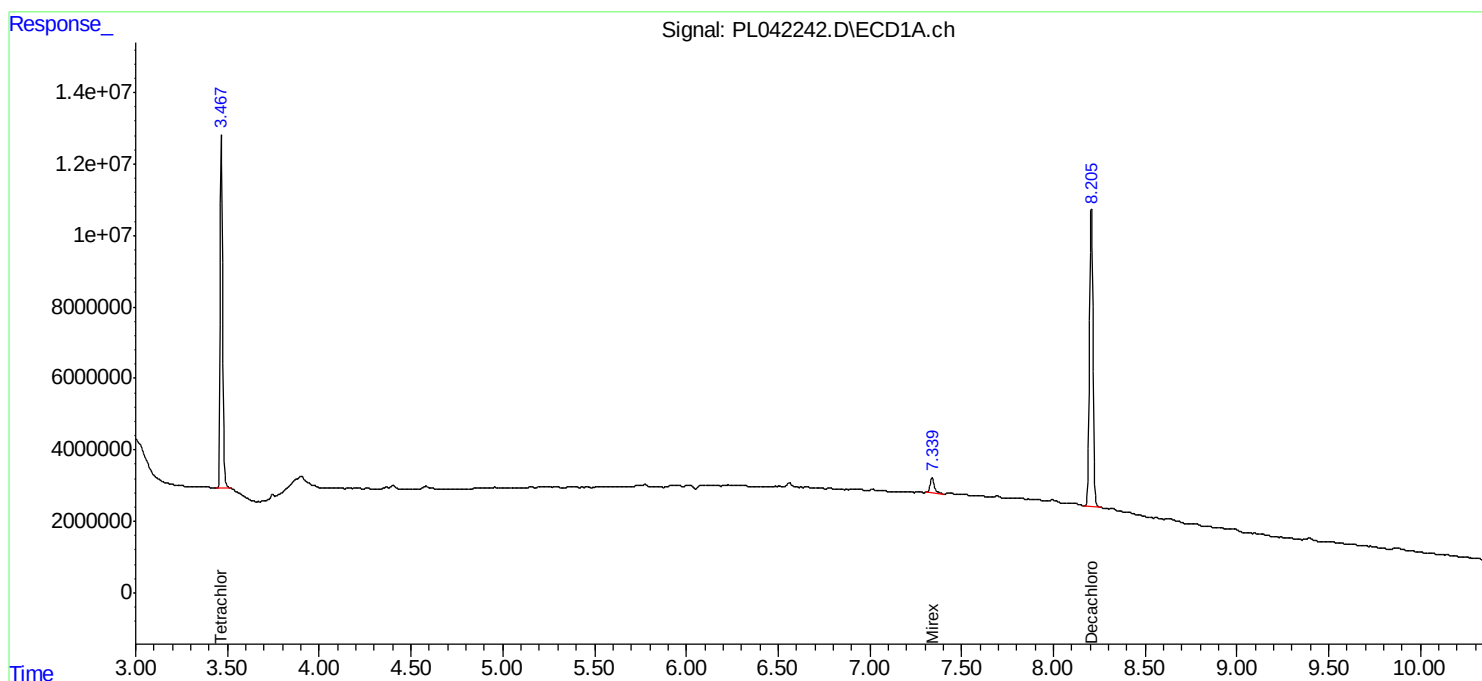

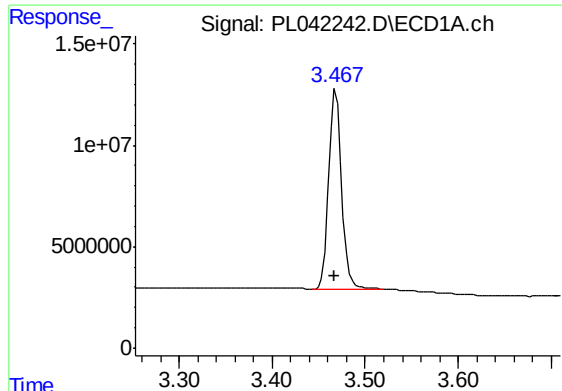


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.002 min
Response: 94382111
Conc: 17.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-01


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:42 PM

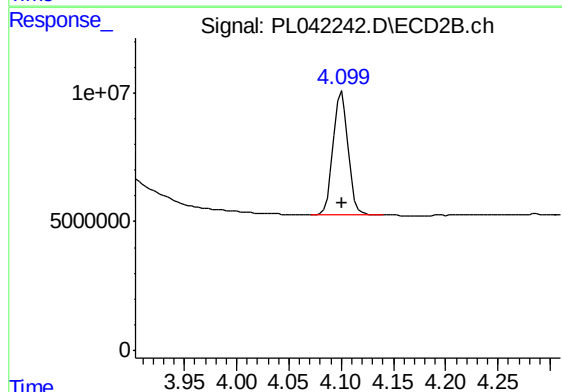


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 48081737
Conc: 17.39 ng/ml

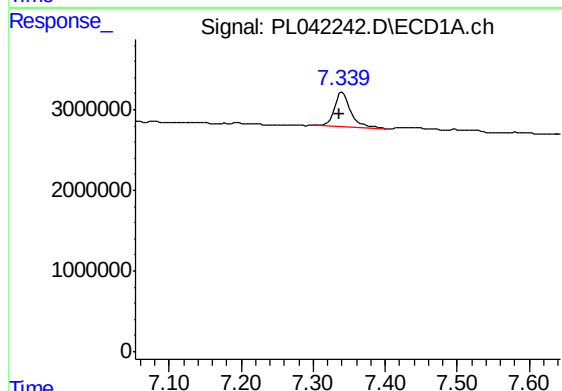


#22 Mirex

R.T.: 7.341 min
Delta R.T.: 0.004 min
Response: 6627618
Conc: 1.16 ng/ml

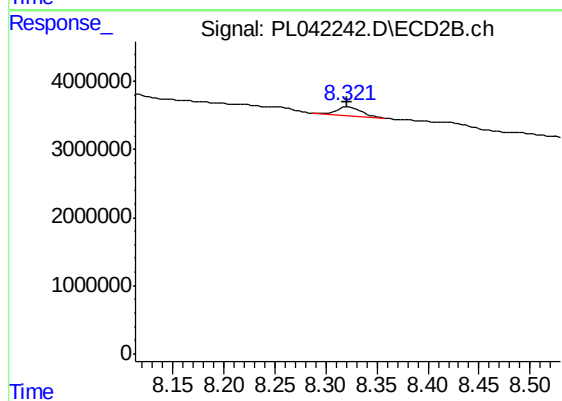

#22 Mirex

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 2185635
Conc: 1.17 ng/ml m

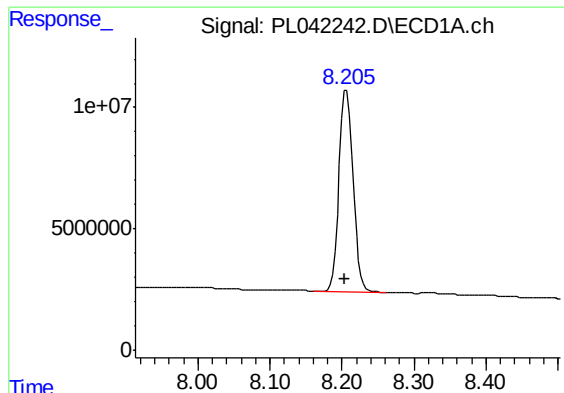


#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.003 min
Response: 112472542
Conc: 18.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-01

Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:42 PM

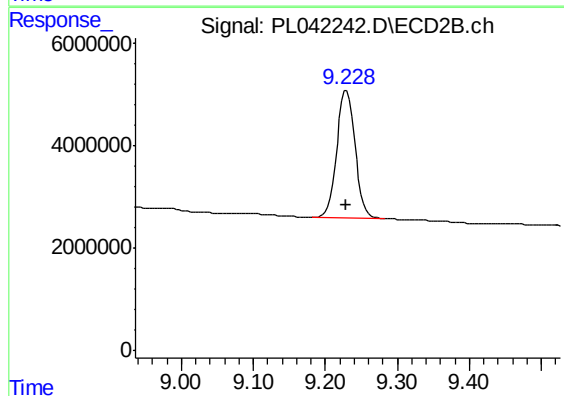

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.001 min
Response: 43754654
Conc: 18.38 ng/ml