

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 14:09
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-02
 Misc : FOR MIREX
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-02

Manual Integrations
 APPROVED

Sohil
 11/16/2018 4:01:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 14:20:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	96809253	50355233	17.442	18.216
28)	SA Decachlor...	8.207	9.231	114.7E6	44514163	18.530	18.700
Target Compounds							
22)	Mirex	7.341	8.323	6285821	1734729	1.103	0.931m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 14:09
Operator : AJ\SJ
Sample : MIREX-MDL-W-02
Misc : FOR MIREX
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-02


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 14:20:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

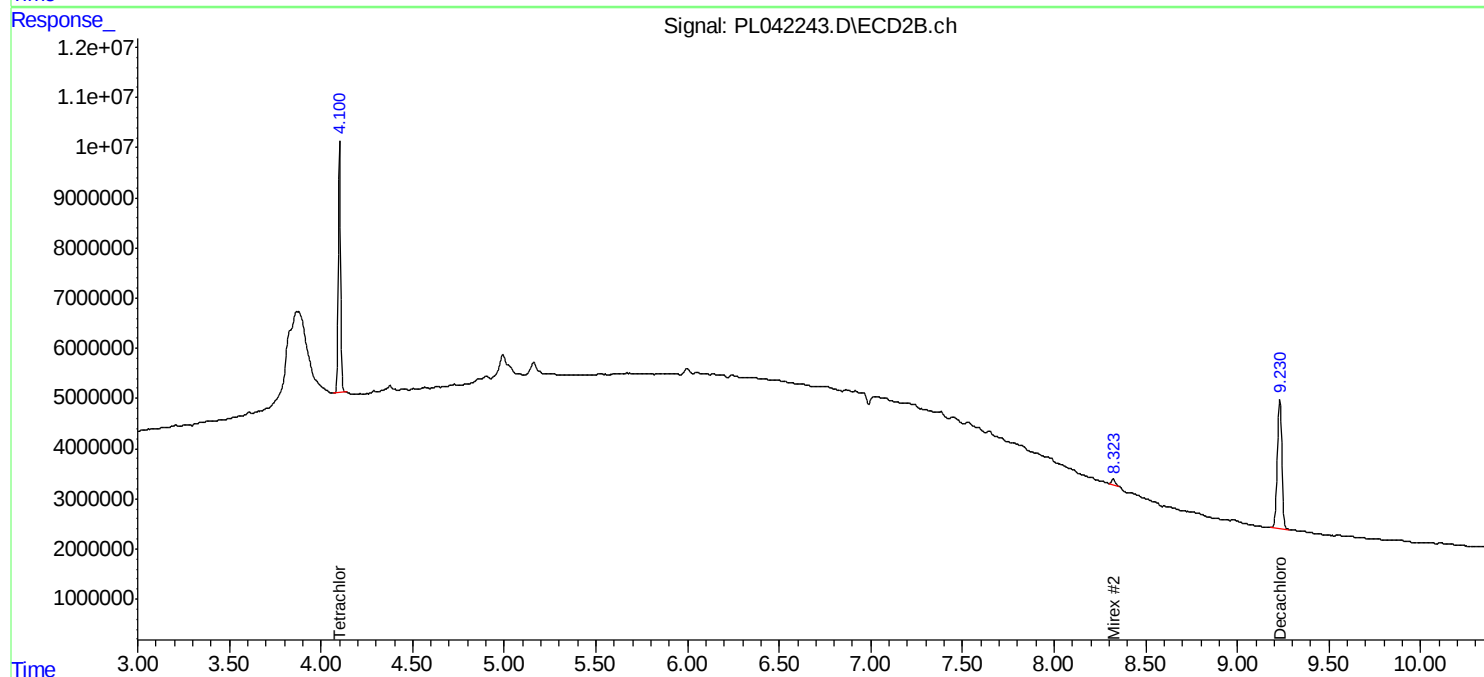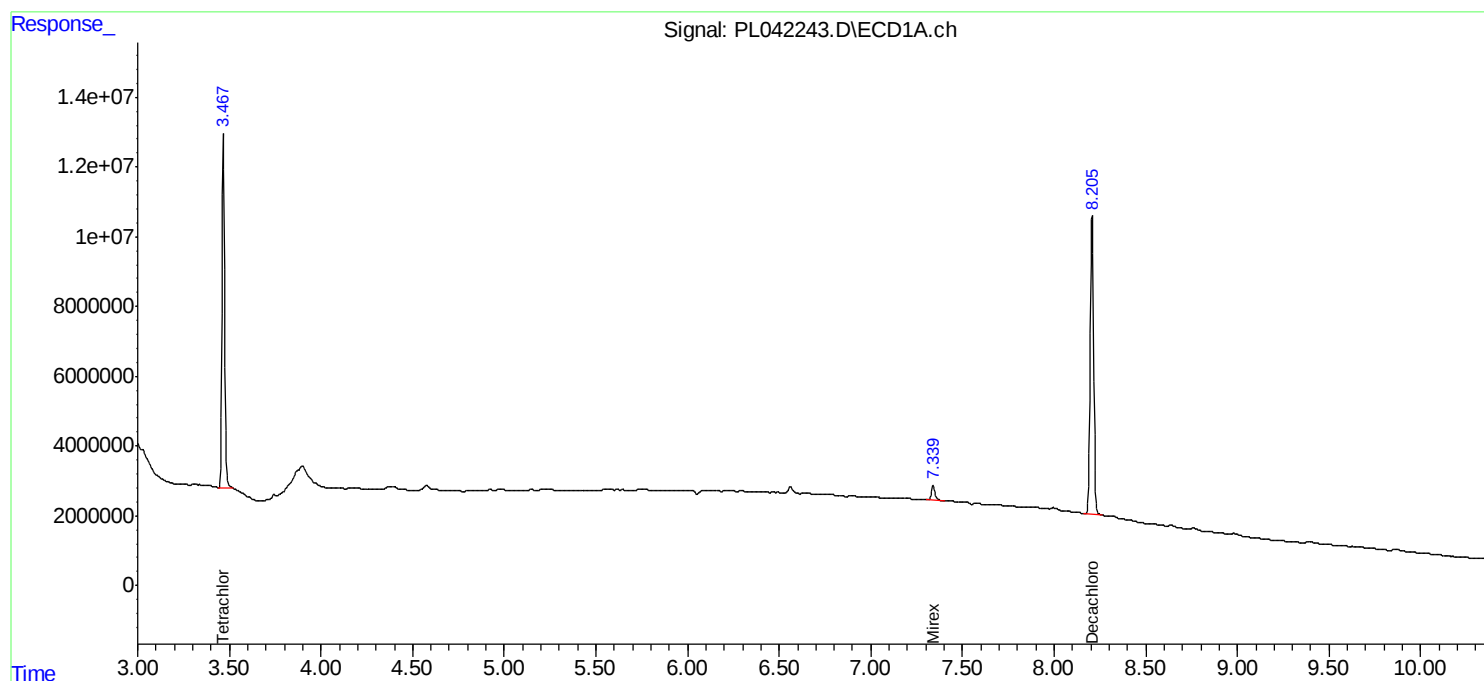

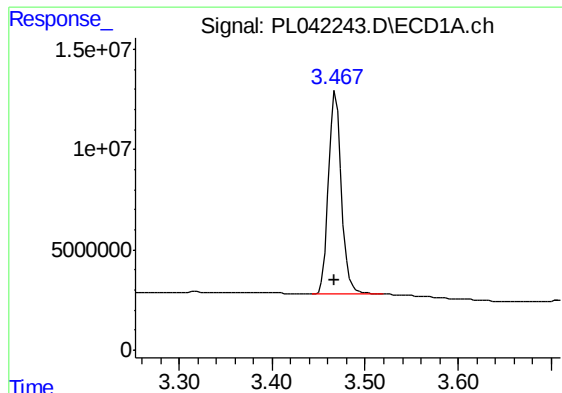


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 96809253
Conc: 17.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-02


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:44 PM

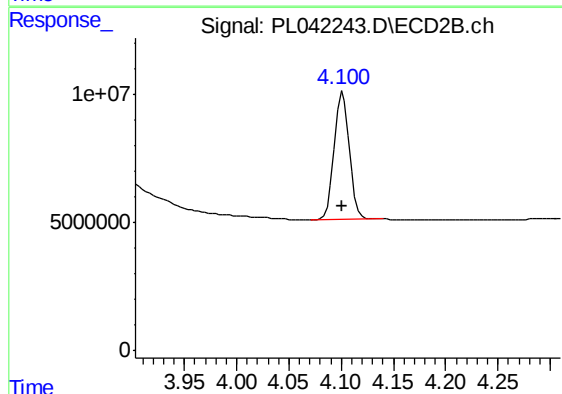


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 50355233
Conc: 18.22 ng/ml

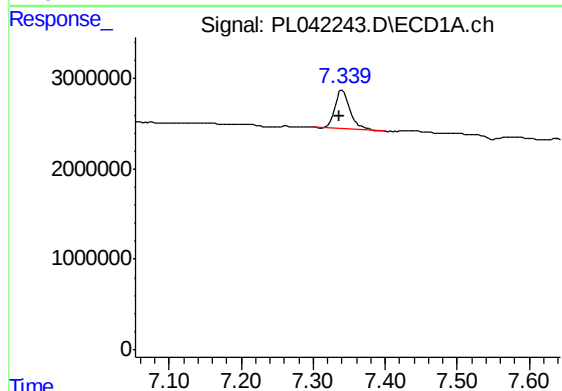


#22 Mirex

R.T.: 7.341 min
Delta R.T.: 0.004 min
Response: 6285821
Conc: 1.10 ng/ml

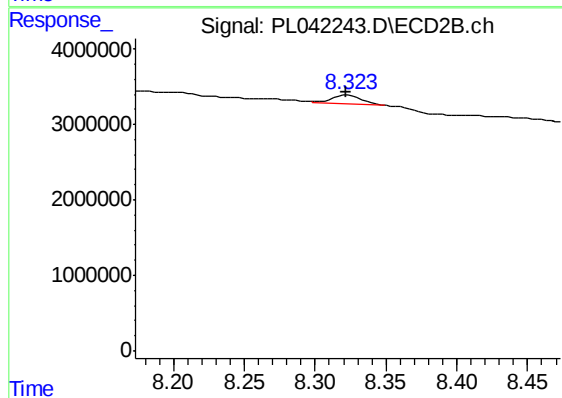

#22 Mirex

R.T.: 8.323 min
Delta R.T.: 0.002 min
Response: 1734729
Conc: 0.93 ng/ml m

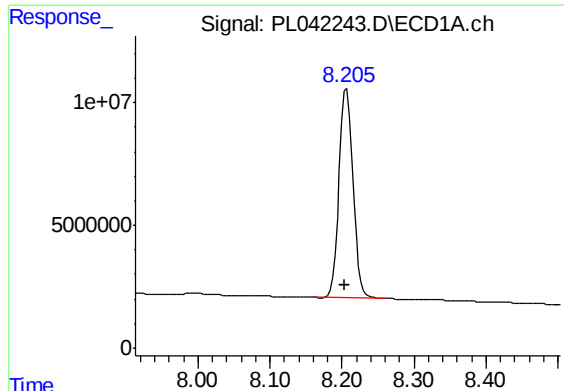


#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.003 min
Response: 114670994
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-02

Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:44 PM

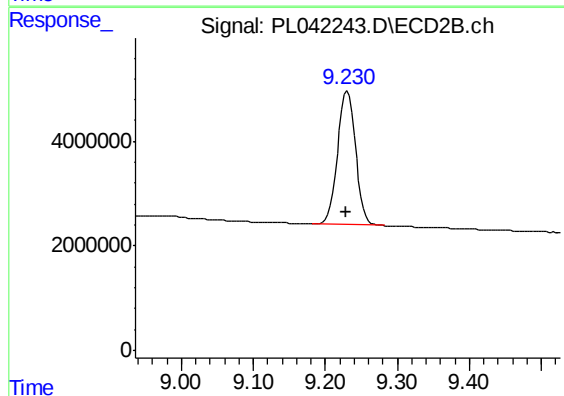

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.003 min
Response: 44514163
Conc: 18.70 ng/ml