

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 14:23
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-03
 Misc : FOR MIREX
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-03

Manual Integrations
 APPROVED

Sohil
 11/16/2018 4:01:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 14:39:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	98290362	51146115	17.709	18.502
28)	SA Decachlor...	8.206	9.231	117.6E6	45707623	19.001	19.201
Target Compounds							
22)	Mirex	7.340	8.323	6782547	1182762	1.190	0.634m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 14:23
Operator : AJ\SJ
Sample : MIREX-MDL-W-03
Misc : FOR MIREX
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-03


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 14:39:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

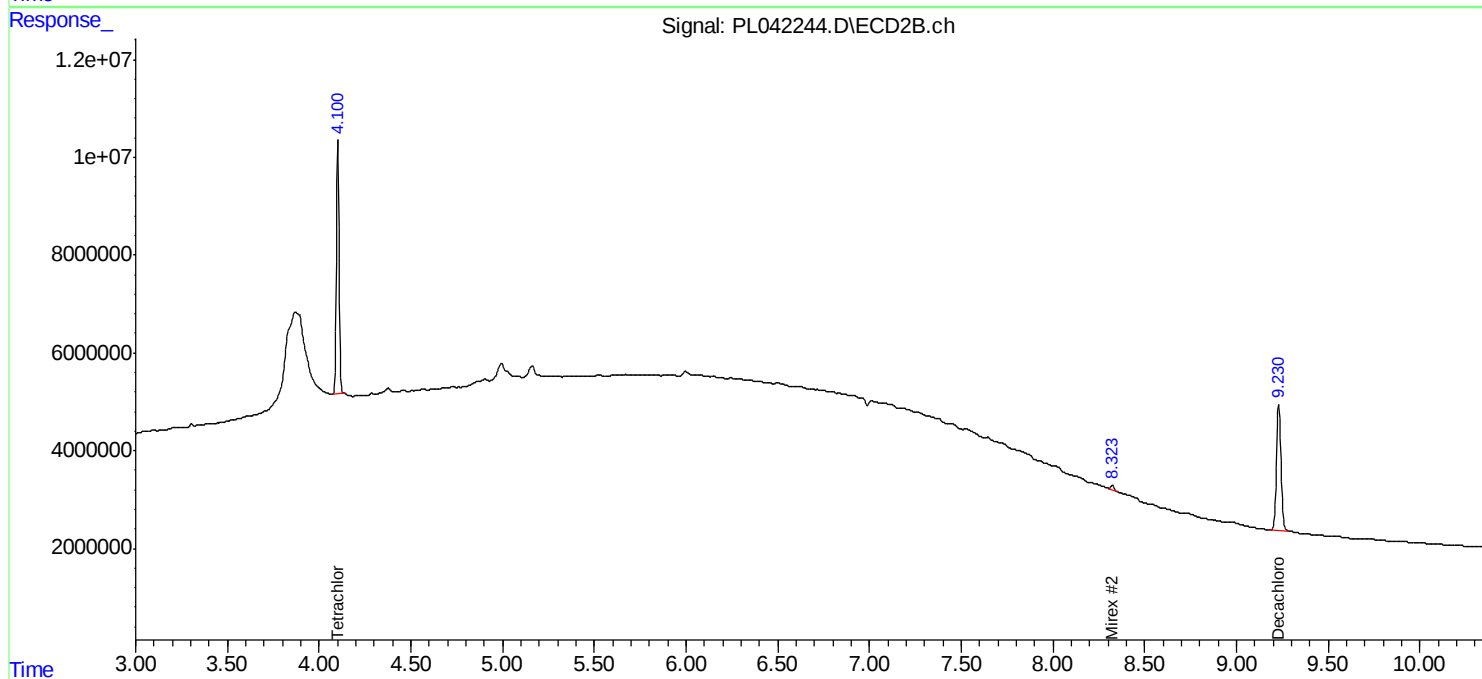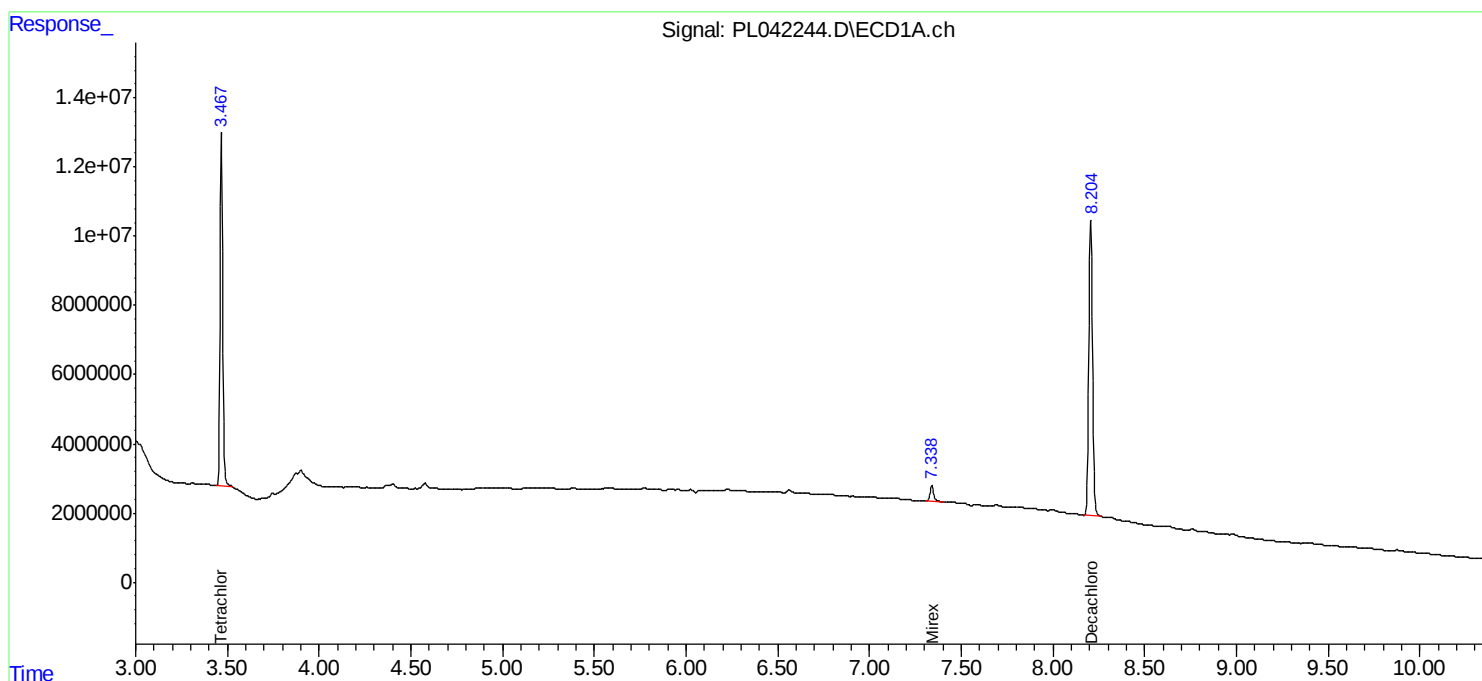

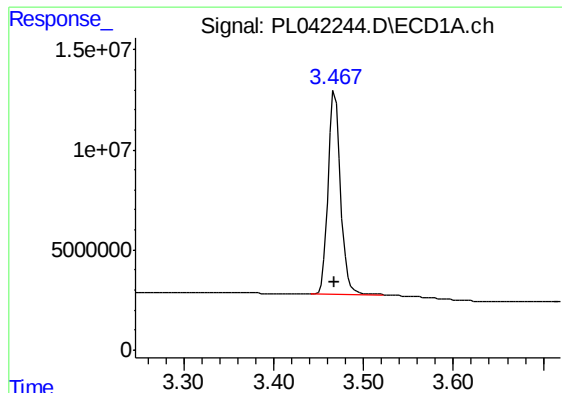


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 98290362
Conc: 17.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-03


Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:45 PM

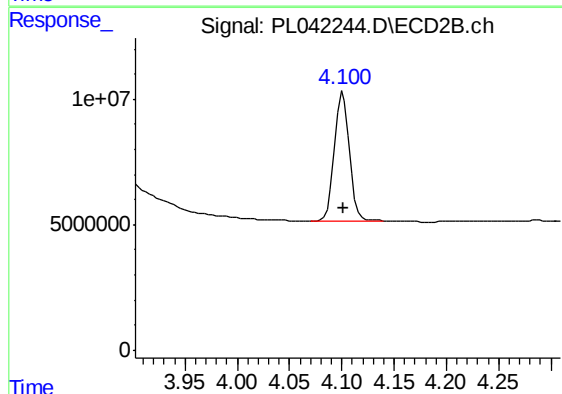


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 51146115
Conc: 18.50 ng/ml

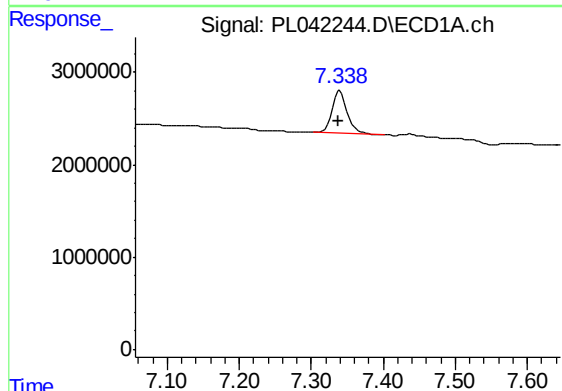


#22 Mirex

R.T.: 7.340 min
Delta R.T.: 0.003 min
Response: 6782547
Conc: 1.19 ng/ml

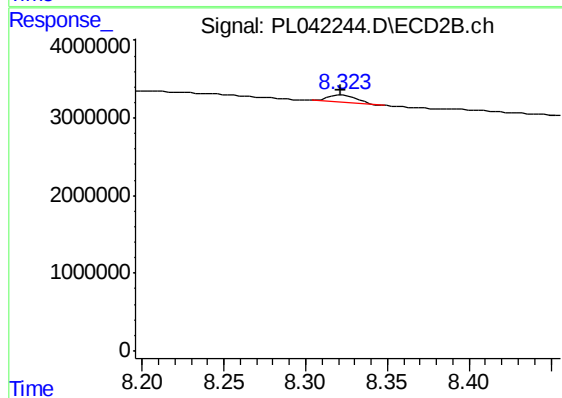

#22 Mirex

R.T.: 8.323 min
Delta R.T.: 0.001 min
Response: 1182762
Conc: 0.63 ng/ml m

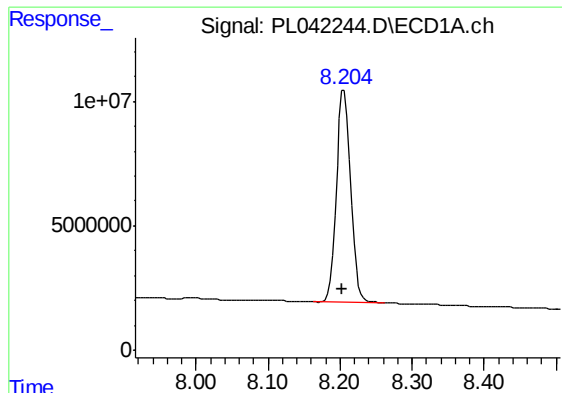


#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.002 min
Response: 117582574
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-03

Manual Integrations
APPROVED

Sohil
11/16/2018 4:01:45 PM

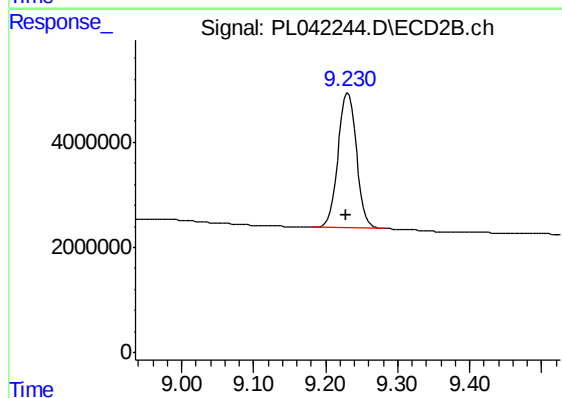

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.003 min
Response: 45707623
Conc: 19.20 ng/ml