

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
 Data File : PL042246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2018 14:51
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc : FOR MIREX
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 15:02:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	278.0E6	140.2E6	50.090	50.733
28)	SA Decachlor...	8.206	9.231	293.9E6	117.2E6	47.499	49.252
Target Compounds							
22)	Mirex	7.340	8.324	273.2E6	94272734	47.934	50.571



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111718\
Data File : PL042246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2018 14:51
Operator : AJ\SJ
Sample : PSTDCCC050
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 15:02:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

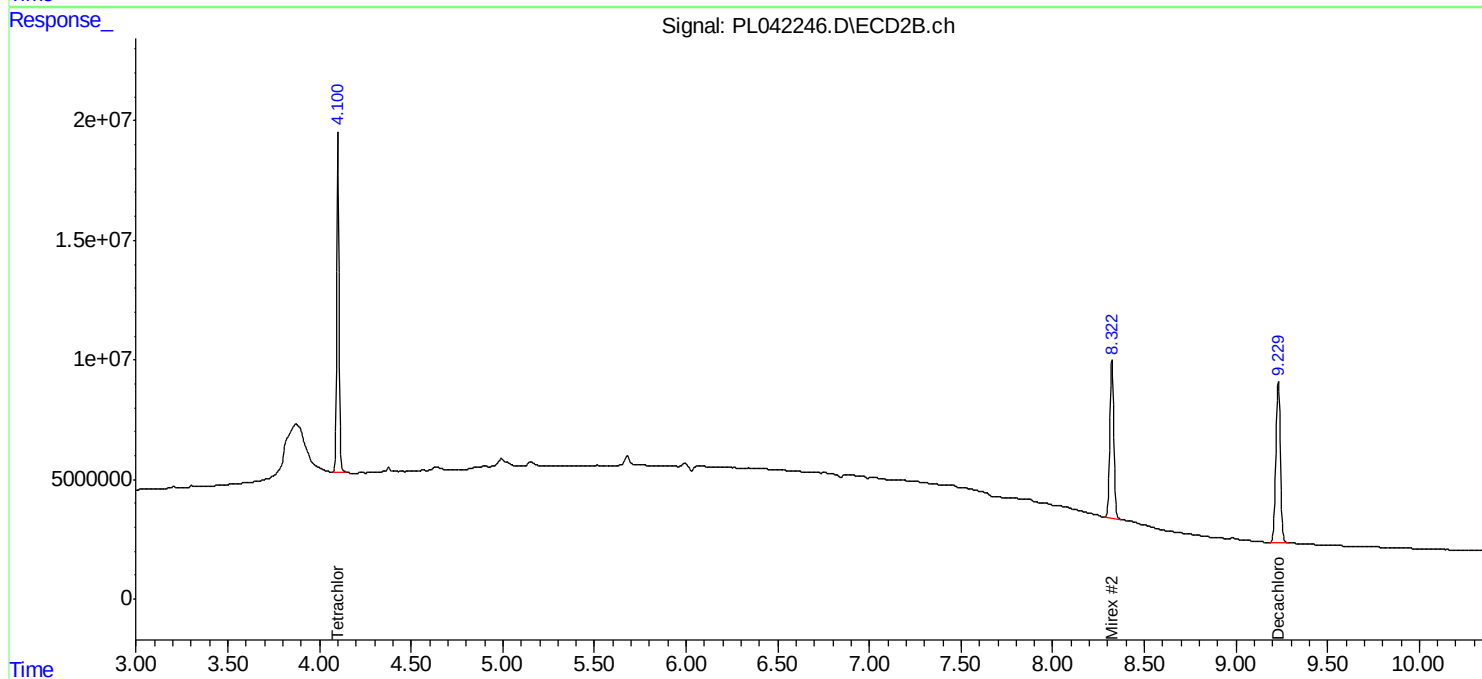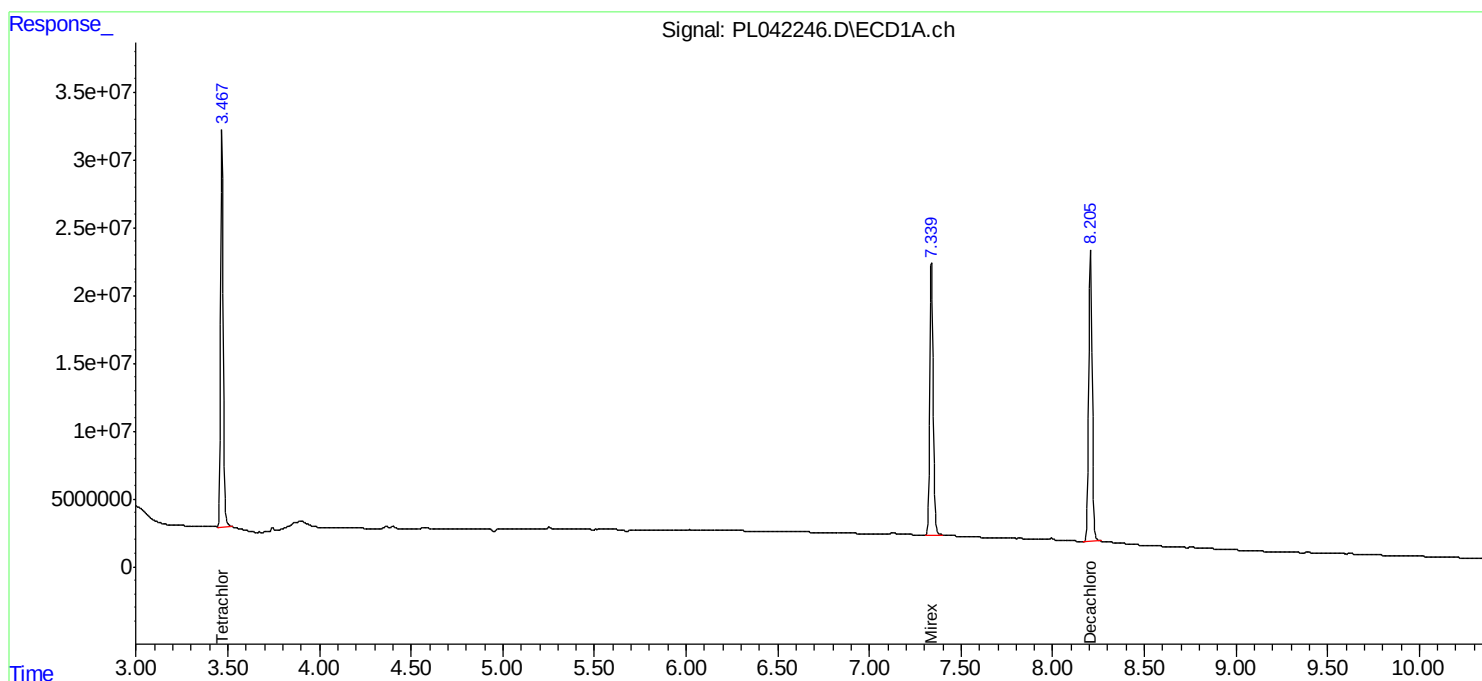


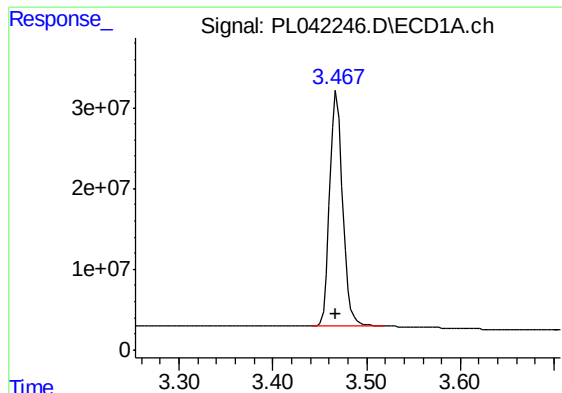

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 278023209
Conc: 50.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

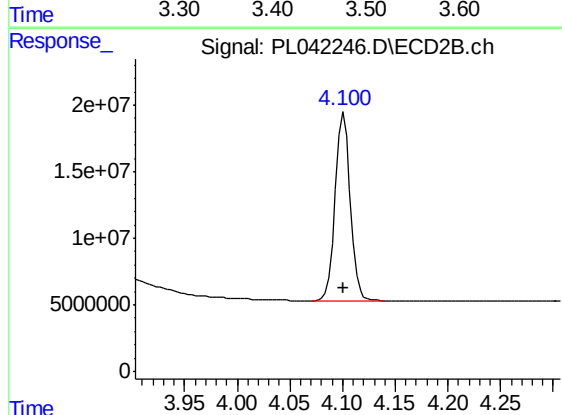


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 140245696
Conc: 50.73 ng/ml

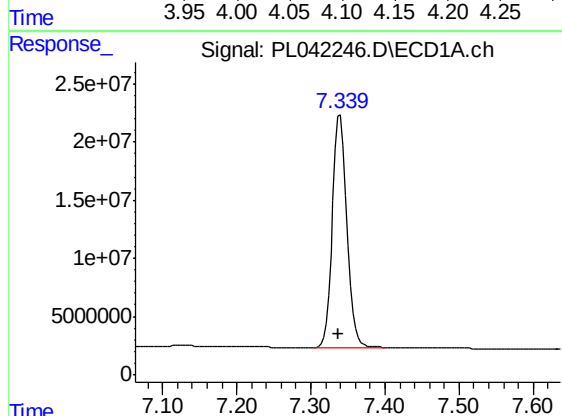


#22 Mirex

R.T.: 7.340 min
Delta R.T.: 0.003 min
Response: 273246930
Conc: 47.93 ng/ml

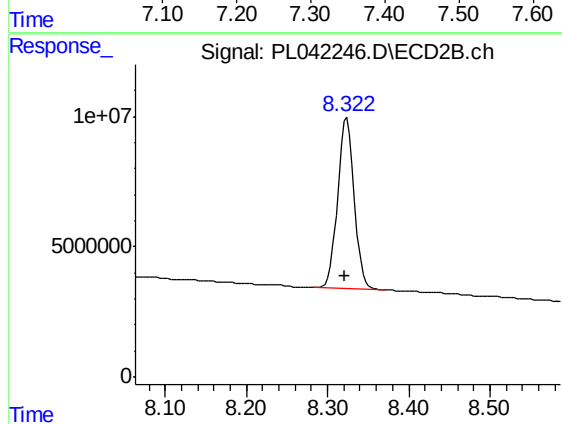

#22 Mirex


R.T.: 8.324 min
Delta R.T.: 0.002 min
Response: 94272734
Conc: 50.57 ng/ml

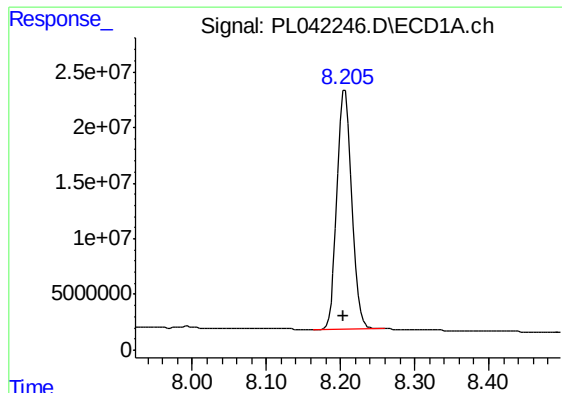

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.003 min
Response: 293942181
Conc: 47.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

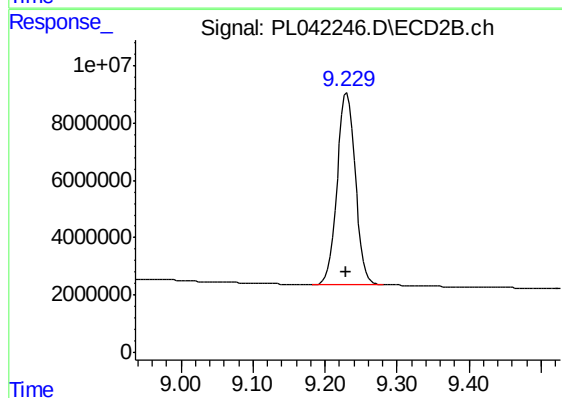

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.002 min
Response: 117241398
Conc: 49.25 ng/ml