

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 15:16
 Operator : DD\AJ
 Sample : L4770-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 03:14:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	25059993	43681900	14.569	14.864
28)	SA Decachlor...	8.128	8.992	21457056	28272406	13.375	13.508
Target Compounds							
2)	A alpha-BHC	0.000	4.361f	0	3211557	N.D.	0.723 #
8)	B Heptachlo...	5.100	5.826	1284296	4322842	0.704	1.335 #
9)	A Endosulfan I	5.449	0.000	1981108	0	1.185	N.D. #
10)	B gamma-Chl...	0.000	6.046	0	4474222	N.D.	1.329 #
11)	B alpha-Chl...	0.000	6.119	0	6097413	N.D.	1.810 #
12)	B 4,4'-DDE	0.000	6.271	0	7513854	N.D.	2.332 #
23)	Chlordane-1	4.260	4.955f	1466381	402500	28.446	4.010 #
25)	Chlordane-3	0.000	6.046	0	4474222	N.D.	11.076 #
26)	Chlordane-4	0.000	6.119	0	6097413	N.D.	12.591 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 15:16
Operator : DD\AJ
Sample : L4770-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 03:14:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

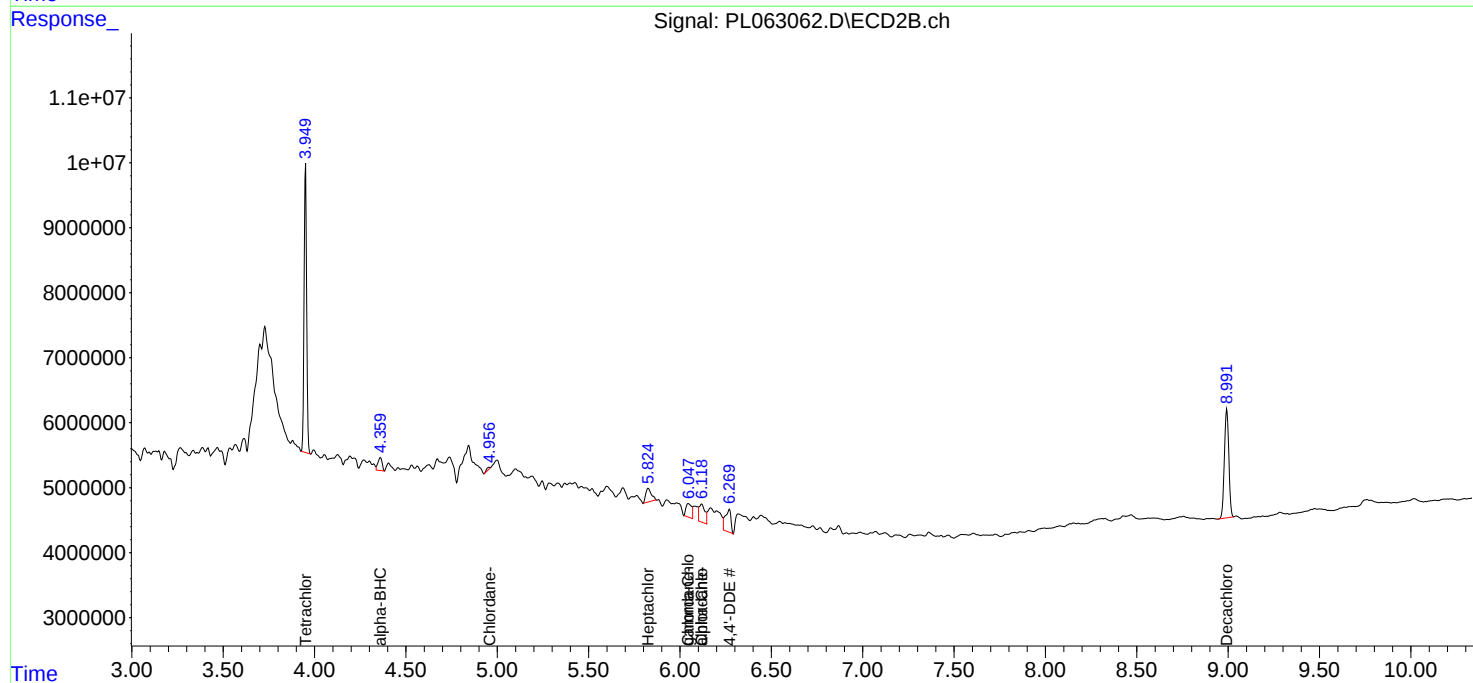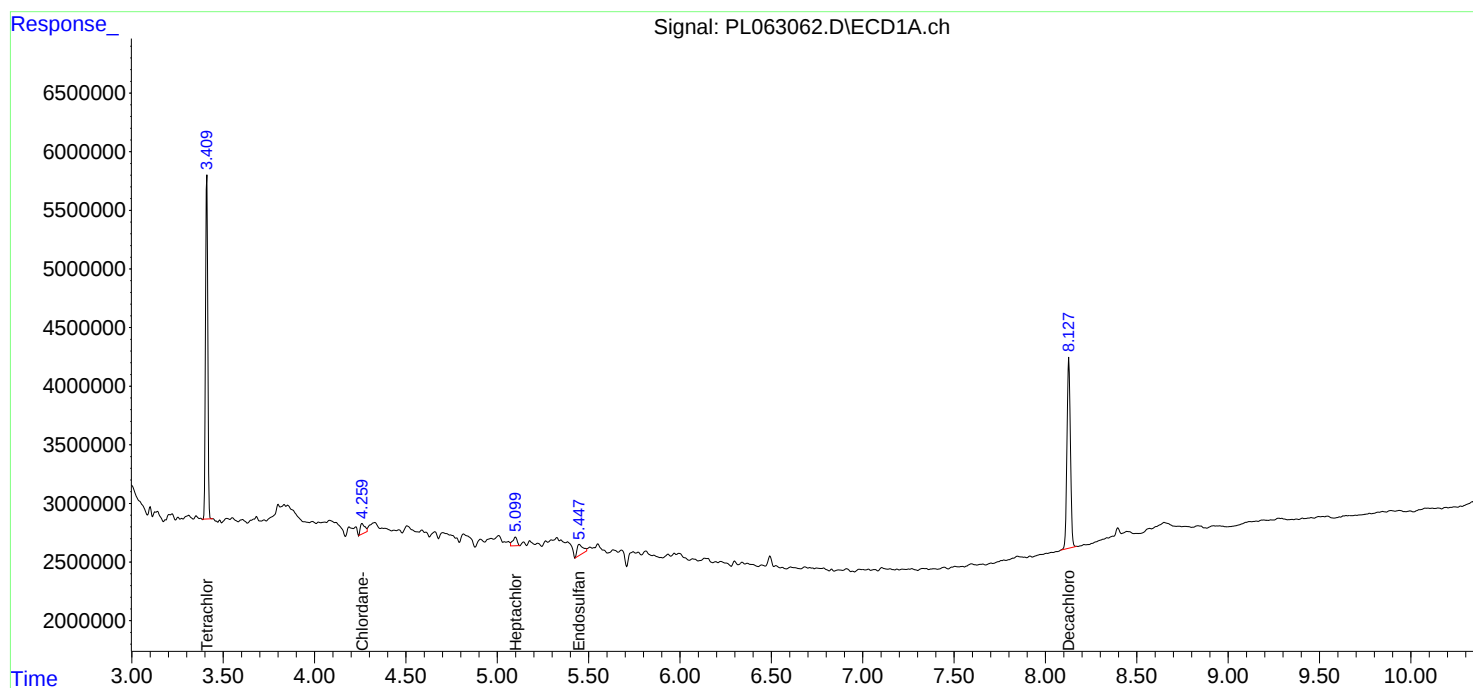


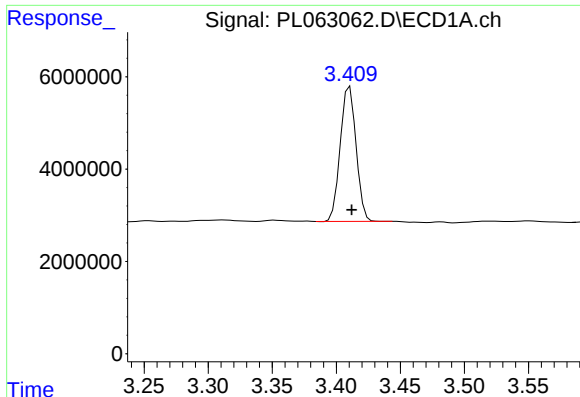

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 25059993
Conc: 14.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

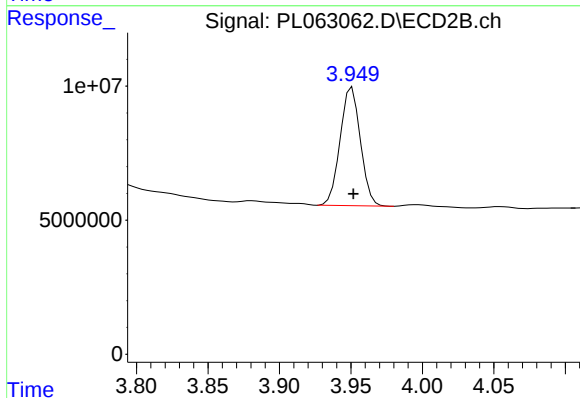


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 43681900
Conc: 14.86 ng/ml

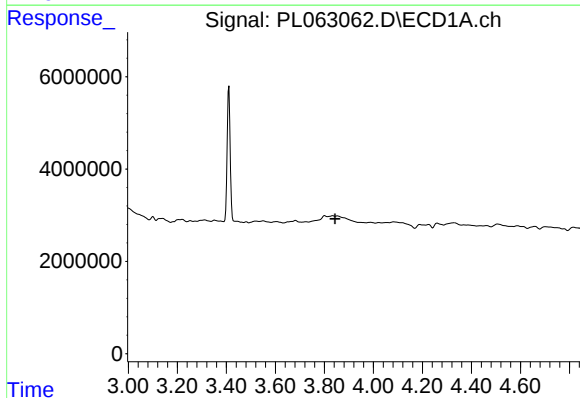


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

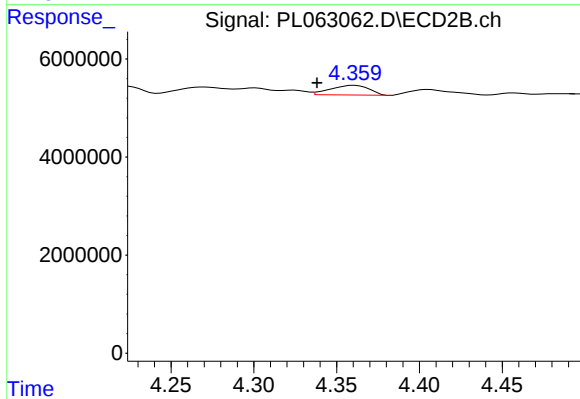

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.023 min
Response: 3211557
Conc: 0.72 ng/ml

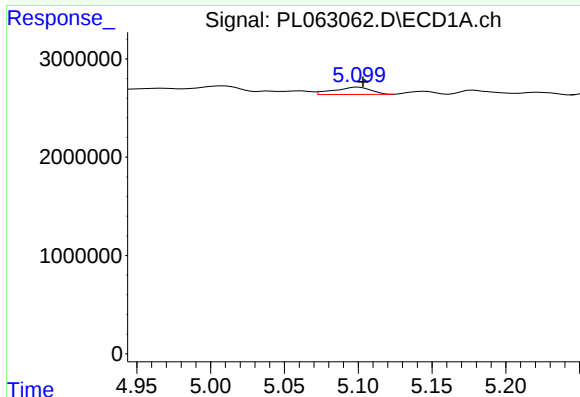

#8 Heptachlor epoxide


R.T.: 5.100 min
Delta R.T.: -0.003 min
Response: 1284296
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

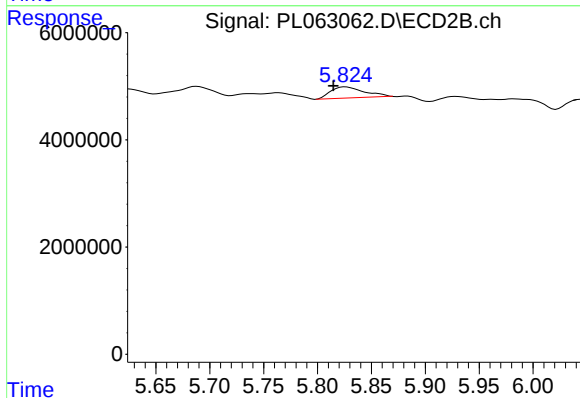


#8 Heptachlor epoxide

R.T.: 5.826 min
Delta R.T.: 0.012 min
Response: 4322842
Conc: 1.33 ng/ml

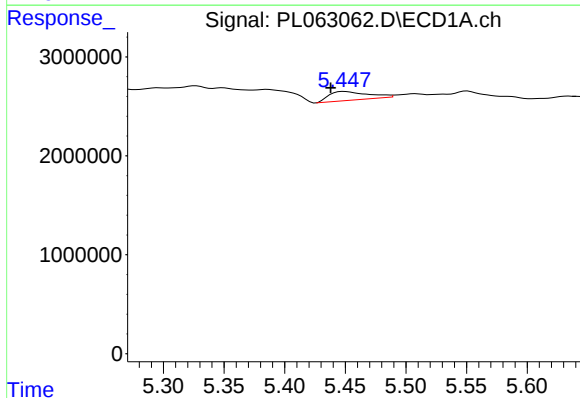


#9 Endosulfan I

R.T.: 5.449 min
Delta R.T.: 0.011 min
Response: 1981108
Conc: 1.19 ng/ml

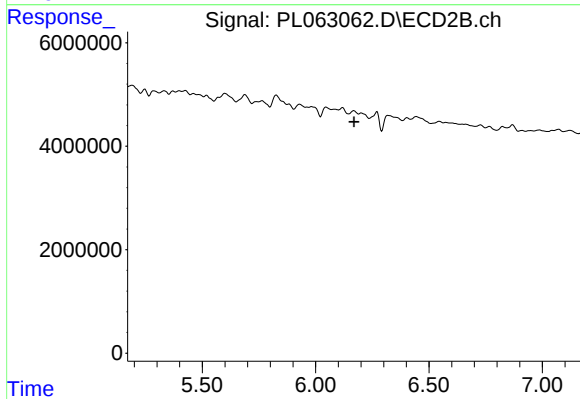

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

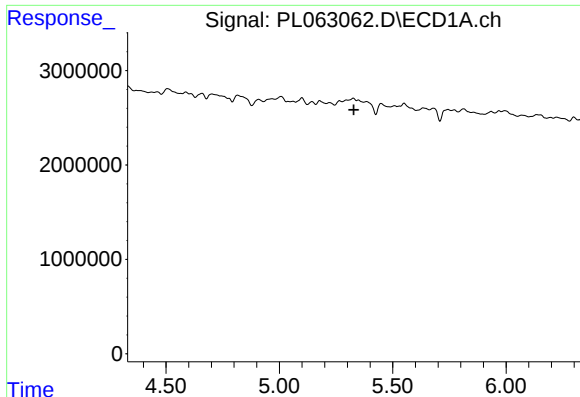

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

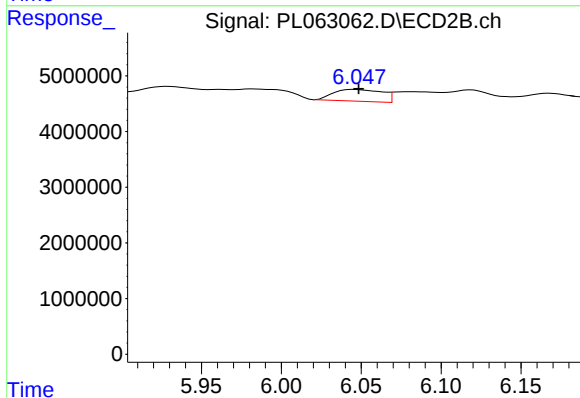


#10 gamma-Chlordane

R.T.: 6.046 min
Delta R.T.: -0.003 min
Response: 4474222
Conc: 1.33 ng/ml

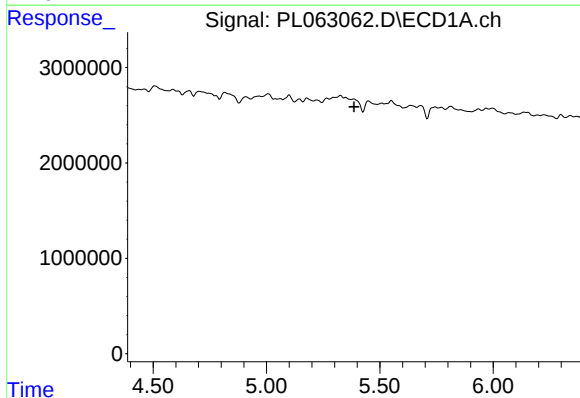


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

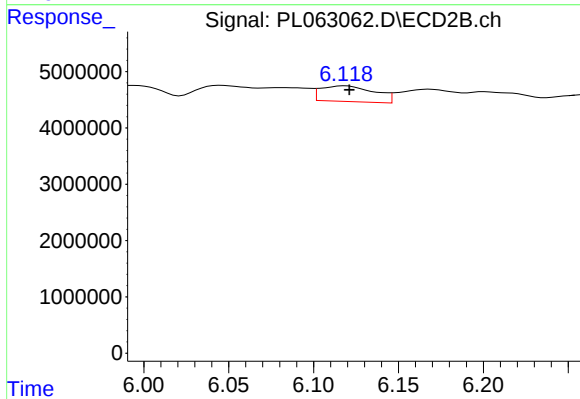

#11 alpha-Chlordane


R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 6097413
Conc: 1.81 ng/ml

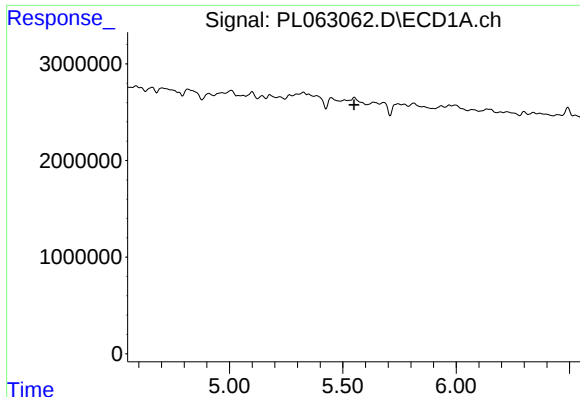

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

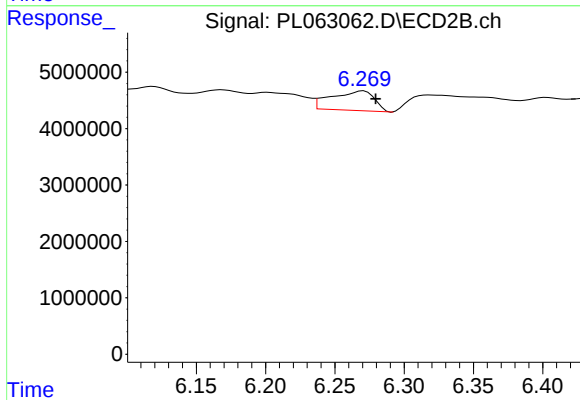


#12 4,4'-DDE

R.T.: 6.271 min
Delta R.T.: -0.009 min
Response: 7513854
Conc: 2.33 ng/ml

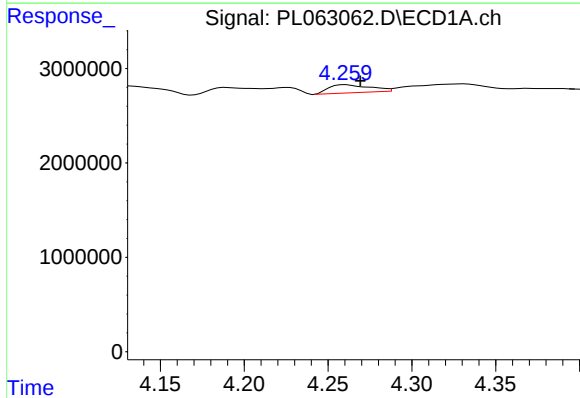


#23 Chlordane-1

R.T.: 4.260 min
Delta R.T.: -0.009 min
Response: 1466381
Conc: 28.45 ng/ml

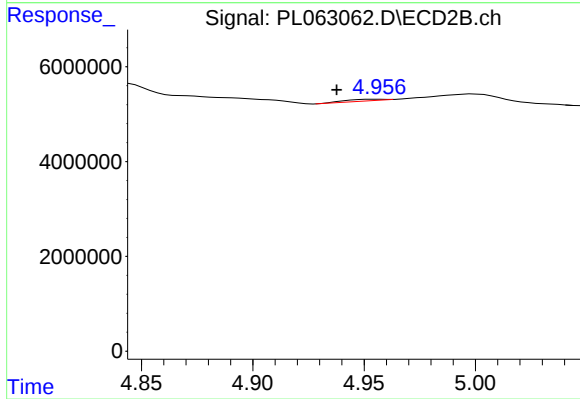

#23 Chlordane-1


R.T.: 4.955 min
Delta R.T.: 0.018 min
Response: 402500
Conc: 4.01 ng/ml

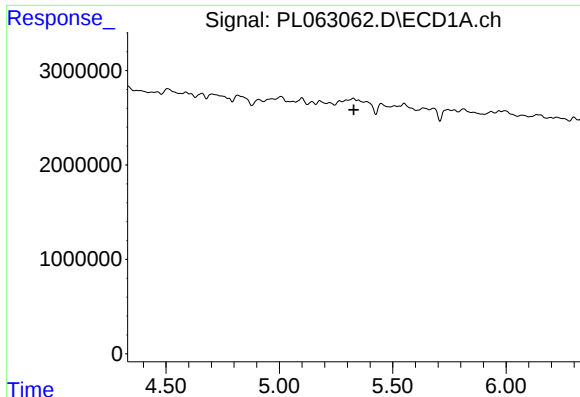

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

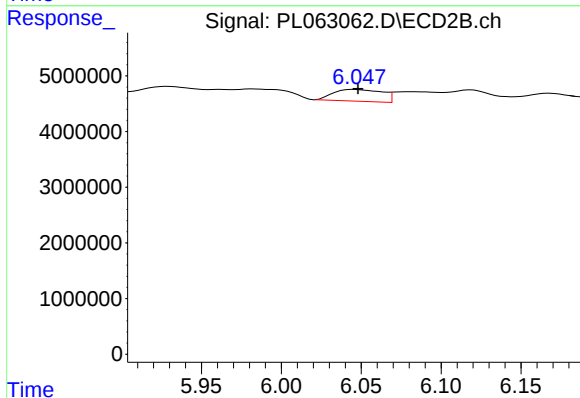


#25 Chlordane-3

R.T.: 6.046 min
Delta R.T.: -0.002 min
Response: 4474222
Conc: 11.08 ng/ml

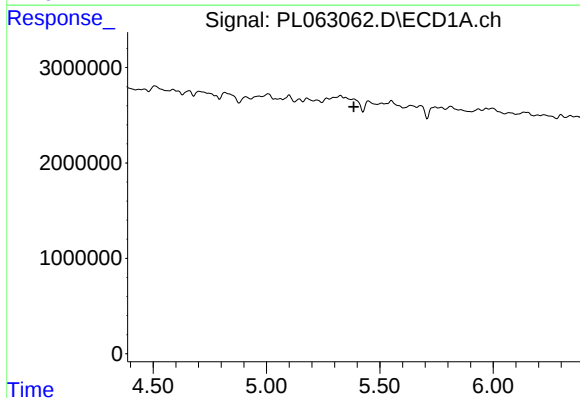


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

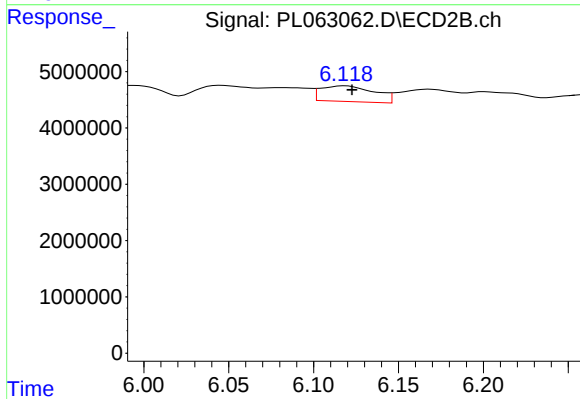

#26 Chlordane-4


R.T.: 6.119 min
Delta R.T.: -0.004 min
Response: 6097413
Conc: 12.59 ng/ml

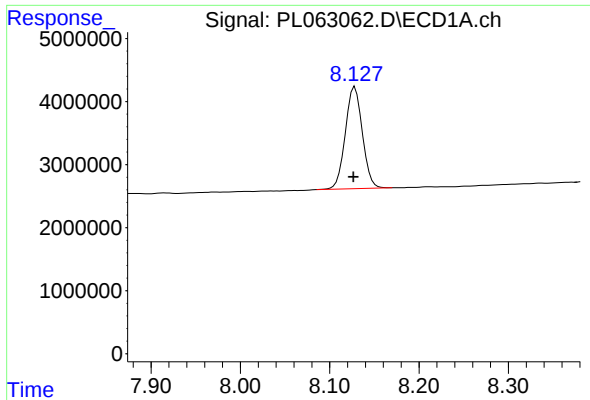

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 21457056
Conc: 13.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

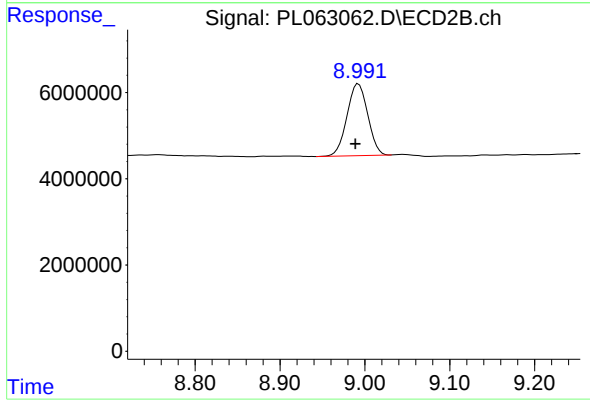

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.004 min
Response: 28272406
Conc: 13.51 ng/ml