

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 11:51
 Operator : DD\AJ
 Sample : L4729-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-658-X

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:43:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 12:20:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	3.950	68759135	58951140	39.974	20.060m#
2) SA Decachlor...	8.128	8.992	32684533	43913152	20.373	20.981m
Target Compounds						
16) A 4,4'-DDD	6.059	6.764	106.3E6	40934881	75.149	15.990 #

Ankita

11/18/2020 10:43:59 AM

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 11:51
Operator : DD\AJ
Sample : L4729-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TI-658-X


Manual Integrations
APPROVED

Ankita
11/18/2020 10:43:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 12:20:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

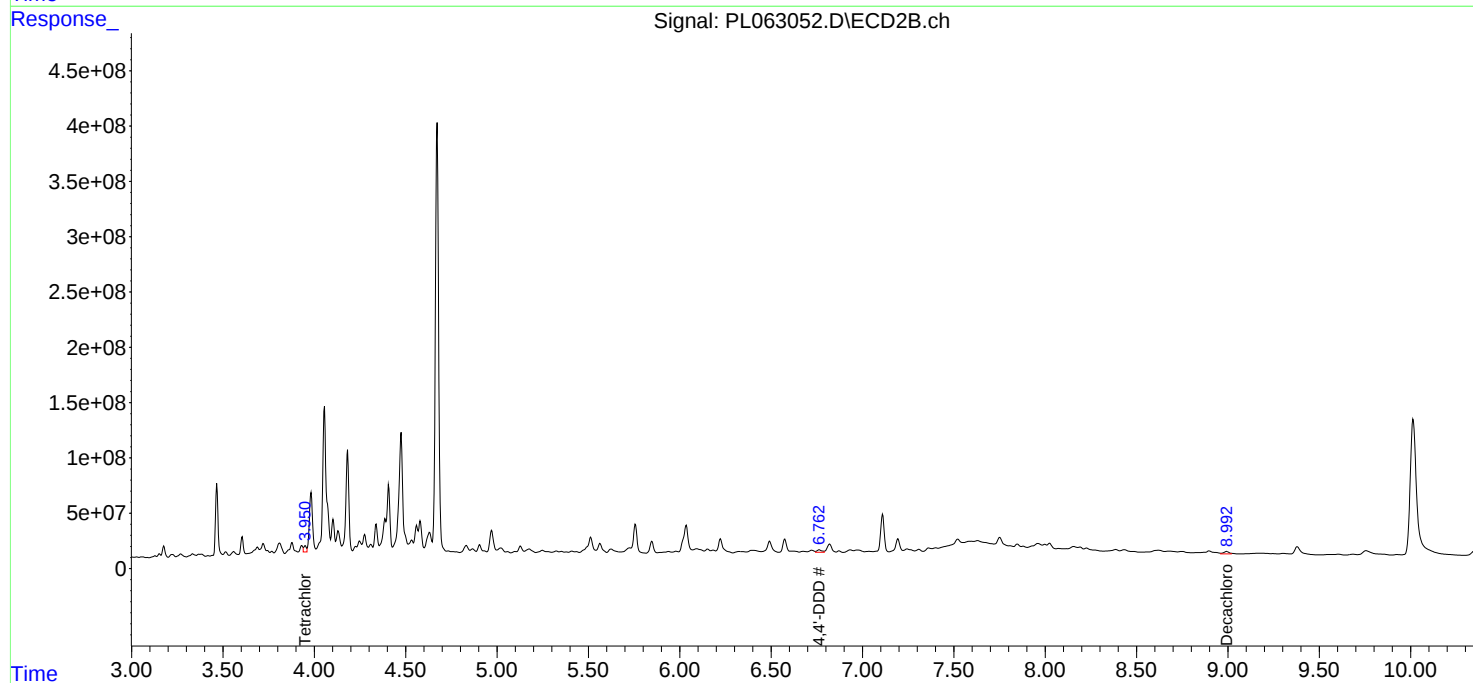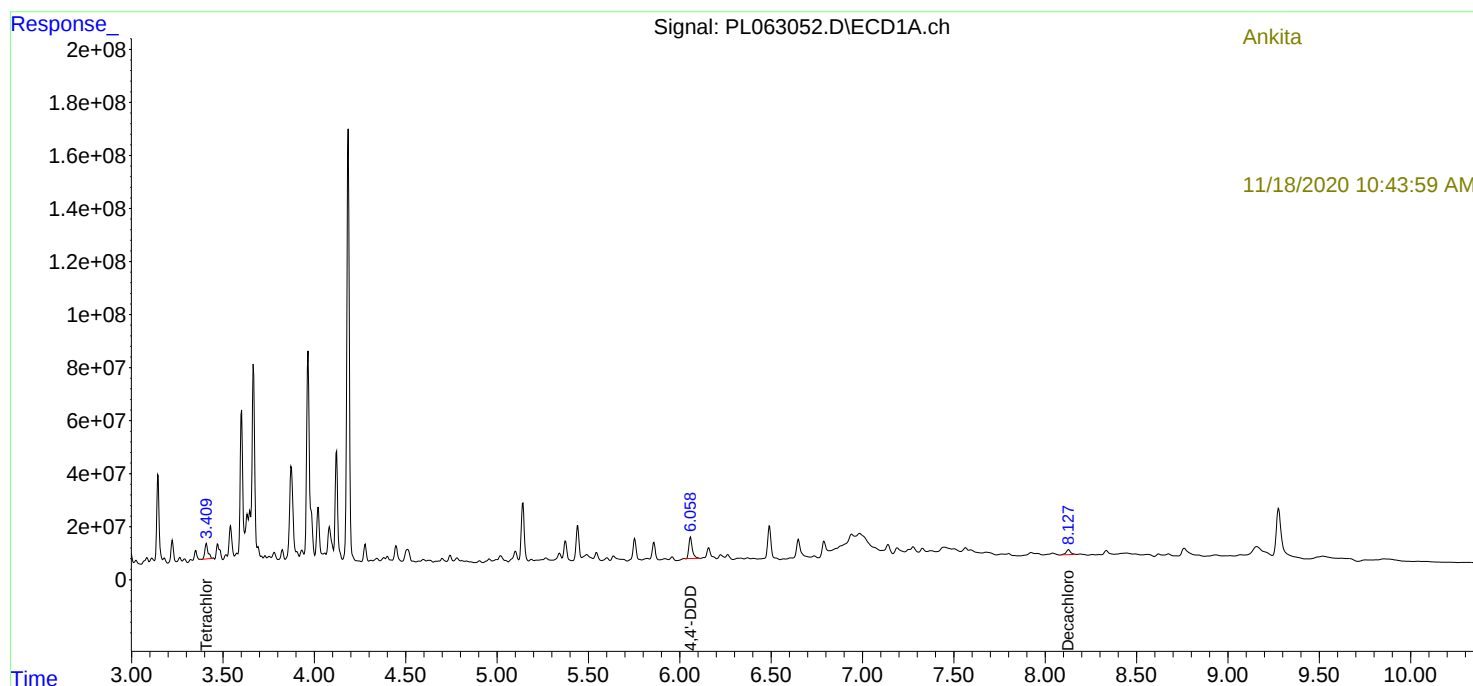

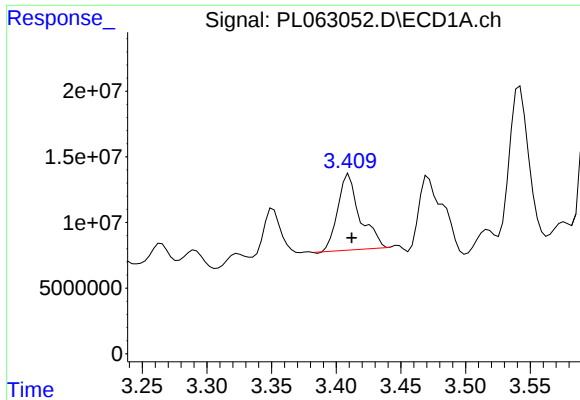


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 68759135
Conc: 39.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-658-X

Manual Integrations
APPROVED


Ankita
11/18/2020 10:43:59 AM

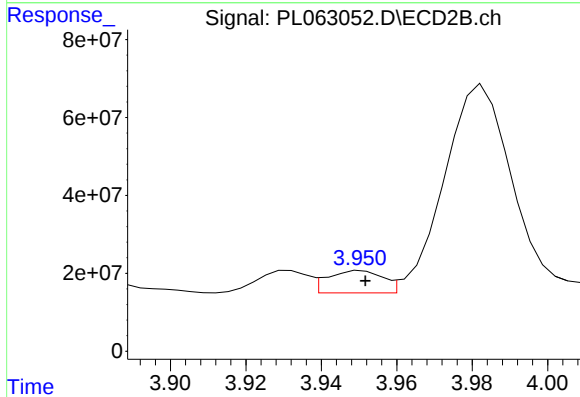

#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 58951140
Conc: 20.06 ng/ml m


Ankita

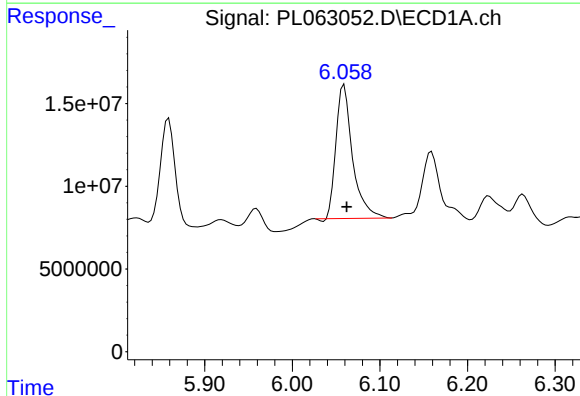

#16 4,4'-DDD


R.T.: 6.059 min
Delta R.T.: -0.003 min
Response: 106298231
Conc: 75.15 ng/ml

11/18/2020 10:43:59 AM

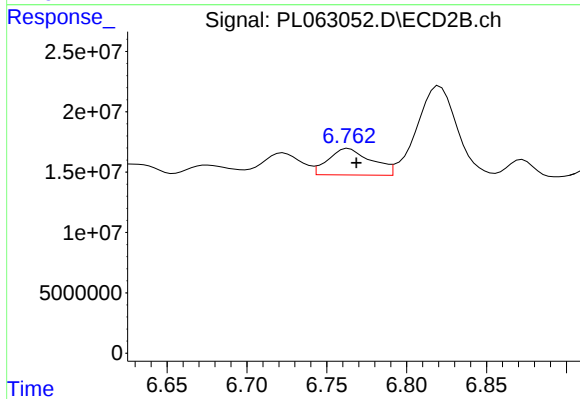

#16 4,4'-DDD

R.T.: 6.764 min
Delta R.T.: -0.005 min
Response: 40934881
Conc: 15.99 ng/ml

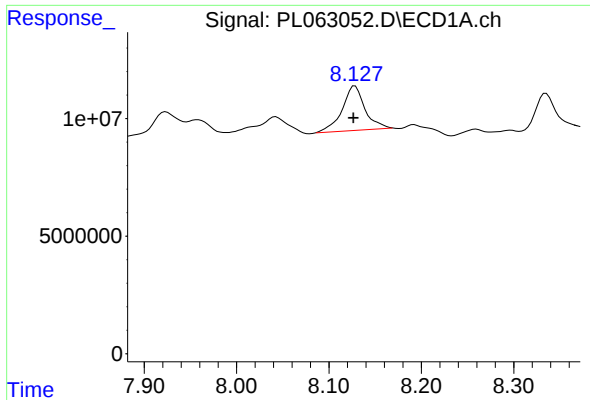

#28 Decachlorobiphenyl

R.T.: 8.128 min

Delta R.T.: 0.002 min


Response: 32684533

Conc: 20.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-658-X

Manual Integrations
APPROVED

Ankita
11/18/2020 10:43:59 AM

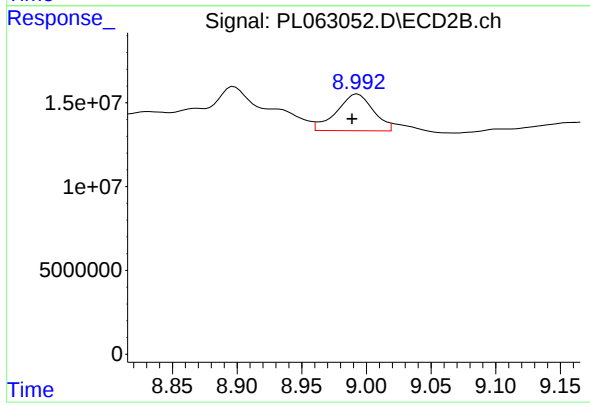

#28 Decachlorobiphenyl

R.T.: 8.992 min

Delta R.T.: 0.003 min

Response: 43913152

Conc: 20.98 ng/ml m

Ankita

11/18/2020 10:43:59 AM