

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 12:21
 Operator : DD\AJ
 Sample : L4730-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-604

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:44:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 13:43:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	77505474	70529927	45.059	24.000m#
28)	SA Decachlor...	8.131	8.995	28690174	42761188	17.883	20.431m
Target Compounds							
4)	MA Heptachlor	4.427	5.129	12095126	94131322	5.637	23.604 #
12)	B 4,4'-DDE	5.549	6.281	6292312	10426504	3.803	3.236

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 12:21
Operator : DD\AJ
Sample : L4730-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TI-604


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 13:43:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

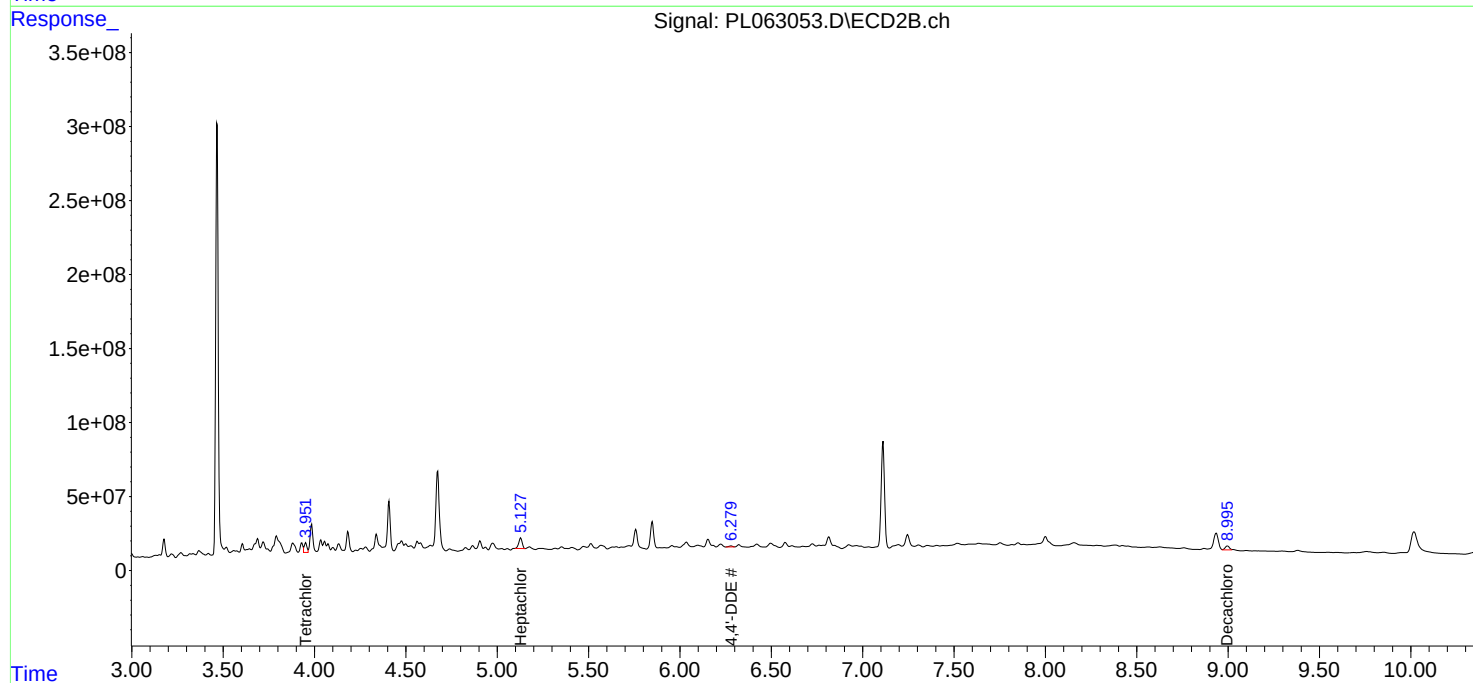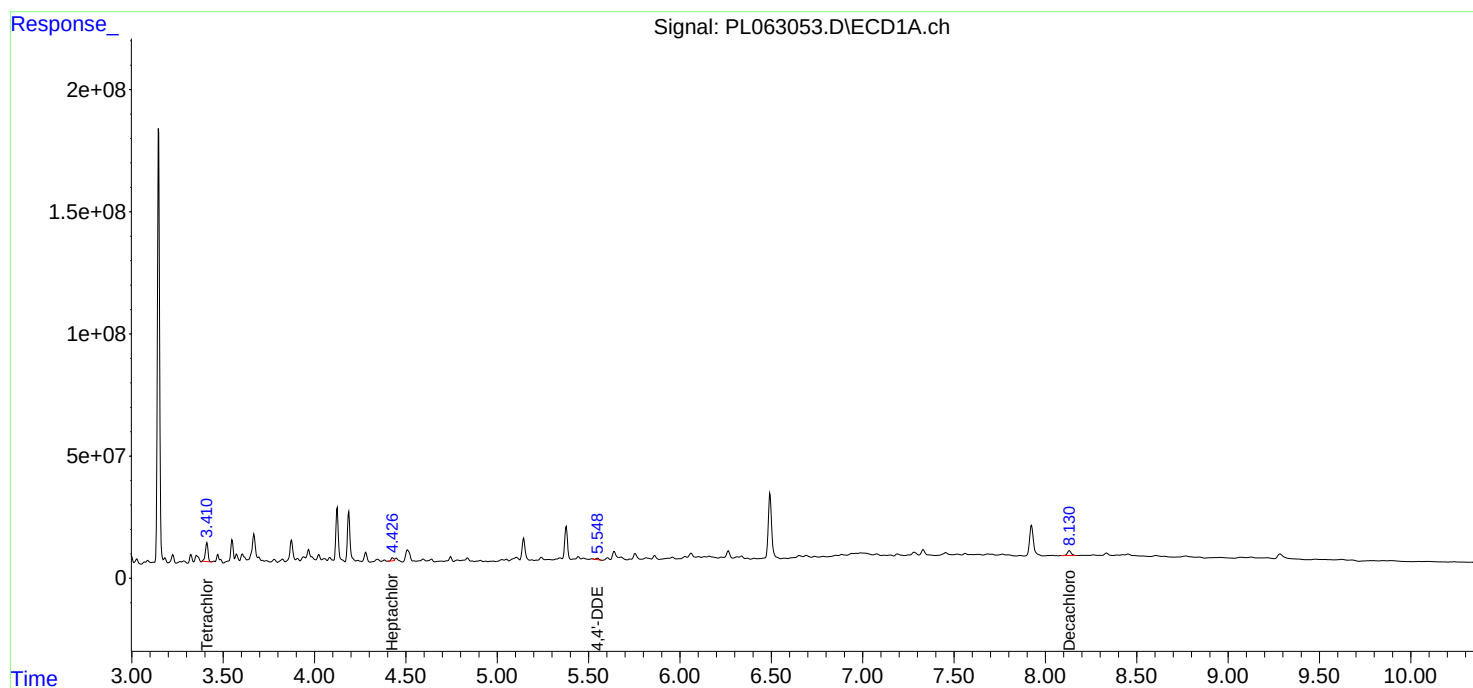

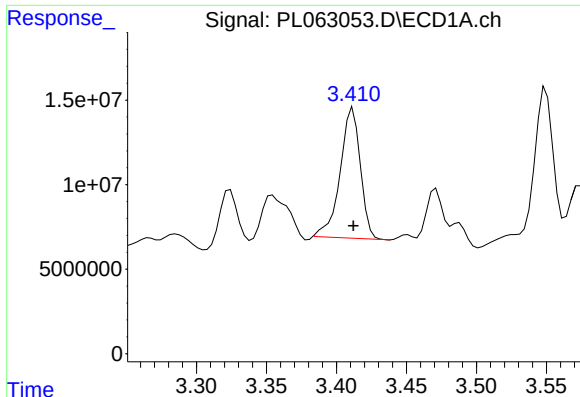


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 77505474
Conc: 45.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-604


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:01 AM

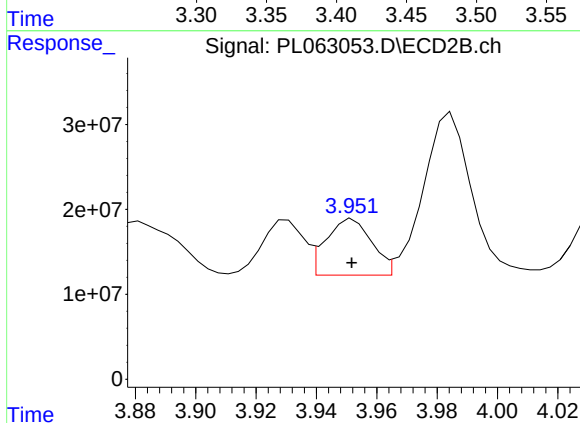


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 70529927
Conc: 24.00 ng/ml m

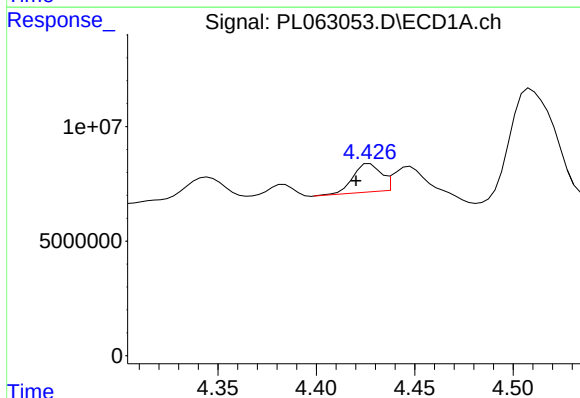


#4 Heptachlor

R.T.: 4.427 min
Delta R.T.: 0.007 min
Response: 12095126
Conc: 5.64 ng/ml

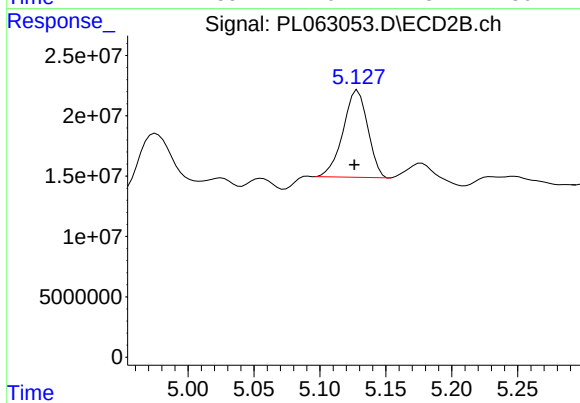

#4 Heptachlor

R.T.: 5.129 min
Delta R.T.: 0.003 min
Response: 94131322
Conc: 23.60 ng/ml

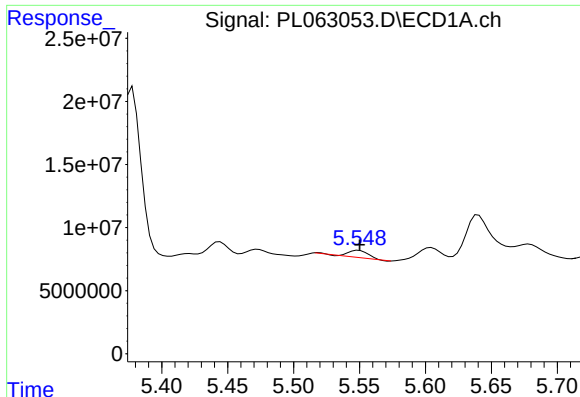


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 6292312
Conc: 3.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-604


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:01 AM

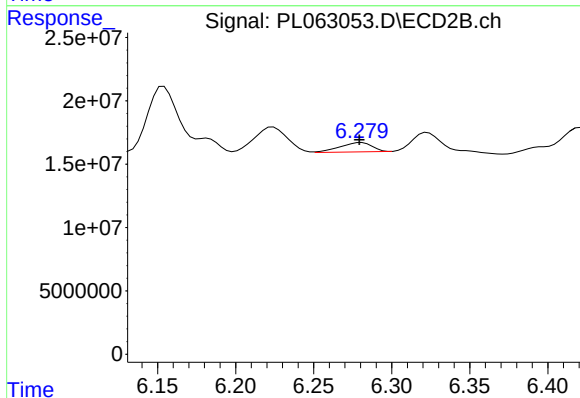


#12 4,4'-DDE

R.T.: 6.281 min
Delta R.T.: 0.001 min
Response: 10426504
Conc: 3.24 ng/ml

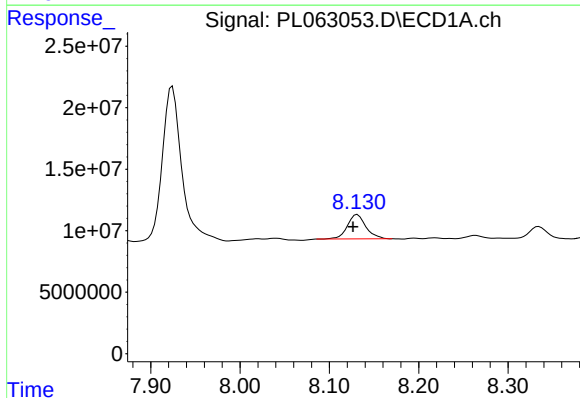

#28 Decachlorobiphenyl

R.T.: 8.131 min
Delta R.T.: 0.005 min
Response: 28690174
Conc: 17.88 ng/ml

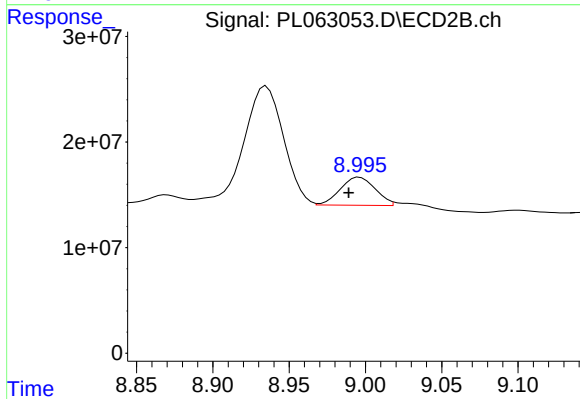

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.006 min
Response: 42761188
Conc: 20.43 ng/ml m