

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 12:35
 Operator : DD\AJ
 Sample : L4731-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-633

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:44:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 13:43:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	74036000	57245693	43.042	19.480m#
28)	SA Decachlor...	8.130	8.992	30974480	37257866	19.307	17.802
Target Compounds							
16)	A 4,4'-DDD	6.060	6.761	62676587	32101153	44.310m	12.540m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 12:35
Operator : DD\AJ
Sample : L4731-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TI-633


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 13:43:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

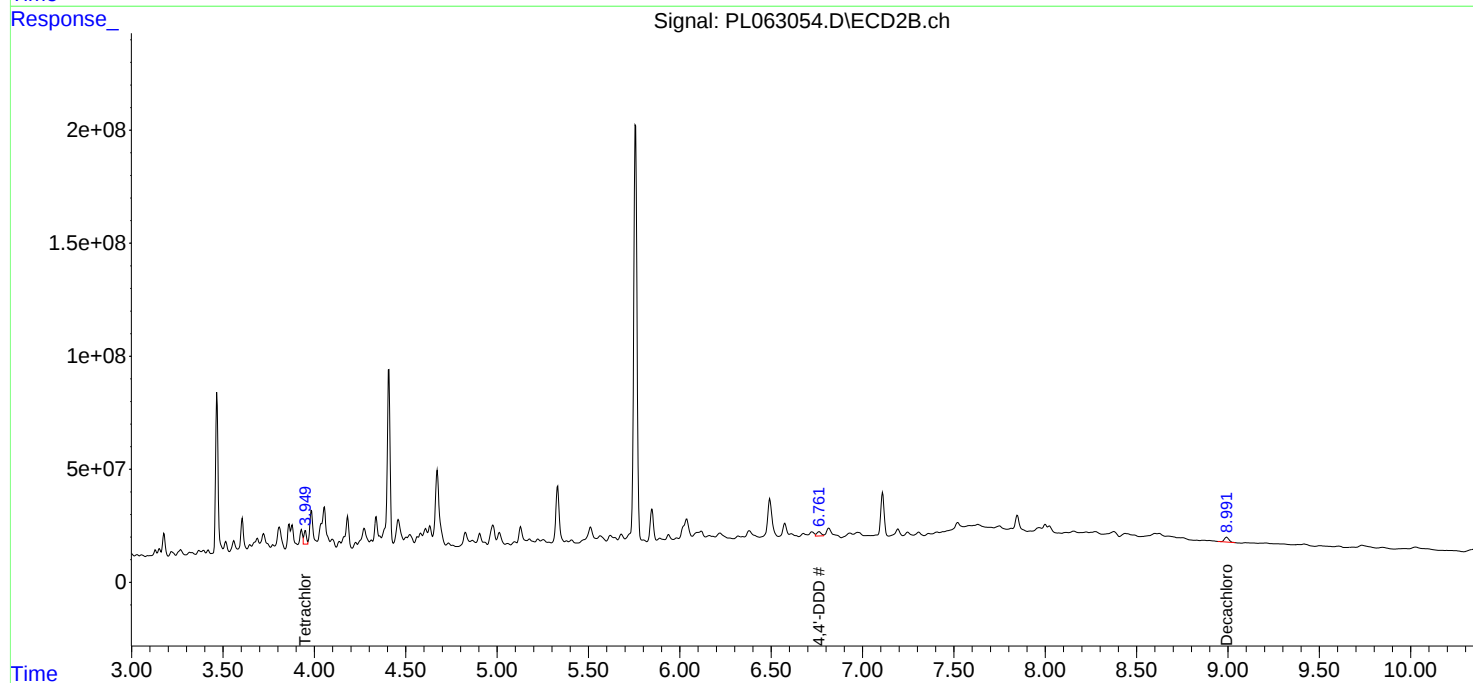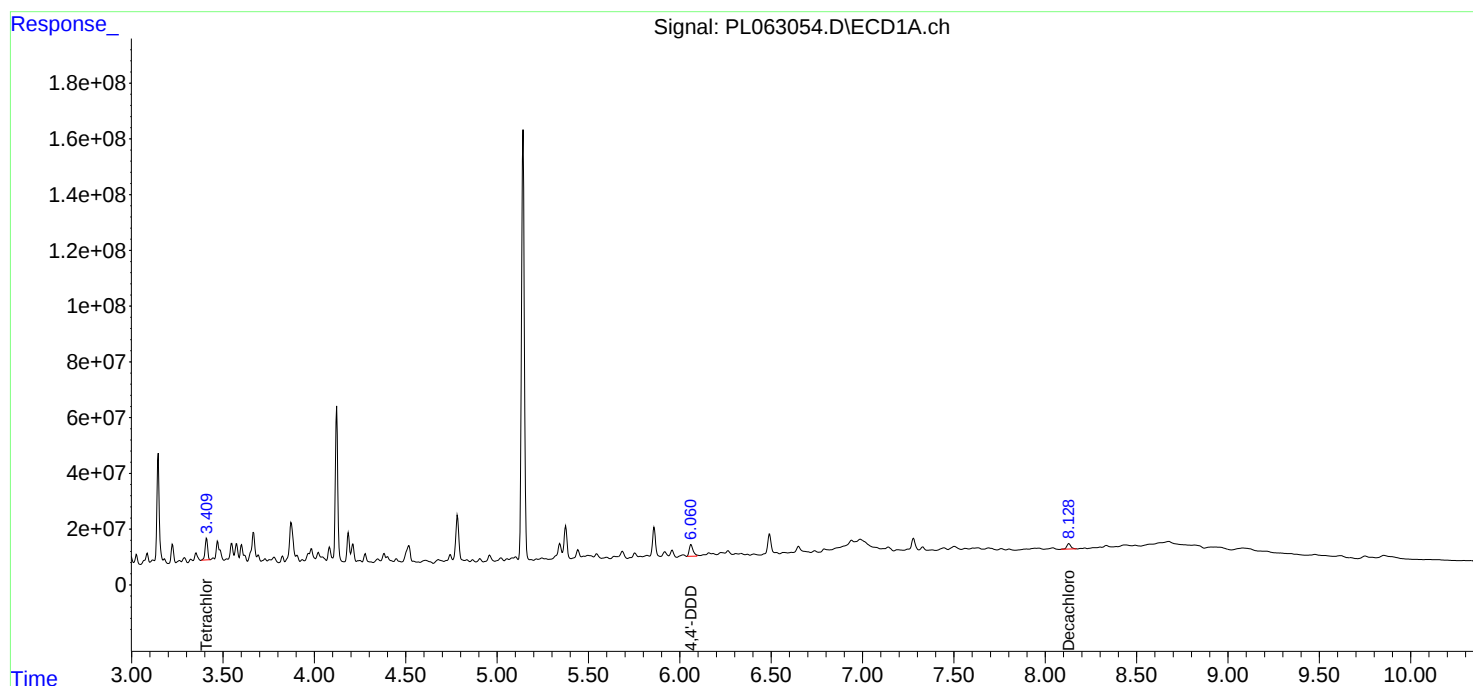

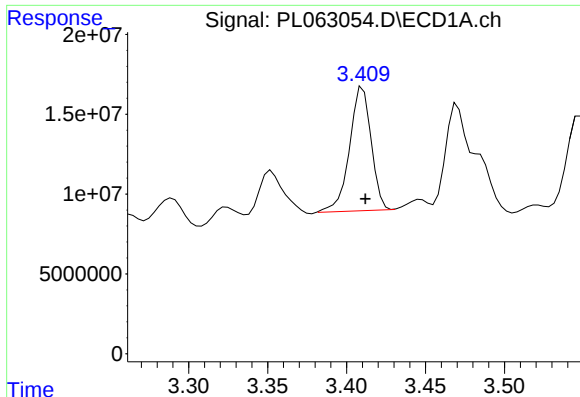


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 74036000
Conc: 43.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-633


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:03 AM

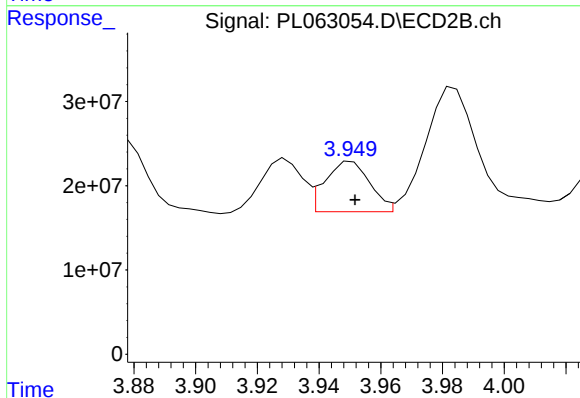


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 57245693
Conc: 19.48 ng/ml m

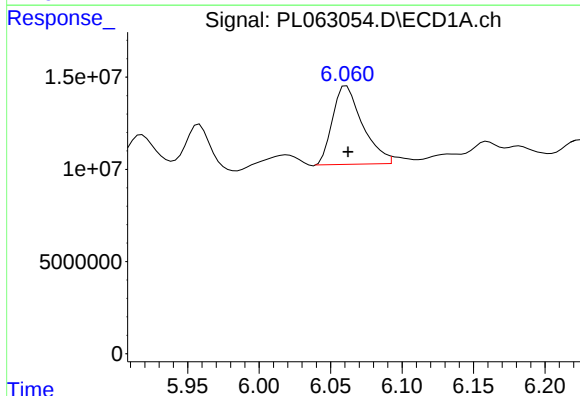


#16 4,4'-DDD

R.T.: 6.060 min
Delta R.T.: -0.002 min
Response: 62676587
Conc: 44.31 ng/ml m

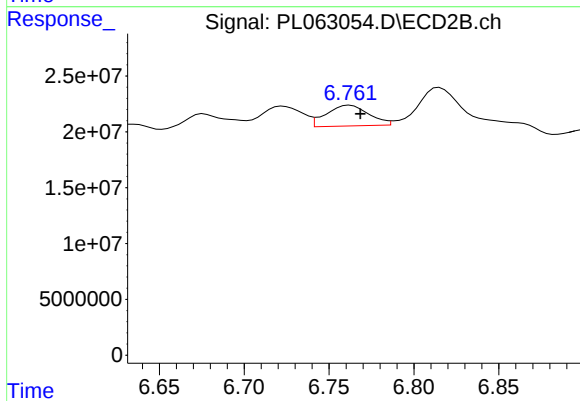

#16 4,4'-DDD

R.T.: 6.761 min
Delta R.T.: -0.007 min
Response: 32101153
Conc: 12.54 ng/ml m

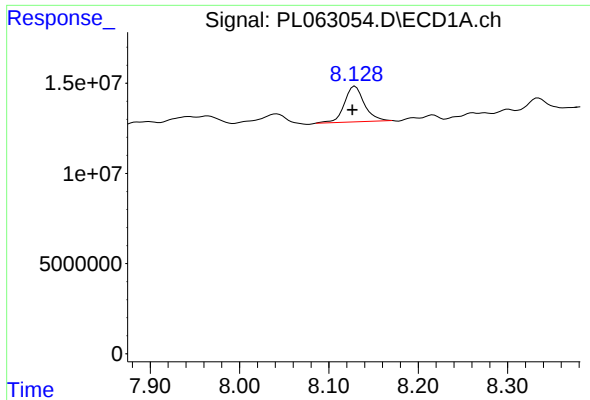


#28 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.003 min
Response: 30974480
Conc: 19.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-633

Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:03 AM

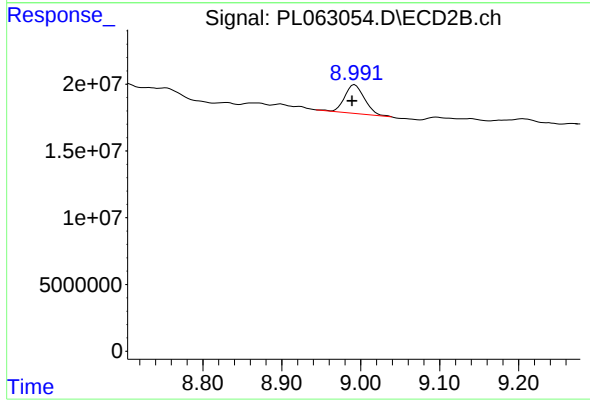

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 37257866
Conc: 17.80 ng/ml