

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 15:30
 Operator : DD\AJ
 Sample : L4770-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FJ-BH-02-0-1

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:44:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 03:14:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	25880800	45116706	15.046	15.353
28)	SA Decachlor...	8.129	8.992	22347817	29856095	13.930	14.265
Target Compounds							
12)	B 4,4'-DDE	5.549	6.278	7783881	12879992	4.705m	3.997

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 15:30
Operator : DD\AJ
Sample : L4770-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FJ-BH-02-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 03:14:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

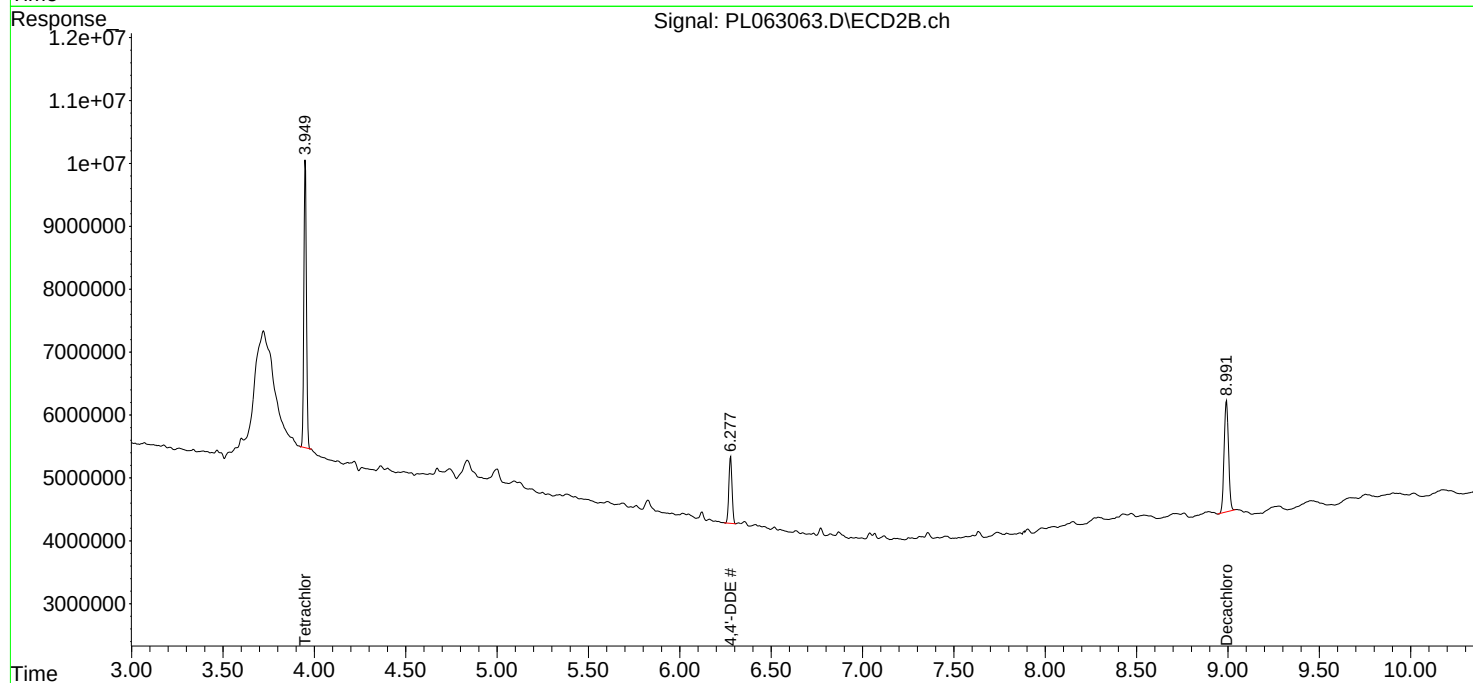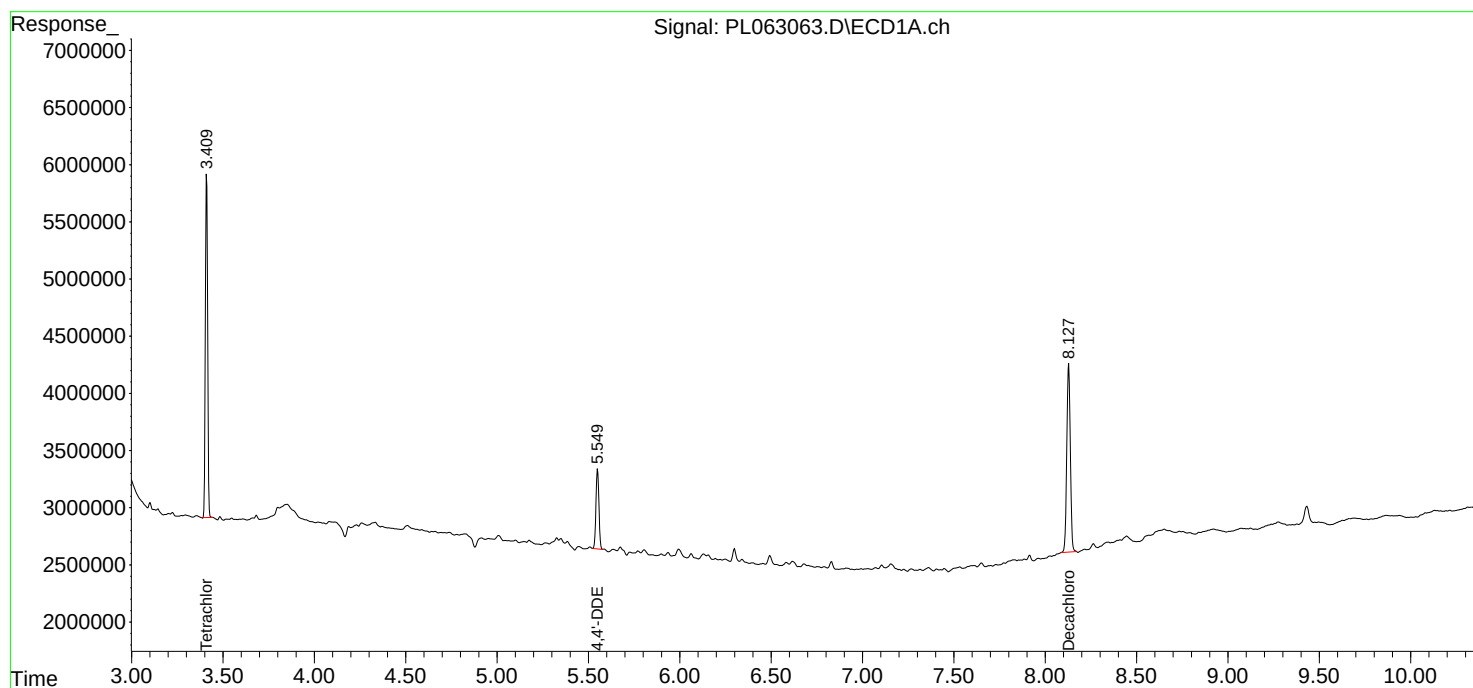

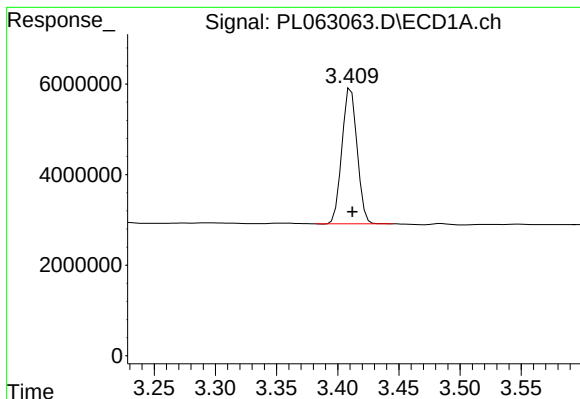


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 25880800
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
FJ-BH-02-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:27 AM

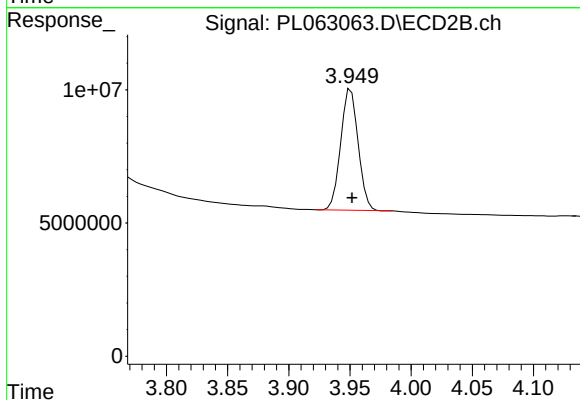


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 45116706
Conc: 15.35 ng/ml

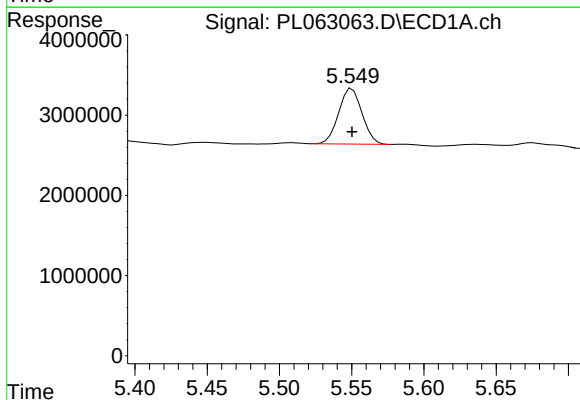


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: -0.001 min
Response: 7783881
Conc: 4.70 ng/ml m

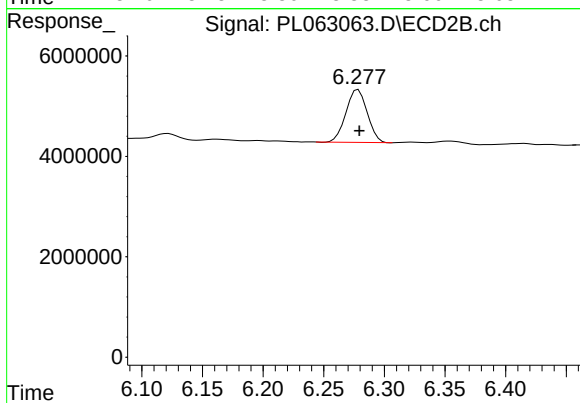

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 12879992
Conc: 4.00 ng/ml

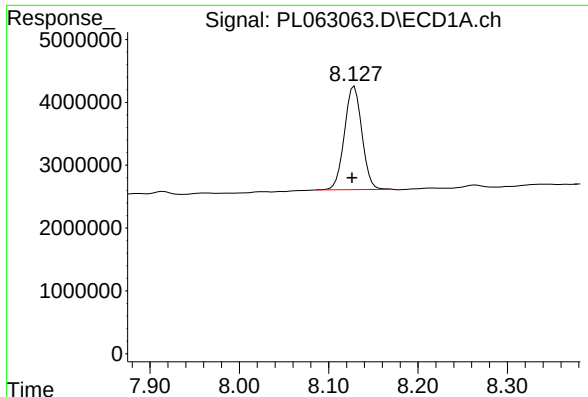

#28 Decachlorobiphenyl

R.T.: 8.129 min

Delta R.T.: 0.002 min


Response: 22347817

Conc: 13.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
FJ-BH-02-0-1

Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:27 AM

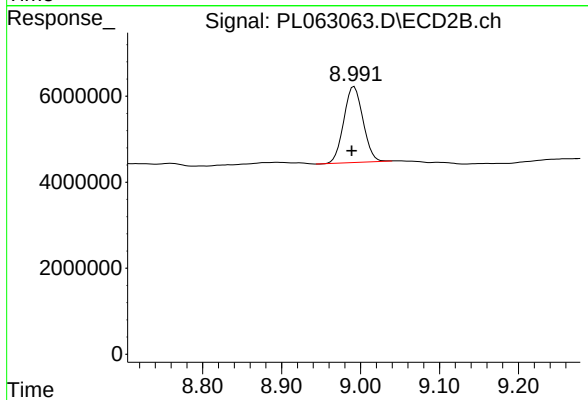

#28 Decachlorobiphenyl

R.T.: 8.992 min

Delta R.T.: 0.003 min

Response: 29856095

Conc: 14.27 ng/ml