

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 16:13
 Operator : DD\AJ
 Sample : L4771-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CD-BH-01-0-1

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:44:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 03:15:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.411	3.952	37682669	60049739	21.907	20.434
28) SA Decachlor...	8.128	8.991	23571829	30300752	14.693	14.477m
Target Compounds						
12) B 4,4'-DDE	5.551	6.278	4049642	6207869	2.448	1.927
17) MA 4,4'-DDT	6.299	7.068	3674985	3454530	2.754m	1.539 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 16:13
Operator : DD\AJ
Sample : L4771-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CD-BH-01-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 03:15:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

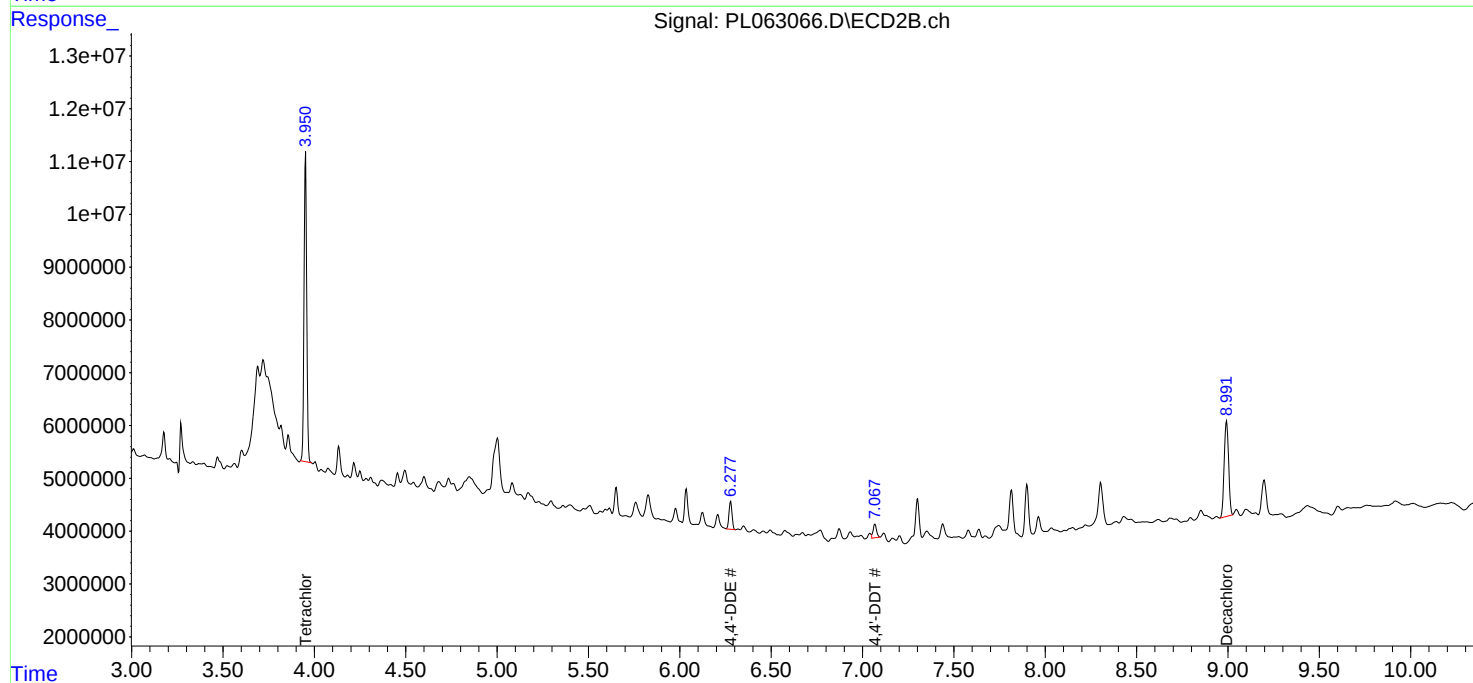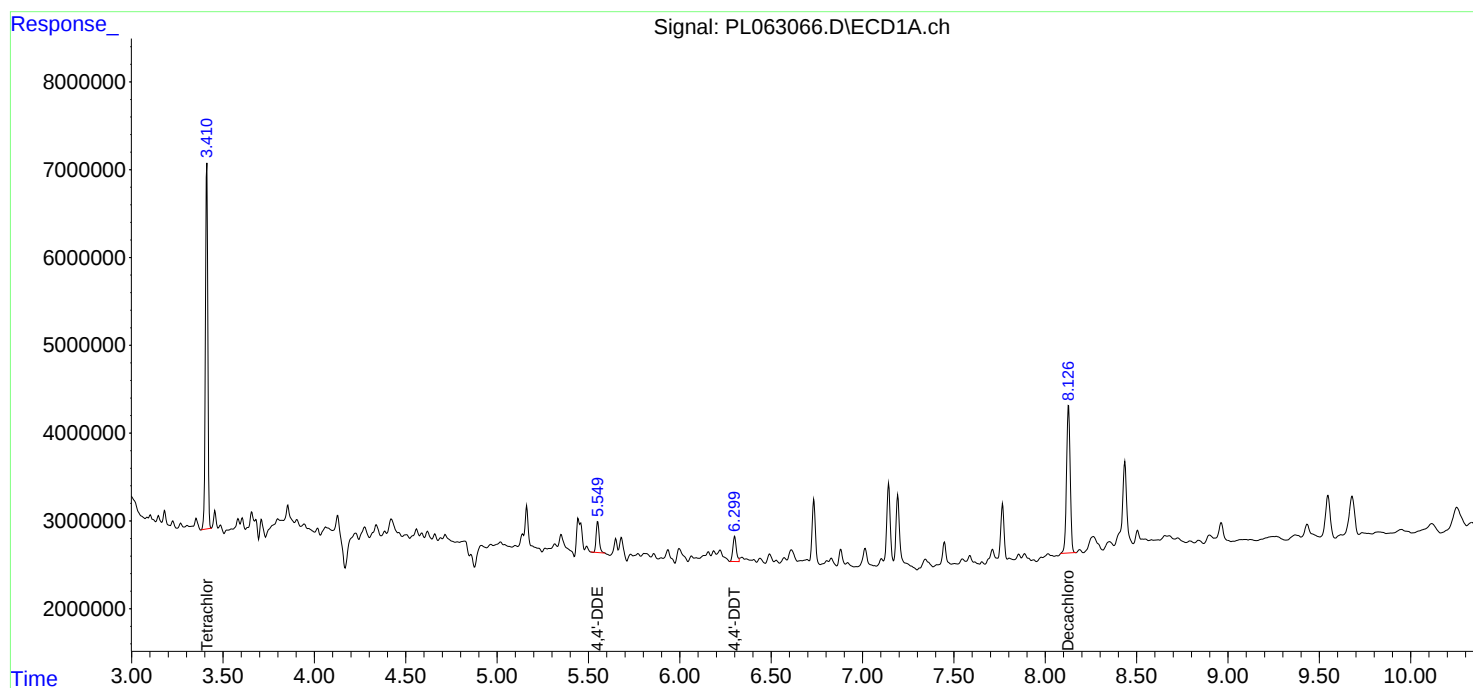

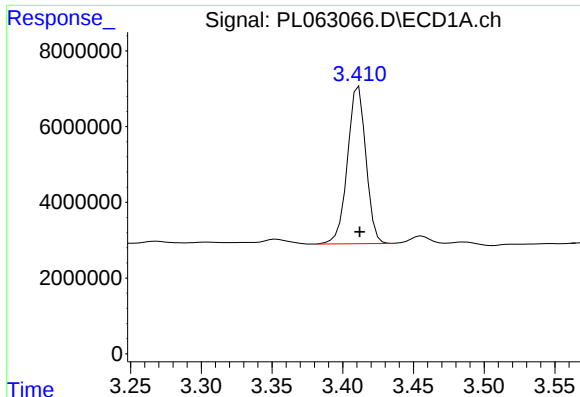


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 37682669
Conc: 21.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
CD-BH-01-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:29 AM

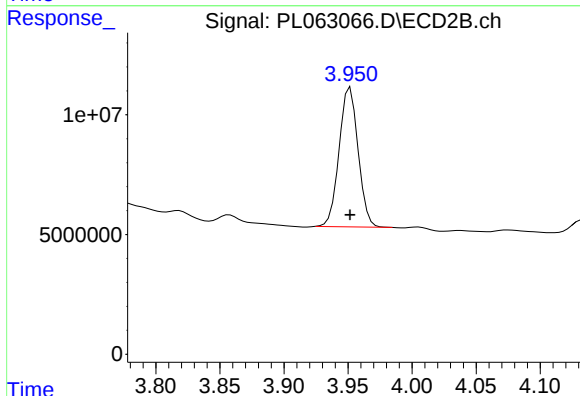


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 60049739
Conc: 20.43 ng/ml

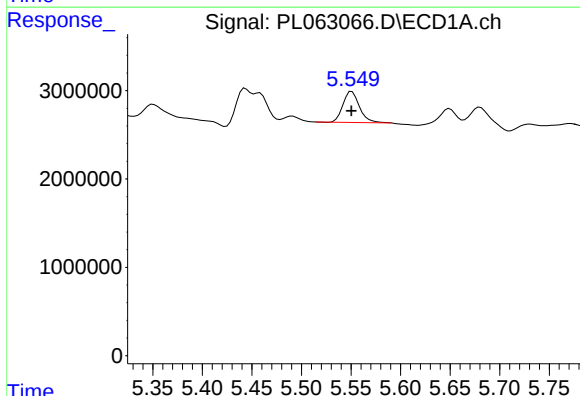


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 4049642
Conc: 2.45 ng/ml

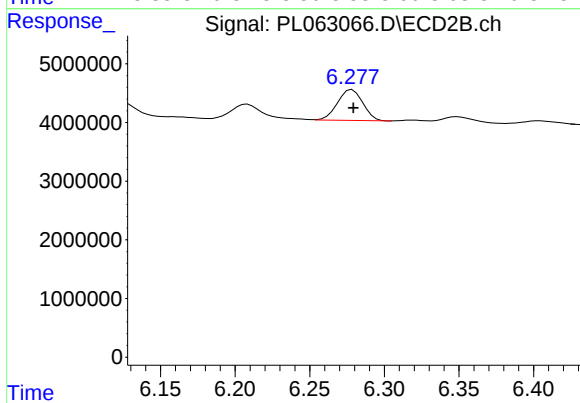

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 6207869
Conc: 1.93 ng/ml

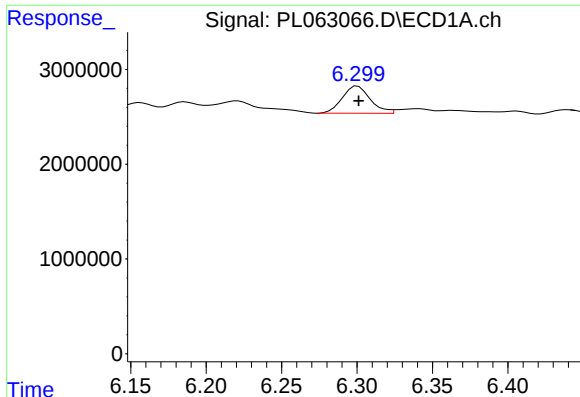


#17 4,4'-DDT

R.T.: 6.299 min
Delta R.T.: -0.002 min
Response: 3674985
Conc: 2.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CD-BH-01-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:29 AM

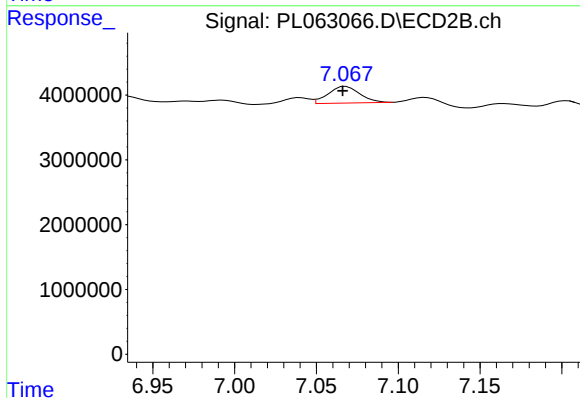


#17 4,4'-DDT

R.T.: 7.068 min
Delta R.T.: 0.002 min
Response: 3454530
Conc: 1.54 ng/ml

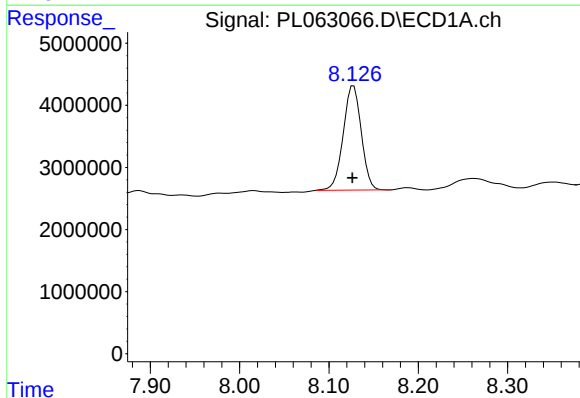

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 23571829
Conc: 14.69 ng/ml

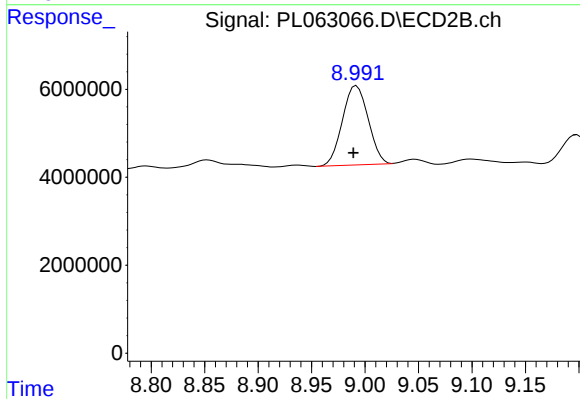

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 30300752
Conc: 14.48 ng/ml m