

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
 Data File : PL063081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 19:47
 Operator : DD\AJ
 Sample : L4734-02MSD
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BARNUM-STREET-TEST-PIT-2MSD

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:44:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 03:18:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	29282109	50788756	17.024	17.283
28)	SA Decachlor...	8.127	8.992	19059683	20144114	11.880	9.625
Target Compounds							
2)	A alpha-BHC	3.843	4.337	118.1E6	219.4E6	46.318	49.381
3)	MA gamma-BHC...	4.123	4.620	106.3E6	201.8E6	45.866	48.328
4)	MA Heptachlor	4.419	5.126	95801580	173.7E6	44.646	43.565
5)	MB Aldrin	4.664	5.429	86789020	169.7E6	45.469	46.894
6)	B beta-BHC	4.372	4.792	44139869	84863792	46.210	45.068
7)	B delta-BHC	4.573	5.007	100.7E6	171.5E6	46.319	48.996
8)	B Heptachlo...	5.103	5.814	85489201	146.3E6	46.854	45.184
9)	A Endosulfan I	5.439	6.170	74930120	132.7E6	44.825	42.061
10)	B gamma-Chl...	5.329	6.048	82024808	141.1E6	45.529	41.918
11)	B alpha-Chl...	5.386	6.121	80388347	139.6E6	44.469	41.448
12)	B 4,4'-DDE	5.551	6.278	72204455	119.9E6	43.643	37.221
13)	MA Dieldrin	5.679	6.426	84669906	131.5E6	47.918	41.088
14)	MA Endrin	5.934	6.643	74113699	113.0E6	44.545	40.484
15)	B Endosulfa...	6.206	6.853	68384453	101.5E6	41.479	35.503
16)	A 4,4'-DDD	6.064	6.769	60829597	107.6E6	43.005	42.026
17)	MA 4,4'-DDT	6.301	7.067	58932446	99786316	44.159	44.443
18)	B Endrin al...	6.373	6.976	56050185	83467607	38.600	36.599m
19)	B Endosulfa...	6.585	7.200	64879195	98912878	39.315	41.227
20)	A Methoxychlor	6.846	7.527	34227479	48659793	39.740	39.384
21)	B Endrin ke...	7.072	7.669	75403255	111.1E6	41.821	46.875
22)	Mirex	7.258	8.123	60156318	68405066	42.433	40.142

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111720\
Data File : PL063081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 19:47
Operator : DD\AJ
Sample : L4734-02MSD
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 03:18:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

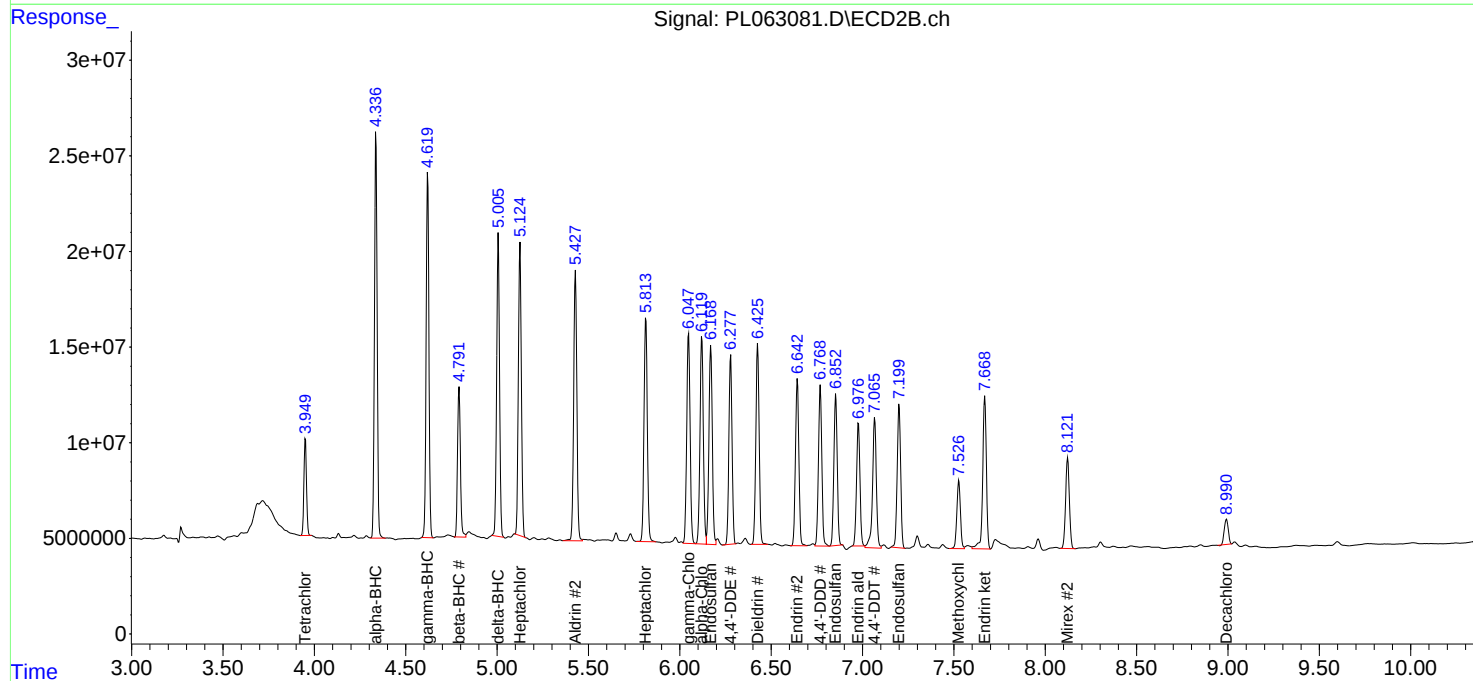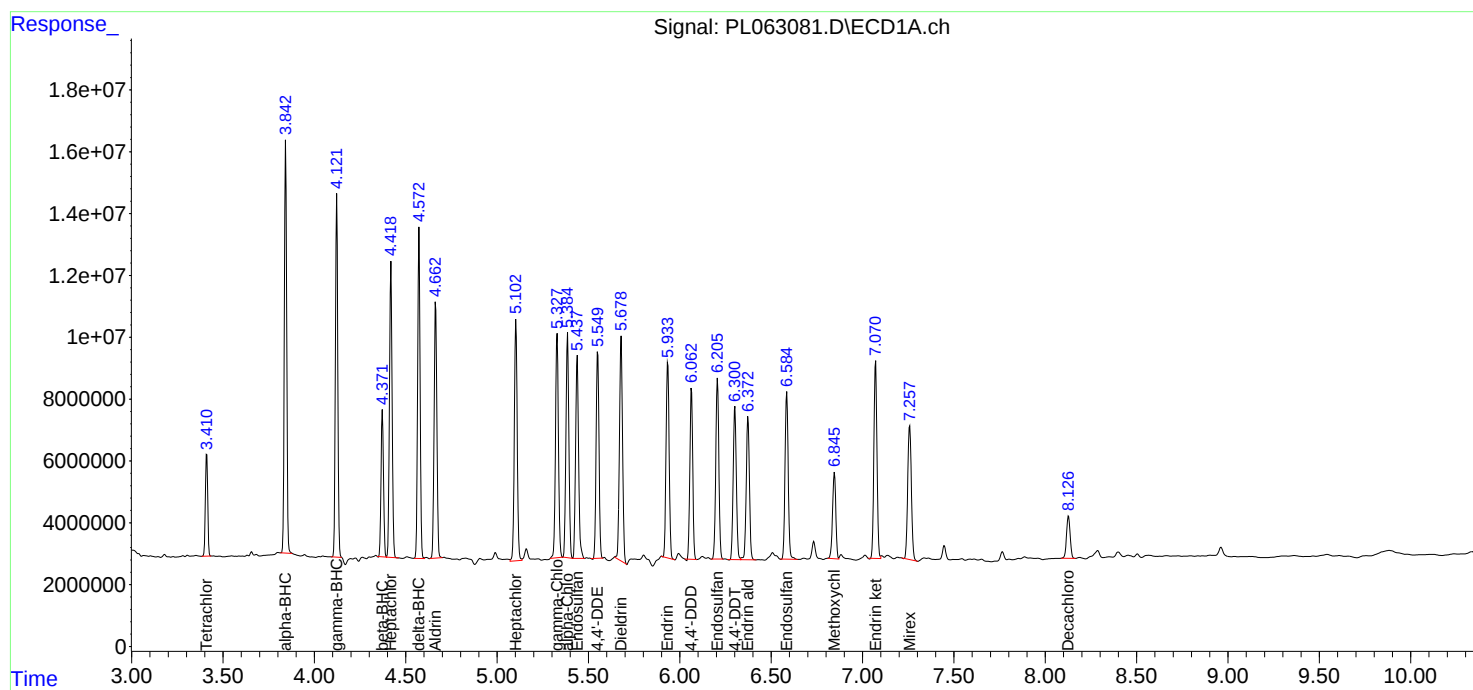

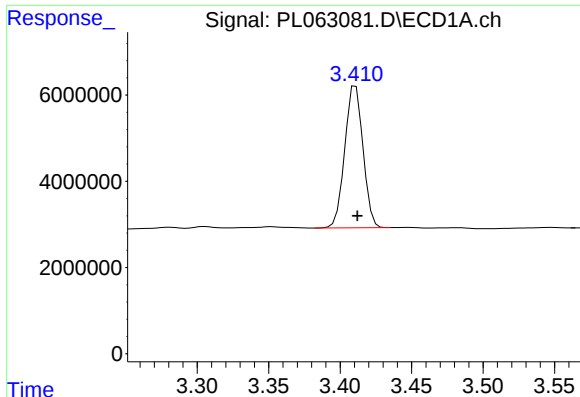


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 29282109
Conc: 17.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

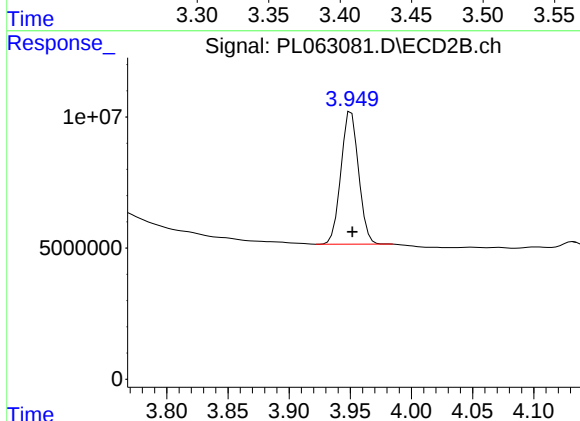


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 50788756
Conc: 17.28 ng/ml

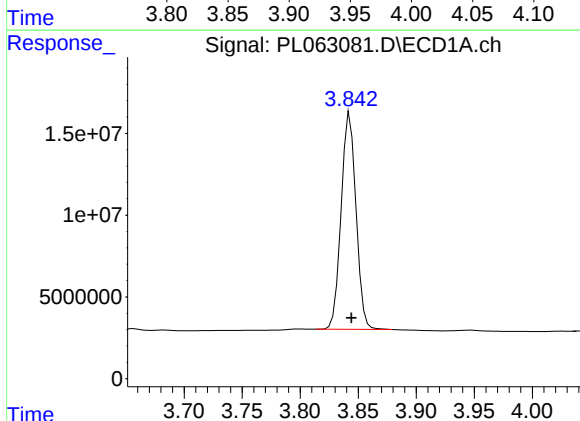


#2 alpha-BHC

R.T.: 3.843 min
Delta R.T.: -0.001 min
Response: 118097482
Conc: 46.32 ng/ml

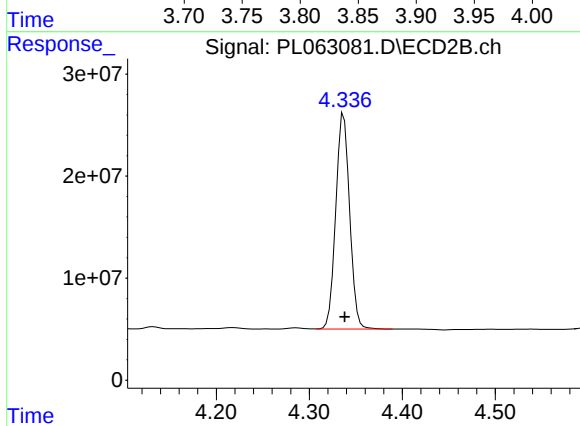

#2 alpha-BHC

R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 219412171
Conc: 49.38 ng/ml

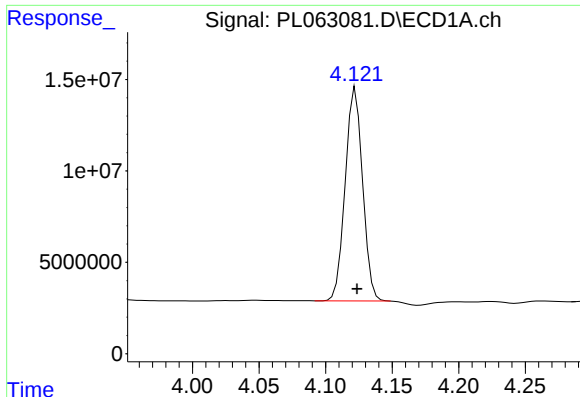


#3 gamma-BHC (Lindane)

R.T.: 4.123 min
Delta R.T.: -0.001 min
Response: 106256919
Conc: 45.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

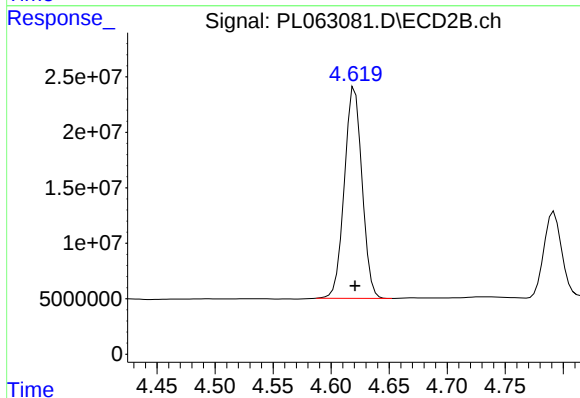


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 201806133
Conc: 48.33 ng/ml

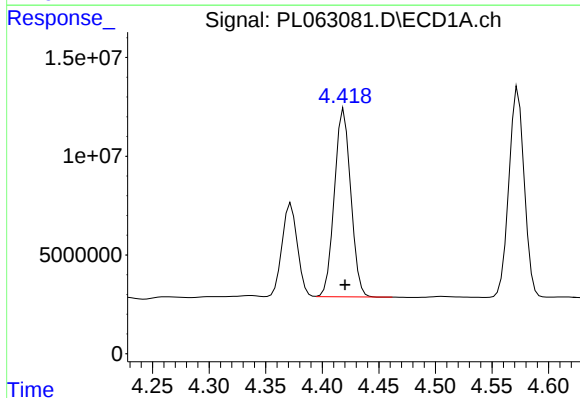


#4 Heptachlor

R.T.: 4.419 min
Delta R.T.: 0.000 min
Response: 95801580
Conc: 44.65 ng/ml

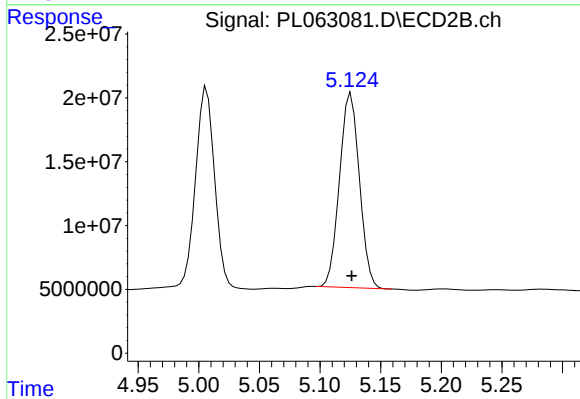

#4 Heptachlor

R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 173732661
Conc: 43.56 ng/ml

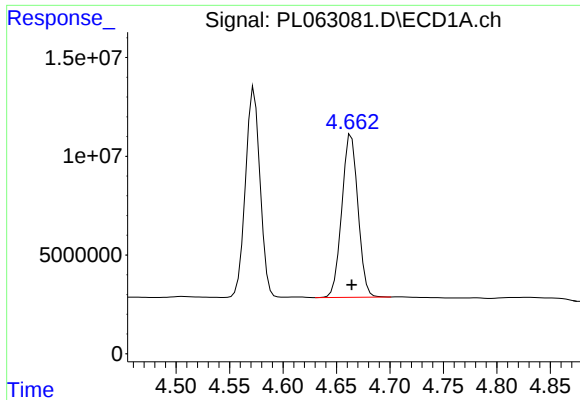


#5 Aldrin

R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 86789020
Conc: 45.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

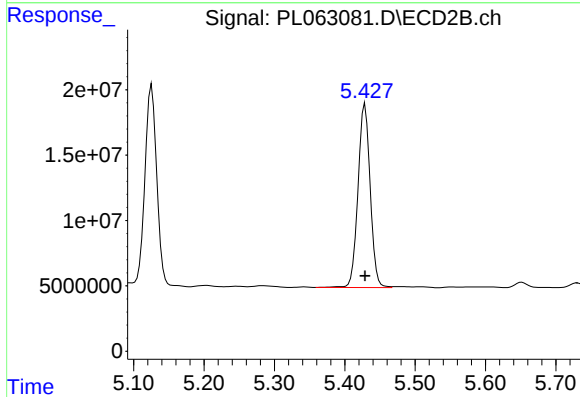


#5 Aldrin

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 169733435
Conc: 46.89 ng/ml

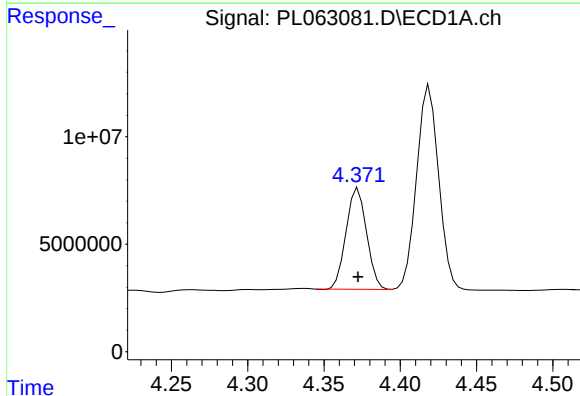


#6 beta-BHC

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 44139869
Conc: 46.21 ng/ml

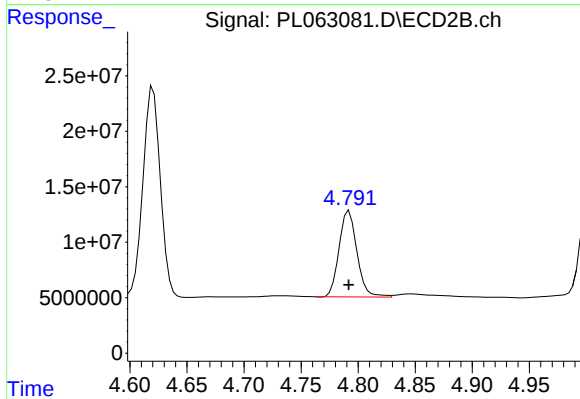

#6 beta-BHC

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 84863792
Conc: 45.07 ng/ml

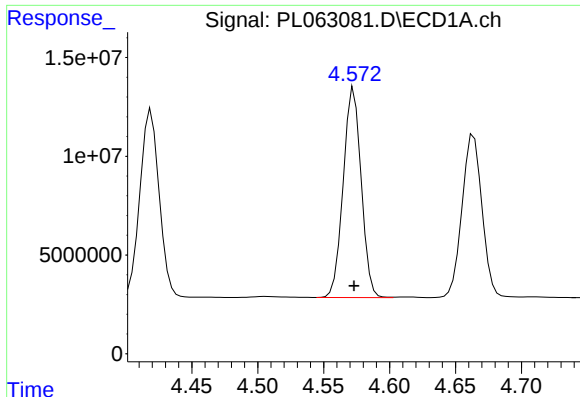


#7 delta-BHC

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 100660425
Conc: 46.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

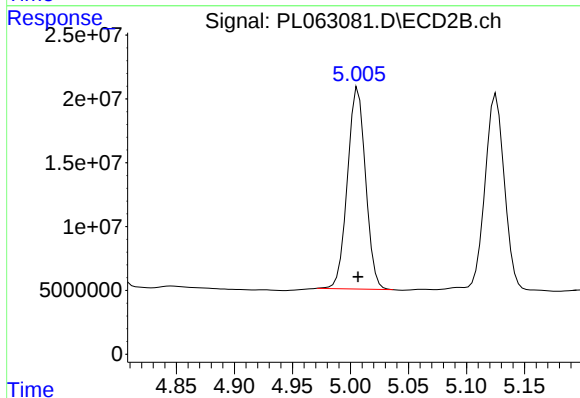


#7 delta-BHC

R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 171459333
Conc: 49.00 ng/ml

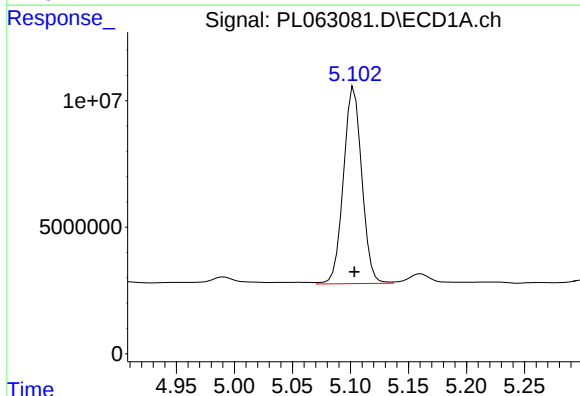


#8 Heptachlor epoxide

R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 85489201
Conc: 46.85 ng/ml

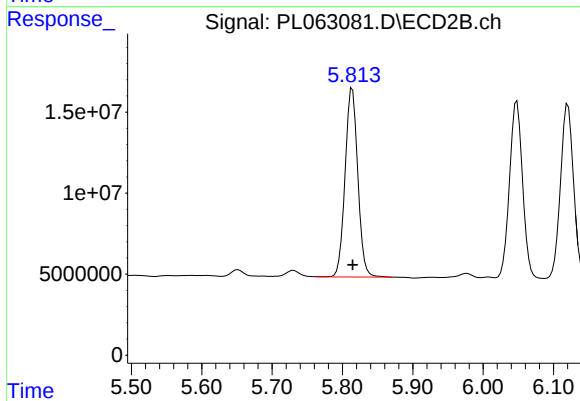

#8 Heptachlor epoxide

R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 146332170
Conc: 45.18 ng/ml

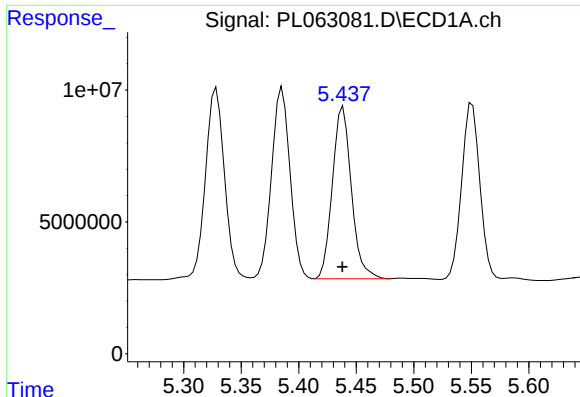


#9 Endosulfan I

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 74930120
Conc: 44.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

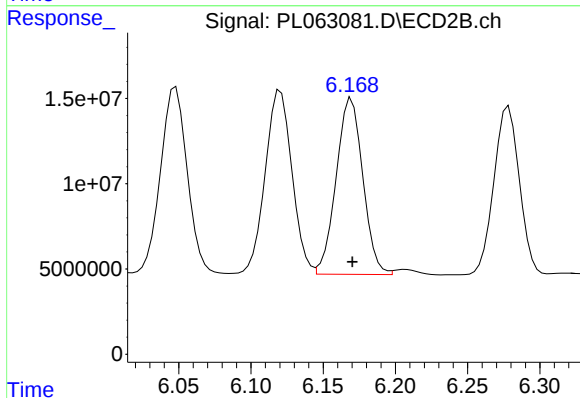


#9 Endosulfan I

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 132652565
Conc: 42.06 ng/ml

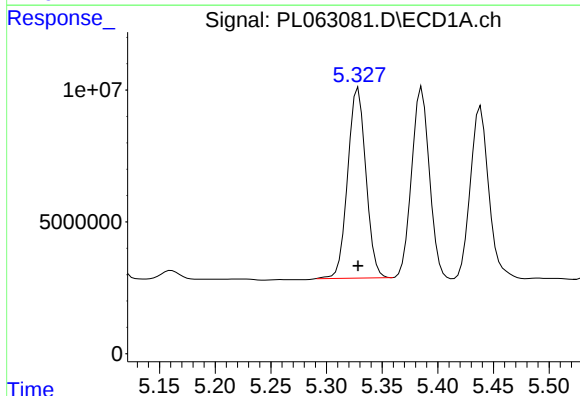


#10 gamma-Chlordane

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 82024808
Conc: 45.53 ng/ml

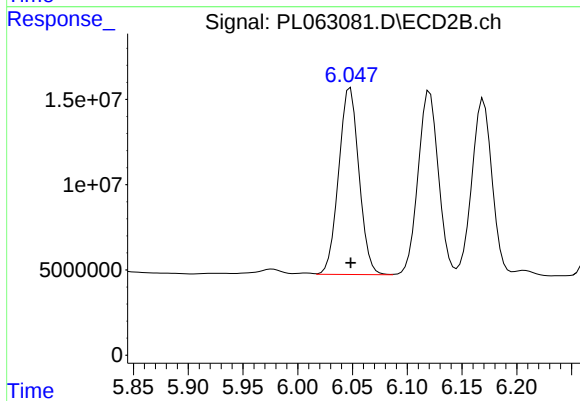

#10 gamma-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 141111225
Conc: 41.92 ng/ml

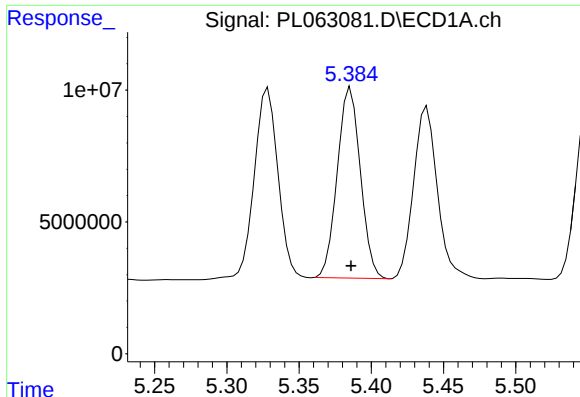


#11 alpha-Chlordane

R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 80388347
Conc: 44.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

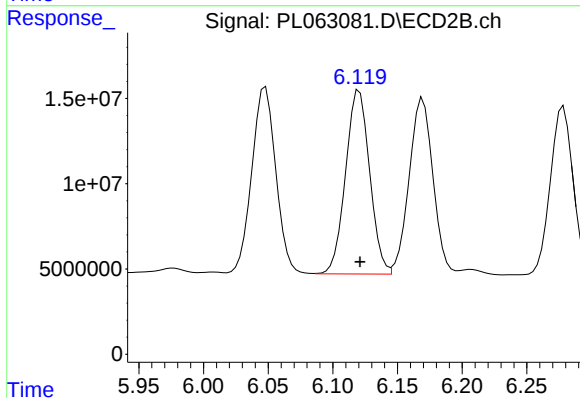


#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 139634286
Conc: 41.45 ng/ml

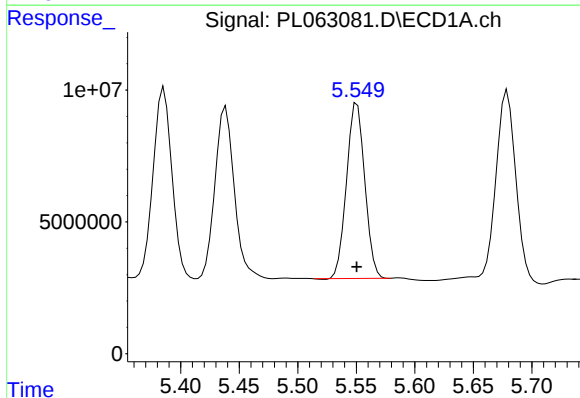


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 72204455
Conc: 43.64 ng/ml

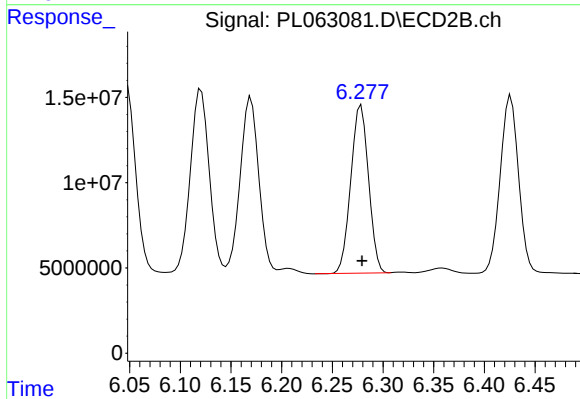

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 119927654
Conc: 37.22 ng/ml

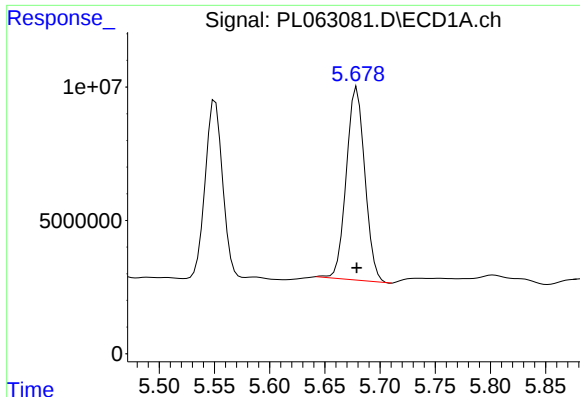


#13 Dieldrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 84669906
Conc: 47.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

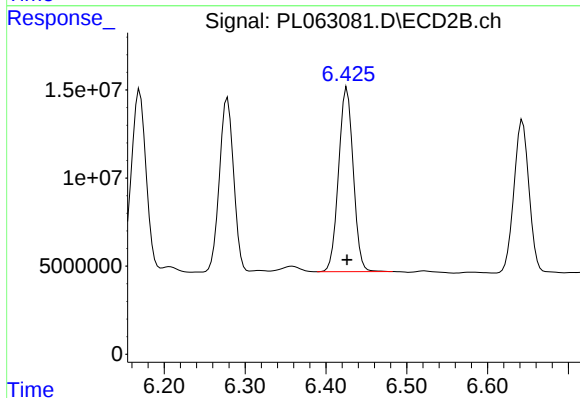


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 131517408
Conc: 41.09 ng/ml

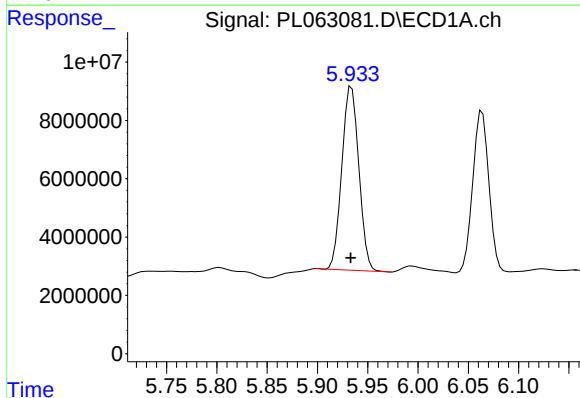


#14 Endrin

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 74113699
Conc: 44.55 ng/ml

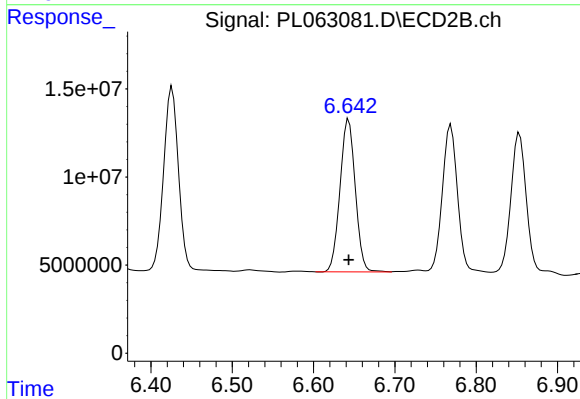

#14 Endrin

R.T.: 6.643 min
Delta R.T.: 0.000 min
Response: 112995987
Conc: 40.48 ng/ml

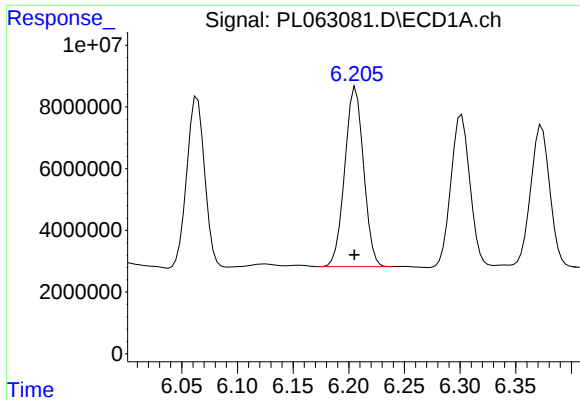


#15 Endosulfan II

R.T.: 6.206 min
Delta R.T.: 0.001 min
Response: 68384453
Conc: 41.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

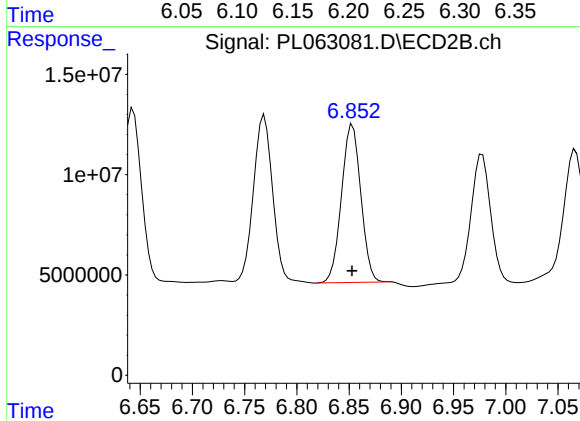


#15 Endosulfan II

R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 101489467
Conc: 35.50 ng/ml

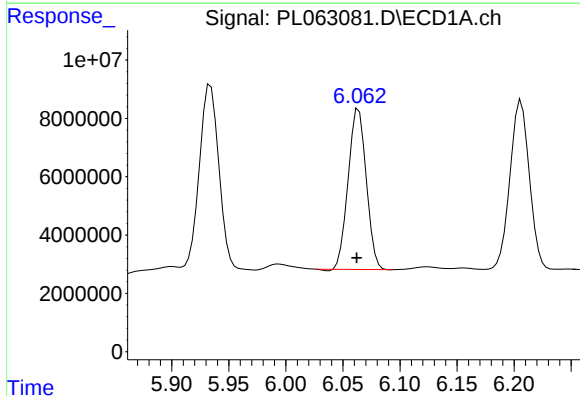


#16 4,4'-DDD

R.T.: 6.064 min
Delta R.T.: 0.002 min
Response: 60829597
Conc: 43.00 ng/ml

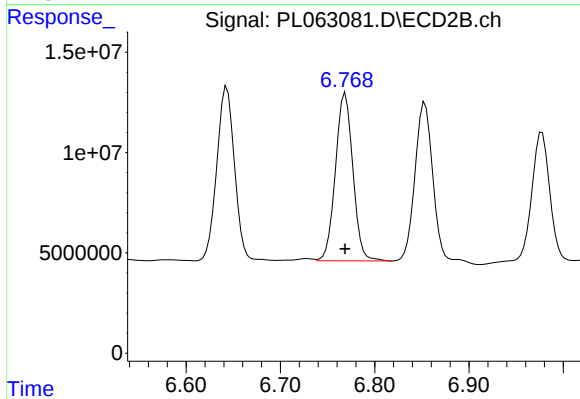

#16 4,4'-DDD

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 107585864
Conc: 42.03 ng/ml

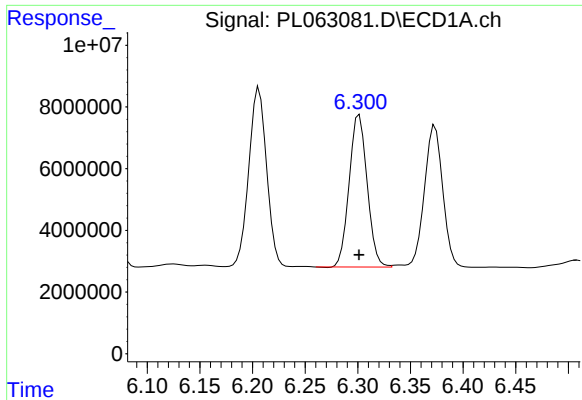


#17 4,4'-DDT

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 58932446
Conc: 44.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

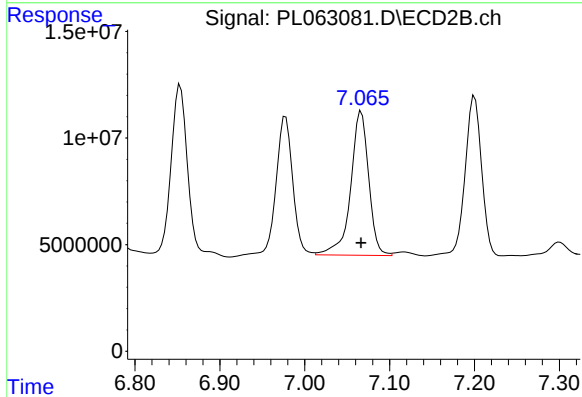


#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 99786316
Conc: 44.44 ng/ml

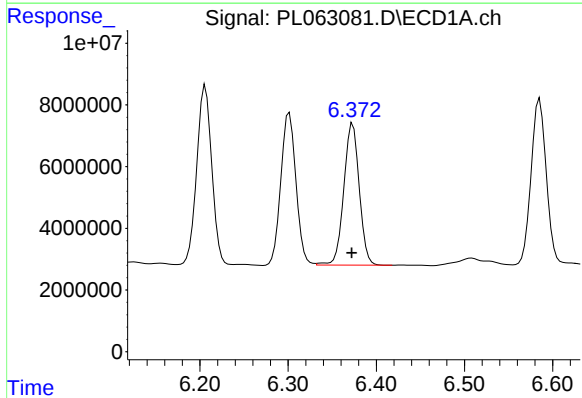


#18 Endrin aldehyde

R.T.: 6.373 min
Delta R.T.: 0.001 min
Response: 56050185
Conc: 38.60 ng/ml

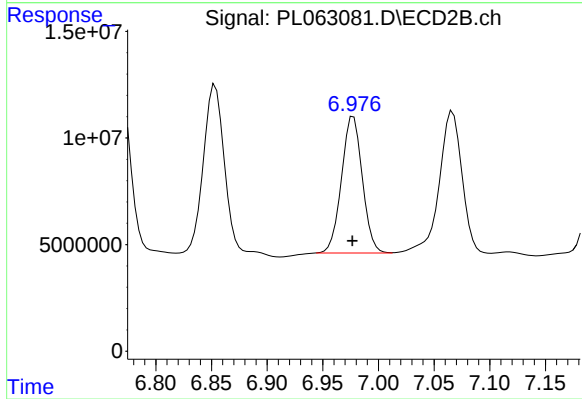

#18 Endrin aldehyde

R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 83467607
Conc: 36.60 ng/ml m

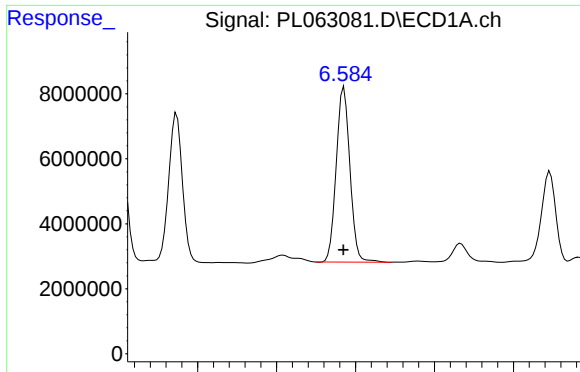


#19 Endosulfan Sulfate

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 64879195
Conc: 39.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

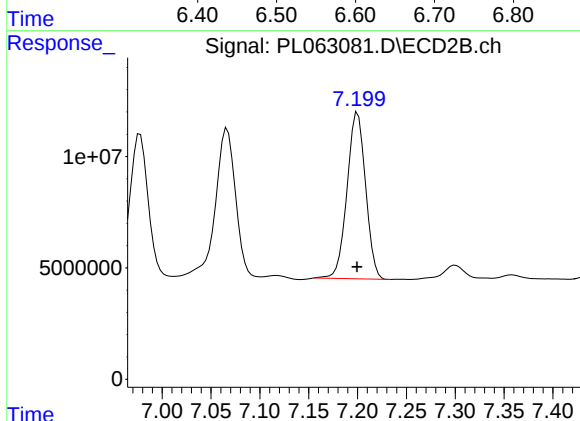


#19 Endosulfan Sulfate

R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 98912878
Conc: 41.23 ng/ml

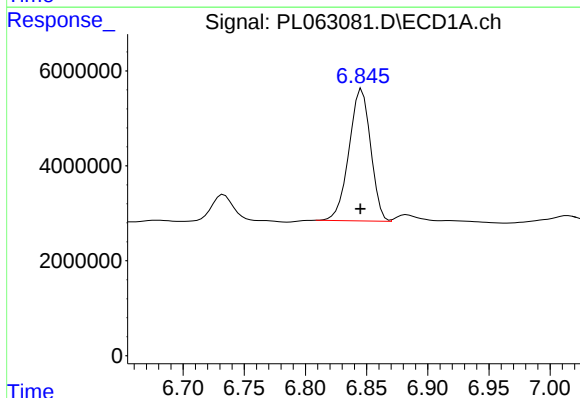


#20 Methoxychlor

R.T.: 6.846 min
Delta R.T.: 0.001 min
Response: 34227479
Conc: 39.74 ng/ml

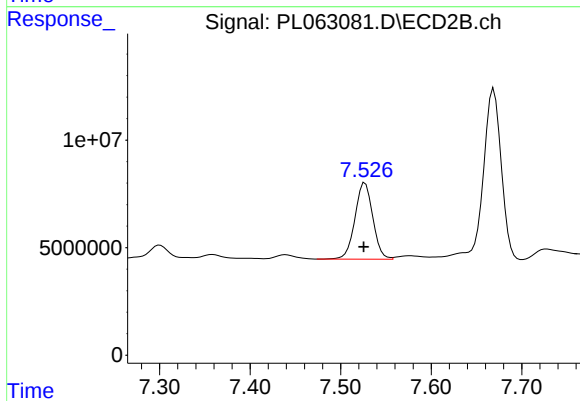

#20 Methoxychlor

R.T.: 7.527 min
Delta R.T.: 0.001 min
Response: 48659793
Conc: 39.38 ng/ml

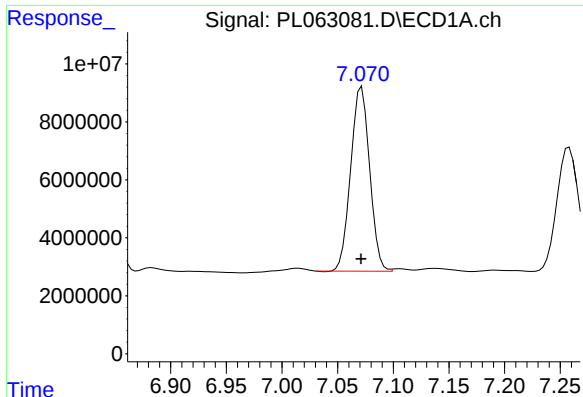


#21 Endrin ketone

R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 75403255
Conc: 41.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

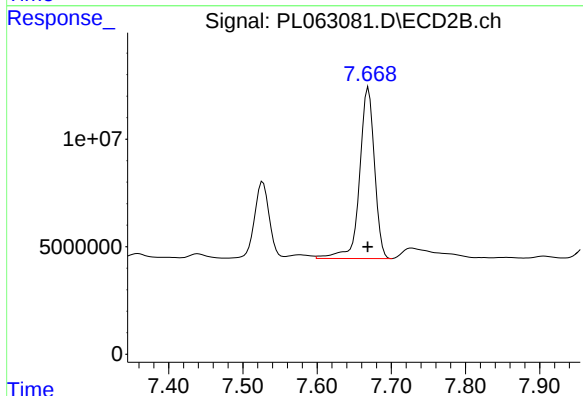


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 111084566
Conc: 46.87 ng/ml

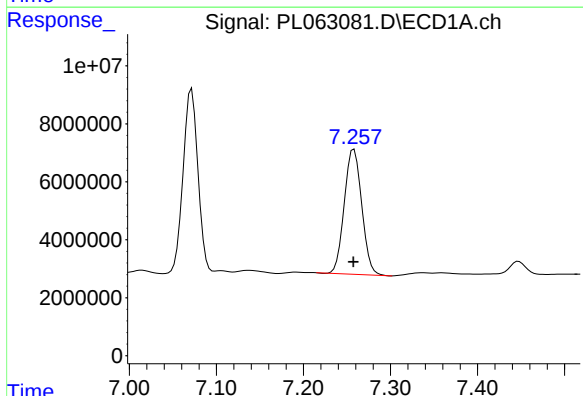


#22 Mirex

R.T.: 7.258 min
Delta R.T.: 0.000 min
Response: 60156318
Conc: 42.43 ng/ml

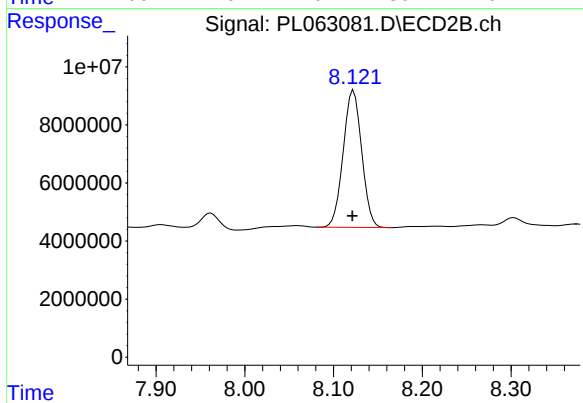

#22 Mirex

R.T.: 8.123 min
Delta R.T.: 0.002 min
Response: 68405066
Conc: 40.14 ng/ml

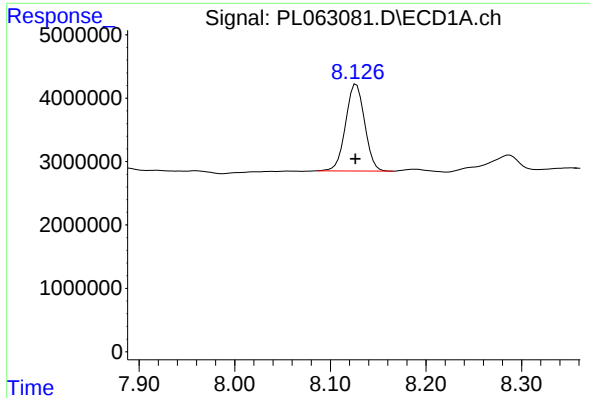


#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 19059683
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2MSD

Manual Integrations
APPROVED

Ankita
11/18/2020 10:44:43 AM

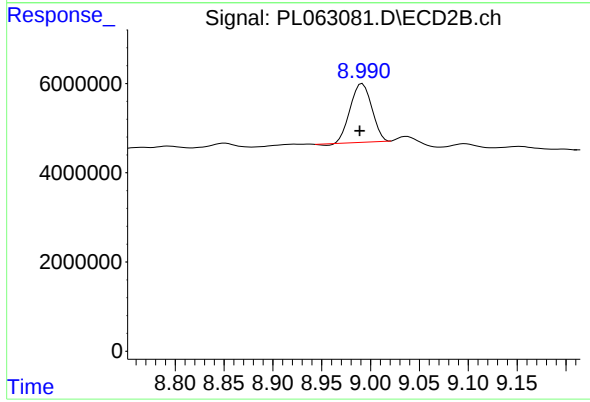

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 20144114
Conc: 9.62 ng/ml