

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
 Data File : PL071011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 10:03
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:46:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	0.000	6.499f	0	590491	N.D.	0.341 #
6) B	beta-BHC	0.000	6.746	0	8468167	N.D.	9.883 #
7) B	delta-BHC	0.000	7.023f	0	593779	N.D.	0.355 #
23)	Chlordane-1	5.866f	6.874	475334	4274086	27.879	88.017 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
Data File : PL071011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 10:03
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:46:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

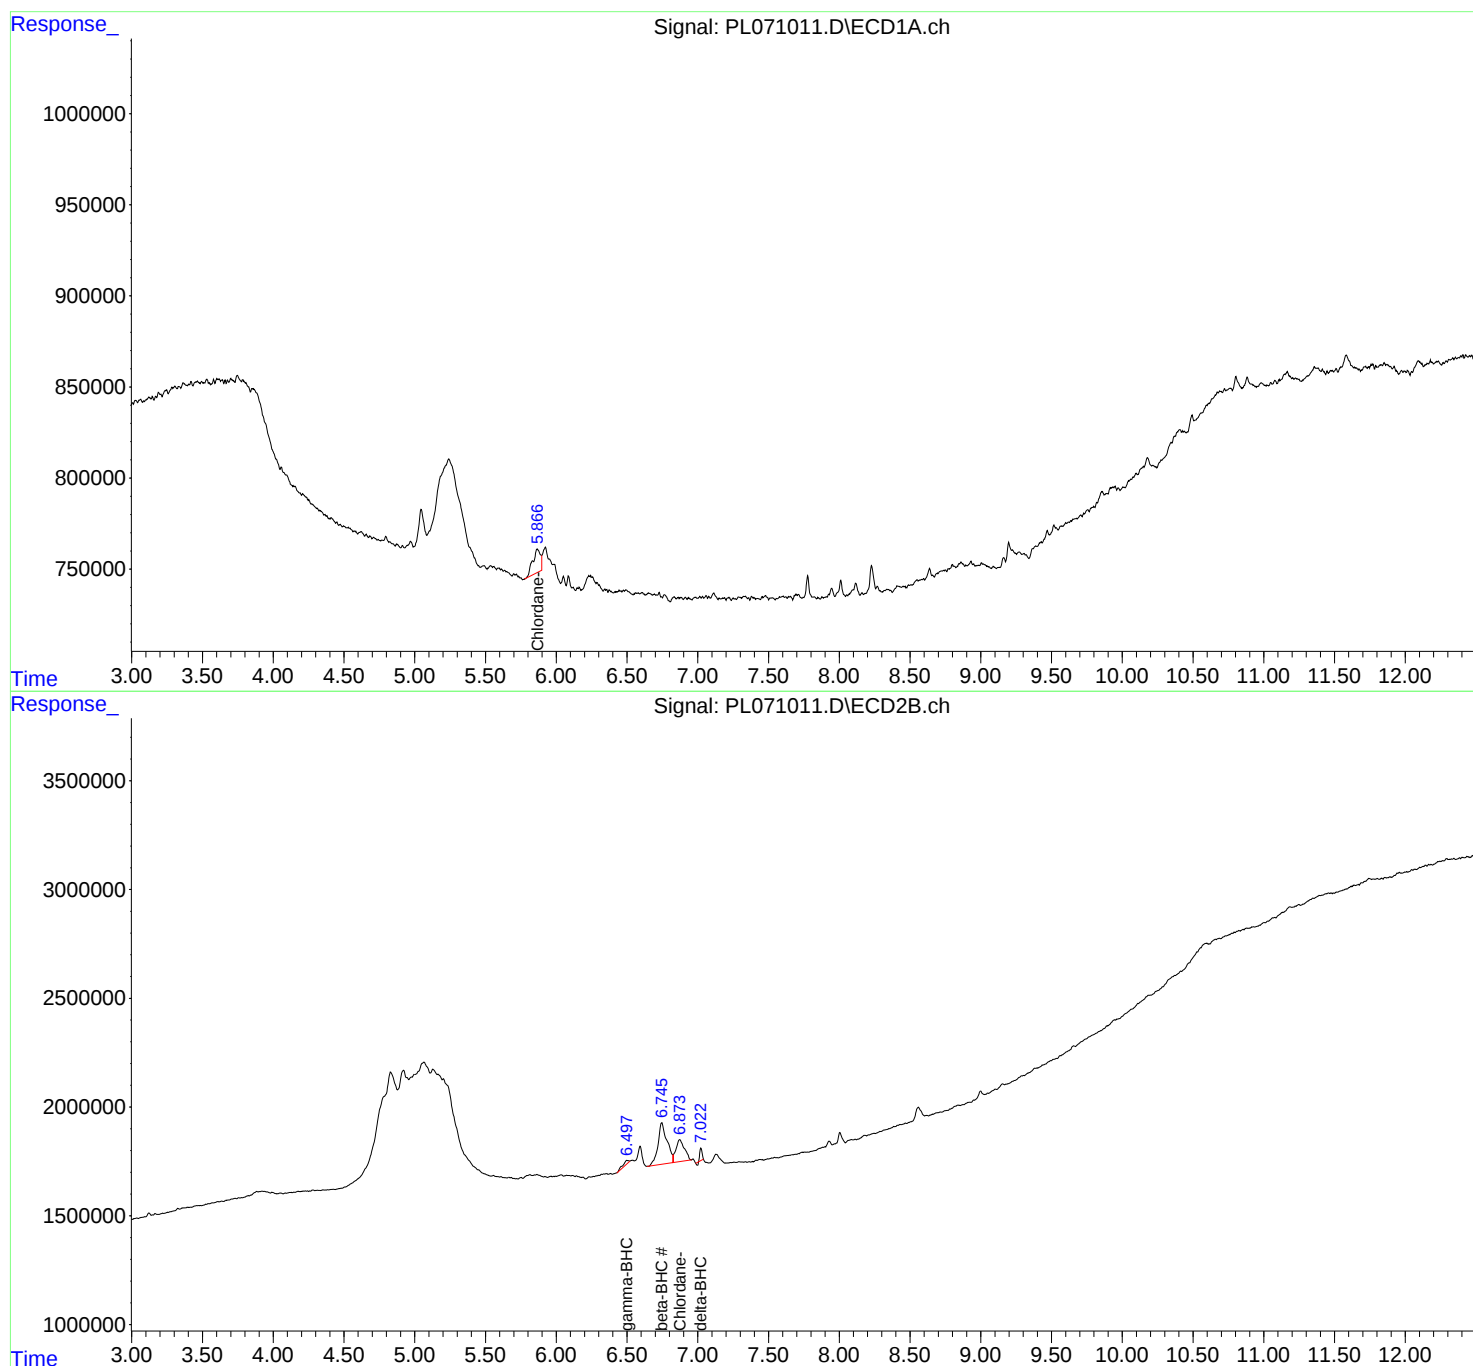


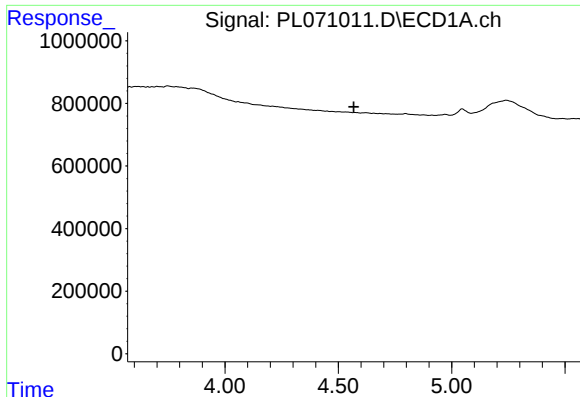

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

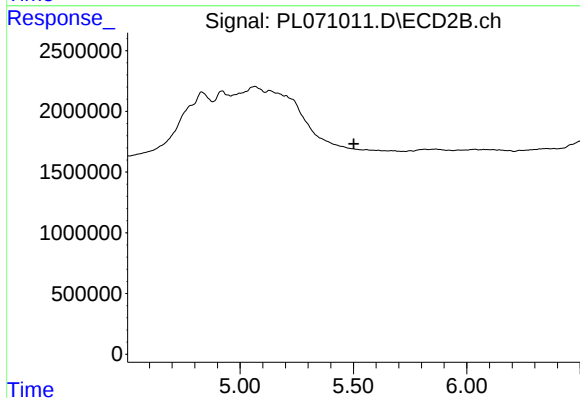


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

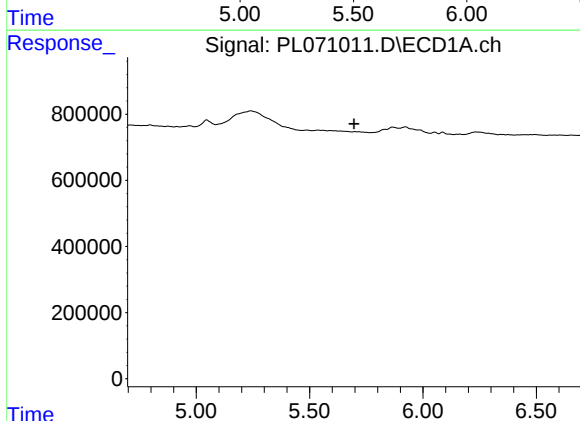


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.697 min
Response: 0
Conc: N.D.

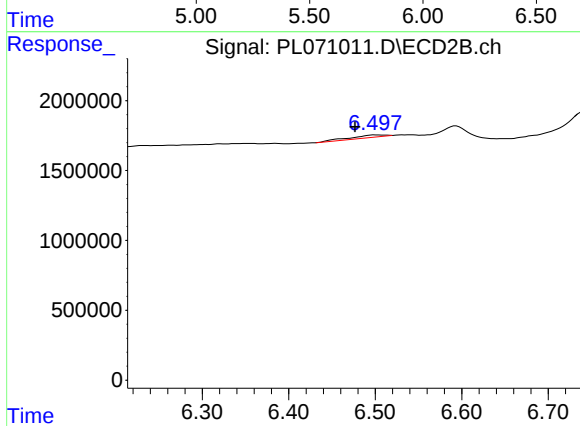

#3 gamma-BHC (Lindane)


R.T.: 6.499 min
Delta R.T.: 0.023 min
Response: 590491
Conc: 0.34 ng/ml

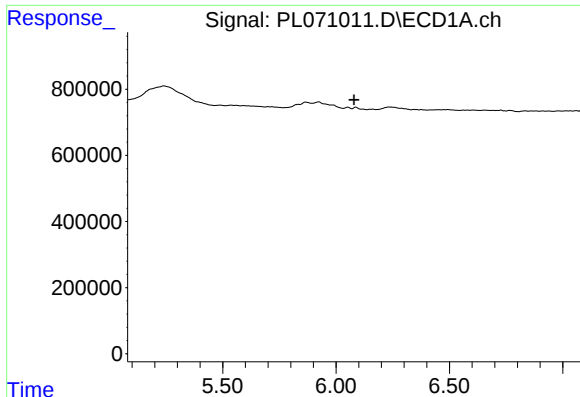

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

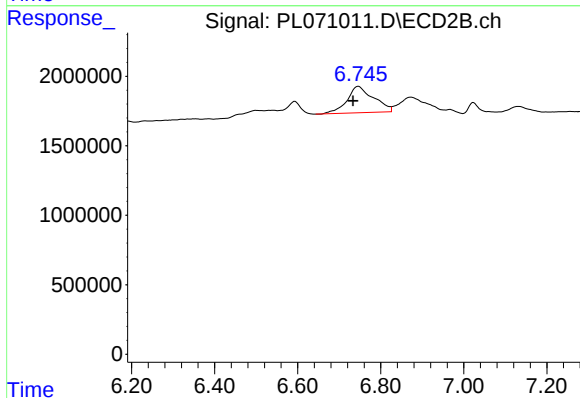


#6 beta-BHC

R.T.: 6.746 min
Delta R.T.: 0.013 min
Response: 8468167
Conc: 9.88 ng/ml

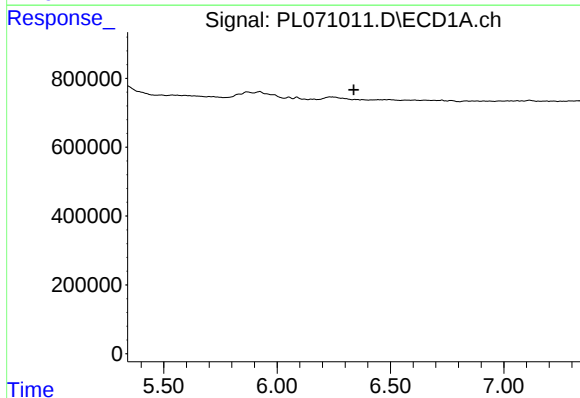


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.338 min
Response: 0
Conc: N.D.

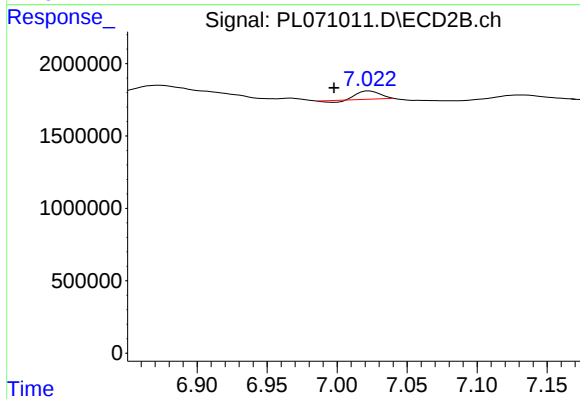

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.025 min
Response: 593779
Conc: 0.36 ng/ml

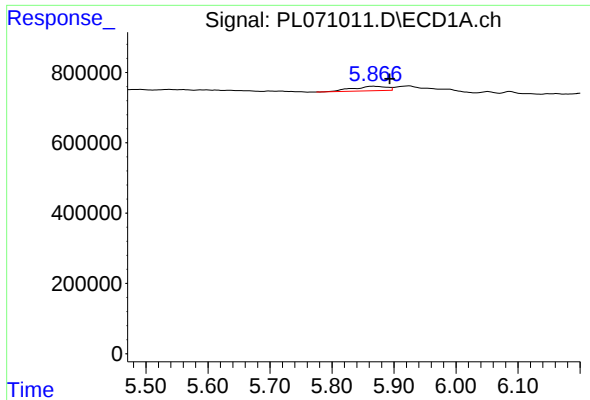

#23 Chlordane-1


R.T.: 5.866 min
Delta R.T.: -0.027 min
Response: 475334
Conc: 27.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

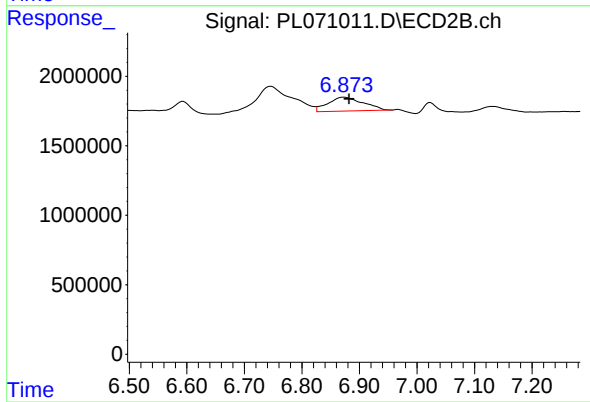


#23 Chlordane-1

R.T.: 6.874 min
Delta R.T.: -0.008 min
Response: 4274086
Conc: 88.02 ng/ml

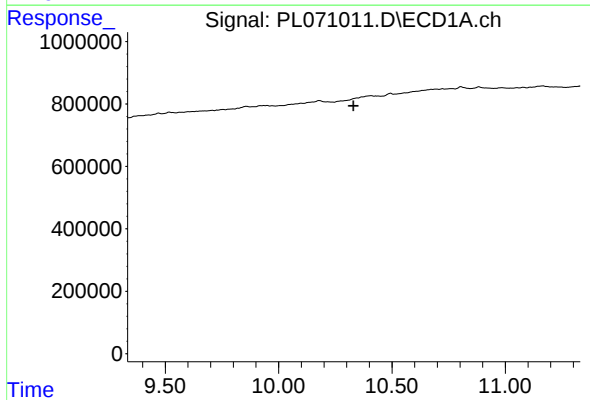

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.330 min
Response: 0
Conc: N.D.

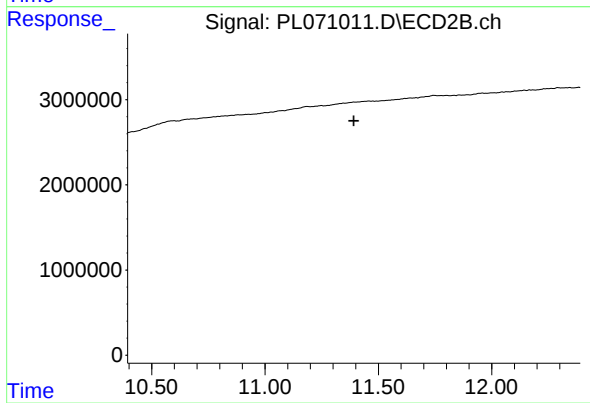

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.