

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
 Data File : PL071033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 18:47
 Operator : AR\AJ
 Sample : M4713-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:53:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.500	10243818	27554596	20.914	21.854
28)	SA Decachlor...	10.327	11.389	12807698	24498790	18.744	18.319
Target Compounds							
14)	MA Endrin	7.956f	0.000	149293	0	0.263	N.D. #
15)	B Endosulfa...	8.274f	0.000	828868	0	1.369	N.D. #
19)	B Endosulfa...	8.723	0.000	762098	0	1.235	N.D. #
20)	A Methoxychlor	8.983f	9.830	1188503	1686666	3.249	2.492
21)	B Endrin ke...	9.203f	10.011	300894	1169223	0.421	0.815 #
24)	Chlordane-2	6.576	0.000	140729	0	6.129	N.D. #
27)	Chlordane-5	8.274f	0.000	828868	0	37.073	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
Data File : PL071033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 18:47
Operator : AR\AJ
Sample : M4713-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:53:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

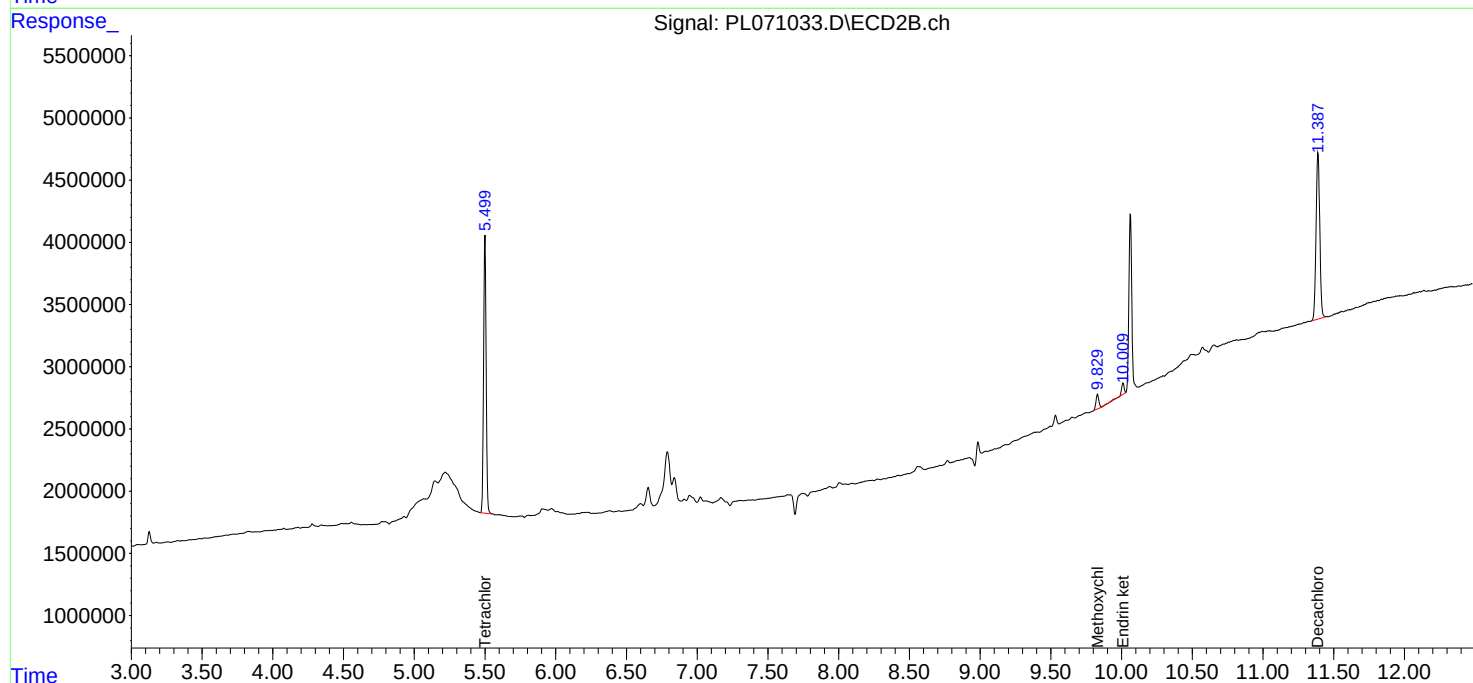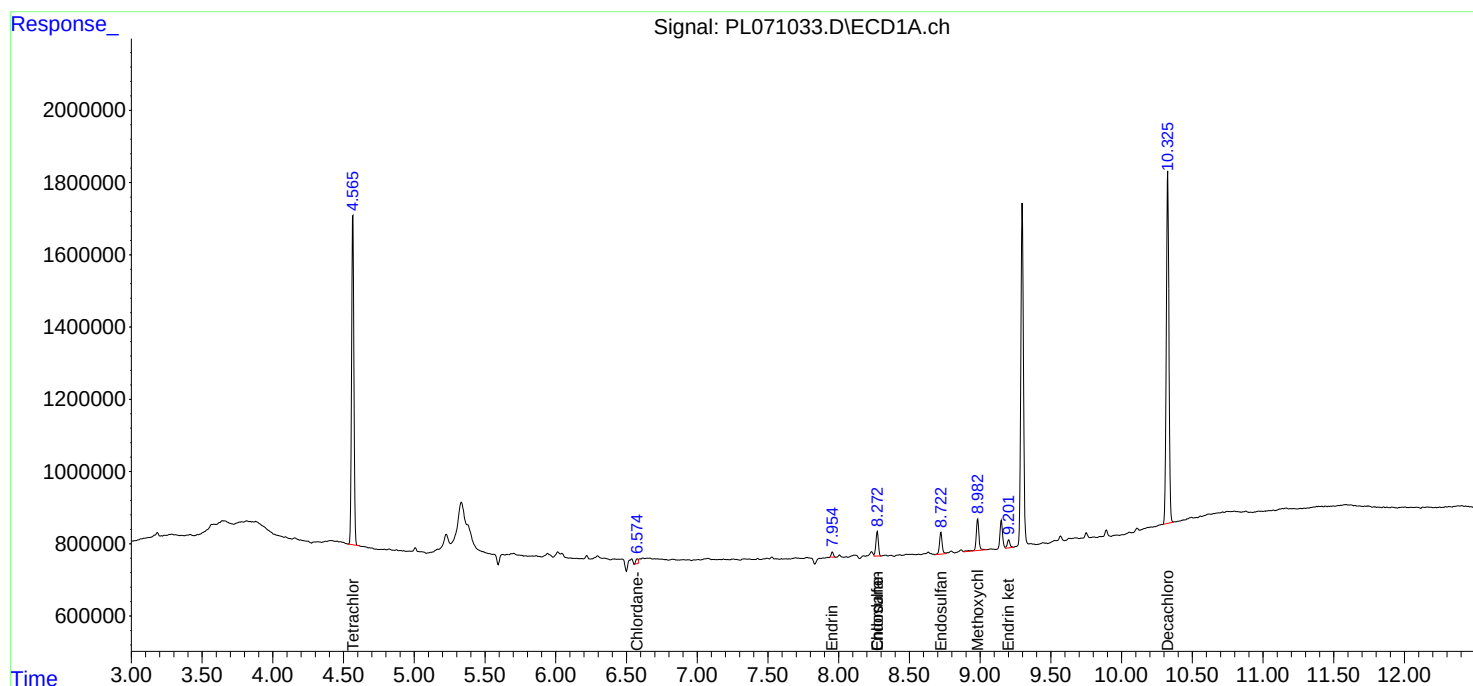


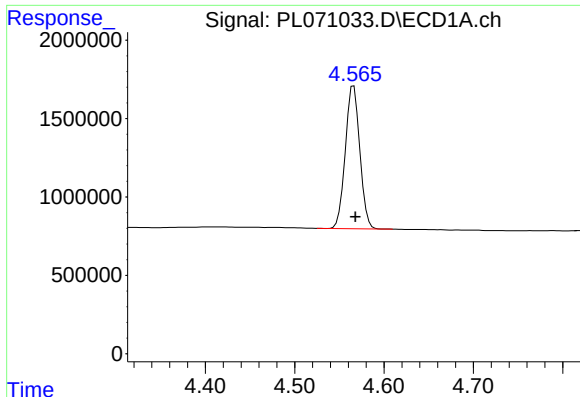

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: -0.002 min
Response: 10243818
Conc: 20.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

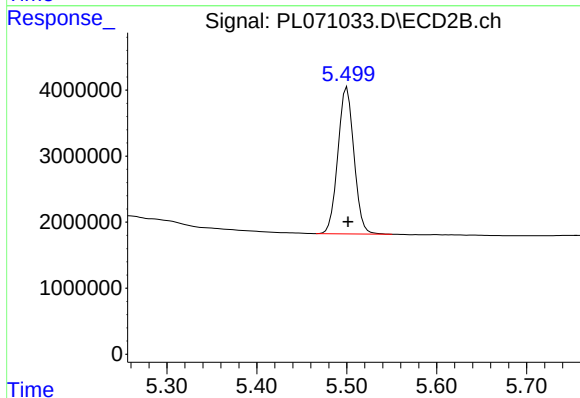


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 27554596
Conc: 21.85 ng/ml

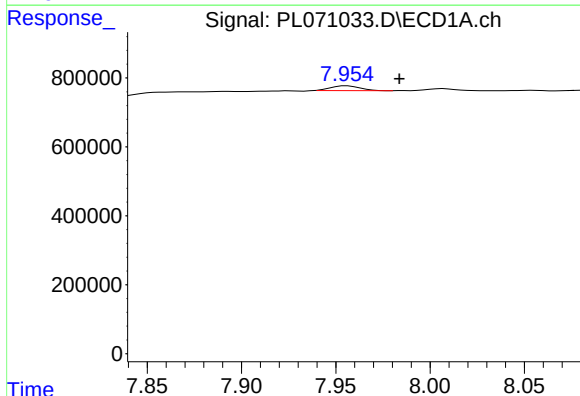


#14 Endrin

R.T.: 7.956 min
Delta R.T.: -0.028 min
Response: 149293
Conc: 0.26 ng/ml

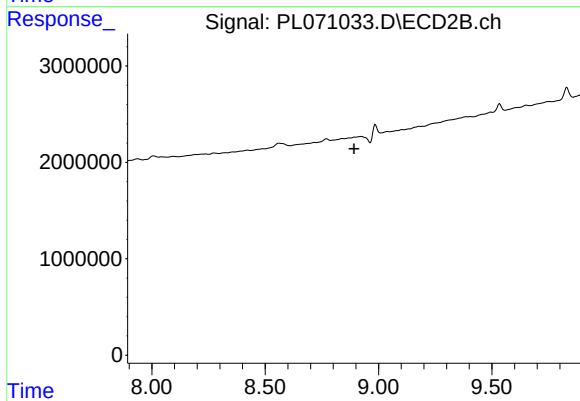

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

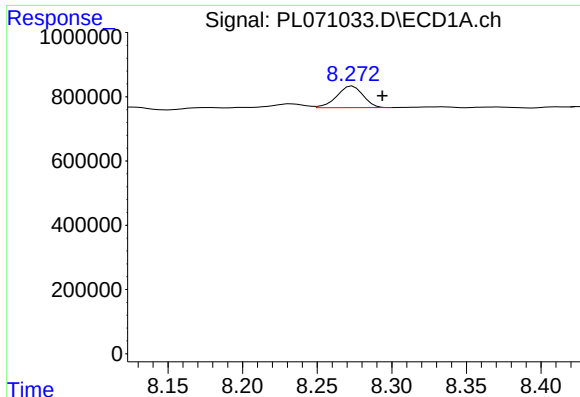

#15 Endosulfan II


R.T.: 8.274 min
Delta R.T.: -0.020 min
Response: 828868
Conc: 1.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

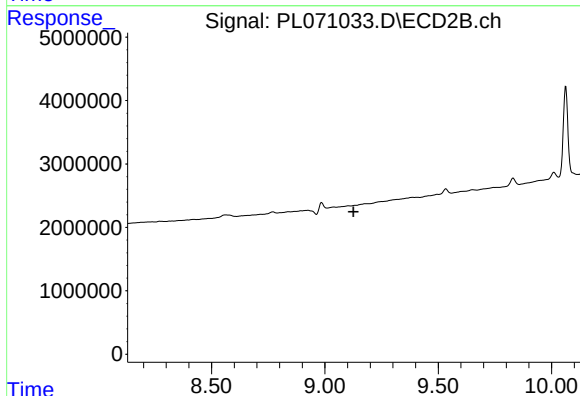


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.

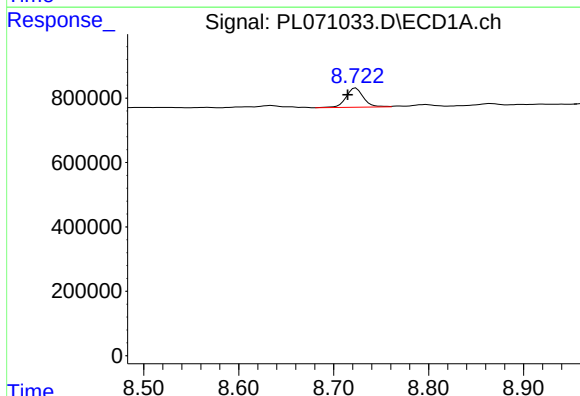


#19 Endosulfan Sulfate

R.T.: 8.723 min
Delta R.T.: 0.009 min
Response: 762098
Conc: 1.24 ng/ml

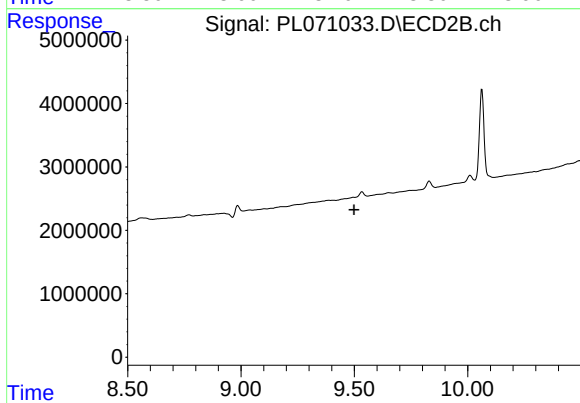

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.500 min
Response: 0
Conc: N.D.

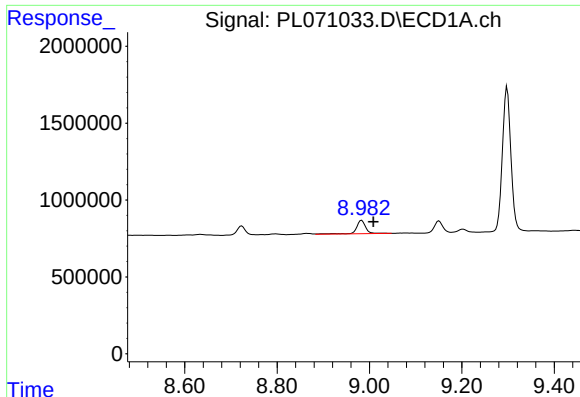

#20 Methoxychlor


R.T.: 8.983 min
Delta R.T.: -0.026 min
Response: 1188503
Conc: 3.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

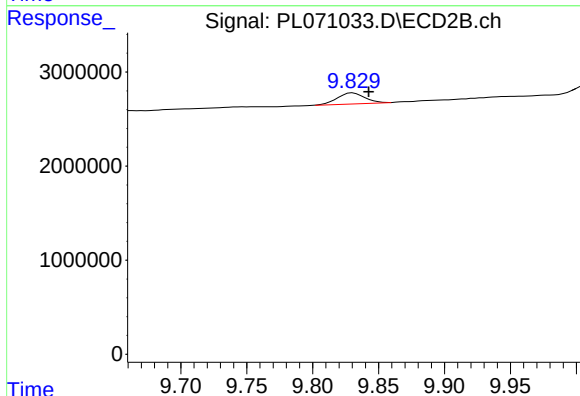


#20 Methoxychlor

R.T.: 9.830 min
Delta R.T.: -0.012 min
Response: 1686666
Conc: 2.49 ng/ml

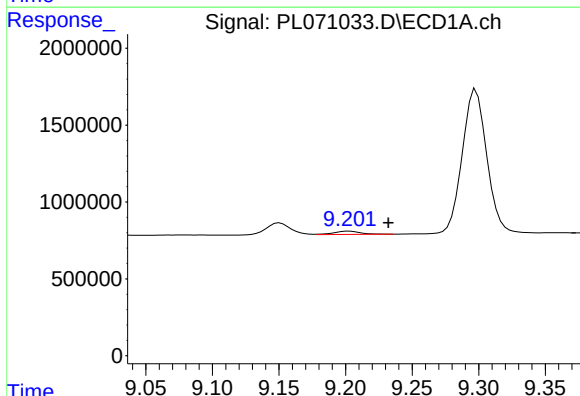


#21 Endrin ketone

R.T.: 9.203 min
Delta R.T.: -0.030 min
Response: 300894
Conc: 0.42 ng/ml

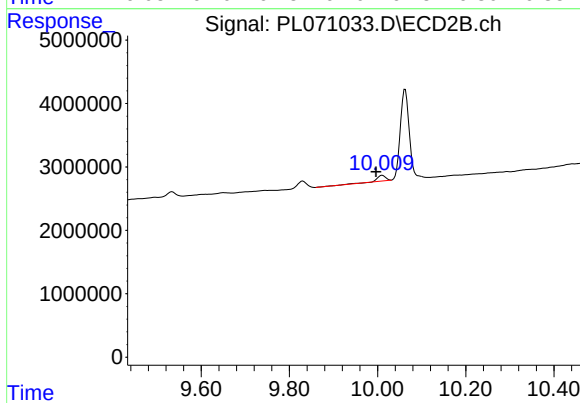

#21 Endrin ketone


R.T.: 10.011 min
Delta R.T.: 0.014 min
Response: 1169223
Conc: 0.81 ng/ml

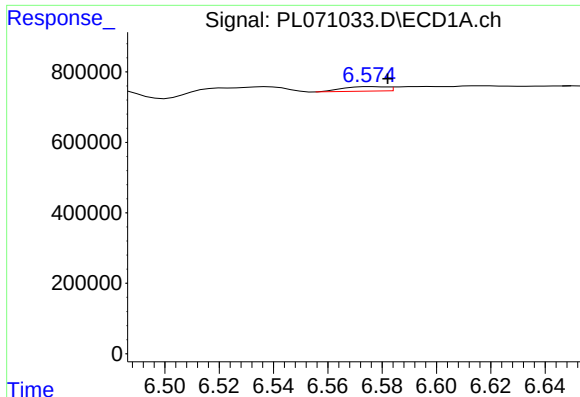

#24 Chlordane-2


R.T.: 6.576 min
Delta R.T.: -0.006 min
Response: 140729
Conc: 6.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

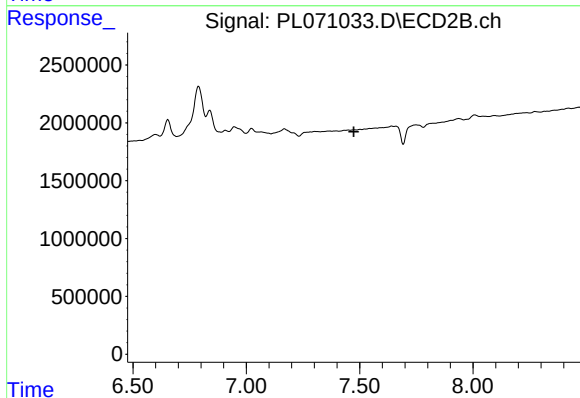


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.474 min
Response: 0
Conc: N.D.

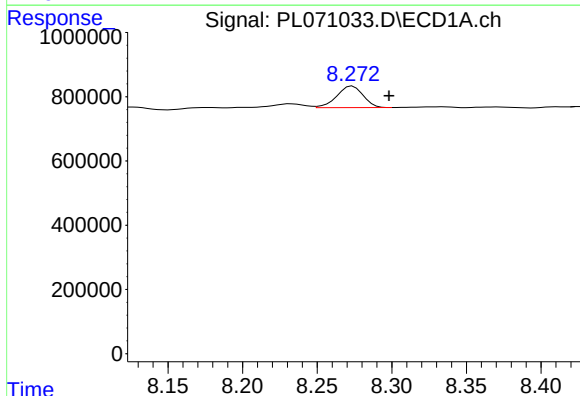


#27 Chlordane-5

R.T.: 8.274 min
Delta R.T.: -0.025 min
Response: 828868
Conc: 37.07 ng/ml

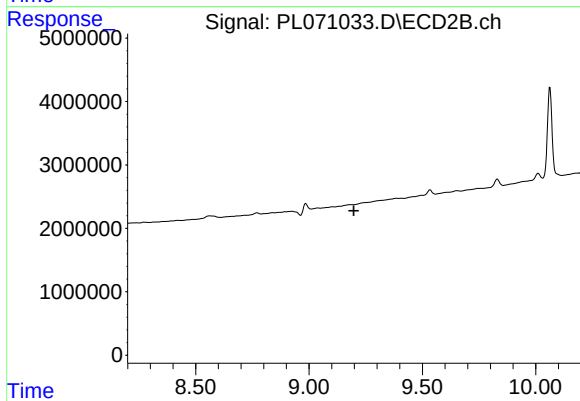

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

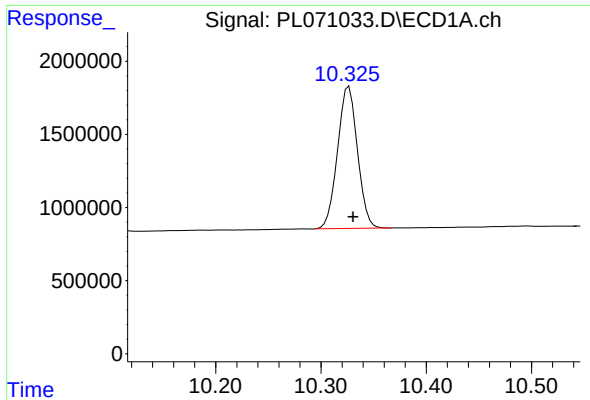

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: -0.004 min
Response: 12807698
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-COMP

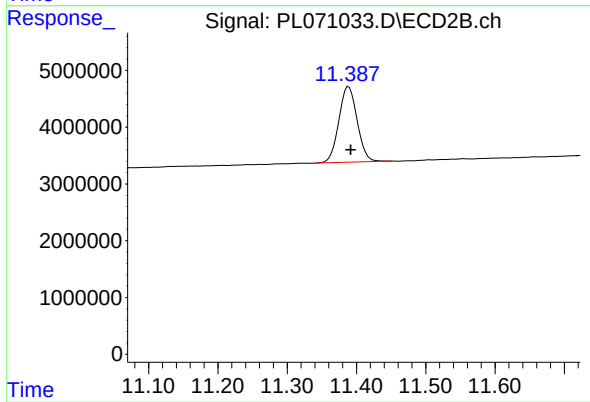

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.003 min
Response: 24498790
Conc: 18.32 ng/ml