

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
 Data File : PL071019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 12:53
 Operator : AR\AJ
 Sample : M4691-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627-EB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2021
 Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:49:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.566	5.500	8583531	23851070	17.524m	18.917m
2) SA Decachlor...	10.328	11.391	7387149	14483802	10.811	10.830

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
Data File : PL071019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 12:53
Operator : AR\AJ
Sample : M4691-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-627-EB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2021
Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:49:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

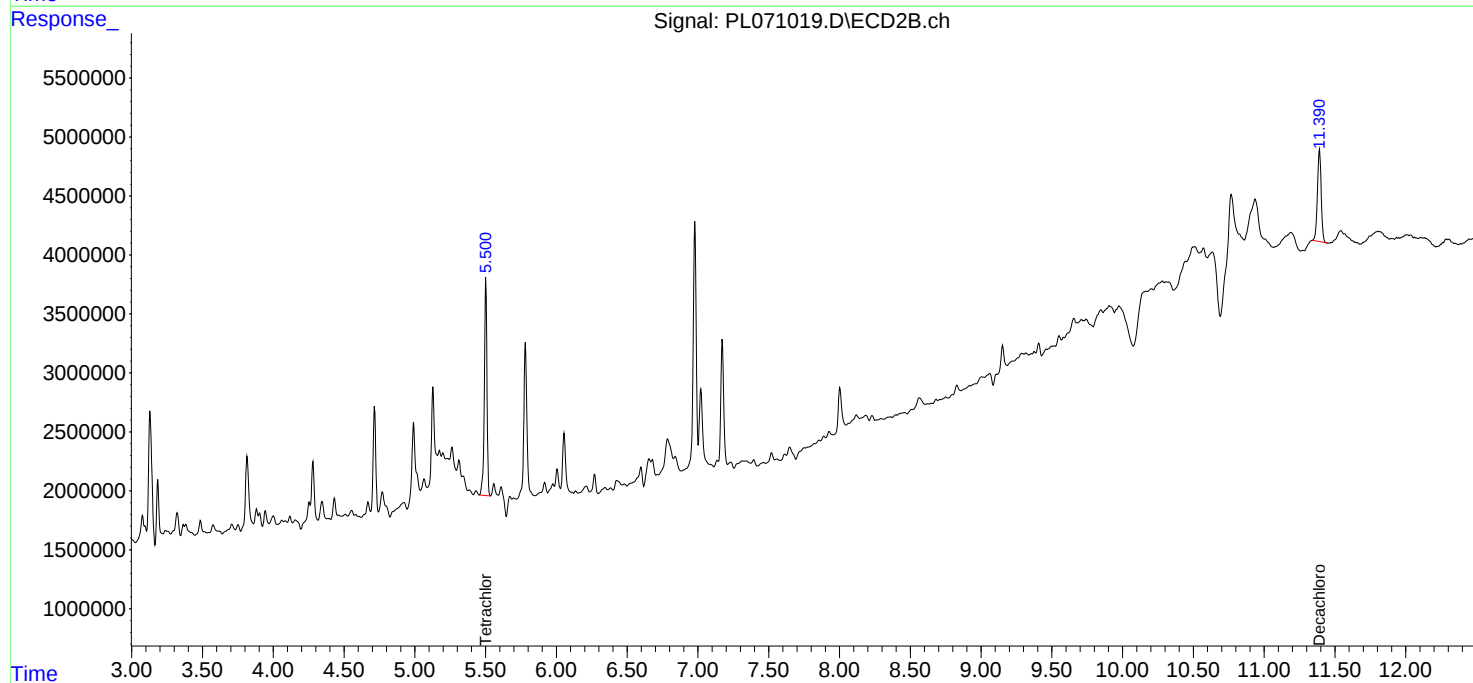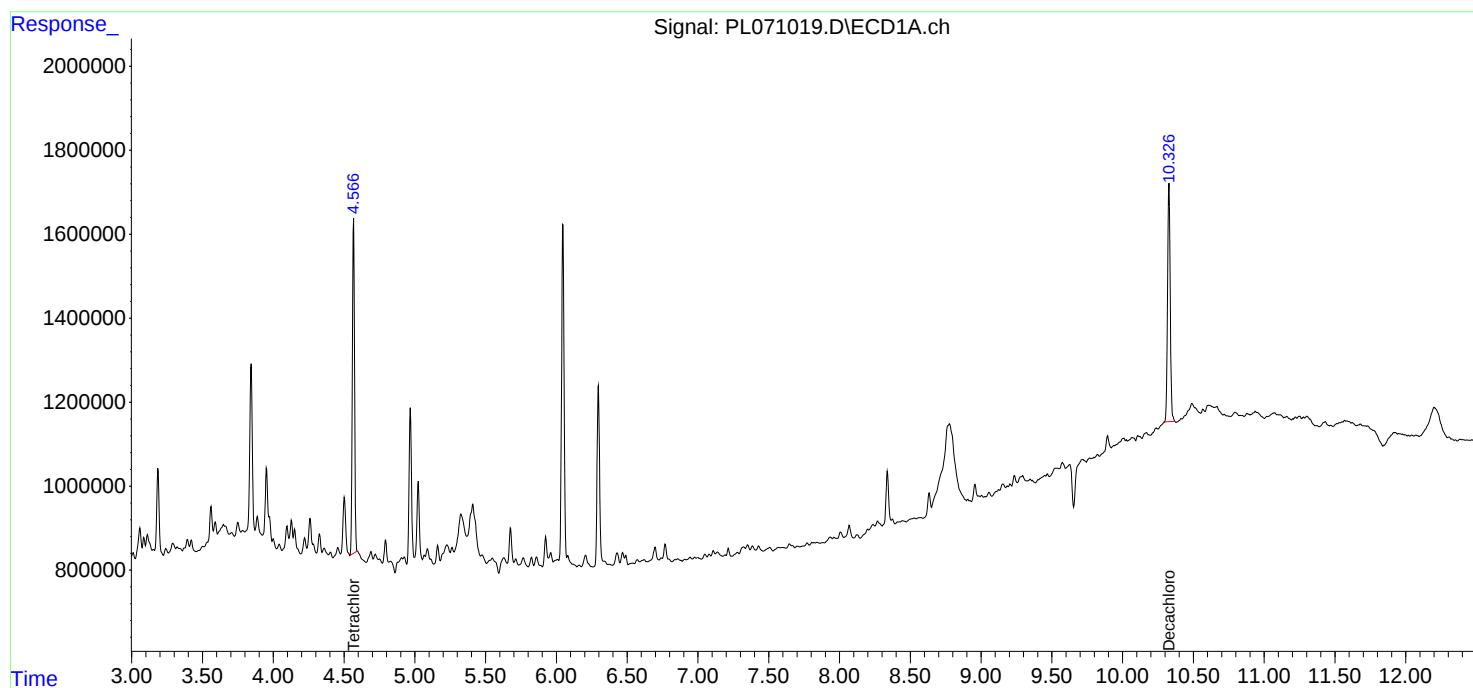

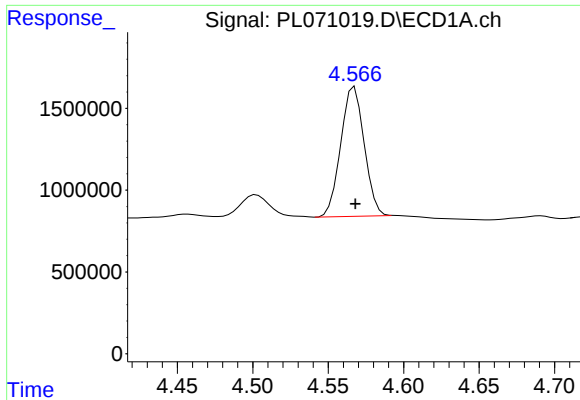


#1 Tetrachloro-m-xylene

R.T.: 4.566 min
Delta R.T.: -0.002 min
Response: 8583531
Conc: 17.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627-EB


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

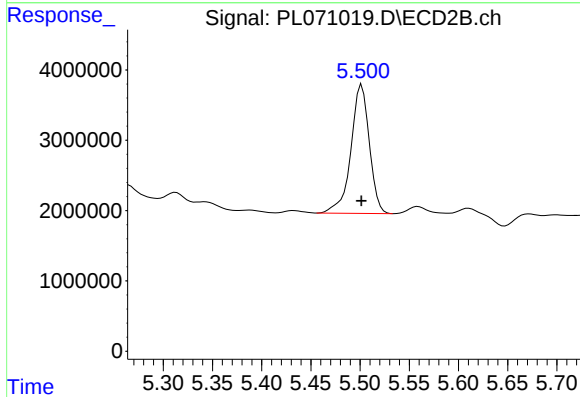


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.001 min
Response: 23851070
Conc: 18.92 ng/ml m

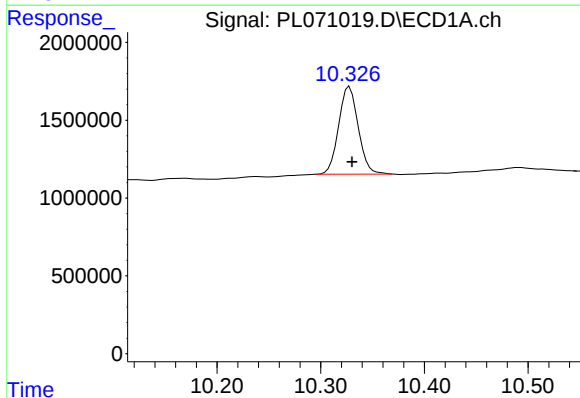

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: -0.003 min
Response: 7387149
Conc: 10.81 ng/ml

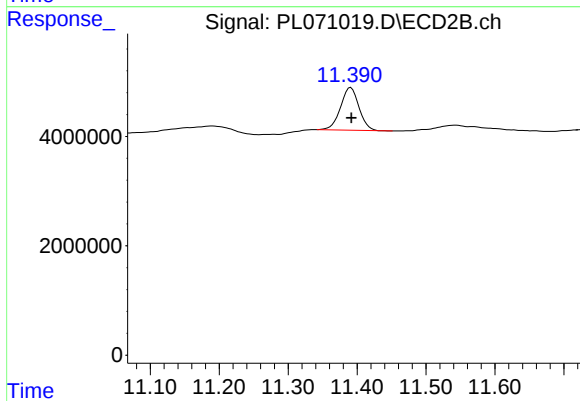

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 14483802
Conc: 10.83 ng/ml