

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
 Data File : PL071042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 23:37
 Operator : AR\AJ
 Sample : M4693-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 UT-COMP-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2021
 Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:55:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.565	5.501	9567733	27694940	19.534m	21.965
2) SA Decachlor...	10.327	11.390	6622869	12259934	9.693	9.167

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111721\
Data File : PL071042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 23:37
Operator : AR\AJ
Sample : M4693-02
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
UT-COMP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2021
Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:55:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

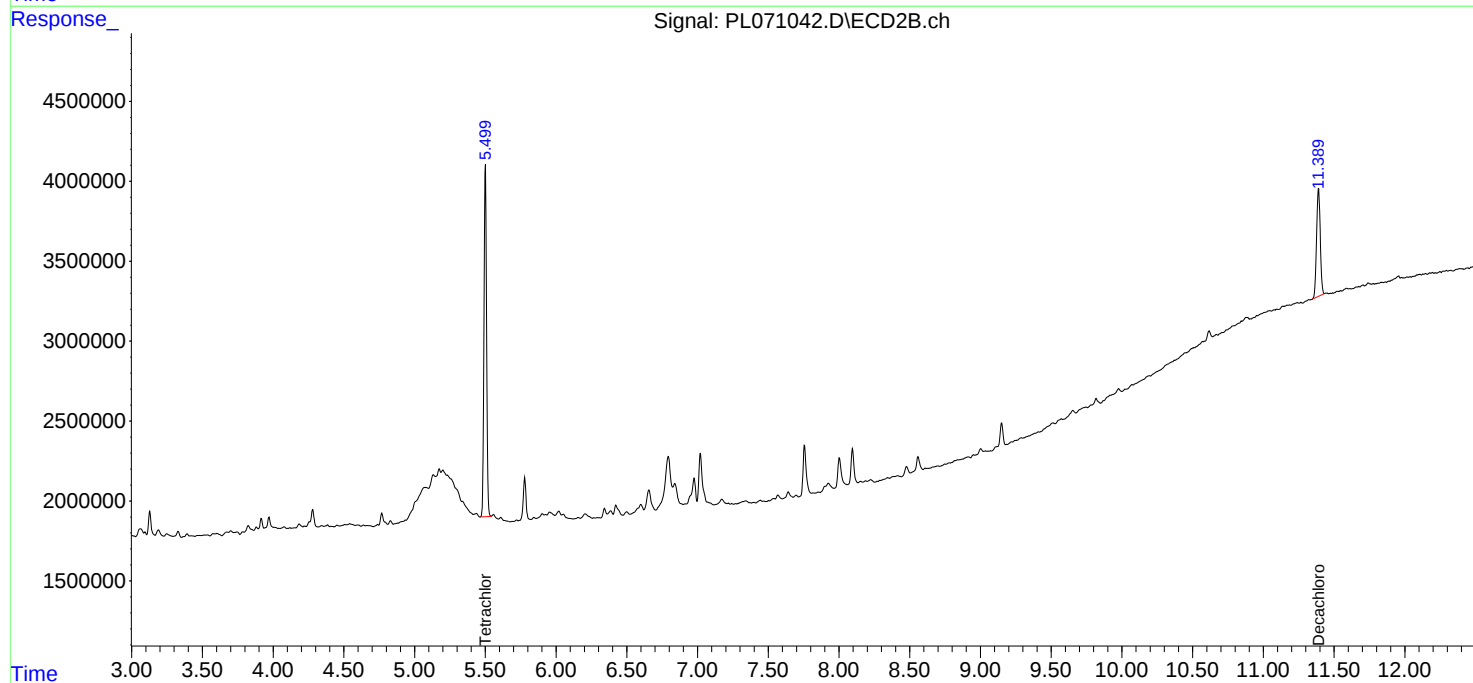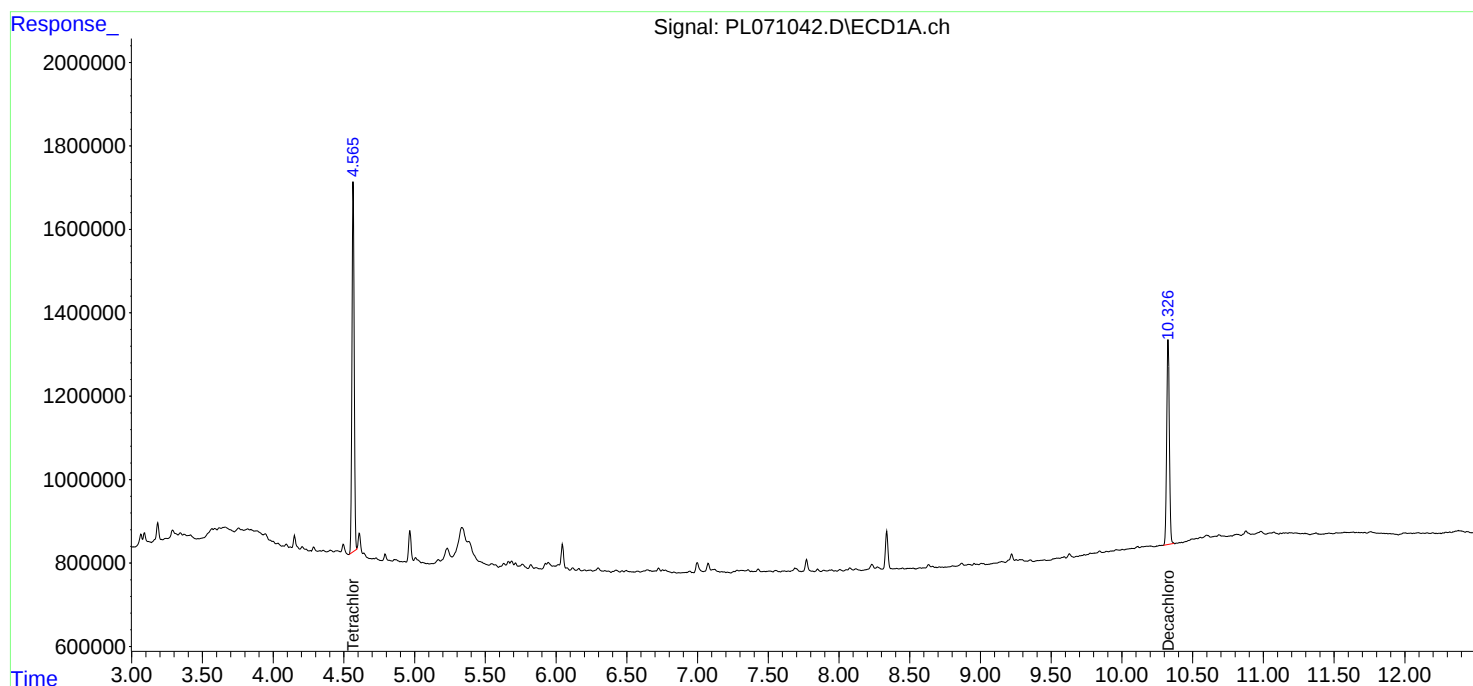

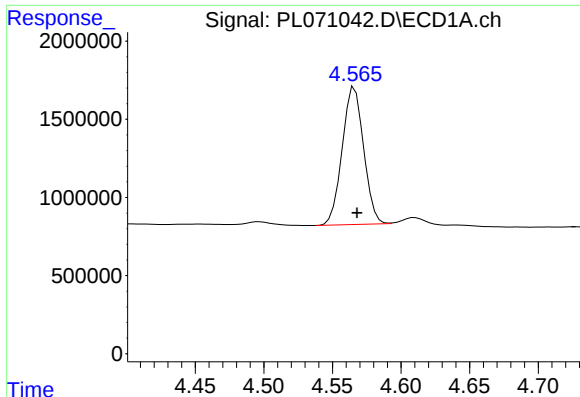


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: -0.003 min
Response: 9567733
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
UT-COMP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

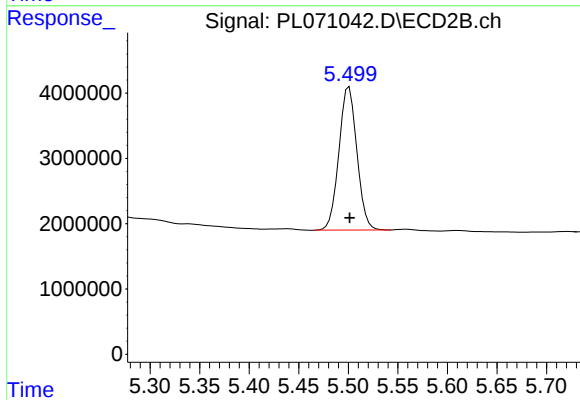


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 27694940
Conc: 21.97 ng/ml

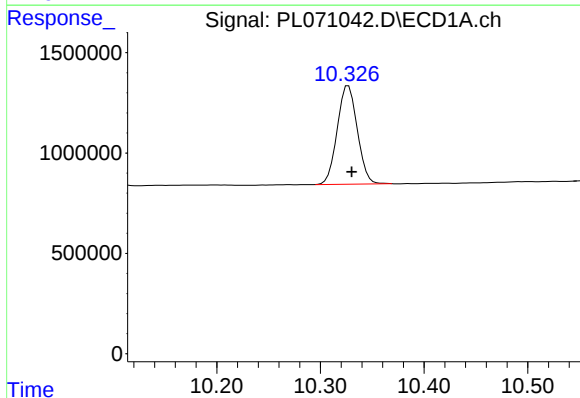

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: -0.003 min
Response: 6622869
Conc: 9.69 ng/ml

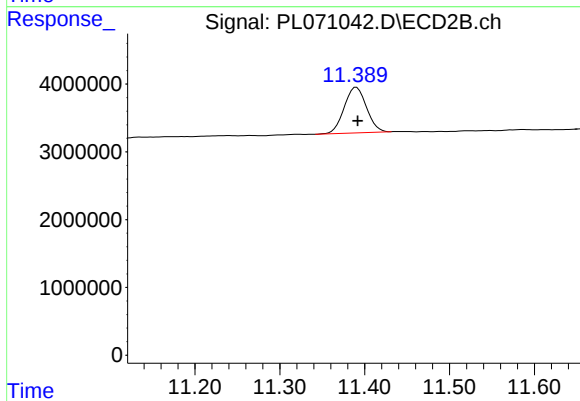

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.002 min
Response: 12259934
Conc: 9.17 ng/ml