

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111722\
 Data File : PL079178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 10:19
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 21:11:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.567	108.4E6	150.0E6	52.051	58.910
28)	SA Decachlor...	8.775	7.637	82103659	99467589	49.083	47.948
Target Compounds							
23)	Chlordane-1	4.471	3.533	45629089	48382272	520.748	468.285
24)	Chlordane-2	5.004	4.099	49967151	49844600	490.905	469.373
25)	Chlordane-3	5.715	4.719	195.3E6	149.7E6	507.086	469.777
26)	Chlordane-4	5.793	4.778	236.7E6	160.6E6	500.244	467.942
27)	Chlordane-5	6.648	5.440	38558448	41869326	519.688	491.027



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111722\
Data File : PL079178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 10:19
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 21:11:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

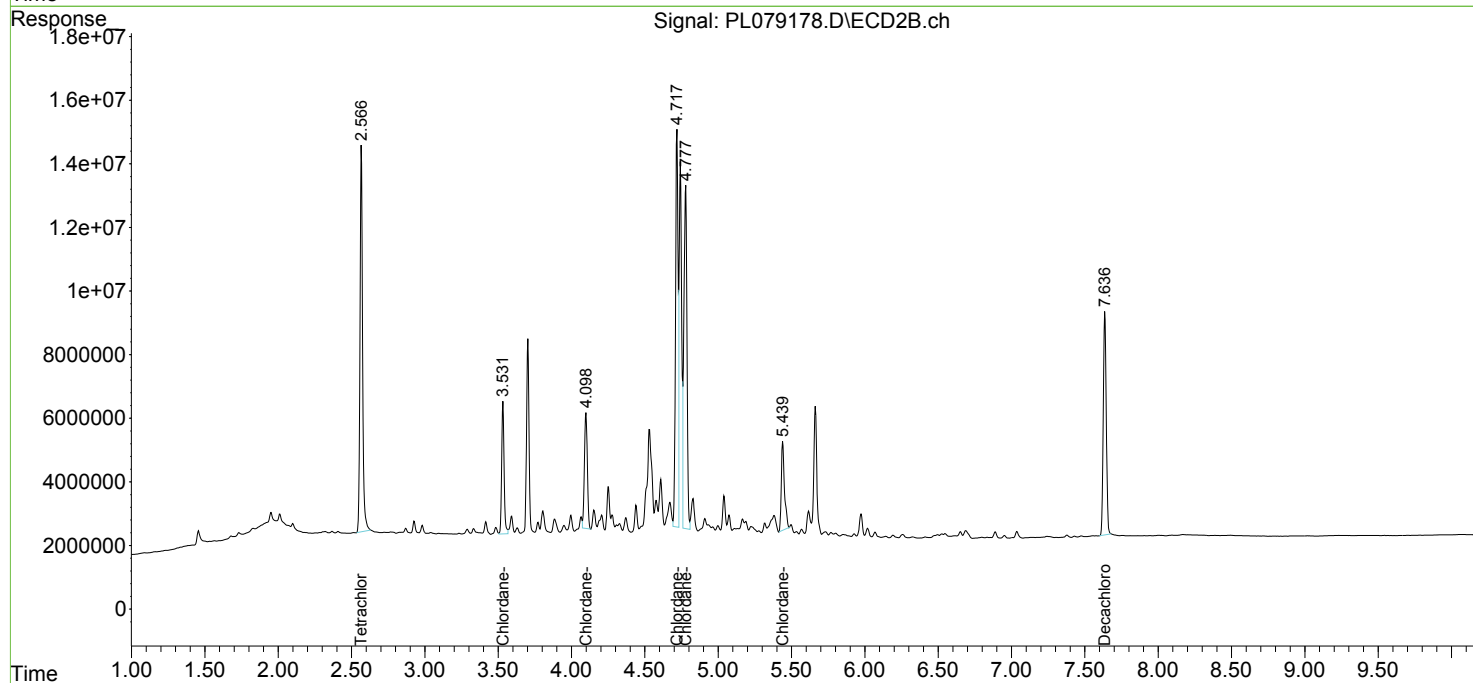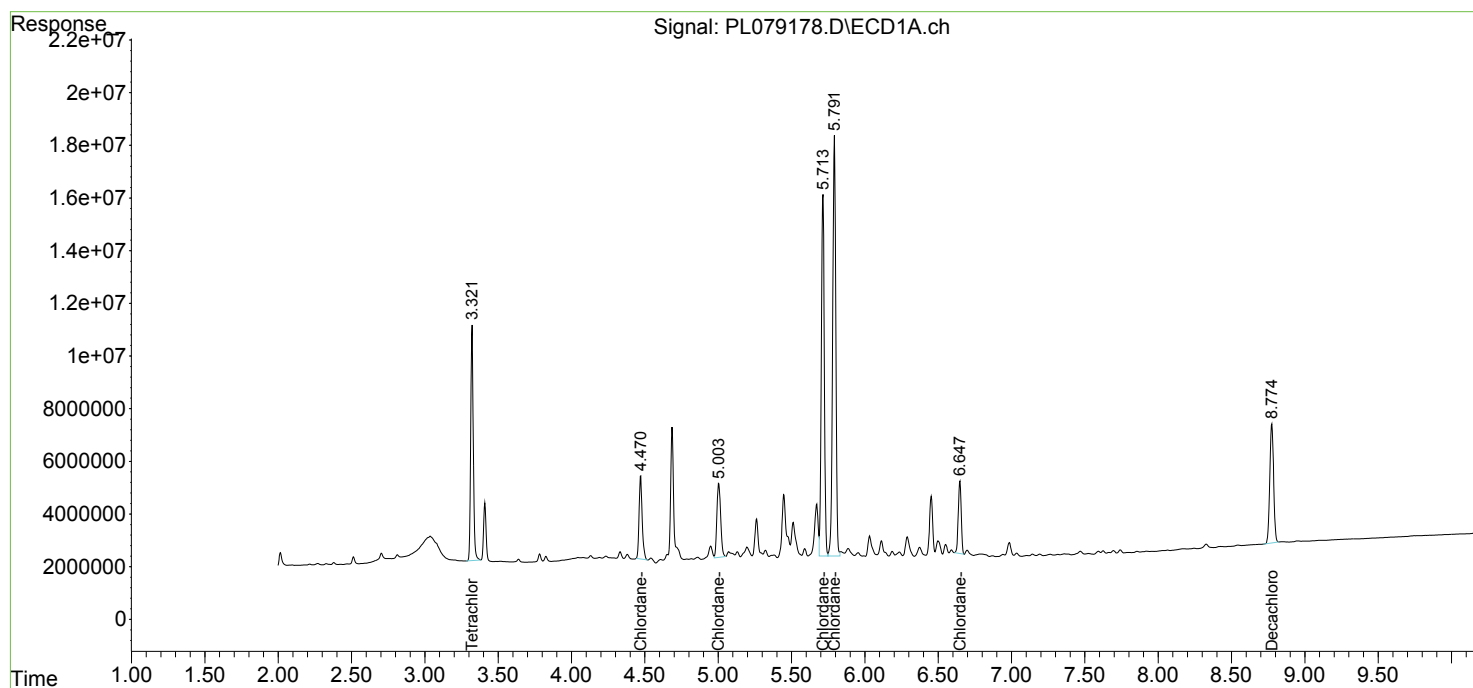


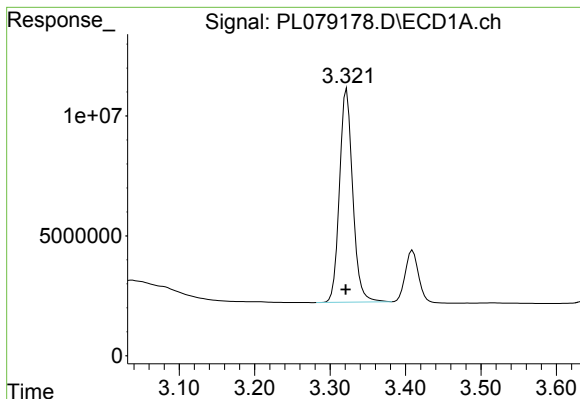

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.001 min
Response: 108392277
Conc: 52.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

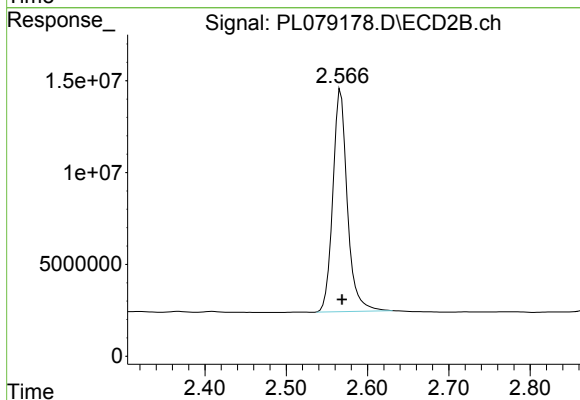


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.001 min
Response: 150035573
Conc: 58.91 ng/ml

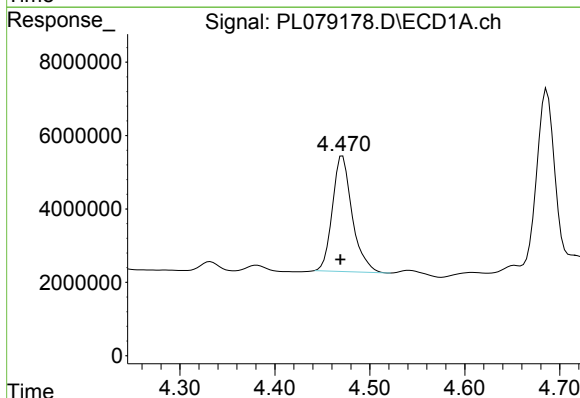


#23 Chlordane-1

R.T.: 4.471 min
Delta R.T.: 0.002 min
Response: 45629089
Conc: 520.75 ng/ml

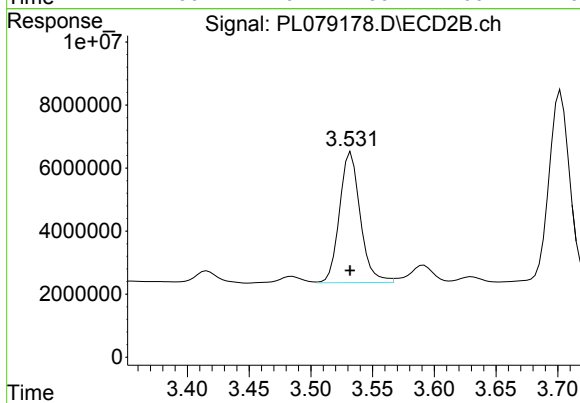

#23 Chlordane-1


R.T.: 3.533 min
Delta R.T.: 0.000 min
Response: 48382272
Conc: 468.29 ng/ml

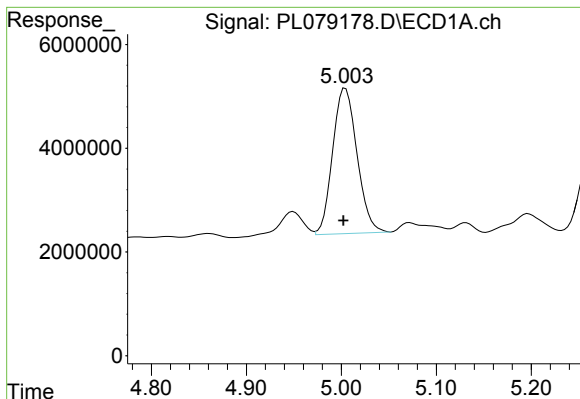

#24 Chlordane-2


R.T.: 5.004 min
Delta R.T.: 0.002 min
Response: 49967151
Conc: 490.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

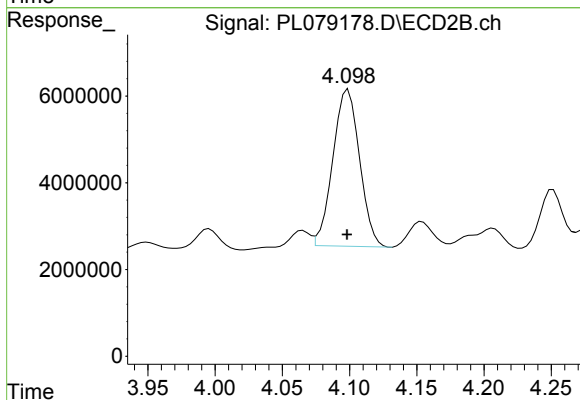


#24 Chlordane-2

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 49844600
Conc: 469.37 ng/ml

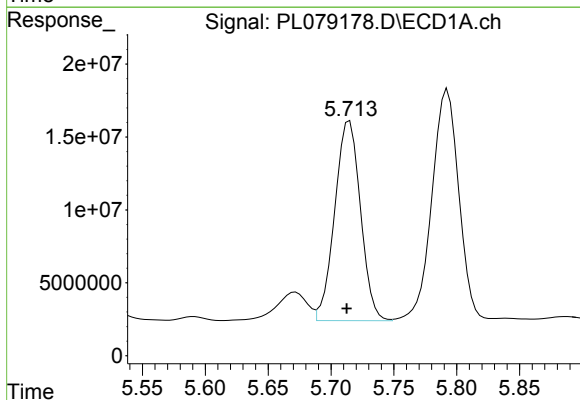


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 195330468
Conc: 507.09 ng/ml

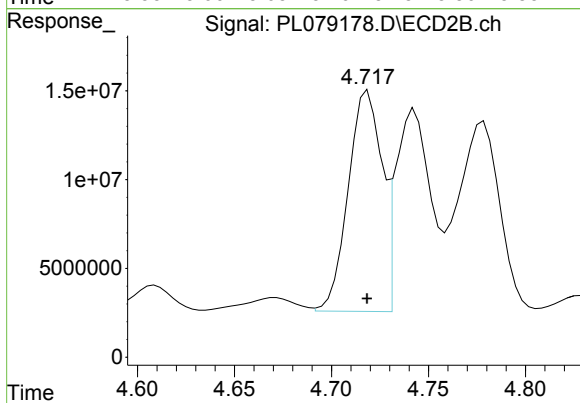

#25 Chlordane-3


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 149678274
Conc: 469.78 ng/ml

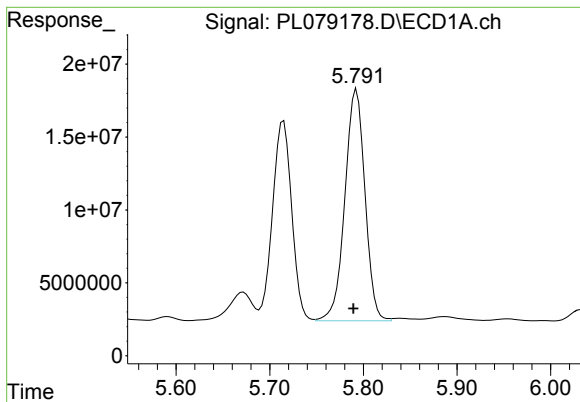

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.003 min
Response: 236696596
Conc: 500.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

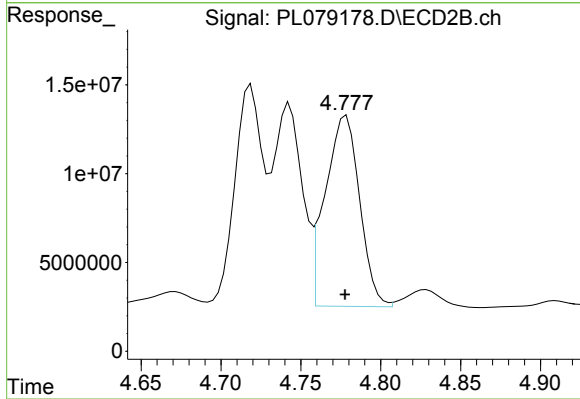


#26 Chlordane-4

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 160580307
Conc: 467.94 ng/ml

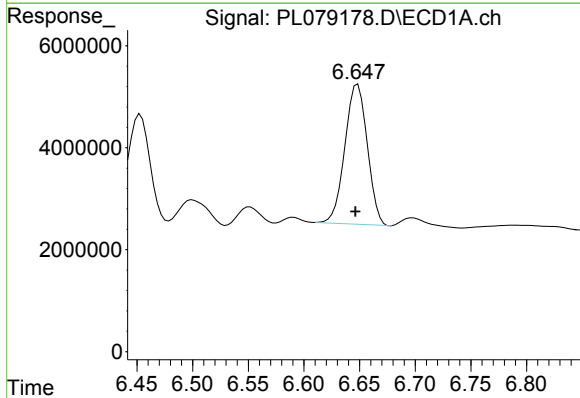


#27 Chlordane-5

R.T.: 6.648 min
Delta R.T.: 0.002 min
Response: 38558448
Conc: 519.69 ng/ml

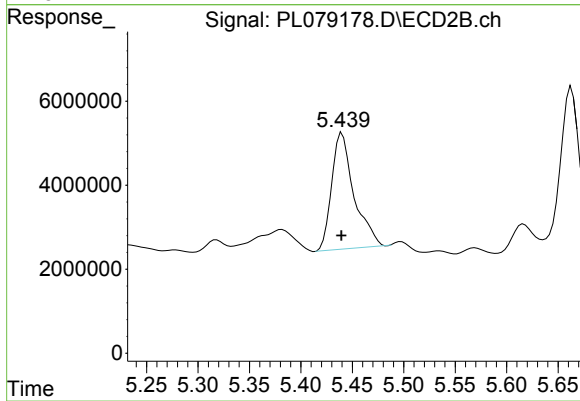

#27 Chlordane-5


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 41869326
Conc: 491.03 ng/ml

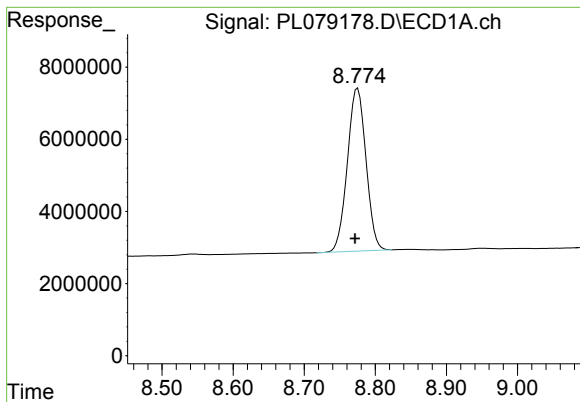

#28 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: 0.003 min
Response: 82103659
Conc: 49.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

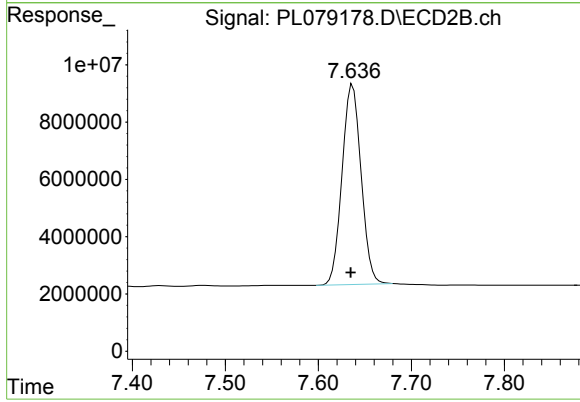

#28 Decachlorobiphenyl

R.T.: 7.637 min
Delta R.T.: 0.002 min
Response: 99467589
Conc: 47.95 ng/ml