

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111722\
 Data File : PL079202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 18:41
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 03:15:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.565	100.6E6	142.5E6	48.329	55.939
28)	SA Decachlor...	8.769	7.633	81485050	99521847	48.713	47.975
Target Compounds							
23)	Chlordane-1	4.468	3.530	41513242	46203183	473.776	447.194
24)	Chlordane-2	5.001	4.097	46712730	46903785	458.932	441.681
25)	Chlordane-3	5.711	4.716	184.4E6	144.6E6	478.625	453.798
26)	Chlordane-4	5.788	4.776	223.6E6	154.7E6	472.629	450.942
27)	Chlordane-5	6.643	5.438	36201101	40136108	487.916	470.700



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111722\
Data File : PL079202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 18:41
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 03:15:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

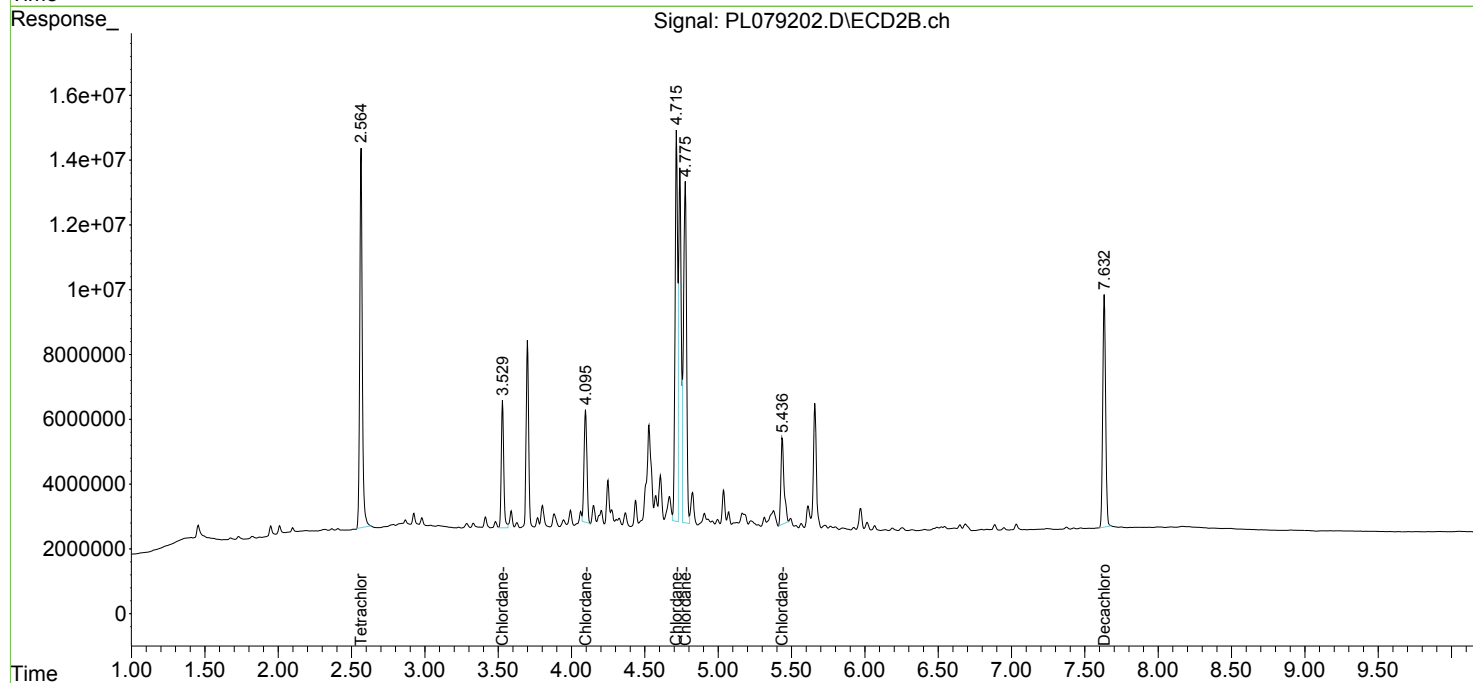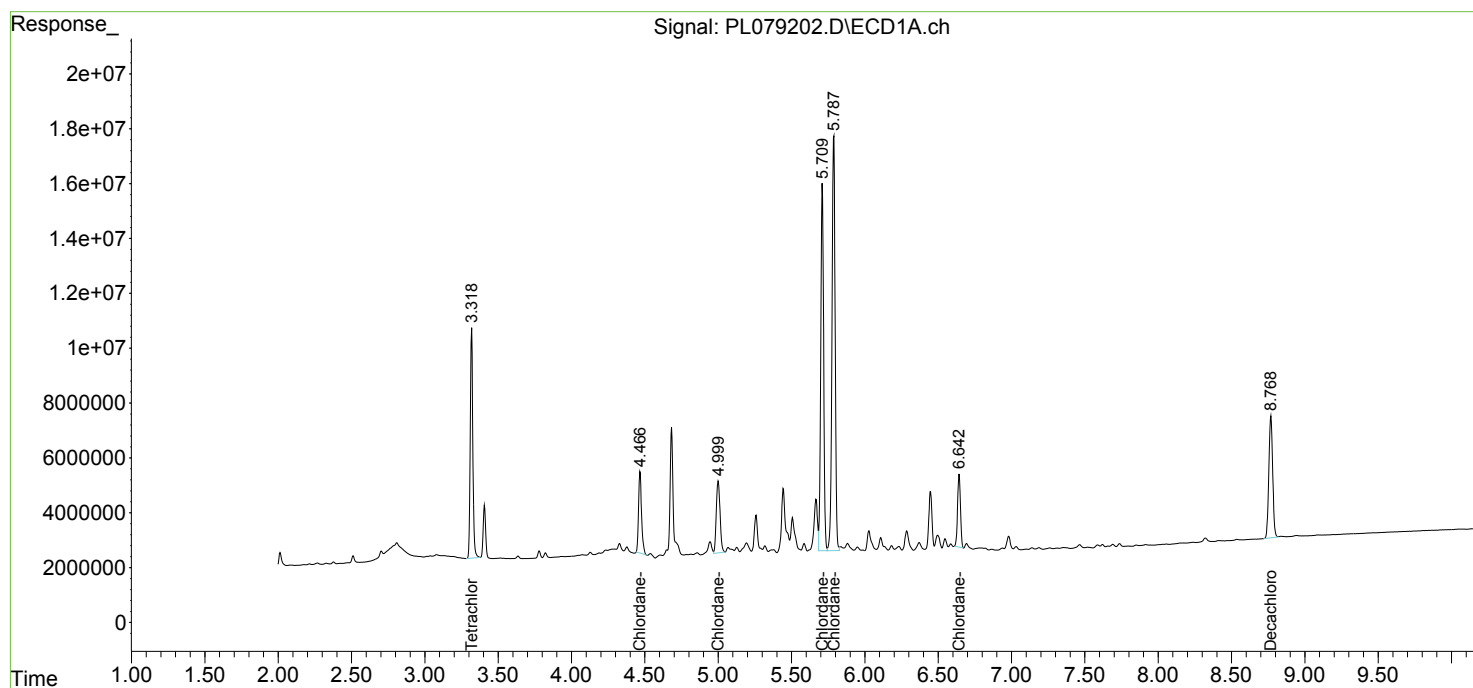


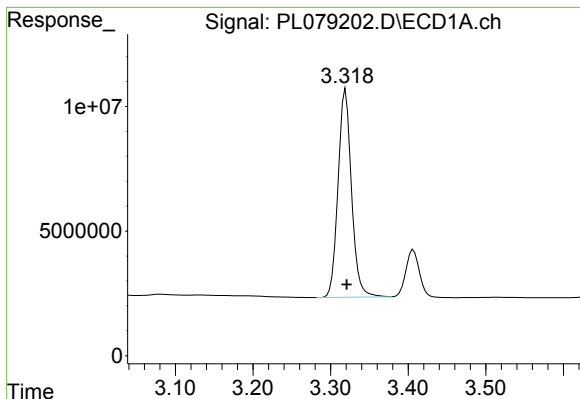

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 100640334
Conc: 48.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

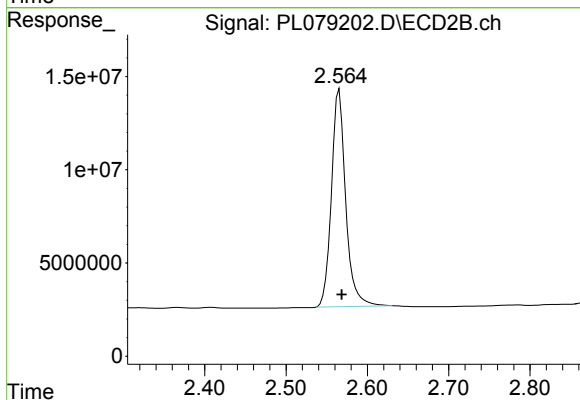


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: -0.003 min
Response: 142467875
Conc: 55.94 ng/ml

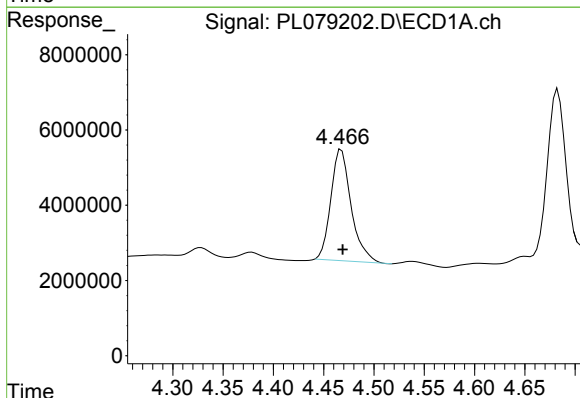


#23 Chlordane-1

R.T.: 4.468 min
Delta R.T.: -0.001 min
Response: 41513242
Conc: 473.78 ng/ml

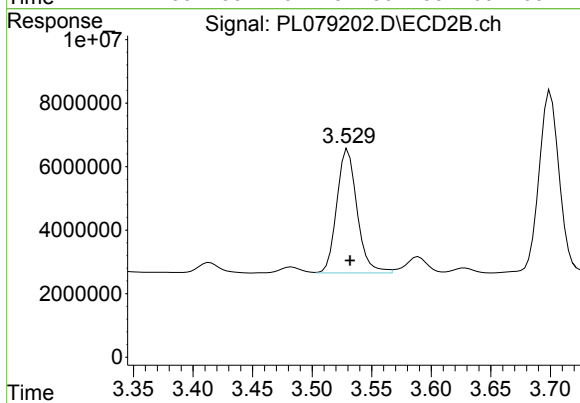

#23 Chlordane-1


R.T.: 3.530 min
Delta R.T.: -0.002 min
Response: 46203183
Conc: 447.19 ng/ml

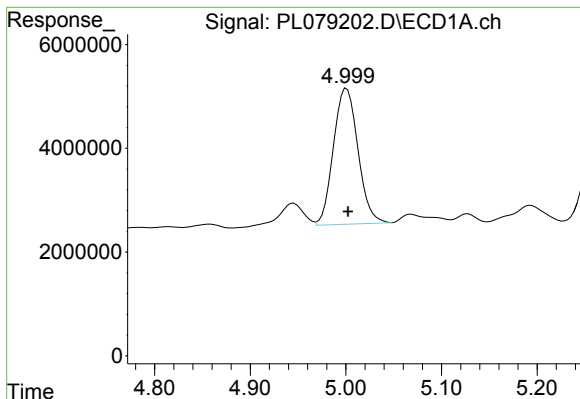

#24 Chlordane-2


R.T.: 5.001 min
Delta R.T.: -0.001 min
Response: 46712730
Conc: 458.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

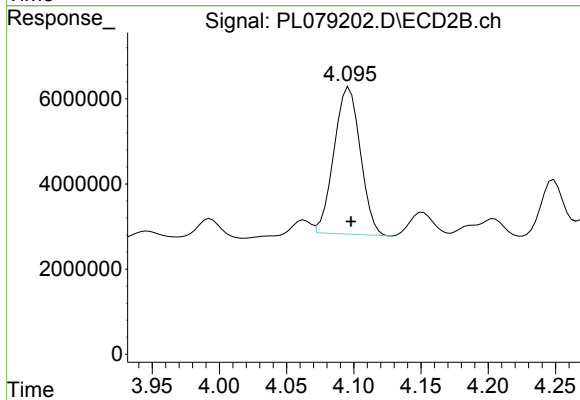


#24 Chlordane-2

R.T.: 4.097 min
Delta R.T.: -0.002 min
Response: 46903785
Conc: 441.68 ng/ml

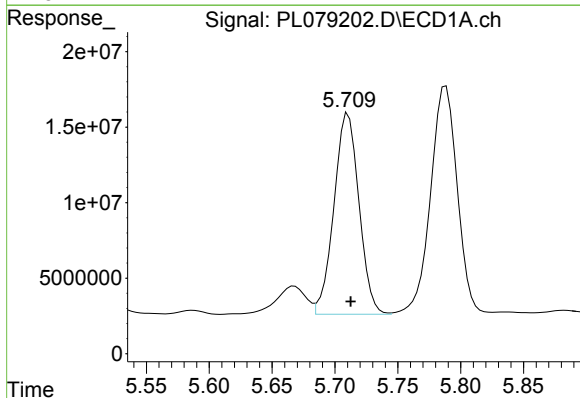


#25 Chlordane-3

R.T.: 5.711 min
Delta R.T.: -0.002 min
Response: 184367443
Conc: 478.63 ng/ml

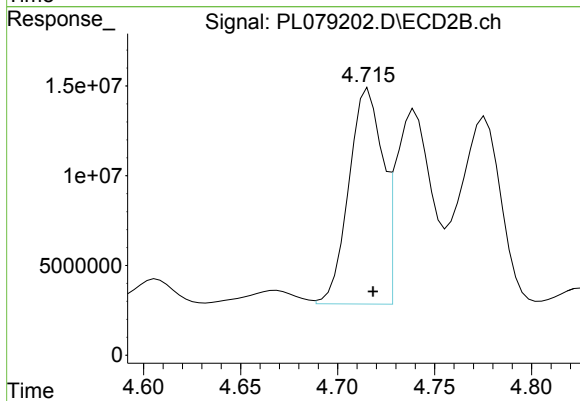

#25 Chlordane-3


R.T.: 4.716 min
Delta R.T.: -0.002 min
Response: 144586831
Conc: 453.80 ng/ml

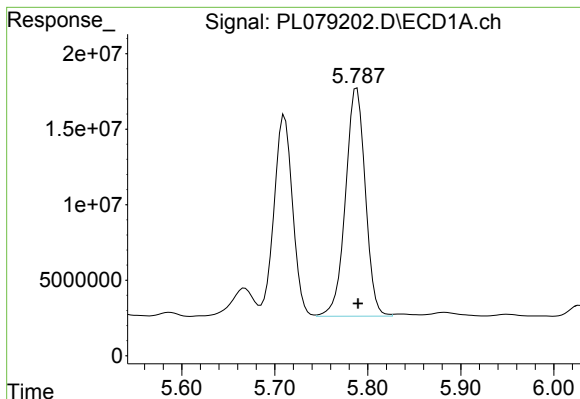

#26 Chlordane-4


R.T.: 5.788 min
Delta R.T.: -0.001 min
Response: 223630548
Conc: 472.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

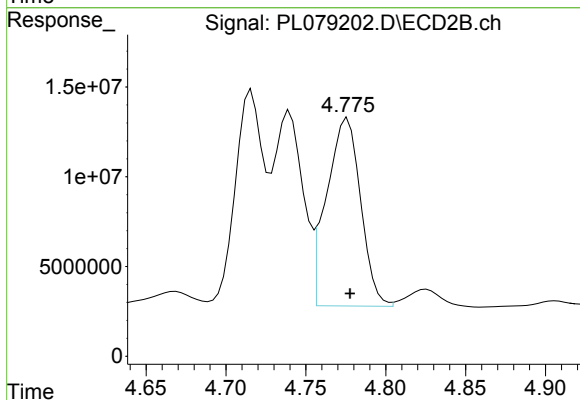


#26 Chlordane-4

R.T.: 4.776 min
Delta R.T.: -0.002 min
Response: 154746625
Conc: 450.94 ng/ml

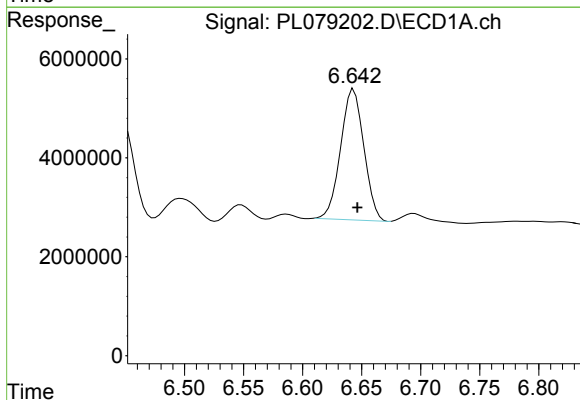


#27 Chlordane-5

R.T.: 6.643 min
Delta R.T.: -0.003 min
Response: 36201101
Conc: 487.92 ng/ml

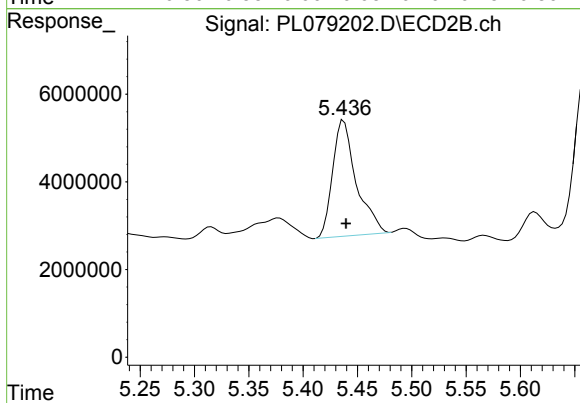

#27 Chlordane-5


R.T.: 5.438 min
Delta R.T.: -0.002 min
Response: 40136108
Conc: 470.70 ng/ml

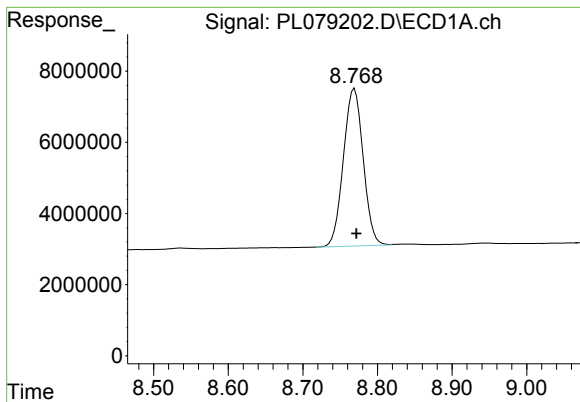

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.002 min
Response: 81485050
Conc: 48.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

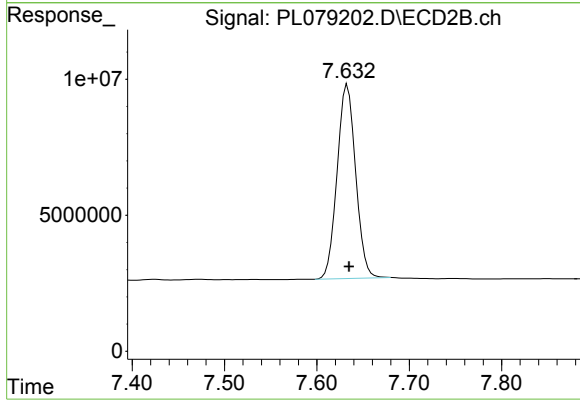

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: -0.002 min
Response: 99521847
Conc: 47.97 ng/ml