

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
 Data File : PL042248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2018 11:07
 Operator : AJ\SJ
 Sample : I.BLK
 Misc : FOR MIREX
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 14:10:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.102	118.5E6	57967986	21.344	20.970
28)	SA Decachlor...	8.211	9.237	124.2E6	48612604	20.074	20.422

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
Data File : PL042248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2018 11:07
Operator : AJ\SJ
Sample : I.BLK
Misc : FOR MIREX
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 14:10:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

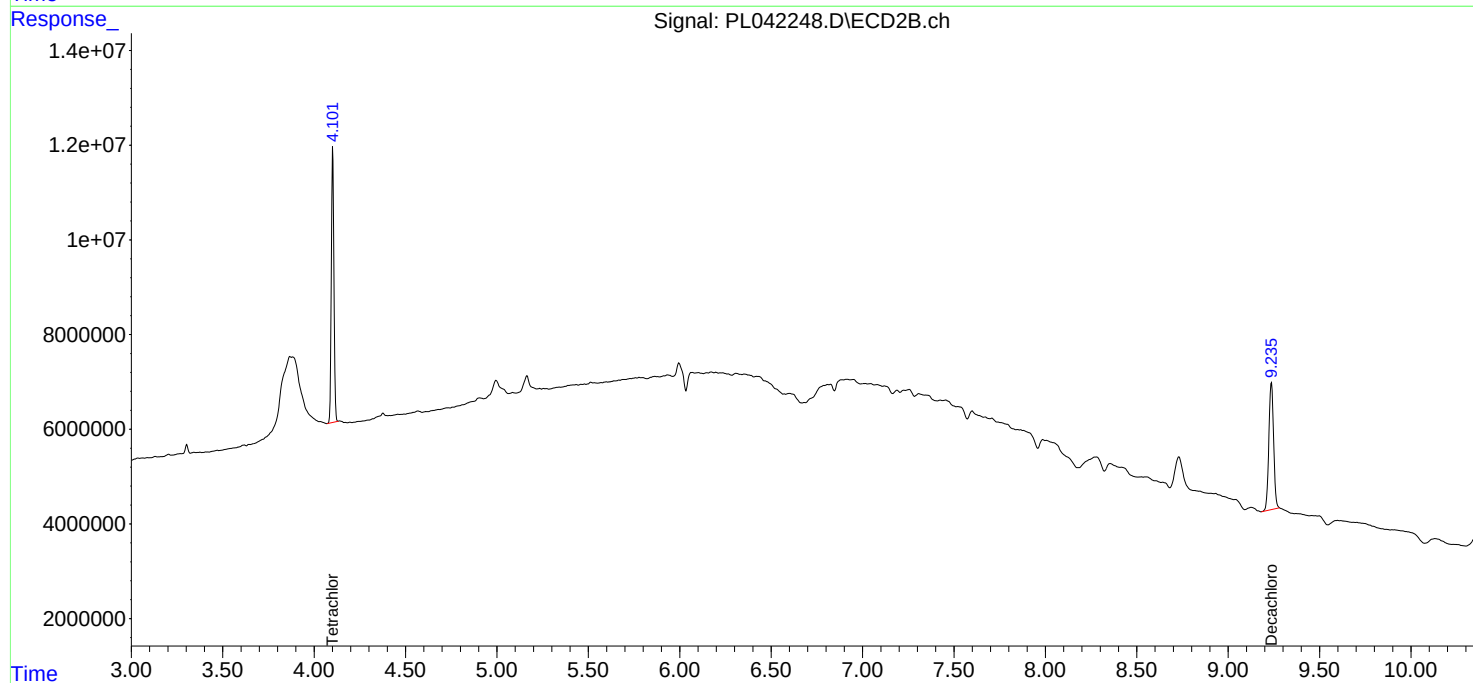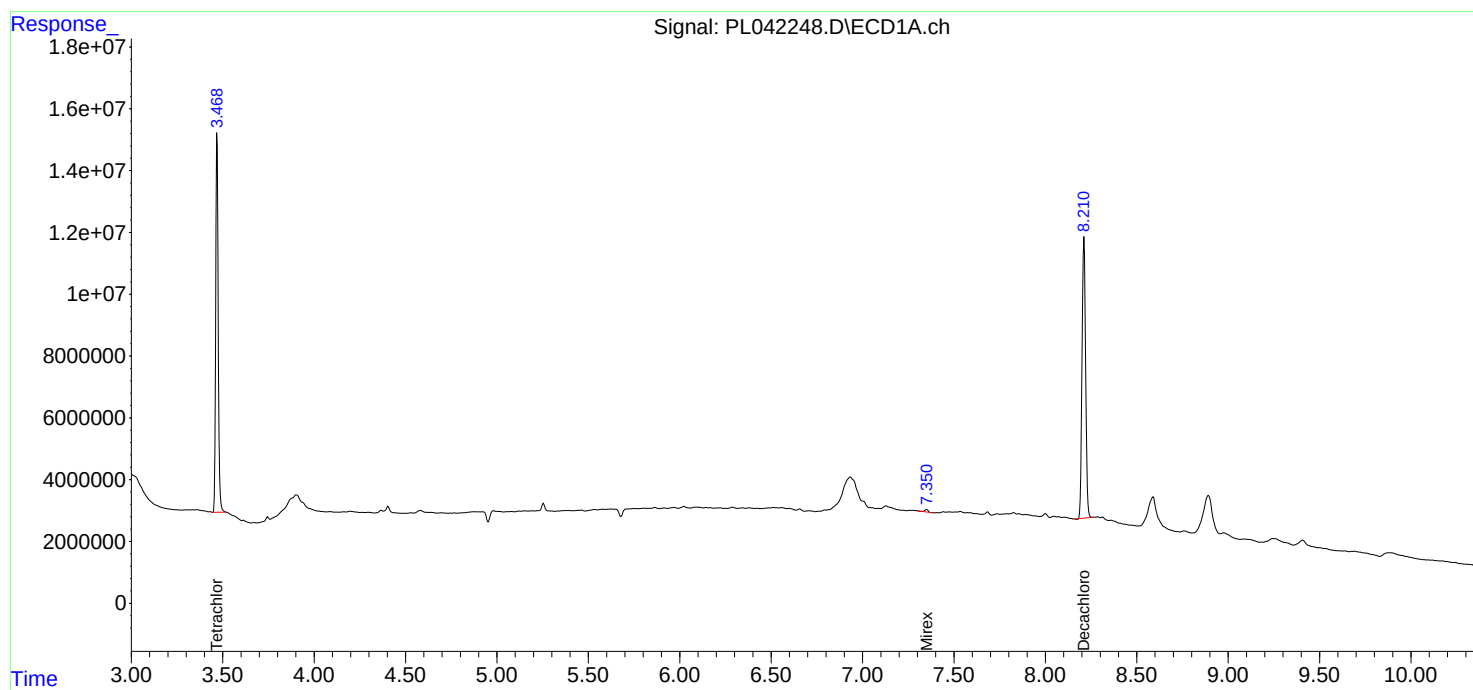


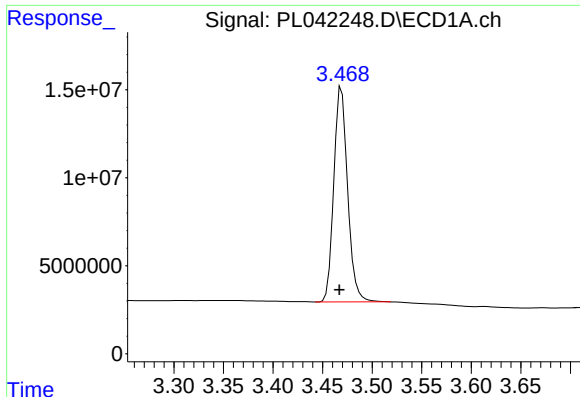

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.002 min
Response: 118466788
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

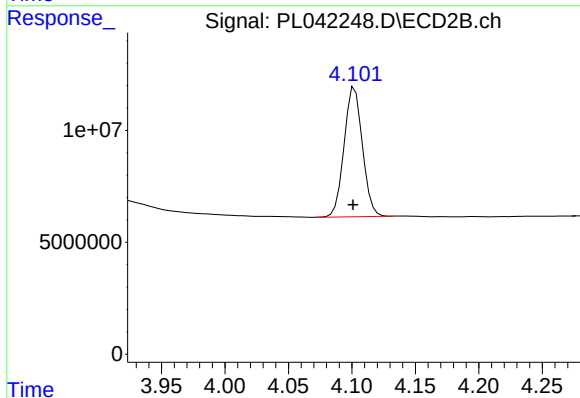


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.001 min
Response: 57967986
Conc: 20.97 ng/ml

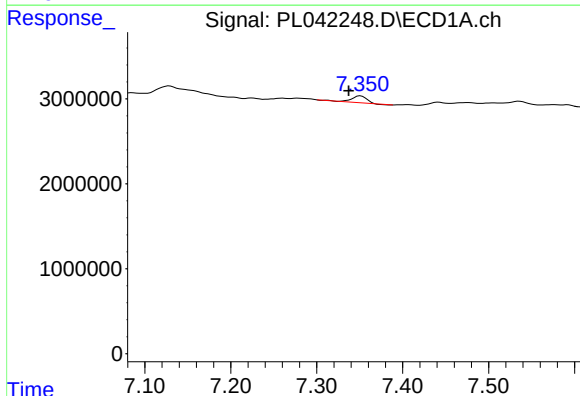


#22 Mirex

R.T.: 7.351 min
Delta R.T.: 0.014 min
Response: 1018109
Conc: 0.18 ng/ml

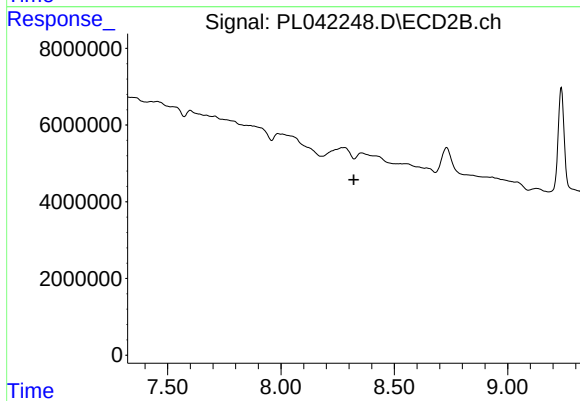

#22 Mirex

R.T.: 8.355 min
Delta R.T.: 0.033 min
Response: -2931709
Conc: N.D.

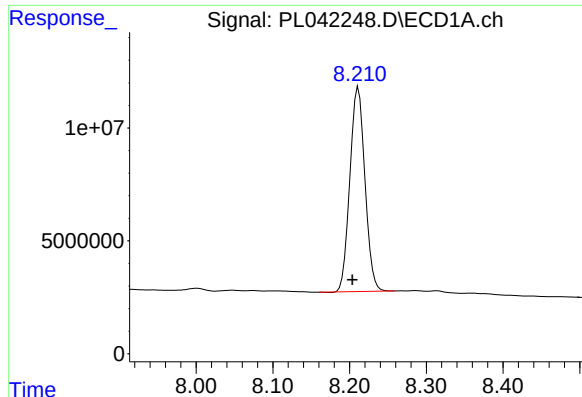

#28 Decachlorobiphenyl


R.T.: 8.211 min

Delta R.T.: 0.008 min

Response: 124224306

Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

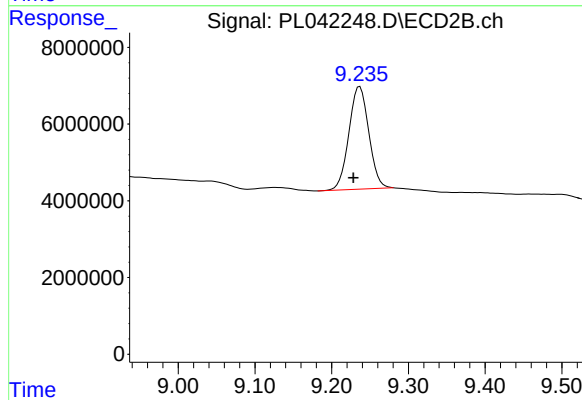

#28 Decachlorobiphenyl

R.T.: 9.237 min

Delta R.T.: 0.008 min

Response: 48612604

Conc: 20.42 ng/ml