

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
 Data File : PL042250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2018 12:05
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc : FOR MIREX
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 14:10:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.103	299.0E6	149.1E6	53.870	53.926
28)	SA Decachlor...	8.210	9.236	304.4E6	119.2E6	49.189	50.055
Target Compounds							
22)	Mirex	7.343	8.327	284.0E6	96711128	49.829	51.879



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
Data File : PL042250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2018 12:05
Operator : AJ\SJ
Sample : PSTDCCC050
Misc : FOR MIREX
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 14:10:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

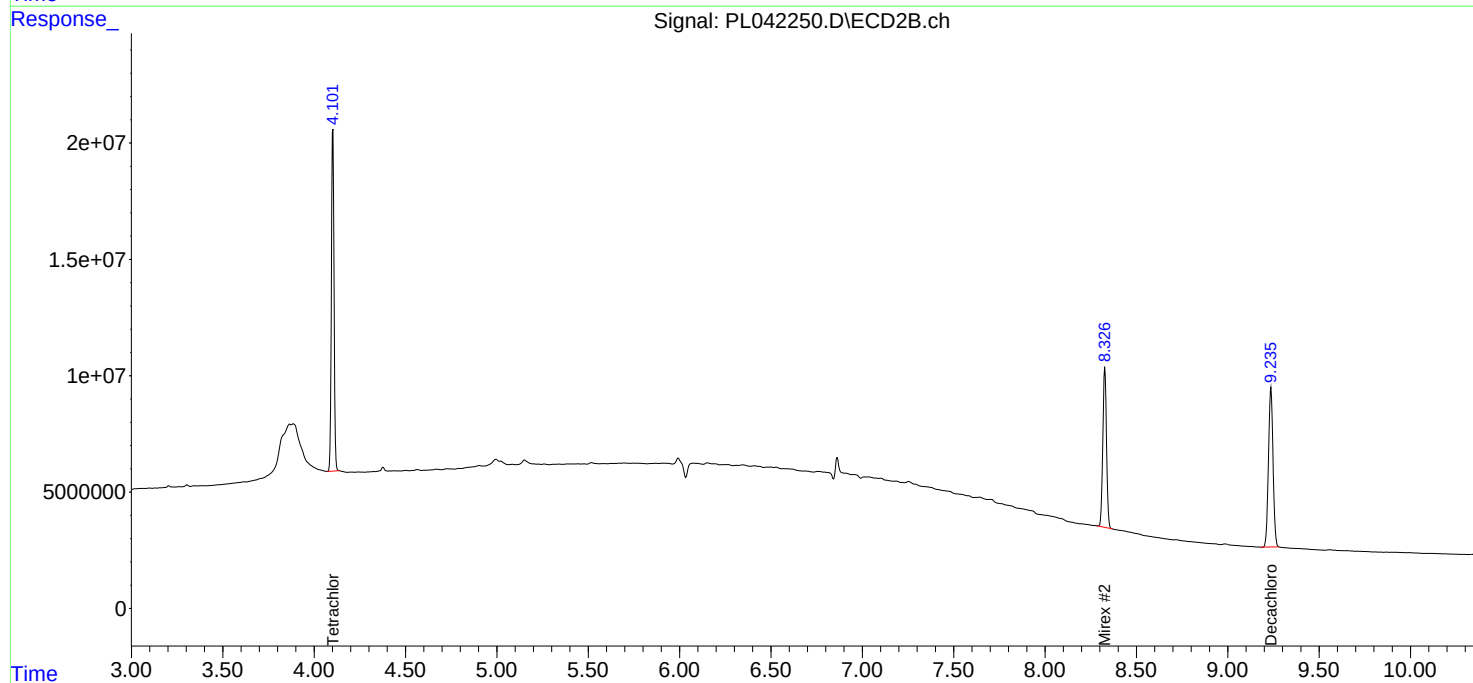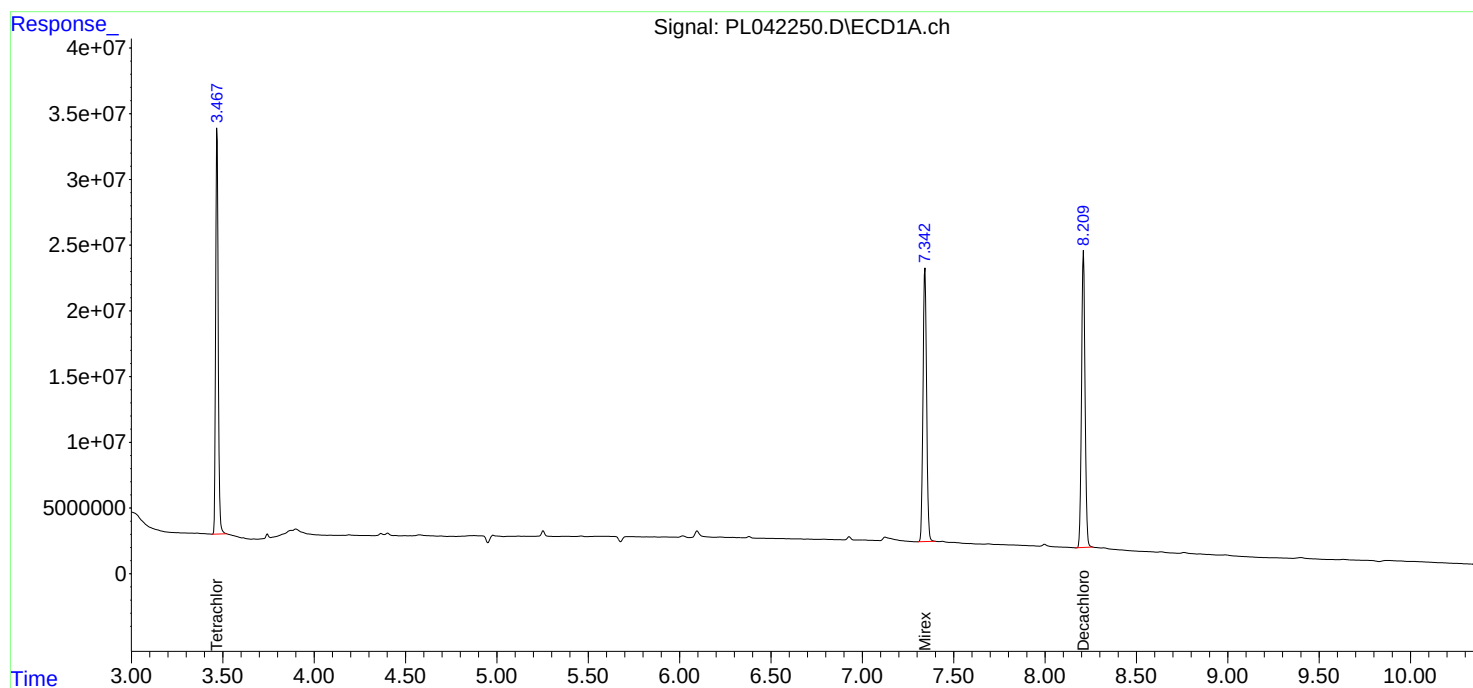


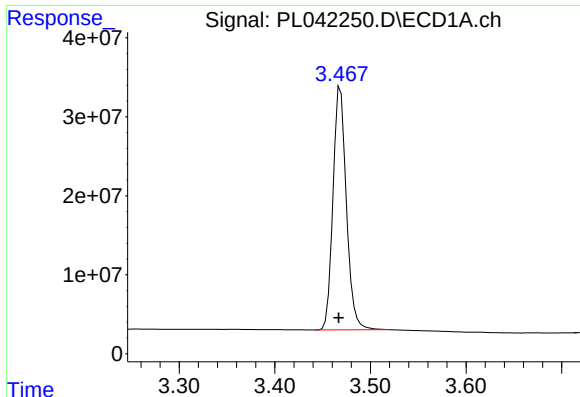

#1 Tetrachloro-m-xylene


R.T.: 3.469 min
Delta R.T.: 0.002 min
Response: 299004405
Conc: 53.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

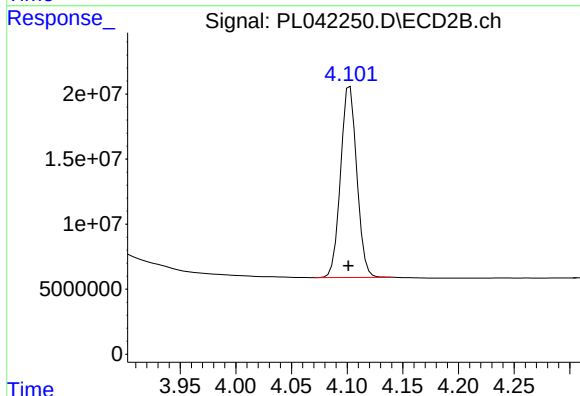


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.002 min
Response: 149072135
Conc: 53.93 ng/ml

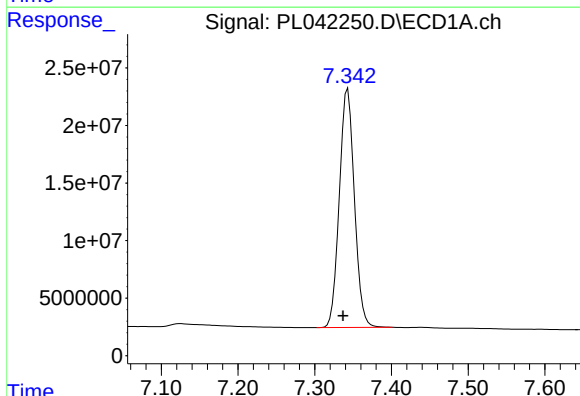


#22 Mirex

R.T.: 7.343 min
Delta R.T.: 0.006 min
Response: 284047973
Conc: 49.83 ng/ml

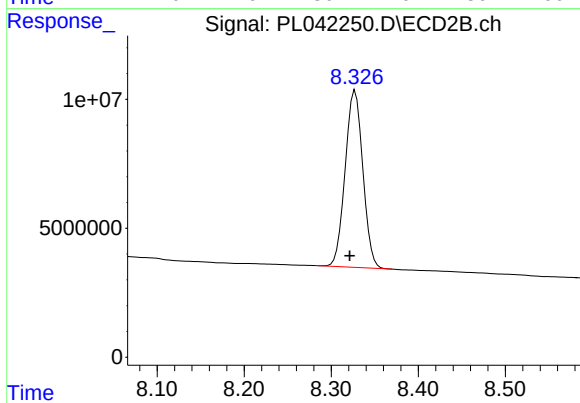

#22 Mirex

R.T.: 8.327 min
Delta R.T.: 0.006 min
Response: 96711128
Conc: 51.88 ng/ml

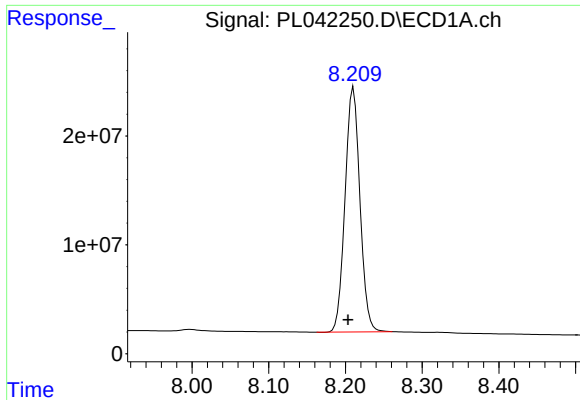

#28 Decachlorobiphenyl


R.T.: 8.210 min

Delta R.T.: 0.007 min

Response: 304400743

Conc: 49.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

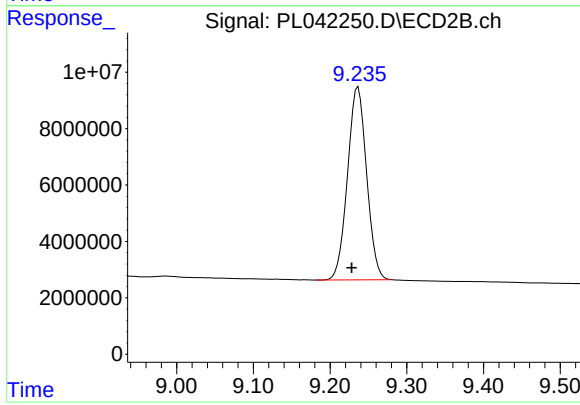

#28 Decachlorobiphenyl

R.T.: 9.236 min

Delta R.T.: 0.008 min

Response: 119153635

Conc: 50.06 ng/ml