

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111818\  
 Data File : PL042251.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 16 Nov 2018 12:19  
 Operator : AJ\SJ  
 Sample : MIREX-MDL-BL-S-02  
 Misc : FOR MIREX  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 MIREX-MDL-BL-S-02

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 16 14:10:55 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\Mirex-PL111718.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 15 11:21:10 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1  | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|---------|----------|--------|--------|
| -----                       |                 |       |       |         |          |        |        |
| System Monitoring Compounds |                 |       |       |         |          |        |        |
| 1)                          | SA Tetrachlo... | 3.468 | 4.103 | 118.3E6 | 60724270 | 21.316 | 21.967 |
| 28)                         | SA Decachlor... | 8.210 | 9.235 | 130.8E6 | 49988930 | 21.139 | 21.000 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111818\  
Data File : PL042251.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Nov 2018 12:19  
Operator : AJ\SJ  
Sample : MIREX-MDL-BL-S-02  
Misc : FOR MIREX  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
MIREX-MDL-BL-S-02

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 16 14:10:55 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\Mirex-PL111718.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 15 11:21:10 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

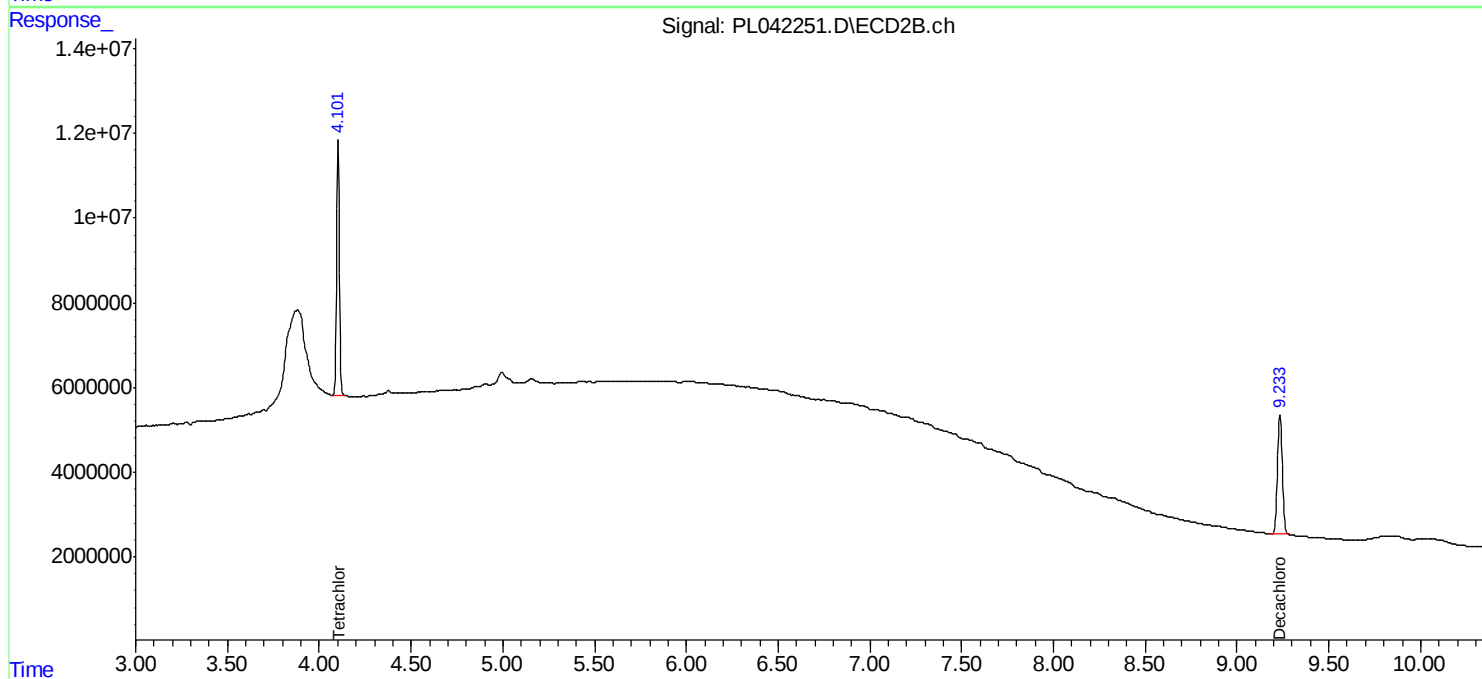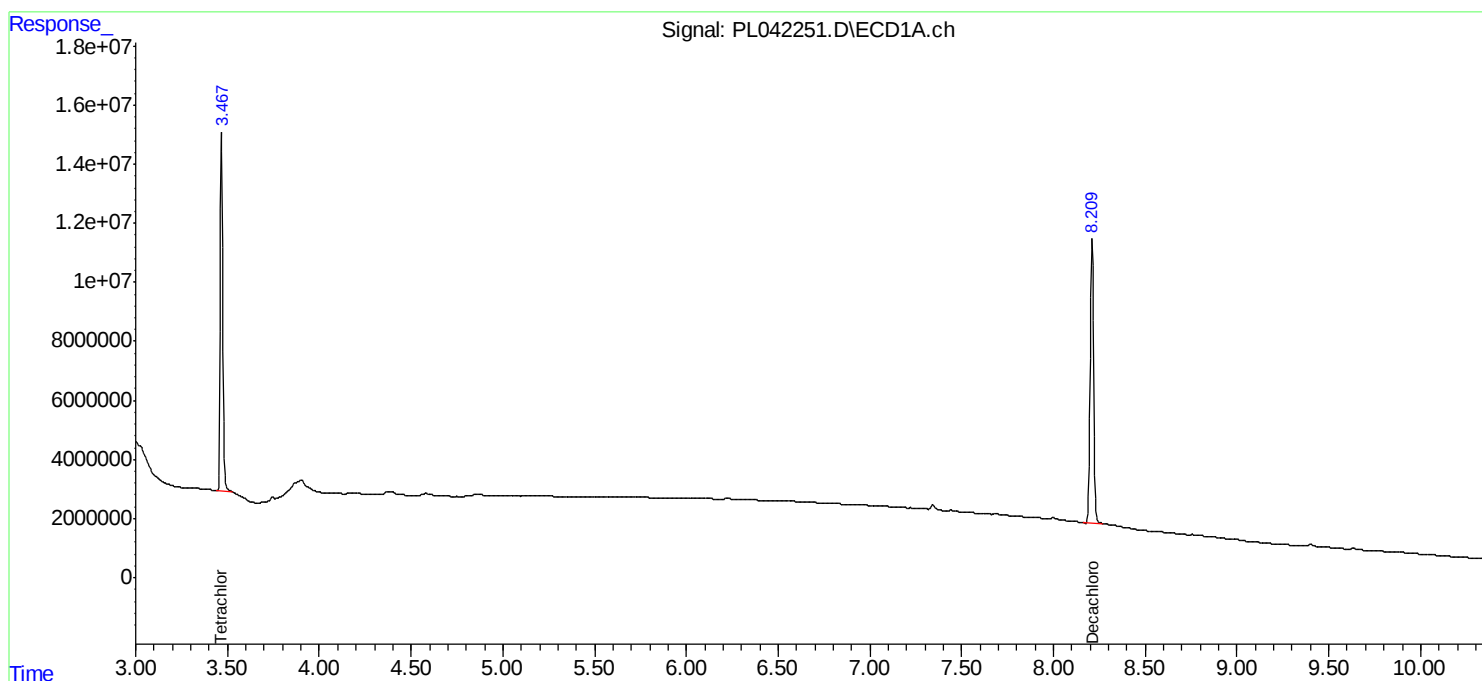


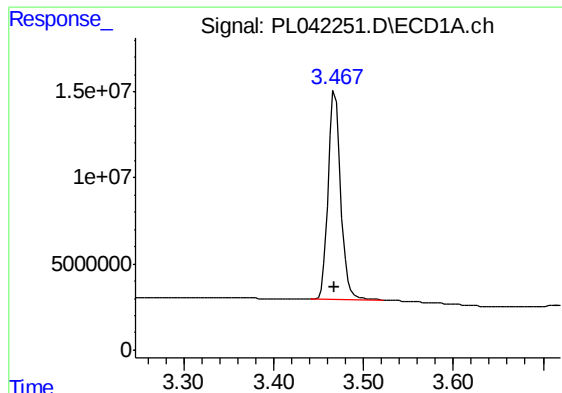

#1 Tetrachloro-m-xylene


R.T.: 3.468 min  
Delta R.T.: 0.001 min  
Response: 118313318  
Conc: 21.32 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
MIREX-MDL-BL-S-02

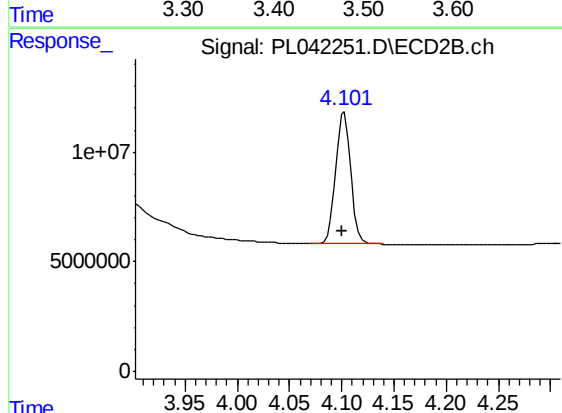


#1 Tetrachloro-m-xylene

R.T.: 4.103 min  
Delta R.T.: 0.002 min  
Response: 60724270  
Conc: 21.97 ng/ml

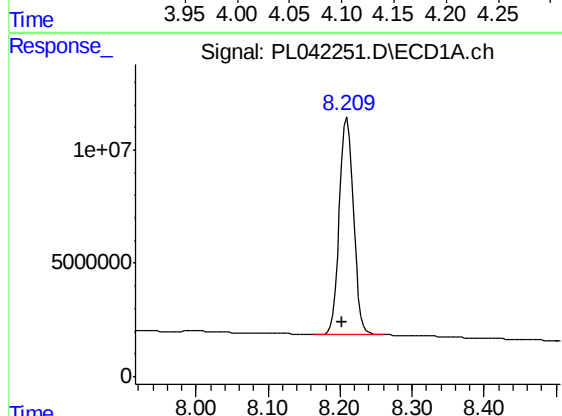

#28 Decachlorobiphenyl

R.T.: 8.210 min  
Delta R.T.: 0.006 min  
Response: 130816957  
Conc: 21.14 ng/ml

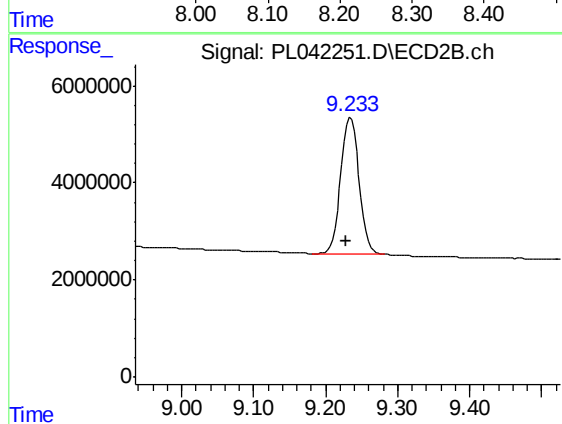

#28 Decachlorobiphenyl

R.T.: 9.235 min  
Delta R.T.: 0.007 min  
Response: 49988930  
Conc: 21.00 ng/ml