

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
 Data File : PL042255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2018 13:15
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-04
 Misc : FOR MIREX
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 14:11:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	91672119	48525640	16.516	17.554
28)	SA Decachlor...	8.210	9.236	108.5E6	42120160	17.530	17.694
Target Compounds							
22)	Mirex	7.342	8.325	5661185	1797323	0.993	0.964m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
Data File : PL042255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2018 13:15
Operator : AJ\SJ
Sample : MIREX-MDL-W-04
Misc : FOR MIREX
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 14:11:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

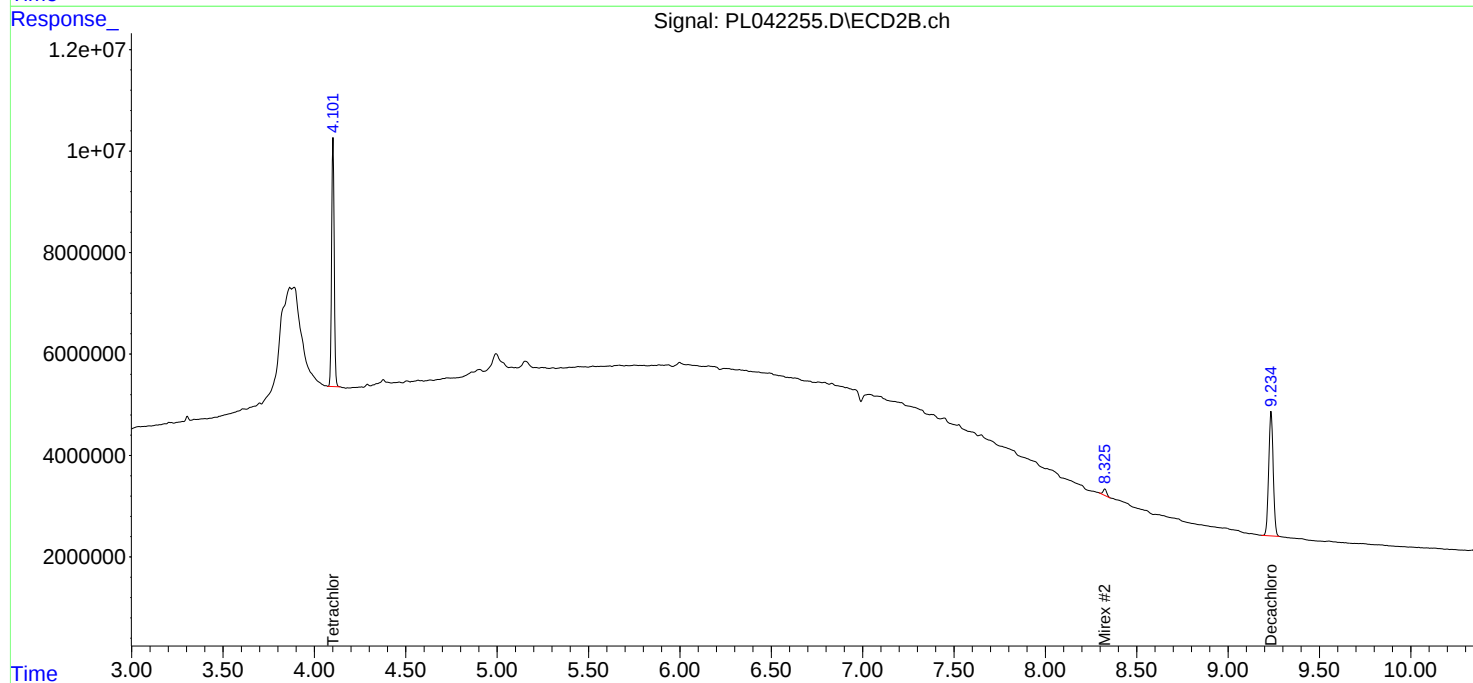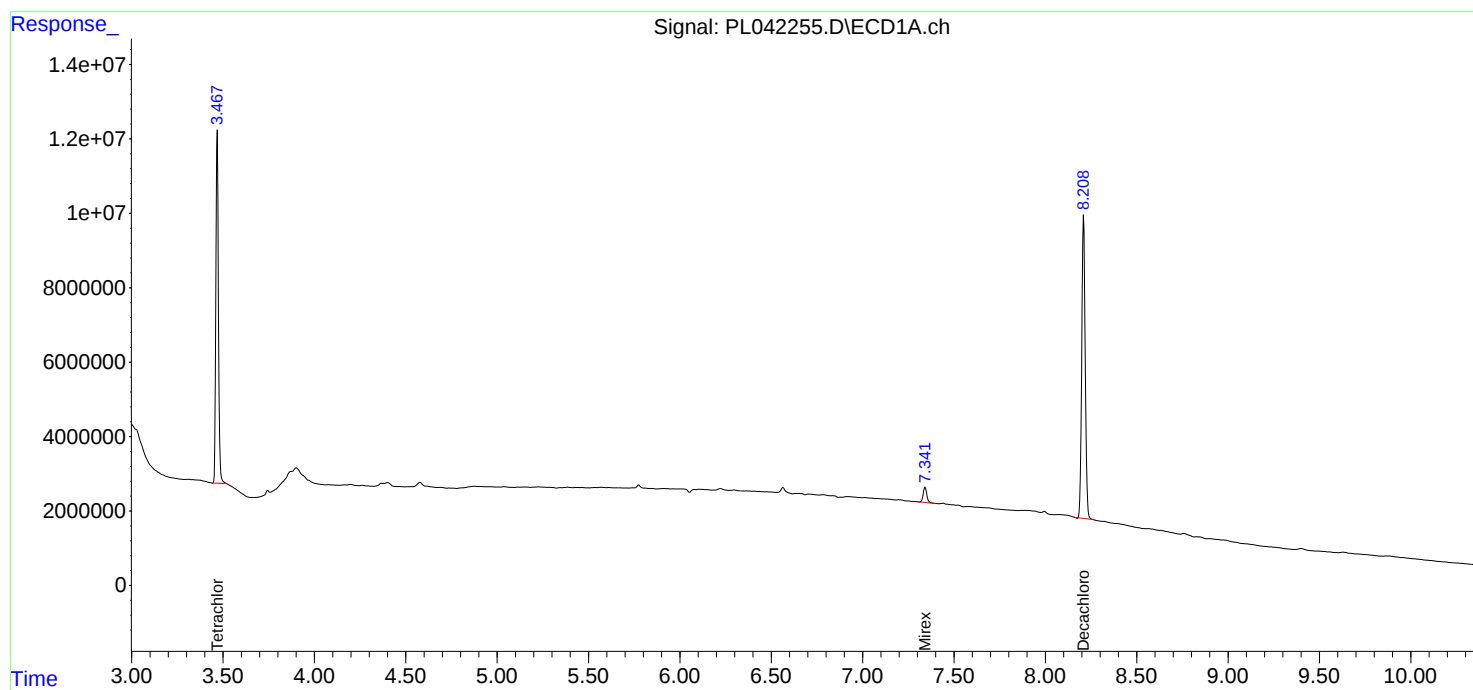


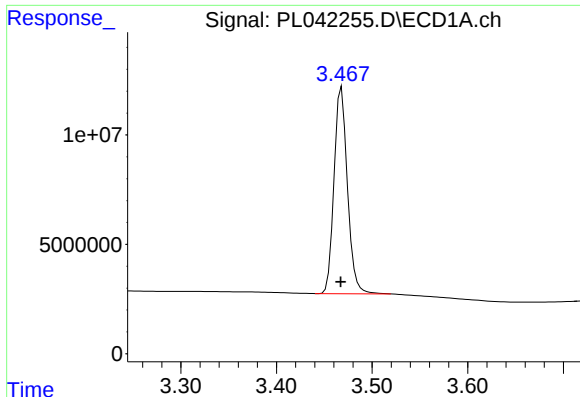

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 91672119
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-04

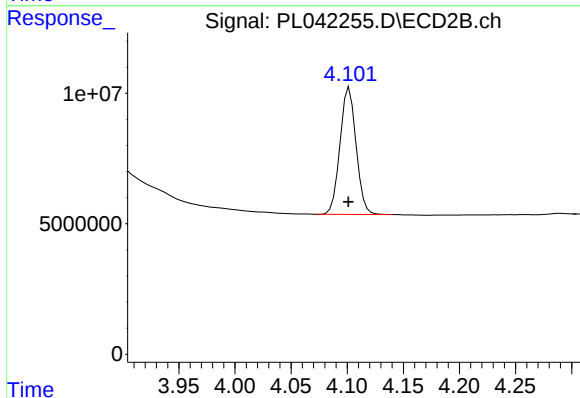


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.001 min
Response: 48525640
Conc: 17.55 ng/ml

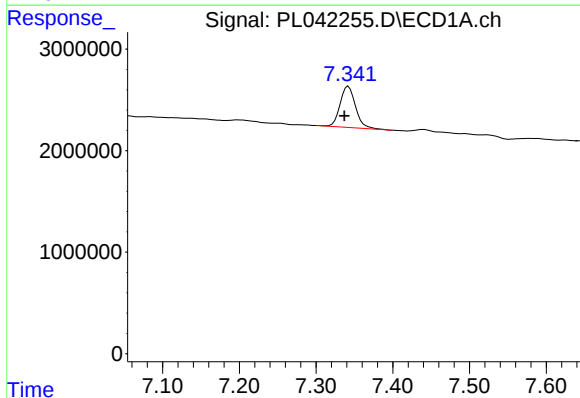


#22 Mirex

R.T.: 7.342 min
Delta R.T.: 0.005 min
Response: 5661185
Conc: 0.99 ng/ml

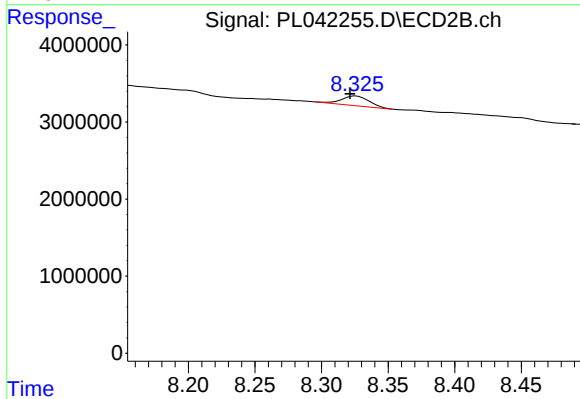

#22 Mirex


R.T.: 8.325 min
Delta R.T.: 0.003 min
Response: 1797323
Conc: 0.96 ng/ml m

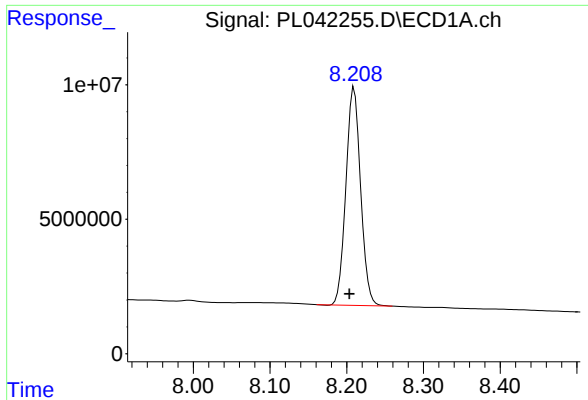

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.006 min
Response: 108481220
Conc: 17.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-04

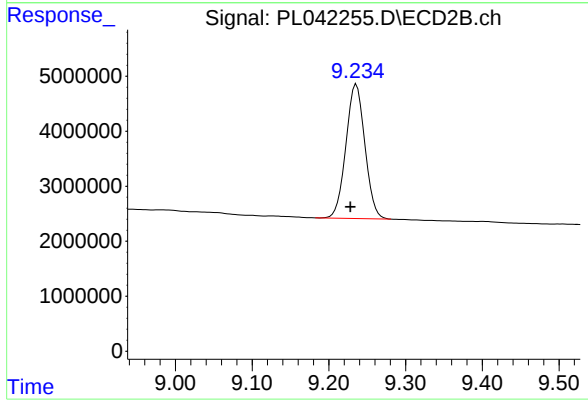

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.007 min
Response: 42120160
Conc: 17.69 ng/ml