

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
 Data File : PL042256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2018 13:29
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-05
 Misc : FOR MIREX
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-W-05

Manual Integrations
 APPROVED

Sohil
 11/16/2018 3:59:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 14:11:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	94136838	50031464	16.960	18.099
28)	SA Decachlor...	8.210	9.235	111.7E6	42898427	18.057	18.021
Target Compounds							
22)	Mirex	7.343	8.326	6309288	1644338	1.107	0.882m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111818\
Data File : PL042256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2018 13:29
Operator : AJ\SJ
Sample : MIREX-MDL-W-05
Misc : FOR MIREX
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-05


Manual Integrations
APPROVED

Sohil
11/16/2018 3:59:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 14:11:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

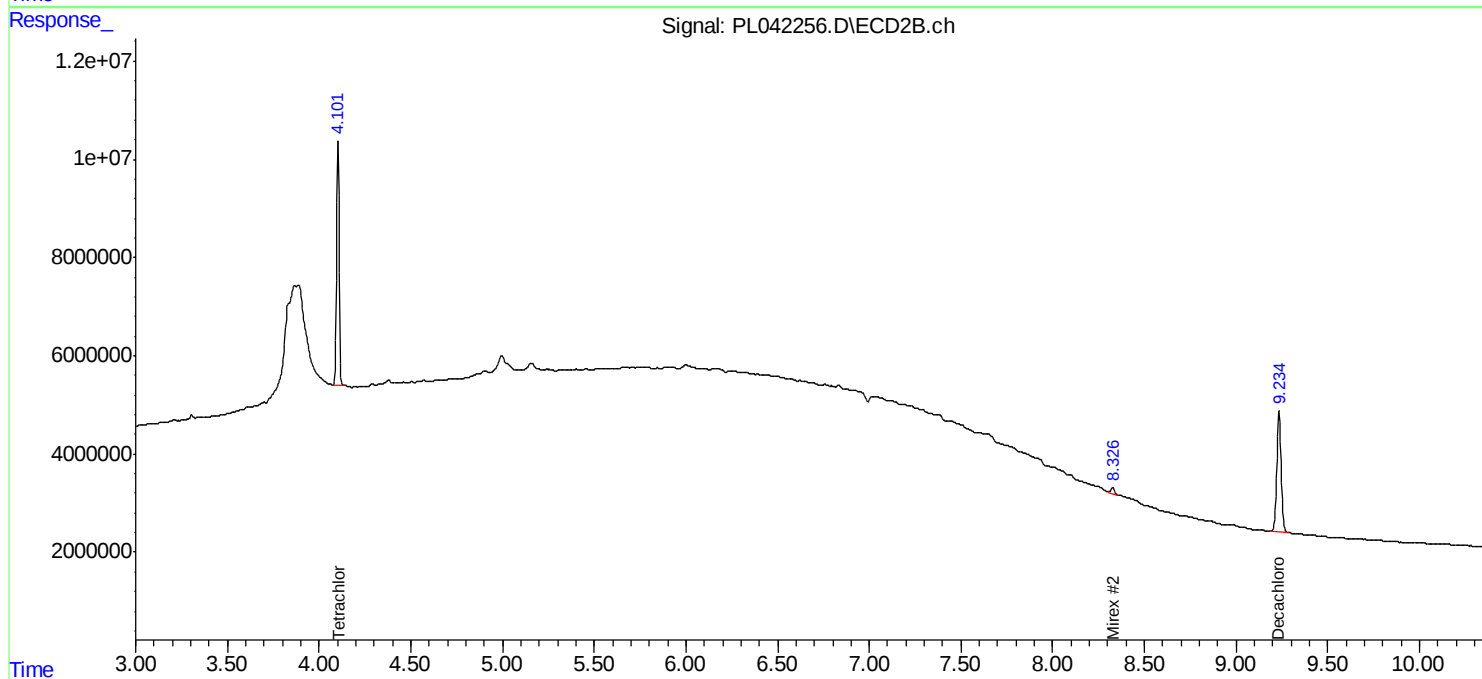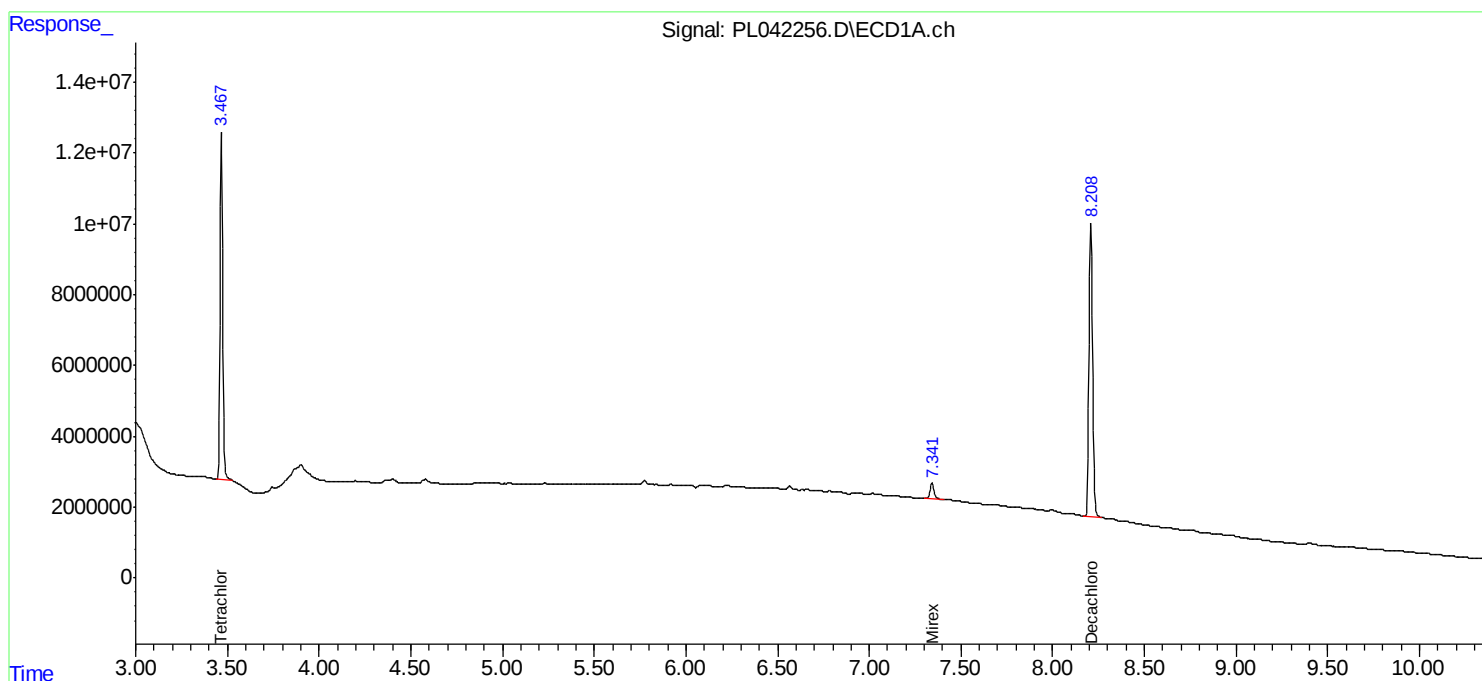

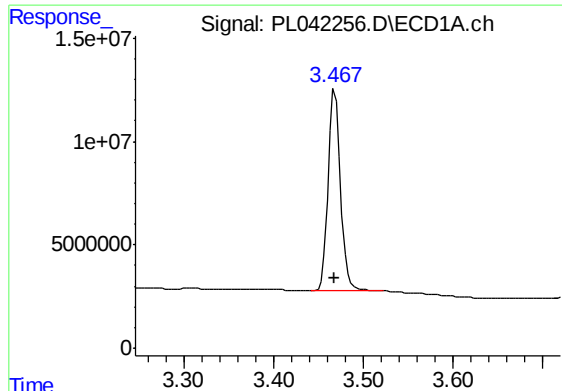


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 94136838
Conc: 16.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-05


Manual Integrations
APPROVED

Sohil
11/16/2018 3:59:32 PM

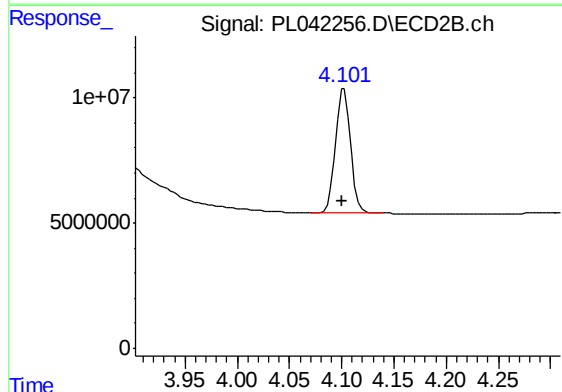


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.001 min
Response: 50031464
Conc: 18.10 ng/ml

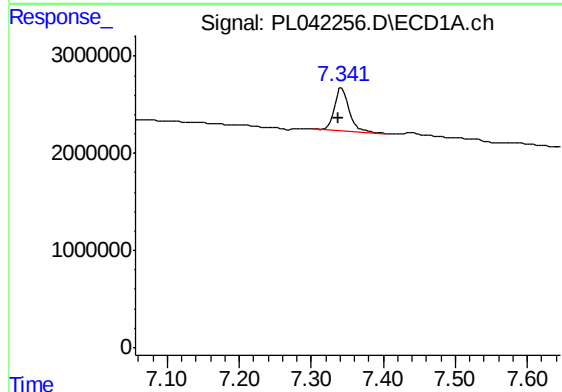


#22 Mirex

R.T.: 7.343 min
Delta R.T.: 0.006 min
Response: 6309288
Conc: 1.11 ng/ml

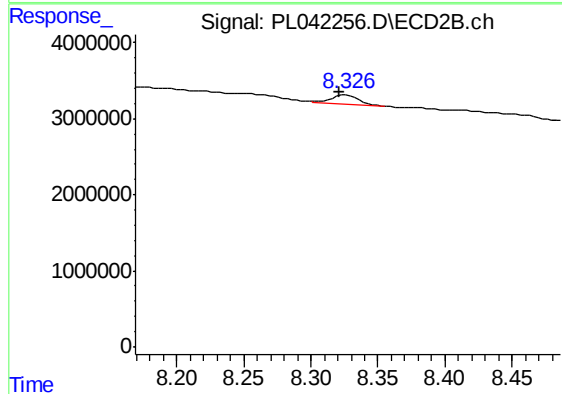

#22 Mirex

R.T.: 8.326 min
Delta R.T.: 0.005 min
Response: 1644338
Conc: 0.88 ng/ml m

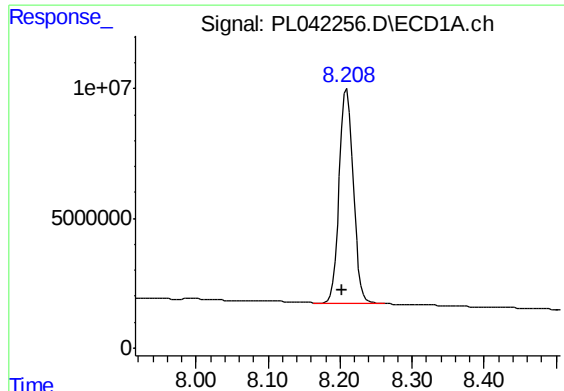


#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.006 min
Response: 111744708
Conc: 18.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-W-05

Manual Integrations
APPROVED

Sohil
11/16/2018 3:59:32 PM

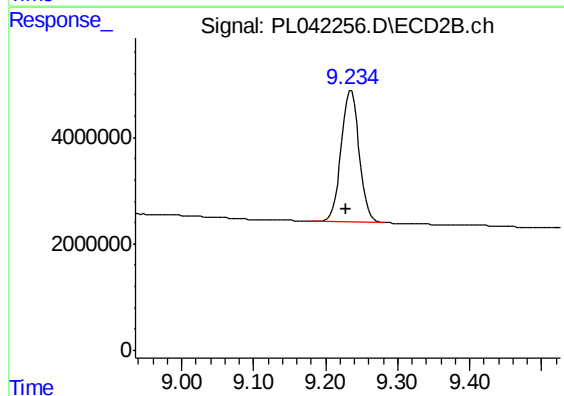

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.007 min
Response: 42898427
Conc: 18.02 ng/ml