

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
 Data File : PL054387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 15:35
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 00:41:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 00:40:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	650.1E6	123.3E6	50.000	50.000
28)	SA Decachlor...	8.323	9.125	459.9E6	125.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.422	5.041	194.2E6	41772295	500.000	500.000
24)	Chlordane-2	4.927	5.510	208.6E6	47400954	500.000	500.000
25)	Chlordane-3	5.502	6.156	615.6E6	166.6E6	500.000	500.000
26)	Chlordane-4	5.559	6.230	506.9E6	202.6E6	500.000	500.000
27)	Chlordane-5	6.401	7.035	184.4E6	36288882	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
Data File : PL054387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 15:35
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 00:41:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 00:40:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

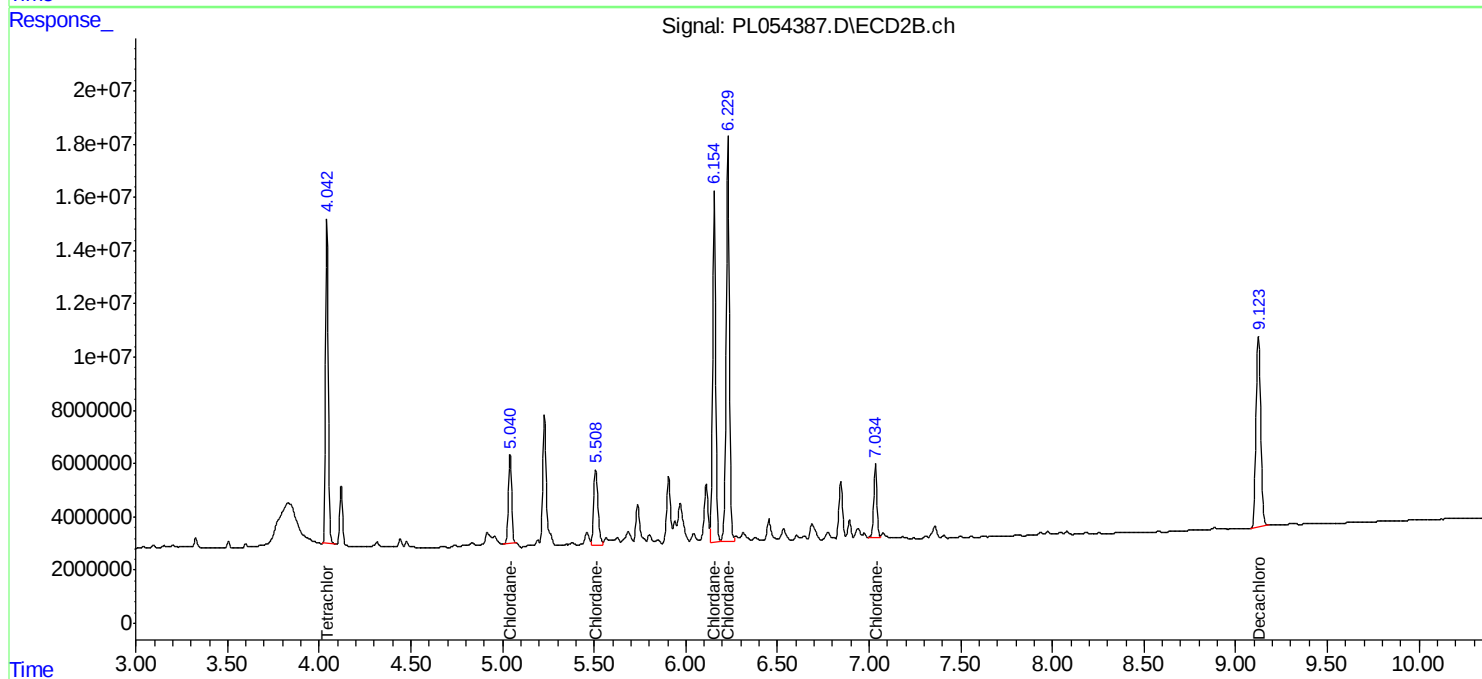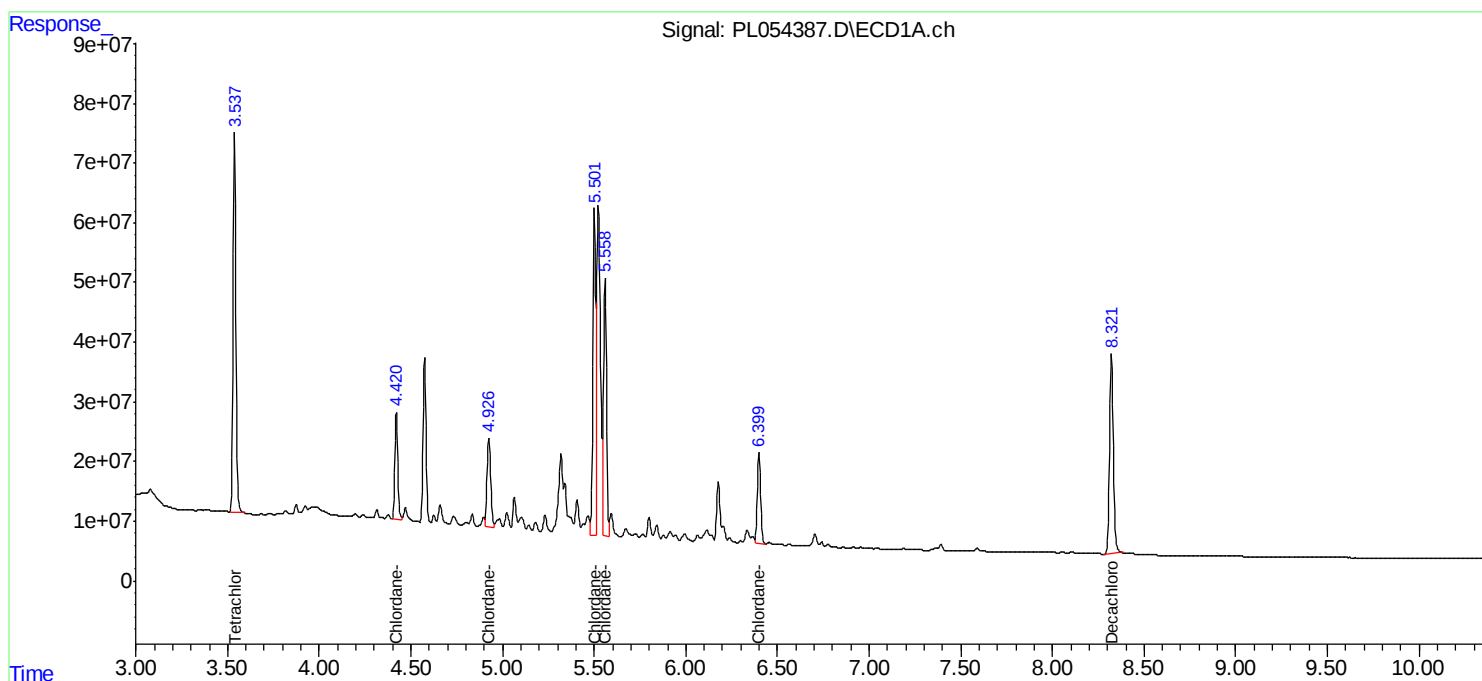


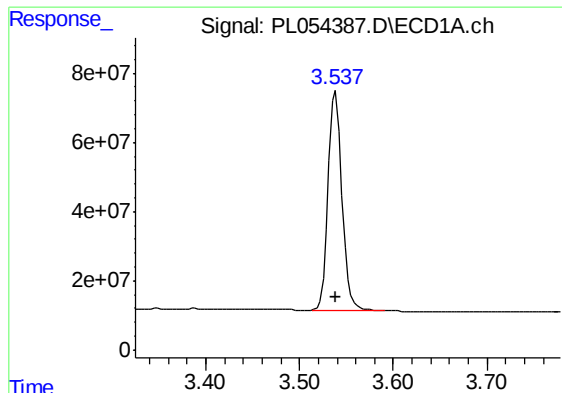

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 650050610
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

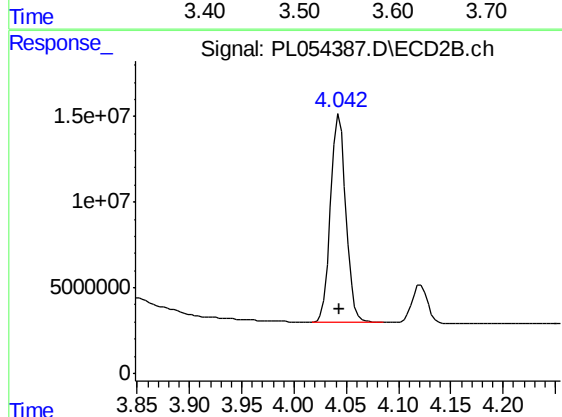


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 123307463
Conc: 50.00 ng/ml

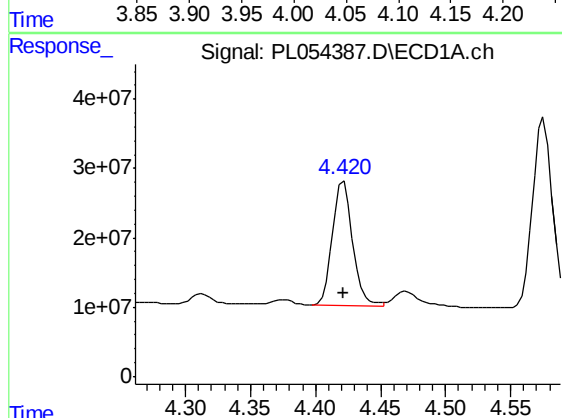


#23 Chlordane-1

R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 194202895
Conc: 500.00 ng/ml

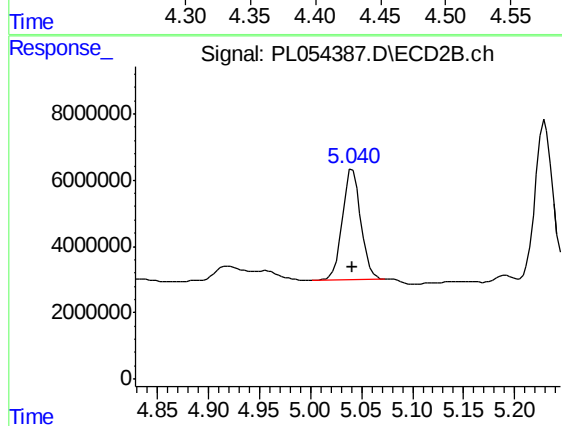

#23 Chlordane-1


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 41772295
Conc: 500.00 ng/ml

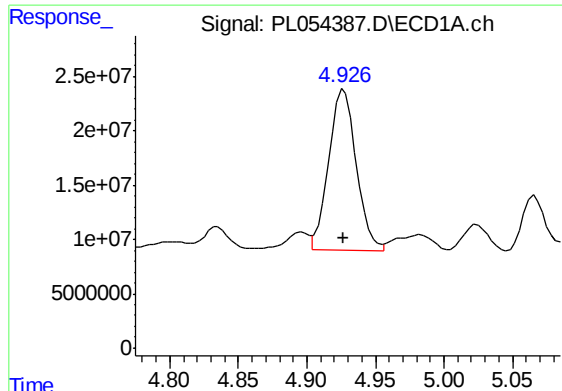

#24 Chlordane-2


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 208555735
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

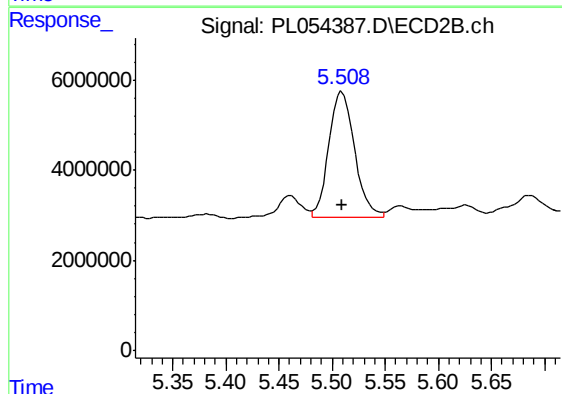


#24 Chlordane-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 47400954
Conc: 500.00 ng/ml

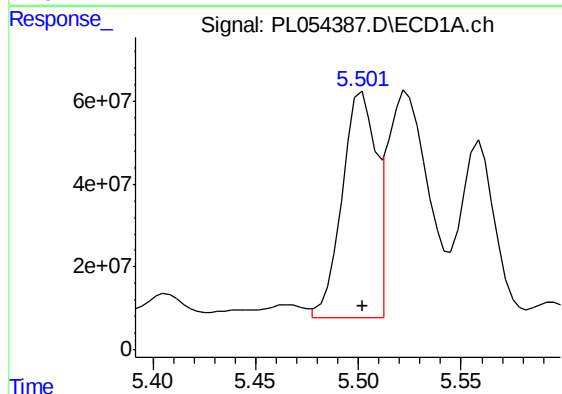


#25 Chlordane-3

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 615603066
Conc: 500.00 ng/ml

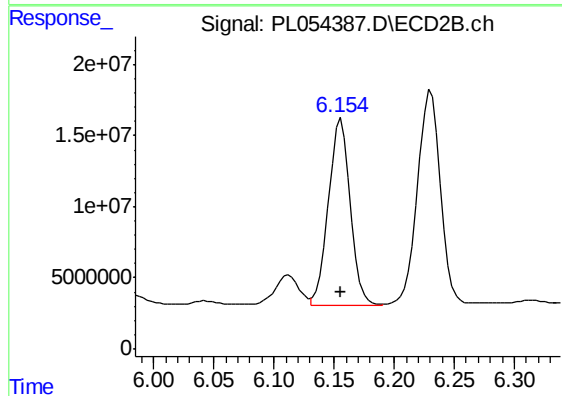

#25 Chlordane-3


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 166582918
Conc: 500.00 ng/ml

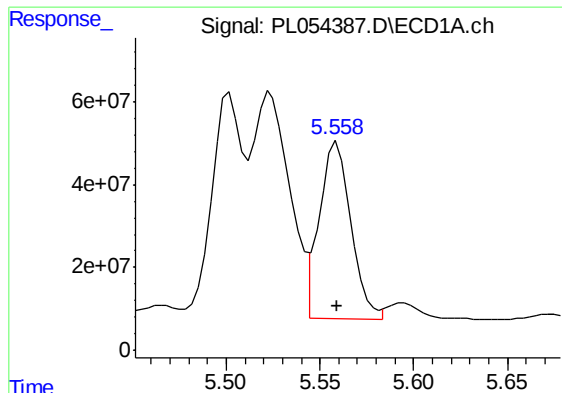

#26 Chlordane-4


R.T.: 5.559 min
Delta R.T.: 0.000 min
Response: 506892595
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

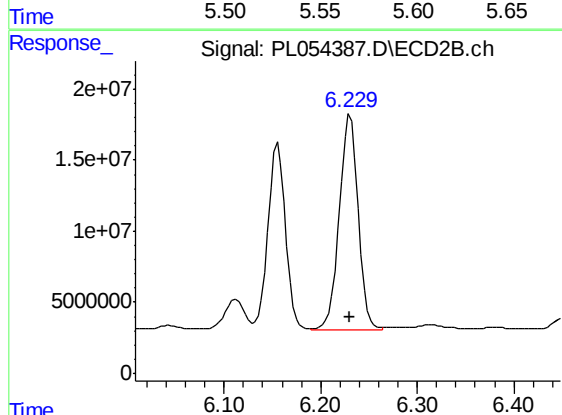


#26 Chlordane-4

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 202556471
Conc: 500.00 ng/ml

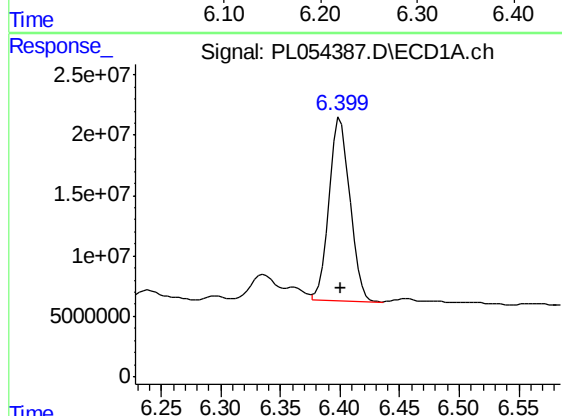


#27 Chlordane-5

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 184418115
Conc: 500.00 ng/ml

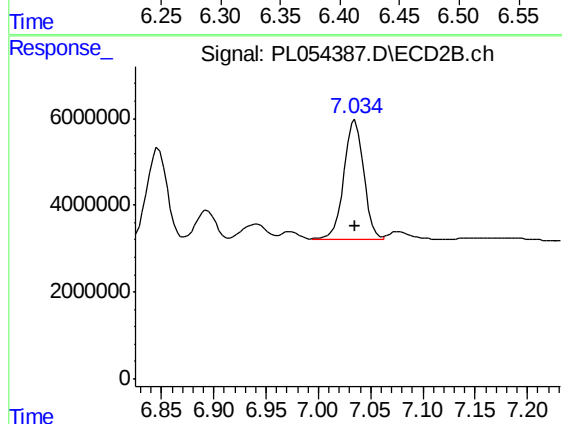

#27 Chlordane-5


R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 36288882
Conc: 500.00 ng/ml

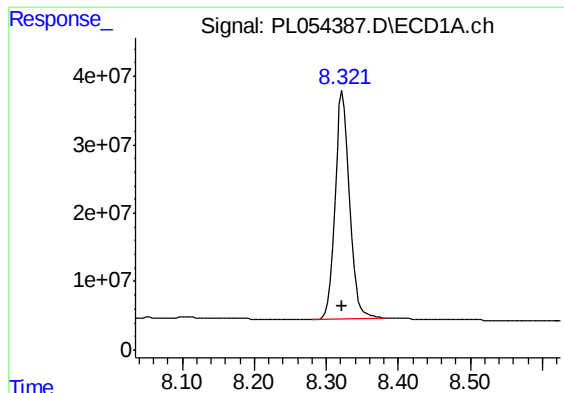

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 459861848
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

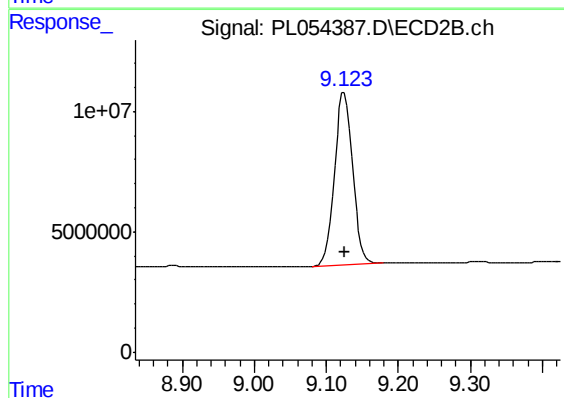

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 125121962
Conc: 50.00 ng/ml