

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
 Data File : PL054402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 19:45
 Operator : SG\AJ
 Sample : K5904-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 1-(6-8)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:53:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.044	249.4E6	60292568	23.990	24.748
28)	SA Decachlor...	8.324	9.127	215.1E6	58770313	24.298	24.307
Target Compounds							
4)	MA Heptachlor	4.559f	0.000	30871568	0	2.016	N.D. #
6)	B beta-BHC	4.536f	0.000	10033787	0	1.561	N.D. #
8)	B Heptachlo...	0.000	5.915	0	1495591	N.D.	0.629 #
9)	A Endosulfan I	0.000	6.278	0	17033274	N.D.	7.266 #
11)	B alpha-Chl...	5.551	0.000	122.4E6	0	9.755	N.D. #
21)	B Endrin ke...	0.000	7.775	0	1711457	N.D.	0.756 #
23)	Chlordane-1	4.440f	0.000	14322074	0	36.874	N.D. #
26)	Chlordane-4	5.551	0.000	122.4E6	0	120.755	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
Data File : PL054402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 19:45
Operator : SG\AJ
Sample : K5904-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:53:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

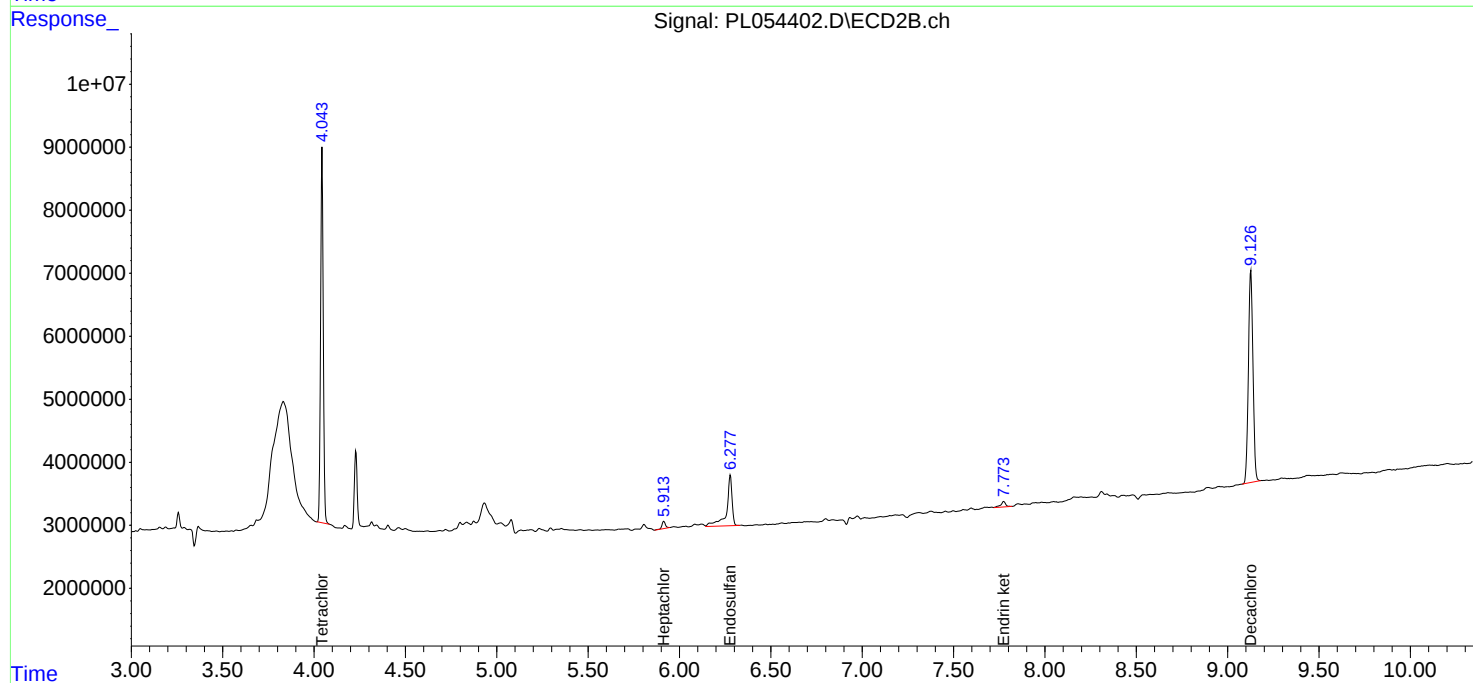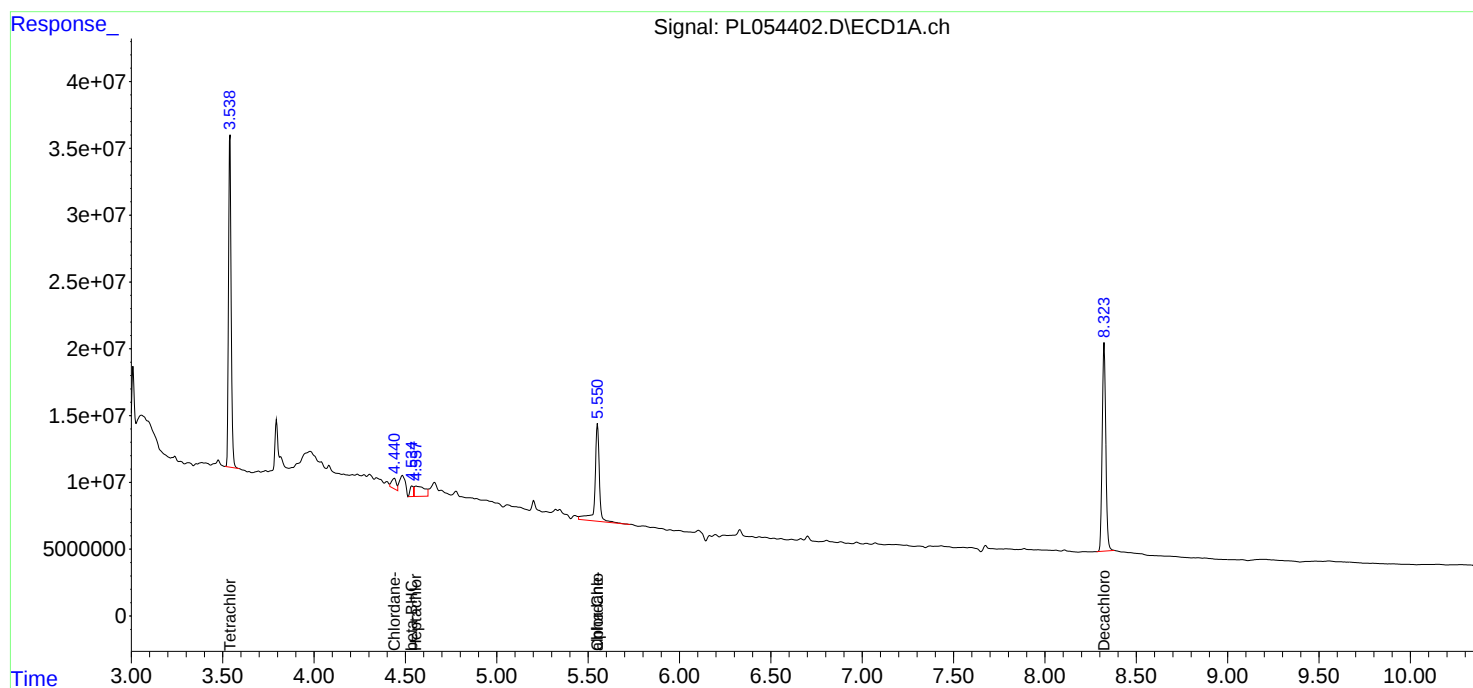


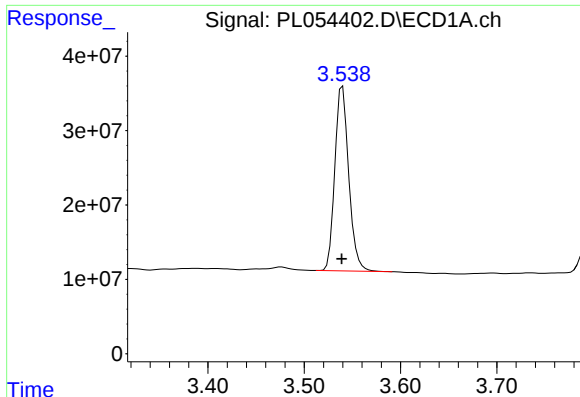

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 249431894
Conc: 23.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

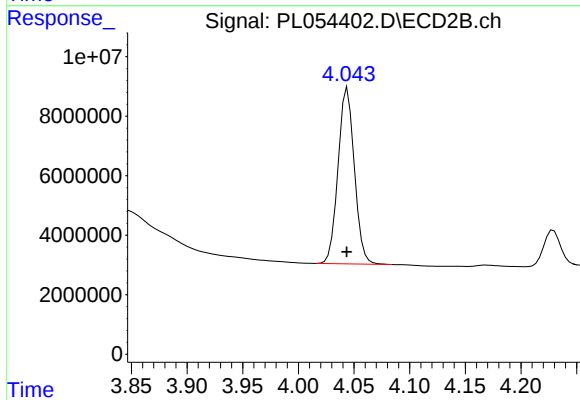


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 60292568
Conc: 24.75 ng/ml

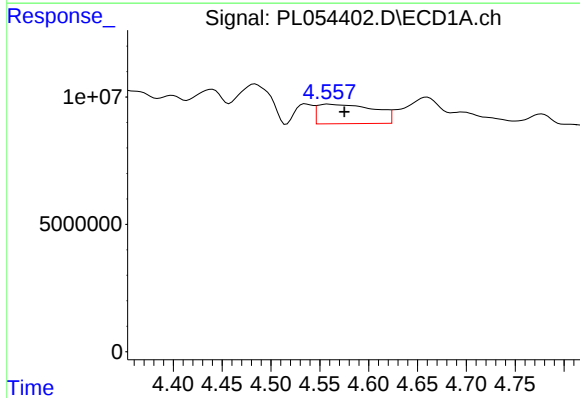


#4 Heptachlor

R.T.: 4.559 min
Delta R.T.: -0.016 min
Response: 30871568
Conc: 2.02 ng/ml

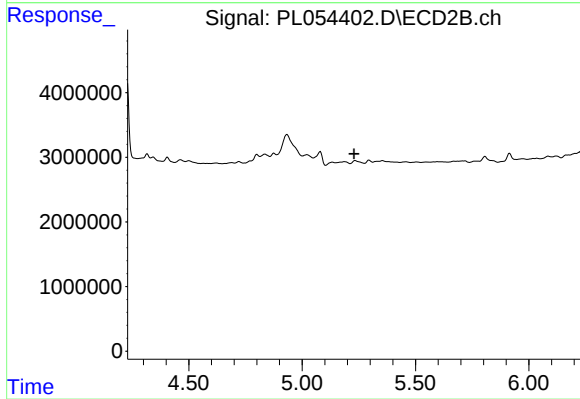

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.230 min
Response: 0
Conc: N.D.

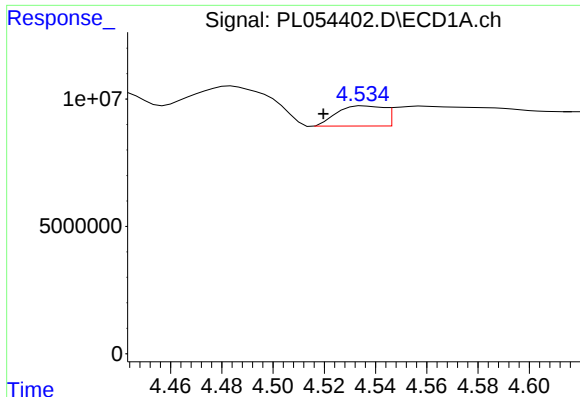

#6 beta-BHC


R.T.: 4.536 min
Delta R.T.: 0.016 min
Response: 10033787
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

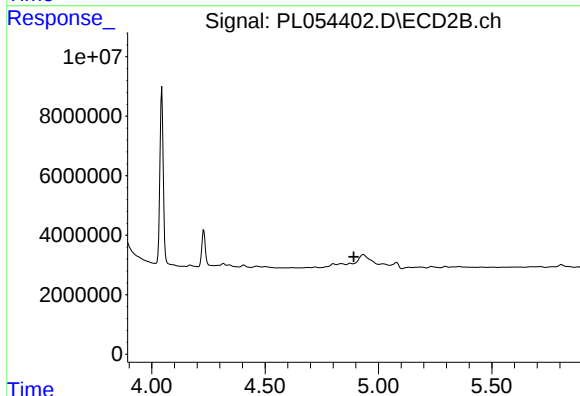


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

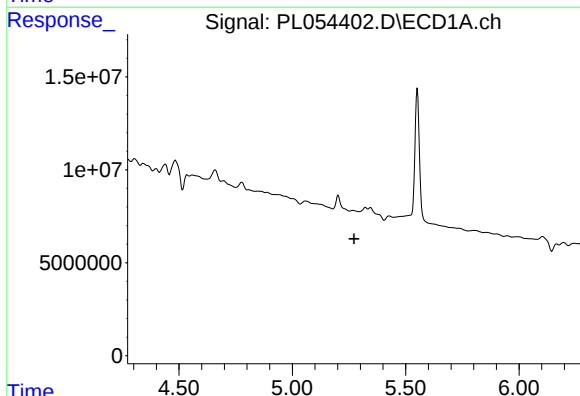


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

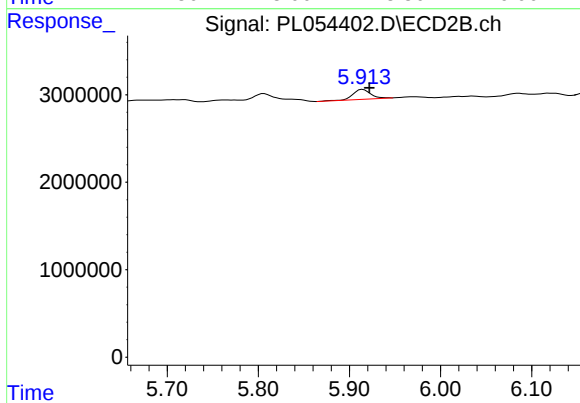

#8 Heptachlor epoxide


R.T.: 5.915 min
Delta R.T.: -0.007 min
Response: 1495591
Conc: 0.63 ng/ml

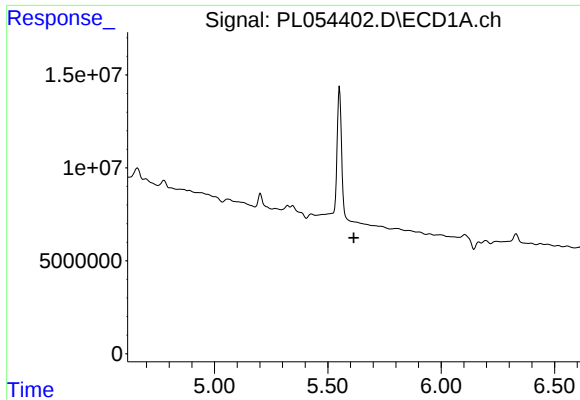

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.615 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

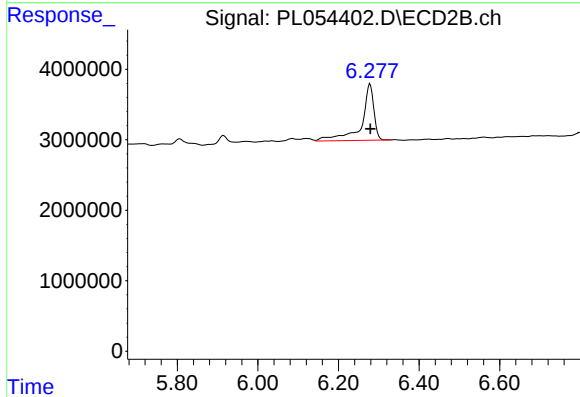


#9 Endosulfan I

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 17033274
Conc: 7.27 ng/ml

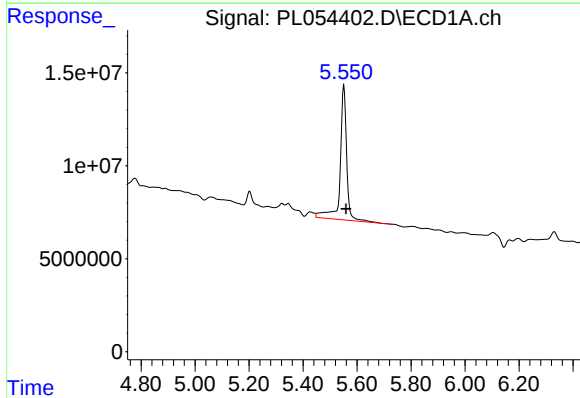


#11 alpha-Chlordane

R.T.: 5.551 min
Delta R.T.: -0.008 min
Response: 122419714
Conc: 9.75 ng/ml

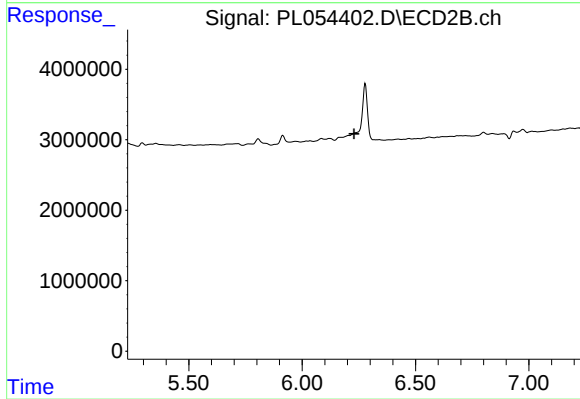

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

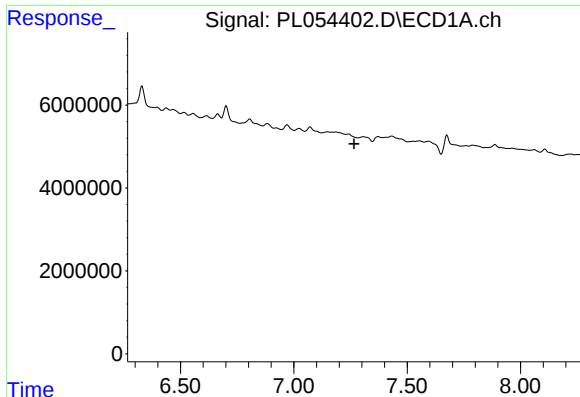

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

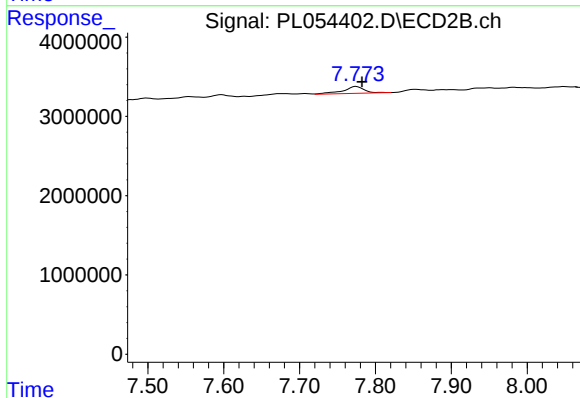


#21 Endrin ketone

R.T.: 7.775 min
Delta R.T.: -0.008 min
Response: 1711457
Conc: 0.76 ng/ml

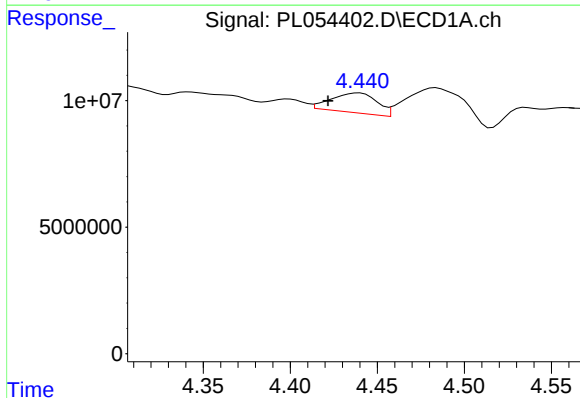


#23 Chlordane-1

R.T.: 4.440 min
Delta R.T.: 0.018 min
Response: 14322074
Conc: 36.87 ng/ml

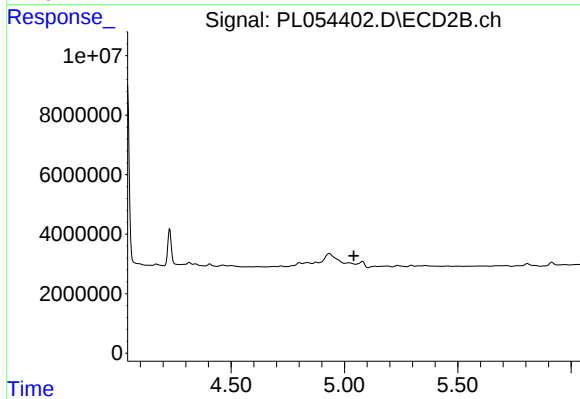

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.041 min
Response: 0
Conc: N.D.

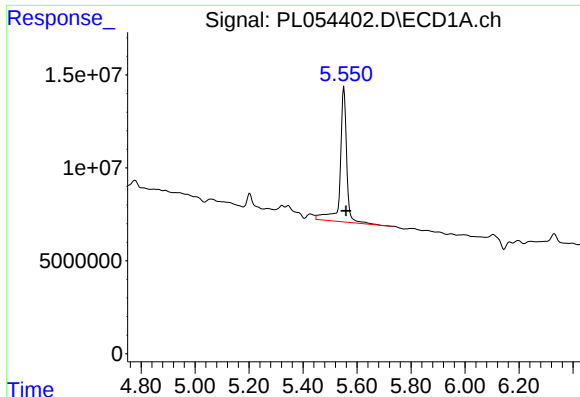

#26 Chlordane-4


R.T.: 5.551 min
Delta R.T.: -0.008 min
Response: 122419714
Conc: 120.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-(6-8)

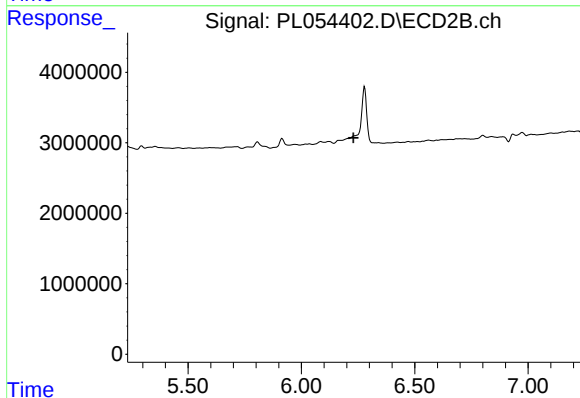


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.230 min
Response: 0
Conc: N.D.

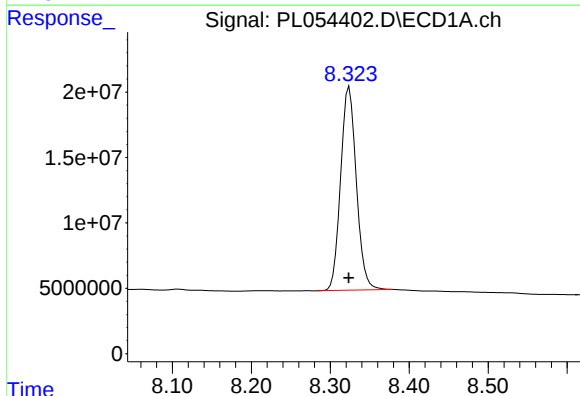

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: 0.000 min
Response: 215062673
Conc: 24.30 ng/ml

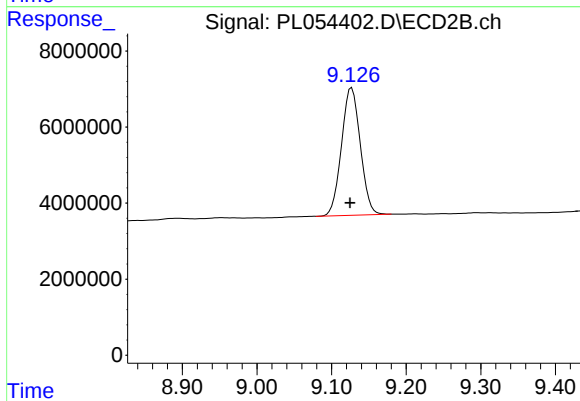

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.002 min
Response: 58770313
Conc: 24.31 ng/ml