

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
 Data File : PL054416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 23:02
 Operator : SG\AJ
 Sample : K5904-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 12-(4-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:56:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.044	186.4E6	45610809	17.926	18.722
28)	SA Decachlor...	8.324	9.126	98667294	27271923	11.148	11.280
Target Compounds							
2)	A alpha-BHC	3.976	0.000	12295574	0	0.722	N.D. #
8)	B Heptachlo...	0.000	5.914	0	1705051	N.D.	0.717 #
9)	A Endosulfan I	5.635f	6.279	10551704	3793169	0.891	1.618 #
11)	B alpha-Chl...	5.551	0.000	43447873	0	3.462	N.D. #
21)	B Endrin ke...	0.000	7.775	0	1583567	N.D.	0.699 #
22)	Mirex	7.437f	0.000	3315704	0	0.435	N.D. #
23)	Chlordane-1	4.444f	0.000	4832823	0	12.443	N.D. #
26)	Chlordane-4	5.551	0.000	43447873	0	42.857	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
Data File : PL054416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 23:02
Operator : SG\AJ
Sample : K5904-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

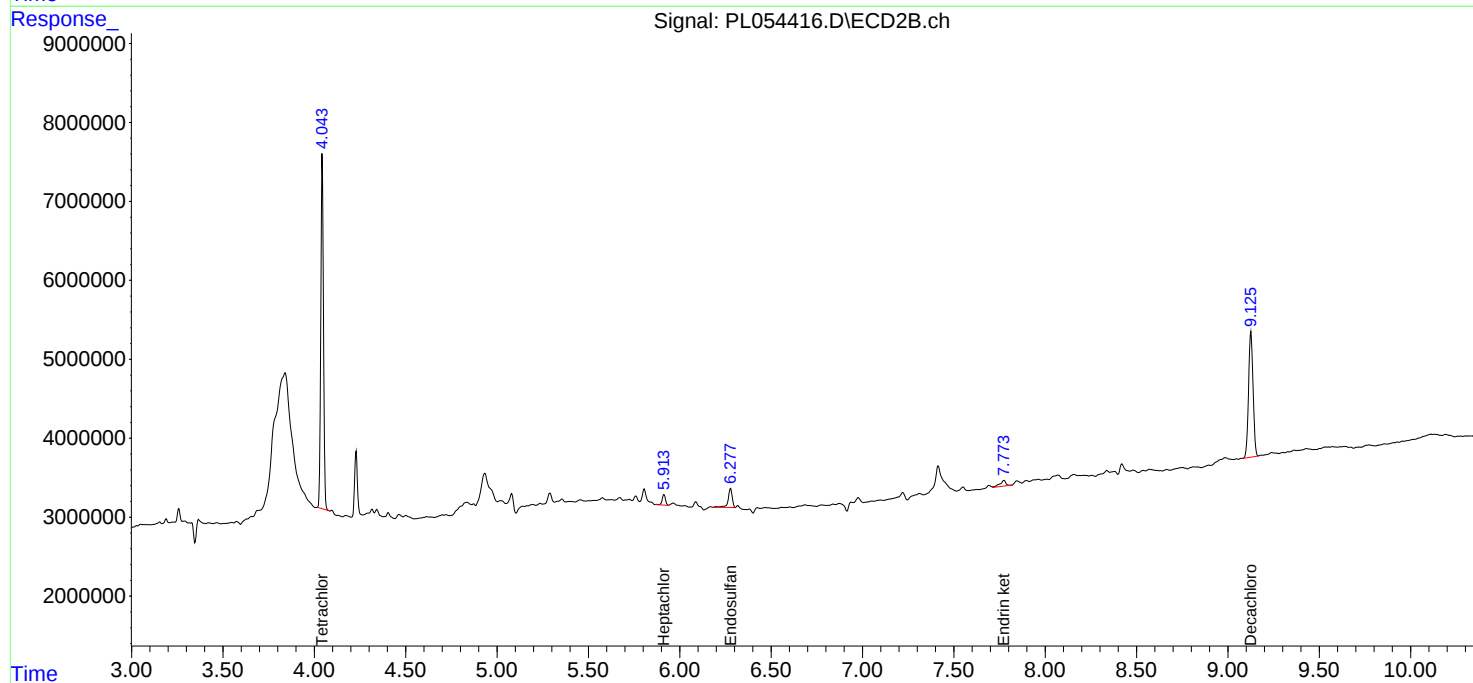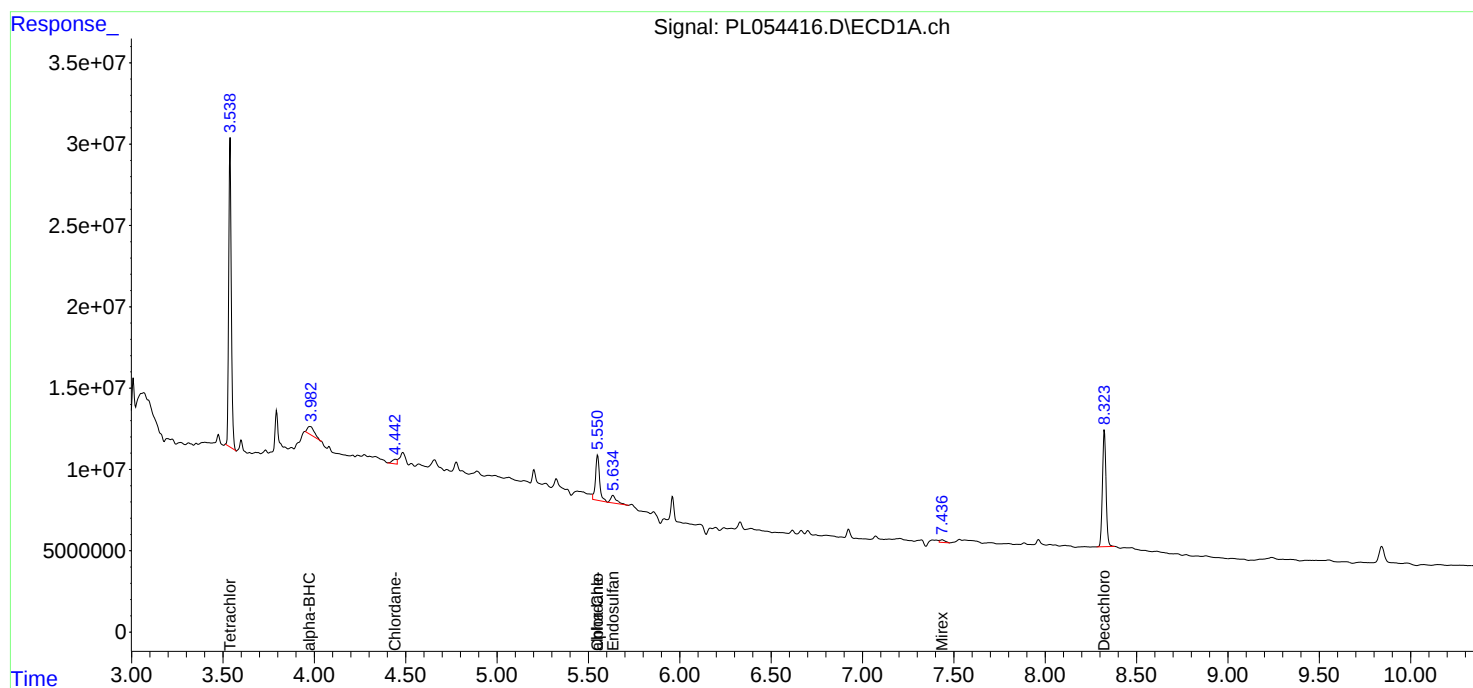


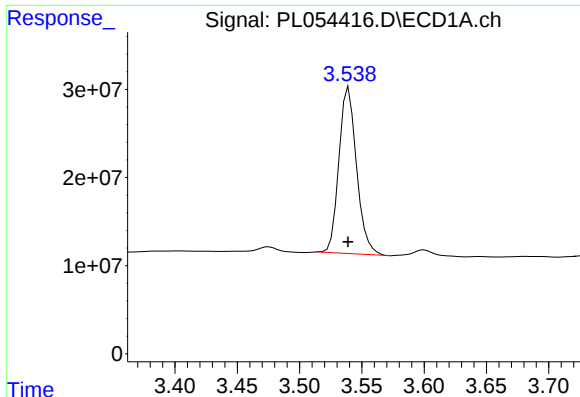

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 186380812
Conc: 17.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

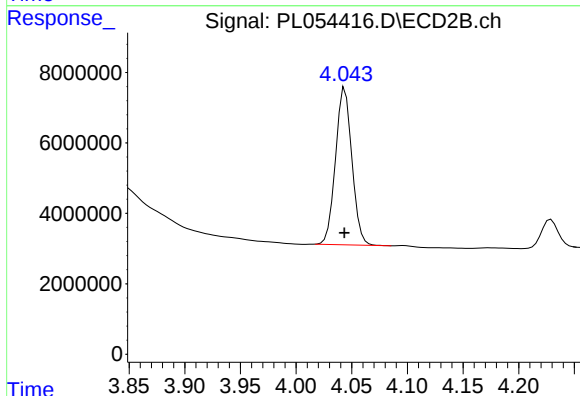


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 45610809
Conc: 18.72 ng/ml

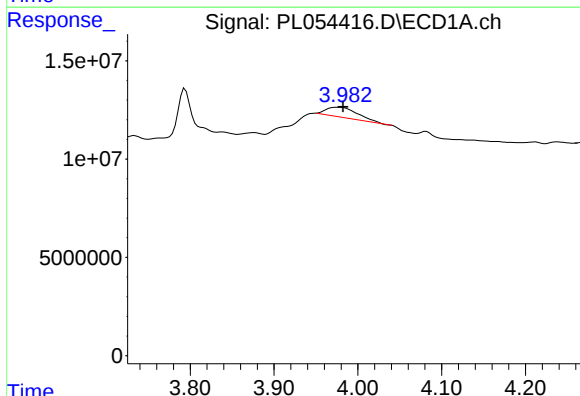


#2 alpha-BHC

R.T.: 3.976 min
Delta R.T.: -0.006 min
Response: 12295574
Conc: 0.72 ng/ml

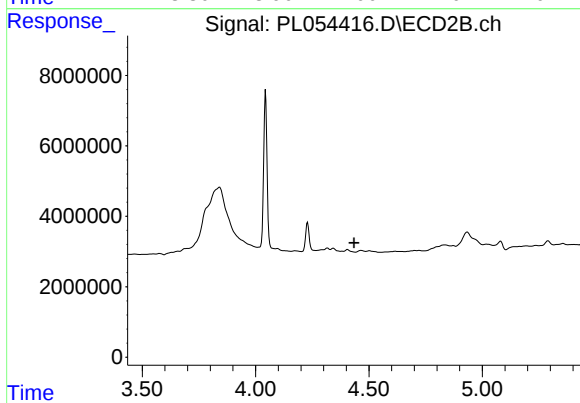

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.435 min
Response: 0
Conc: N.D.

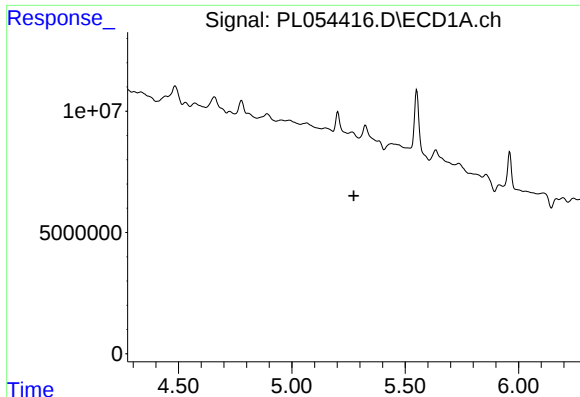

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

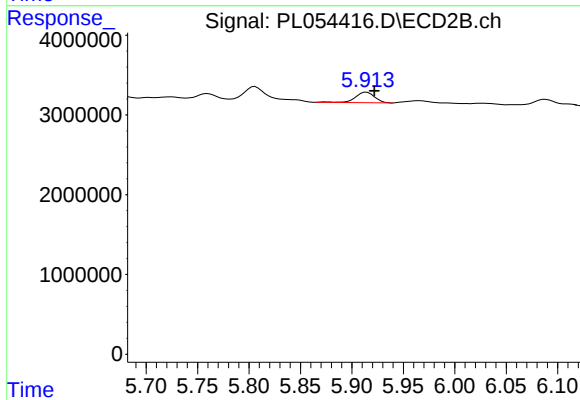


#8 Heptachlor epoxide

R.T.: 5.914 min
Delta R.T.: -0.008 min
Response: 1705051
Conc: 0.72 ng/ml

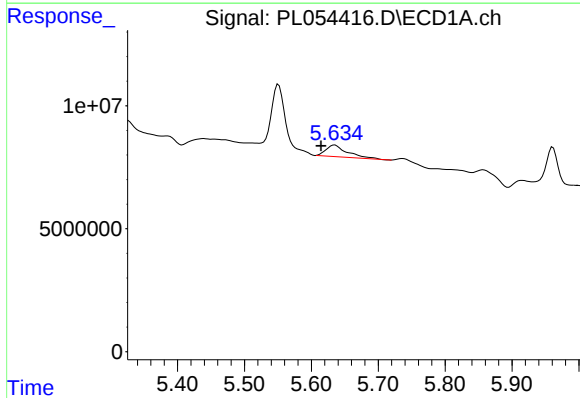


#9 Endosulfan I

R.T.: 5.635 min
Delta R.T.: 0.020 min
Response: 10551704
Conc: 0.89 ng/ml

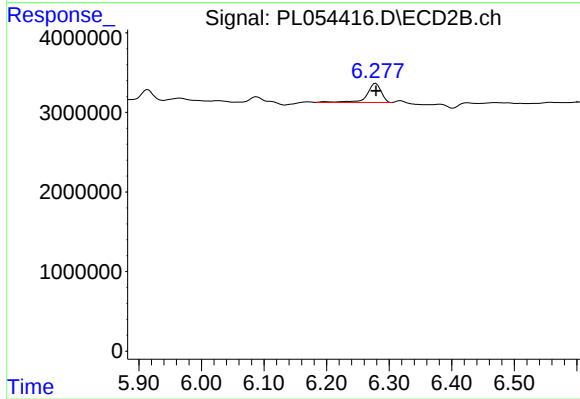

#9 Endosulfan I


R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 3793169
Conc: 1.62 ng/ml

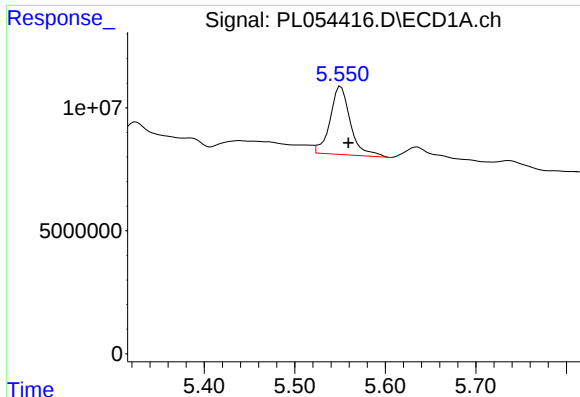

#11 alpha-Chlordane


R.T.: 5.551 min
Delta R.T.: -0.008 min
Response: 43447873
Conc: 3.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

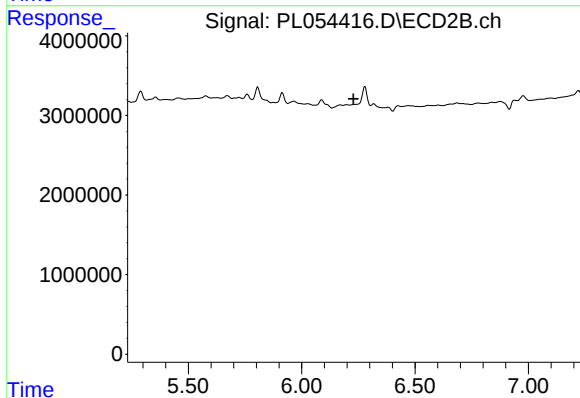


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.229 min
Response: 0
Conc: N.D.

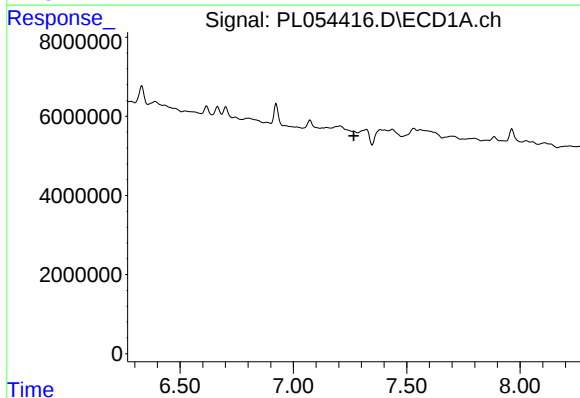


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.267 min
Response: 0
Conc: N.D.

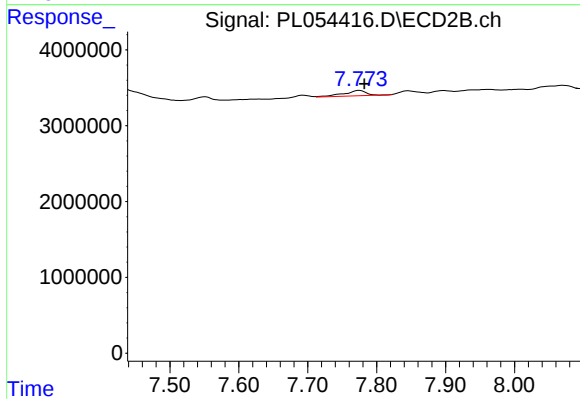

#21 Endrin ketone


R.T.: 7.775 min
Delta R.T.: -0.007 min
Response: 1583567
Conc: 0.70 ng/ml

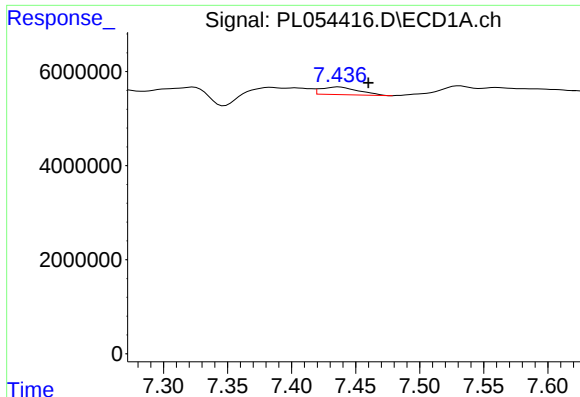

#22 Mirex


R.T.: 7.437 min
Delta R.T.: -0.023 min
Response: 3315704
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

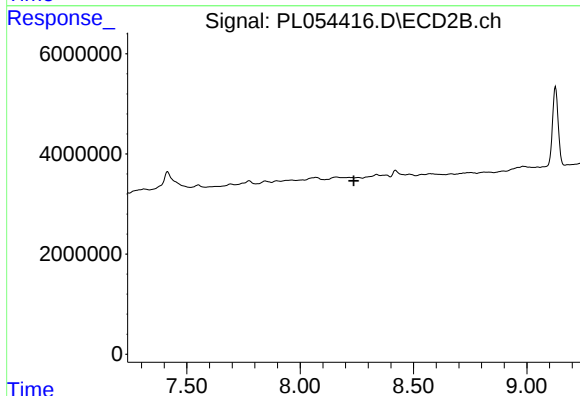


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

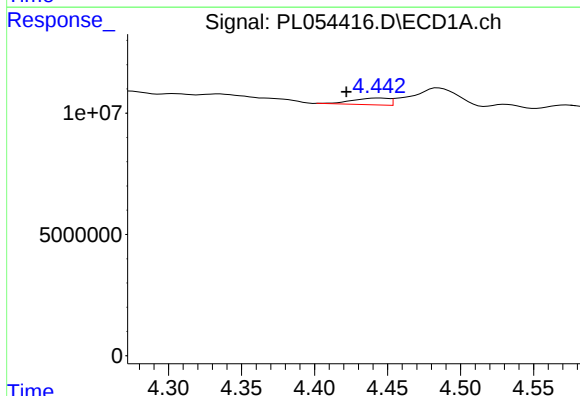


#23 Chlordane-1

R.T.: 4.444 min
Delta R.T.: 0.022 min
Response: 4832823
Conc: 12.44 ng/ml

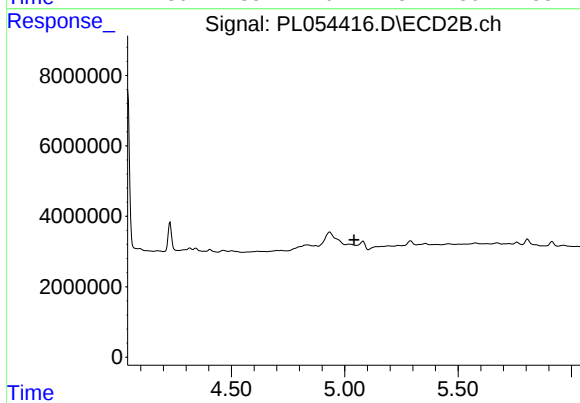

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.041 min
Response: 0
Conc: N.D.

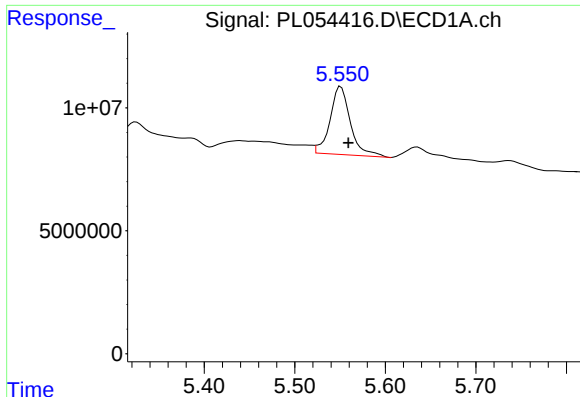

#26 Chlordane-4


R.T.: 5.551 min
Delta R.T.: -0.008 min
Response: 43447873
Conc: 42.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
12-(4-6)

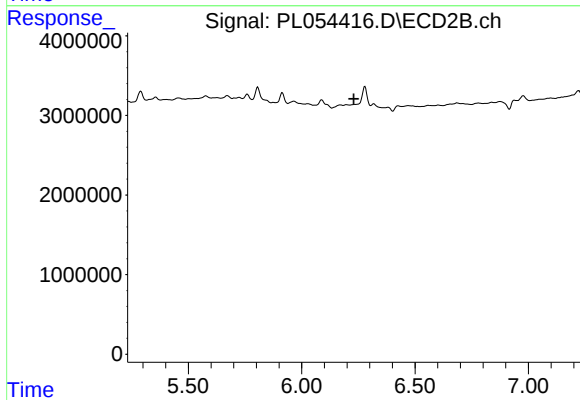


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.230 min
Response: 0
Conc: N.D.

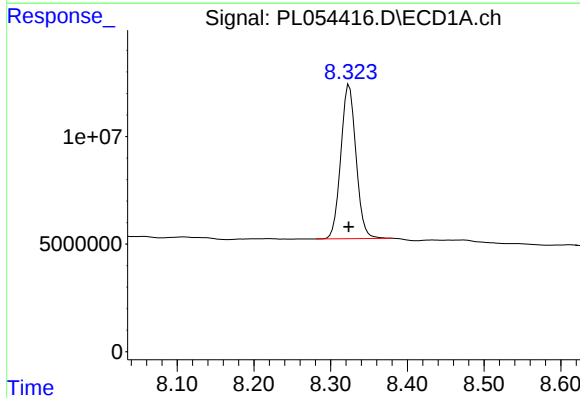

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: 0.000 min
Response: 98667294
Conc: 11.15 ng/ml

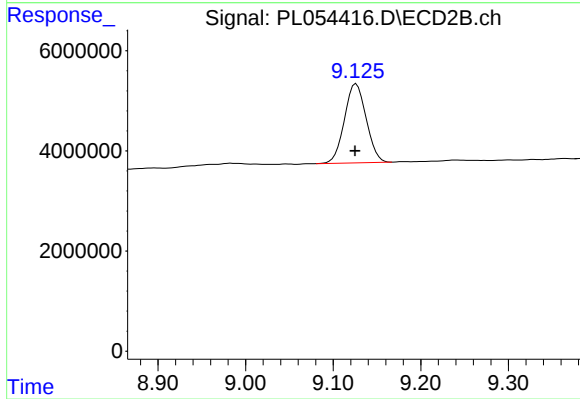

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.001 min
Response: 27271923
Conc: 11.28 ng/ml