

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
 Data File : PL054436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 04:41
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 06:00:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	4.044	298.1E6	71495422	28.669	29.347
28)	SA Decachlor...	8.324	9.126	242.8E6	69996181	27.428	28.950
Target Compounds							
2)	A alpha-BHC	3.977	0.000	12110309	0	0.711	N.D. #
23)	Chlordane-1	4.450f	0.000	4821441	0	12.413	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
Data File : PL054436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 04:41
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:00:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

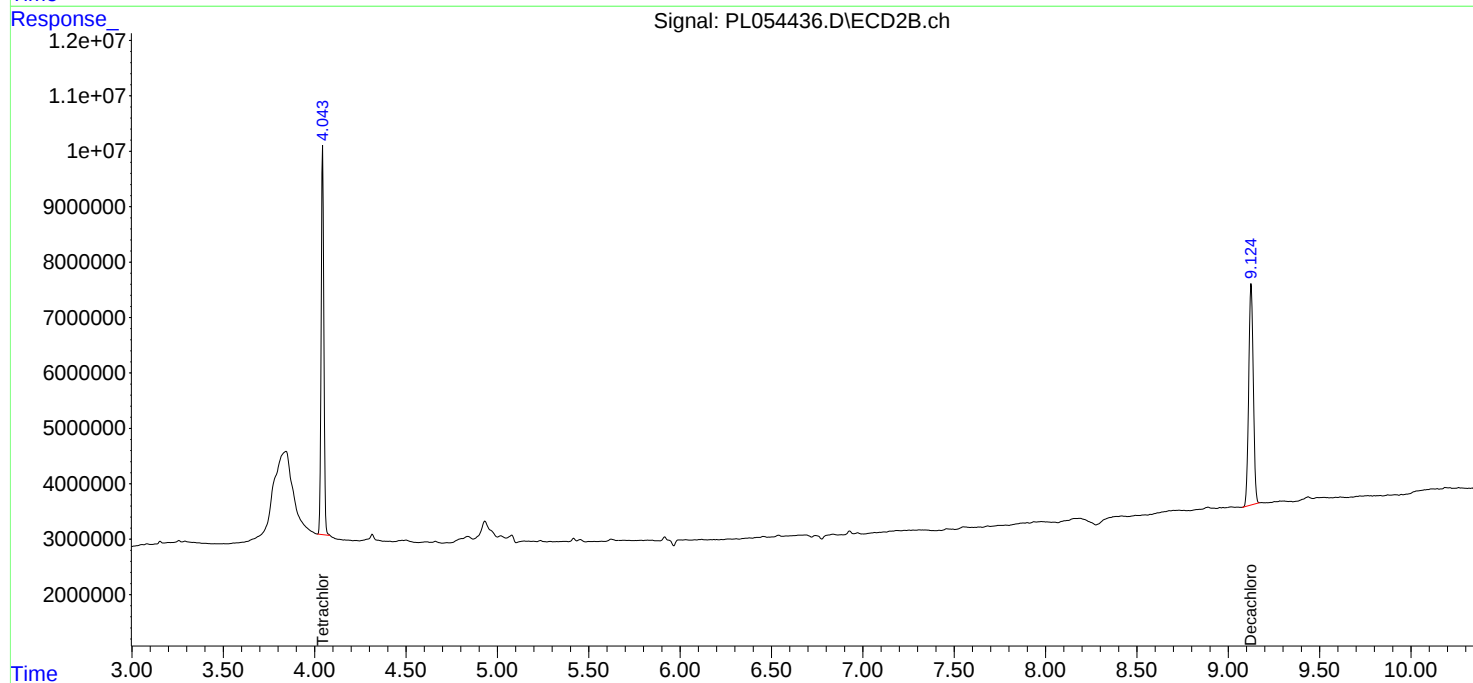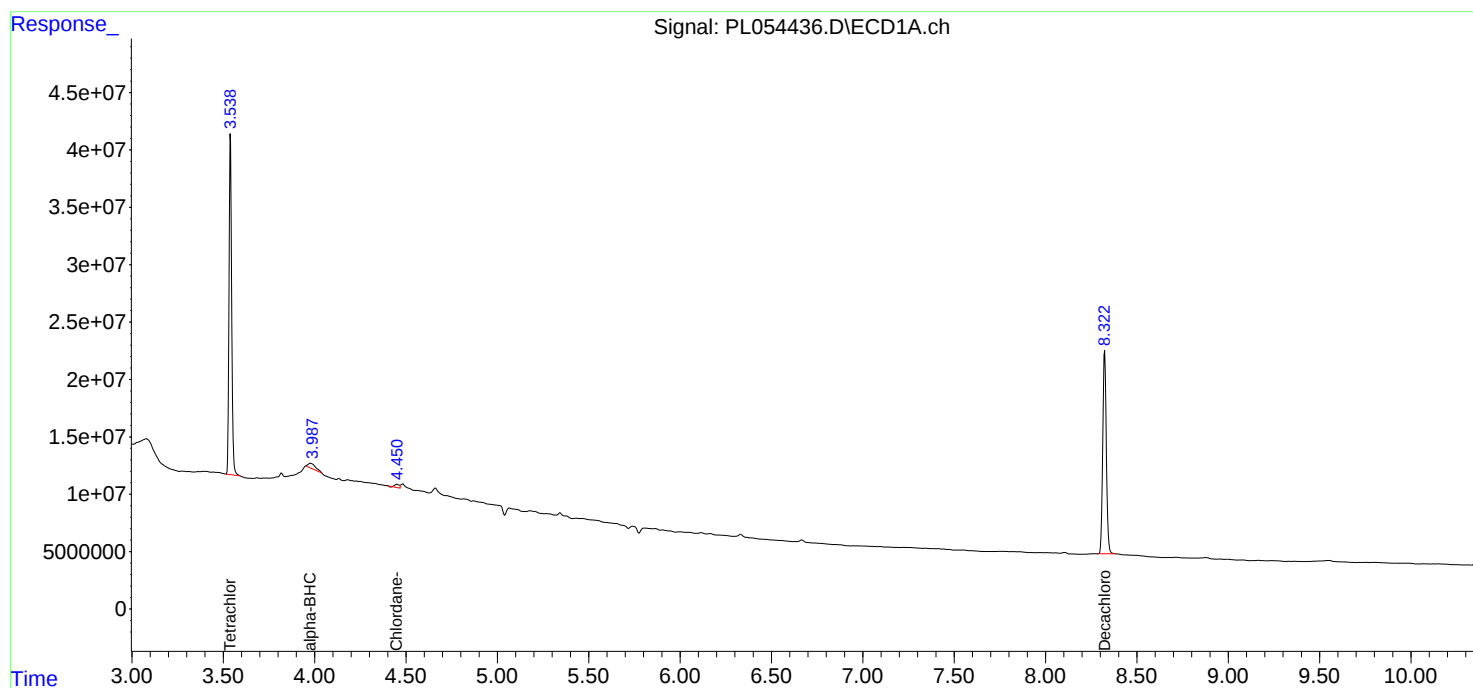


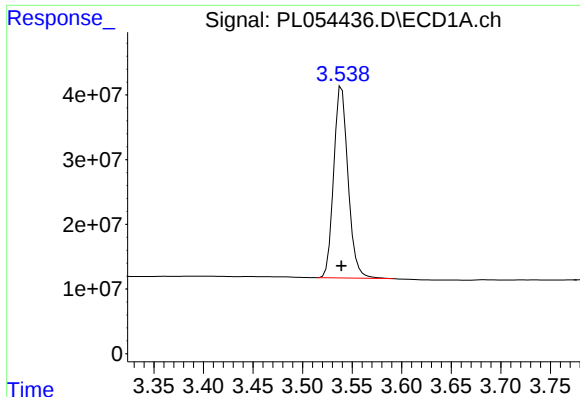

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 298081354
Conc: 28.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

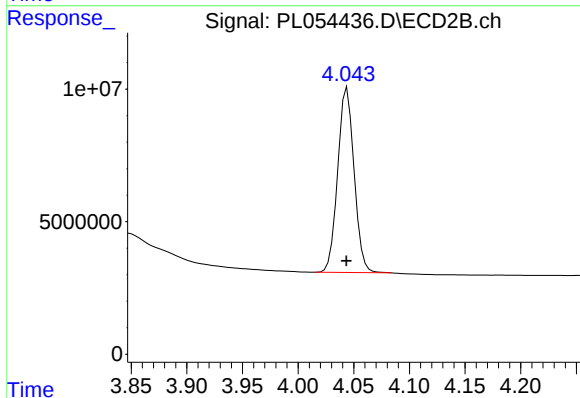


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 71495422
Conc: 29.35 ng/ml

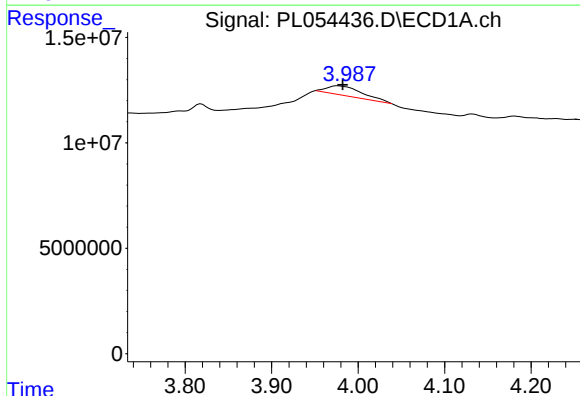


#2 alpha-BHC

R.T.: 3.977 min
Delta R.T.: -0.006 min
Response: 12110309
Conc: 0.71 ng/ml

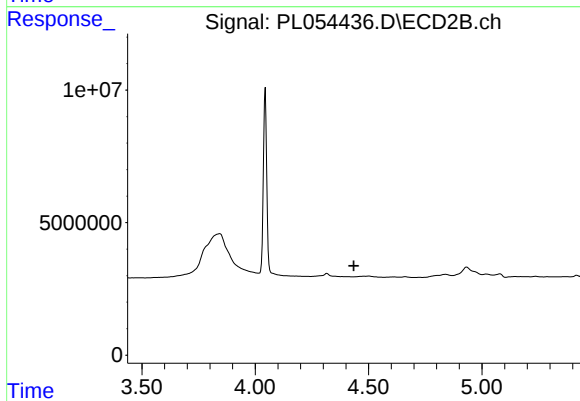

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.435 min
Response: 0
Conc: N.D.

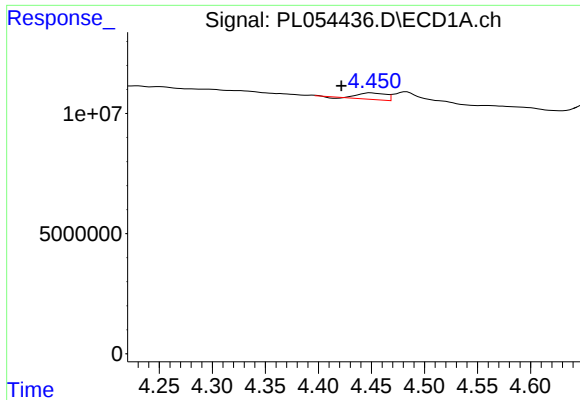

#23 Chlordane-1


R.T.: 4.450 min
Delta R.T.: 0.028 min
Response: 4821441
Conc: 12.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

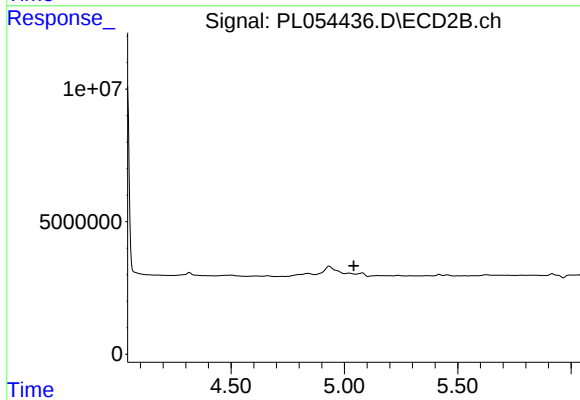


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.041 min
Response: 0
Conc: N.D.

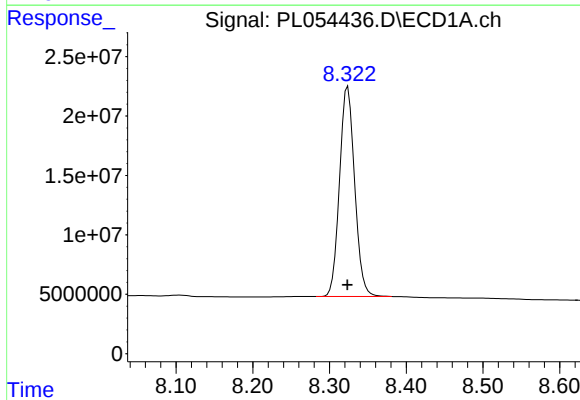

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: 0.000 min
Response: 242763576
Conc: 27.43 ng/ml

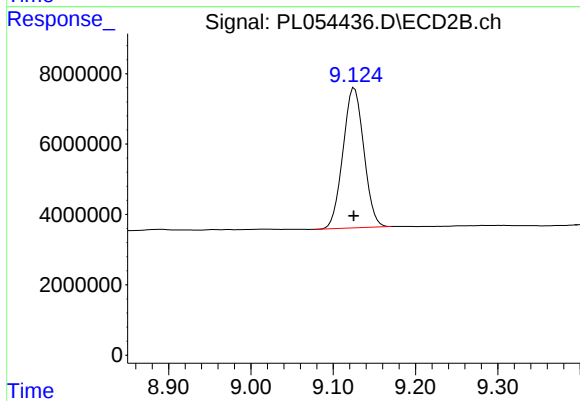

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 69996181
Conc: 28.95 ng/ml