

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
 Data File : PL054435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 03:30
 Operator : SG\AJ
 Sample : K5840-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHIPPS-BH-NE-01

Manual Integrations
 APPROVED

Ankita
 11/19/2019 1:07:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 06:00:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.044	125.9E6	33489555	12.109	13.746
28)	SA Decachlor...	8.324	9.126	132.6E6	38377170	14.987	15.873
Target Compounds							
11)	B alpha-Chl...	5.556	6.231	13013438	3627964	1.037m	1.458 #
12)	B 4,4'-DDE	5.721	6.385	5850463	1738458	0.506m	0.728 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111819\
Data File : PL054435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 03:30
Operator : SG\AJ
Sample : K5840-03
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PHIPPS-BH-NE-01


Manual Integrations
APPROVED

Ankita
11/19/2019 1:07:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:00:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

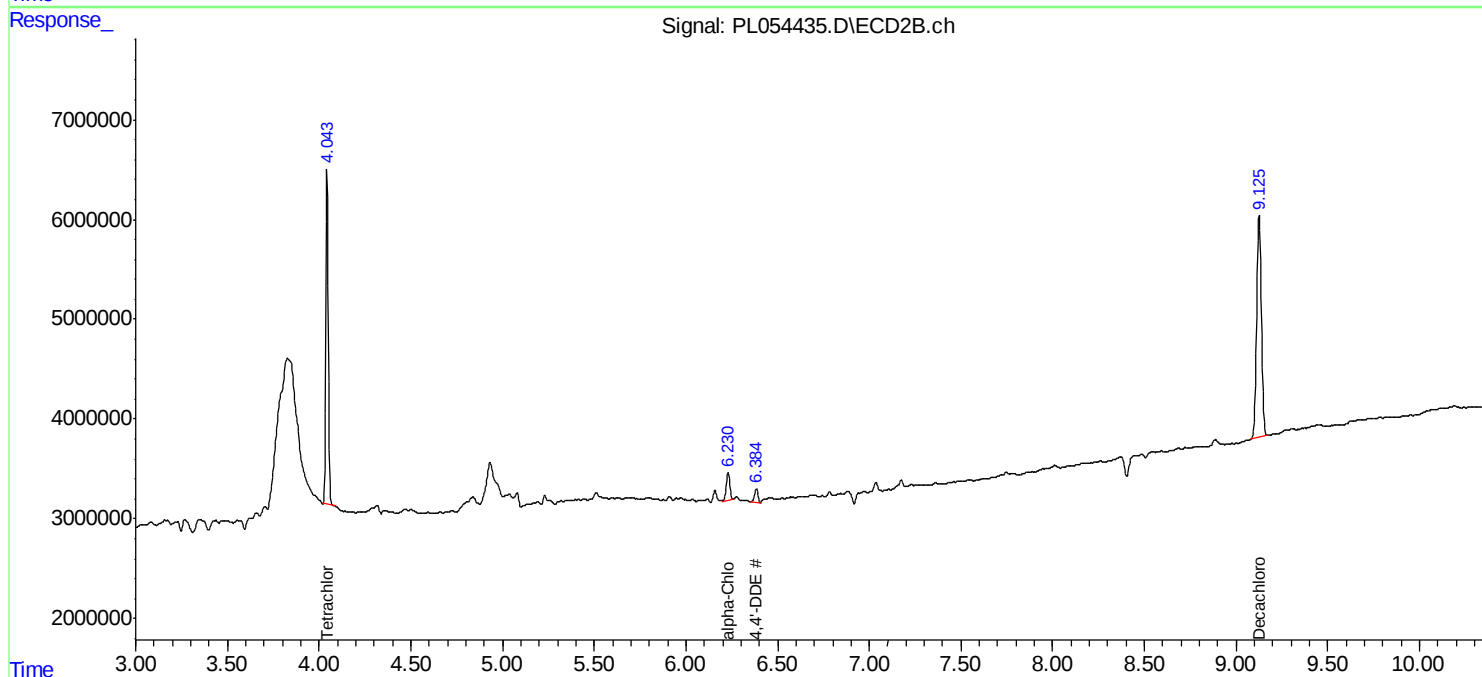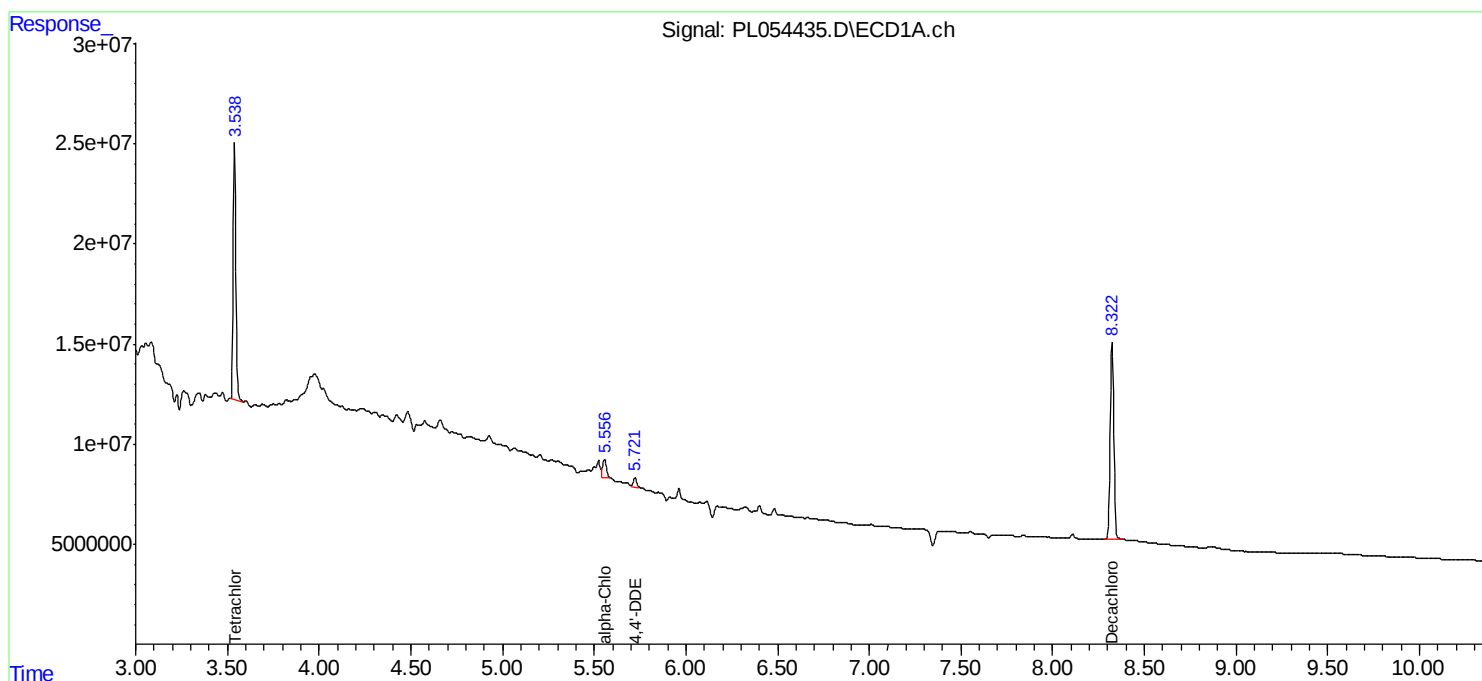

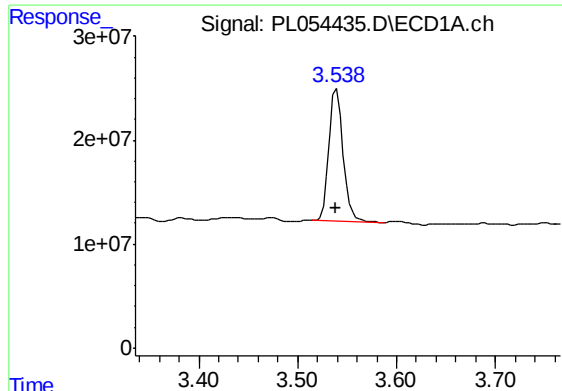


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 125904174
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHIPPS-BH-NE-01


Manual Integrations
APPROVED

Ankita
11/19/2019 1:07:19 PM

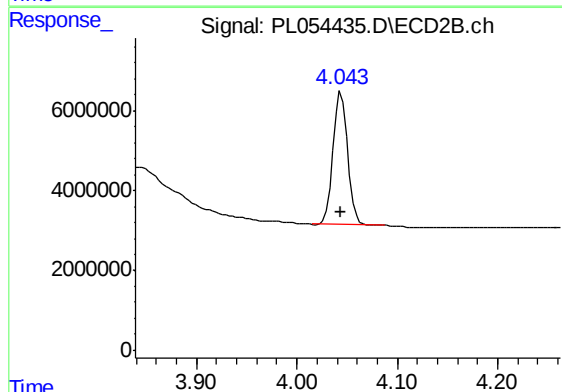


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 33489555
Conc: 13.75 ng/ml

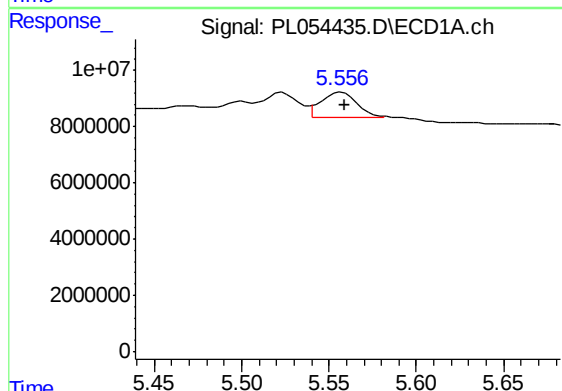


#11 alpha-Chlordane

R.T.: 5.556 min
Delta R.T.: -0.004 min
Response: 13013438
Conc: 1.04 ng/ml m

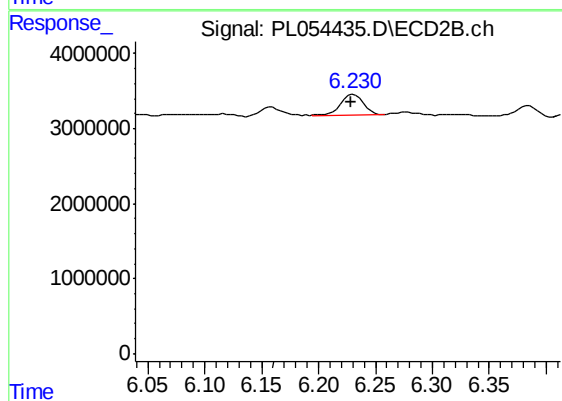

#11 alpha-Chlordane

R.T.: 6.231 min
Delta R.T.: 0.002 min
Response: 3627964
Conc: 1.46 ng/ml

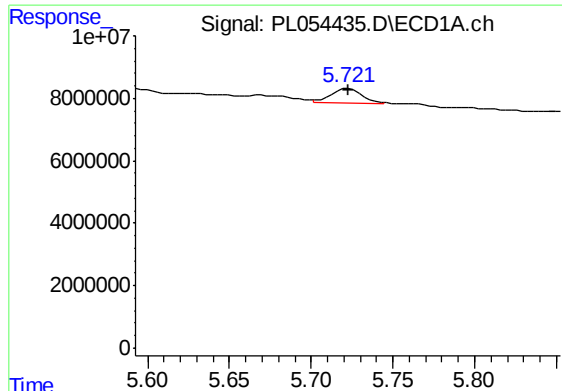


#12 4,4'-DDE

R.T.: 5.721 min
Delta R.T.: -0.001 min
Response: 5850463
Conc: 0.51 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PHIPPS-BH-NE-01


Manual Integrations
APPROVED

Ankita
11/19/2019 1:07:19 PM

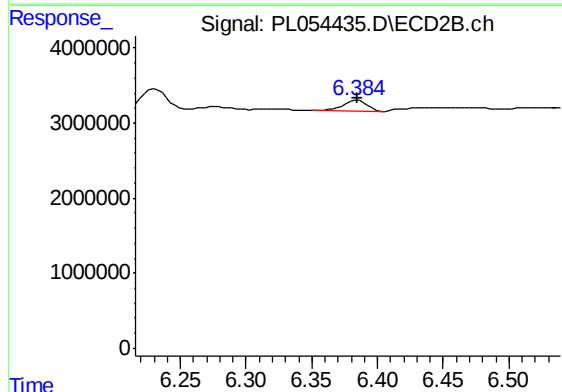


#12 4,4'-DDE

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 1738458
Conc: 0.73 ng/ml

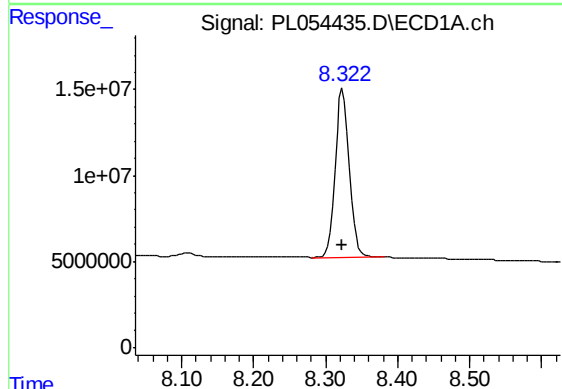

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: 0.000 min
Response: 132644918
Conc: 14.99 ng/ml

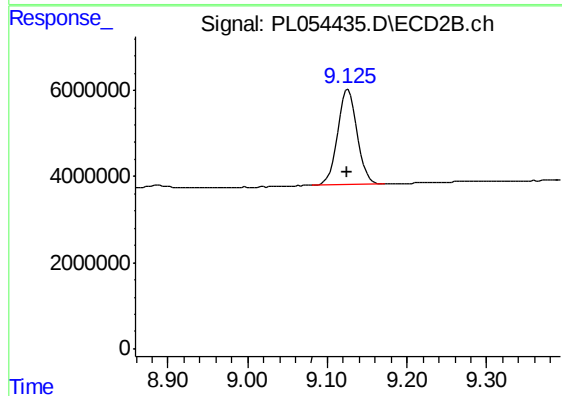

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.001 min
Response: 38377170
Conc: 15.87 ng/ml