

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111820\
 Data File : PL063093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 11:17
 Operator : DD\AJ
 Sample : L4734-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BARNUM-STREET-TEST-PIT-2

Manual Integrations
 APPROVED

Ankita
 11/19/2020 11:00:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:29:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	3.950	33095171	53119418	19.240	18.076
28) SA Decachlor...	8.123	8.986	18265851	19836030	11.386m	9.478m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111820\
Data File : PL063093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 11:17
Operator : DD\AJ
Sample : L4734-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2


Manual Integrations
APPROVED

Ankita
11/19/2020 11:00:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:29:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

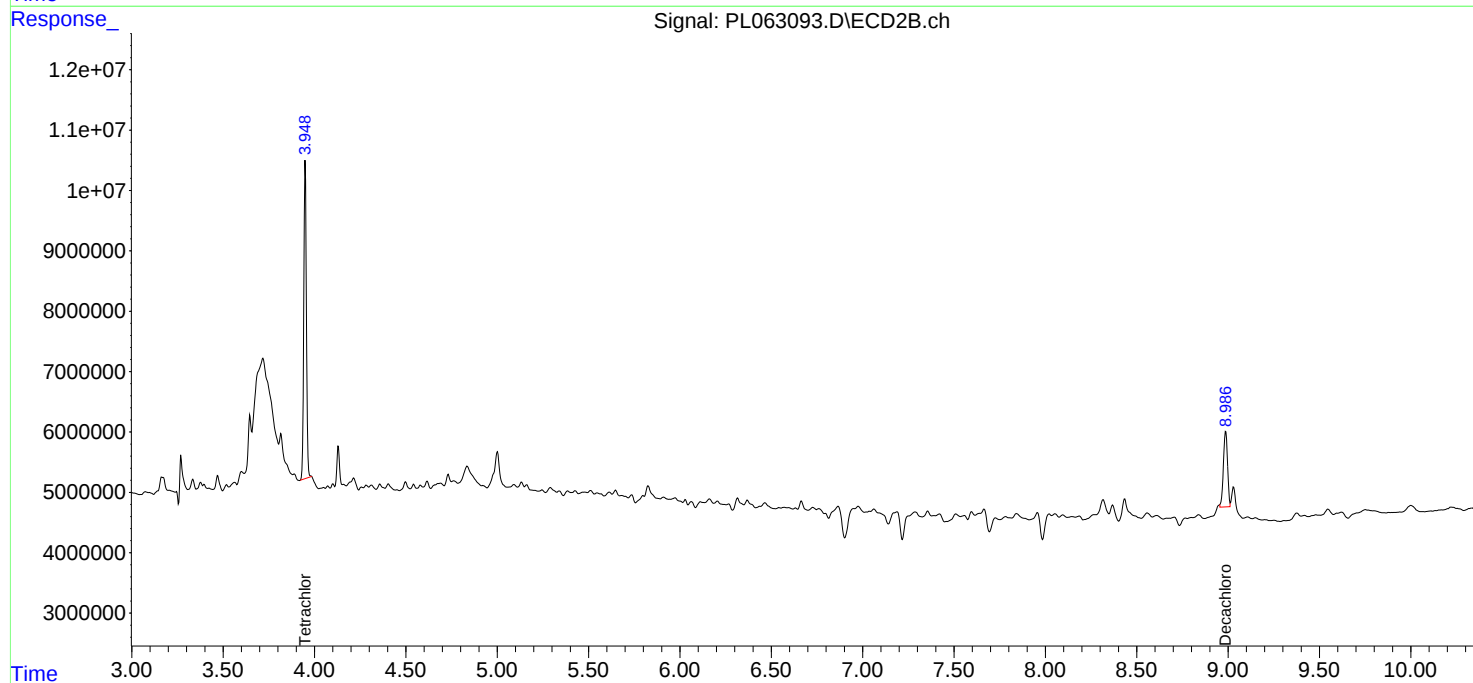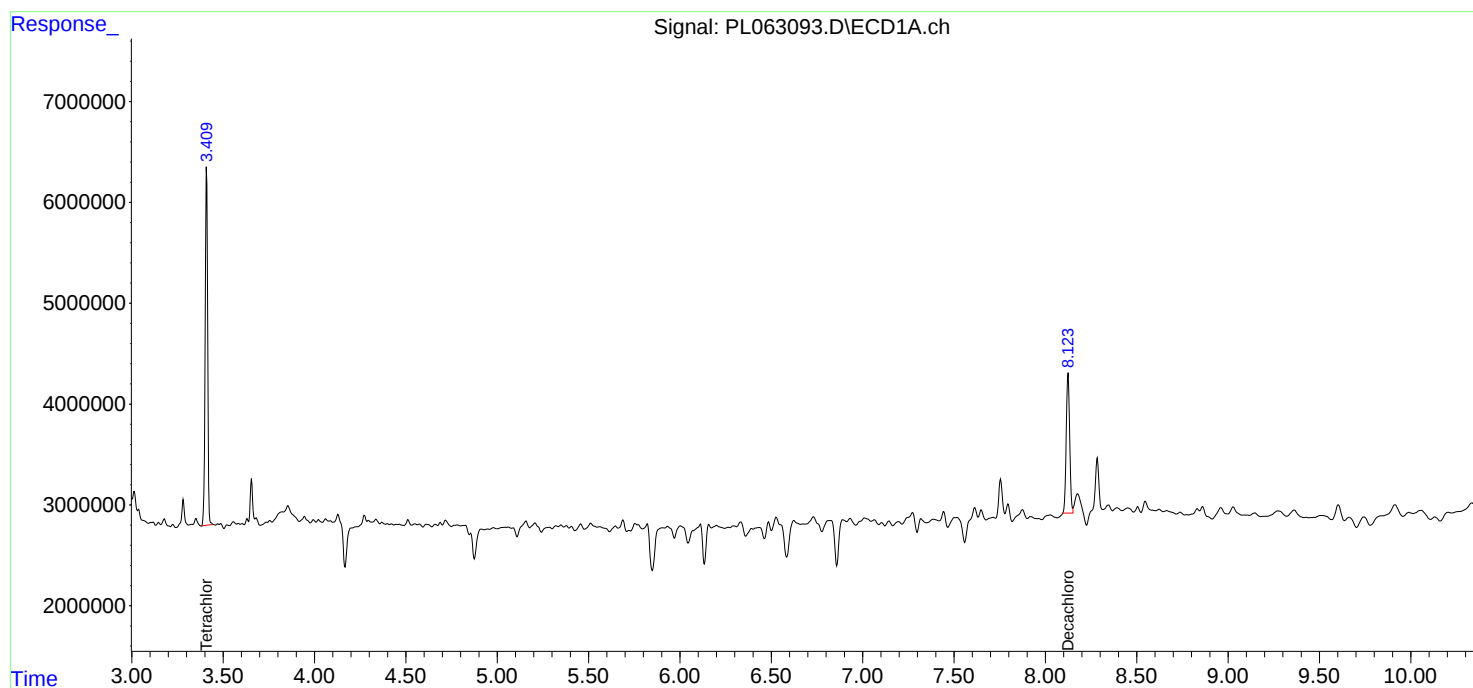

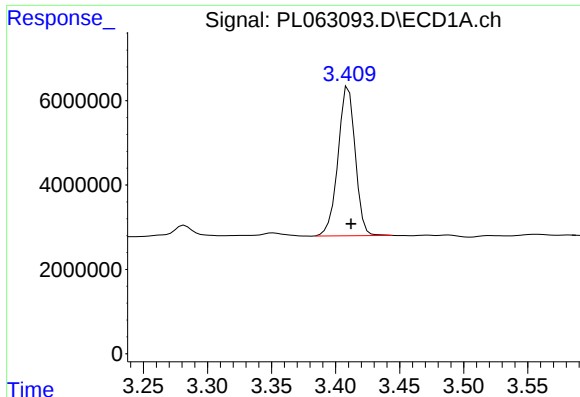


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 33095171
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
BARNUM-STREET-TEST-PIT-2


Manual Integrations
APPROVED

Ankita
11/19/2020 11:00:30 AM

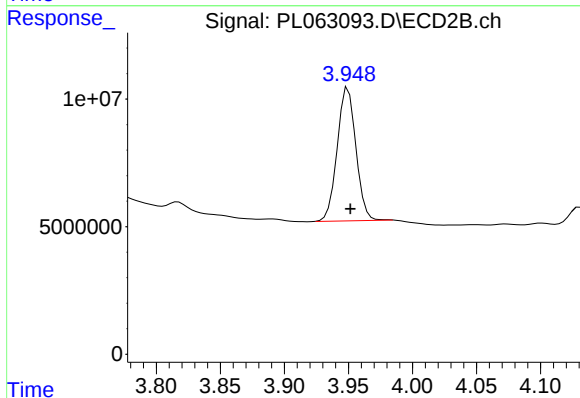


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 53119418
Conc: 18.08 ng/ml

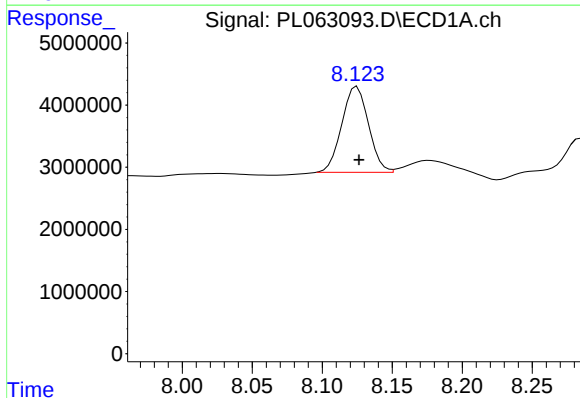

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.003 min
Response: 18265851
Conc: 11.39 ng/ml m

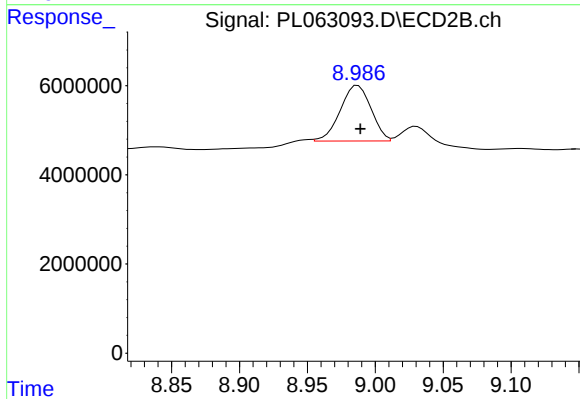

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: -0.003 min
Response: 19836030
Conc: 9.48 ng/ml m