

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
 Data File : PL079249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 18:19
 Operator : AR\AJ
 Sample : PB149151BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:26:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.566	40100773	49470062	19.257	19.424
28)	SA Decachlor...	8.770	7.634	34036709	45142453	20.348	21.761
Target Compounds							
4)	MA Heptachlor	4.713f	0.000	209980	0	0.070	N.D. #
6)	B beta-BHC	4.311f	0.000	1408956	0	1.071	N.D. #
9)	A Endosulfan I	5.856f	0.000	1657937	0	0.690	N.D. #
10)	B gamma-Chl...	5.715	0.000	593383	0	0.232	N.D. #
11)	B alpha-Chl...	5.789	0.000	527768	0	0.205	N.D. #
12)	B 4,4'-DDE	5.974	0.000	79933	0	0.035	N.D. #
15)	B Endosulfa...	6.550f	0.000	642933	0	0.285	N.D. #
25)	Chlordane-3	5.715	0.000	593383	0	1.540	N.D. #
26)	Chlordane-4	5.789	0.000	527768	0	1.115	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
Data File : PL079249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 18:19
Operator : AR\AJ
Sample : PB149151BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:26:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

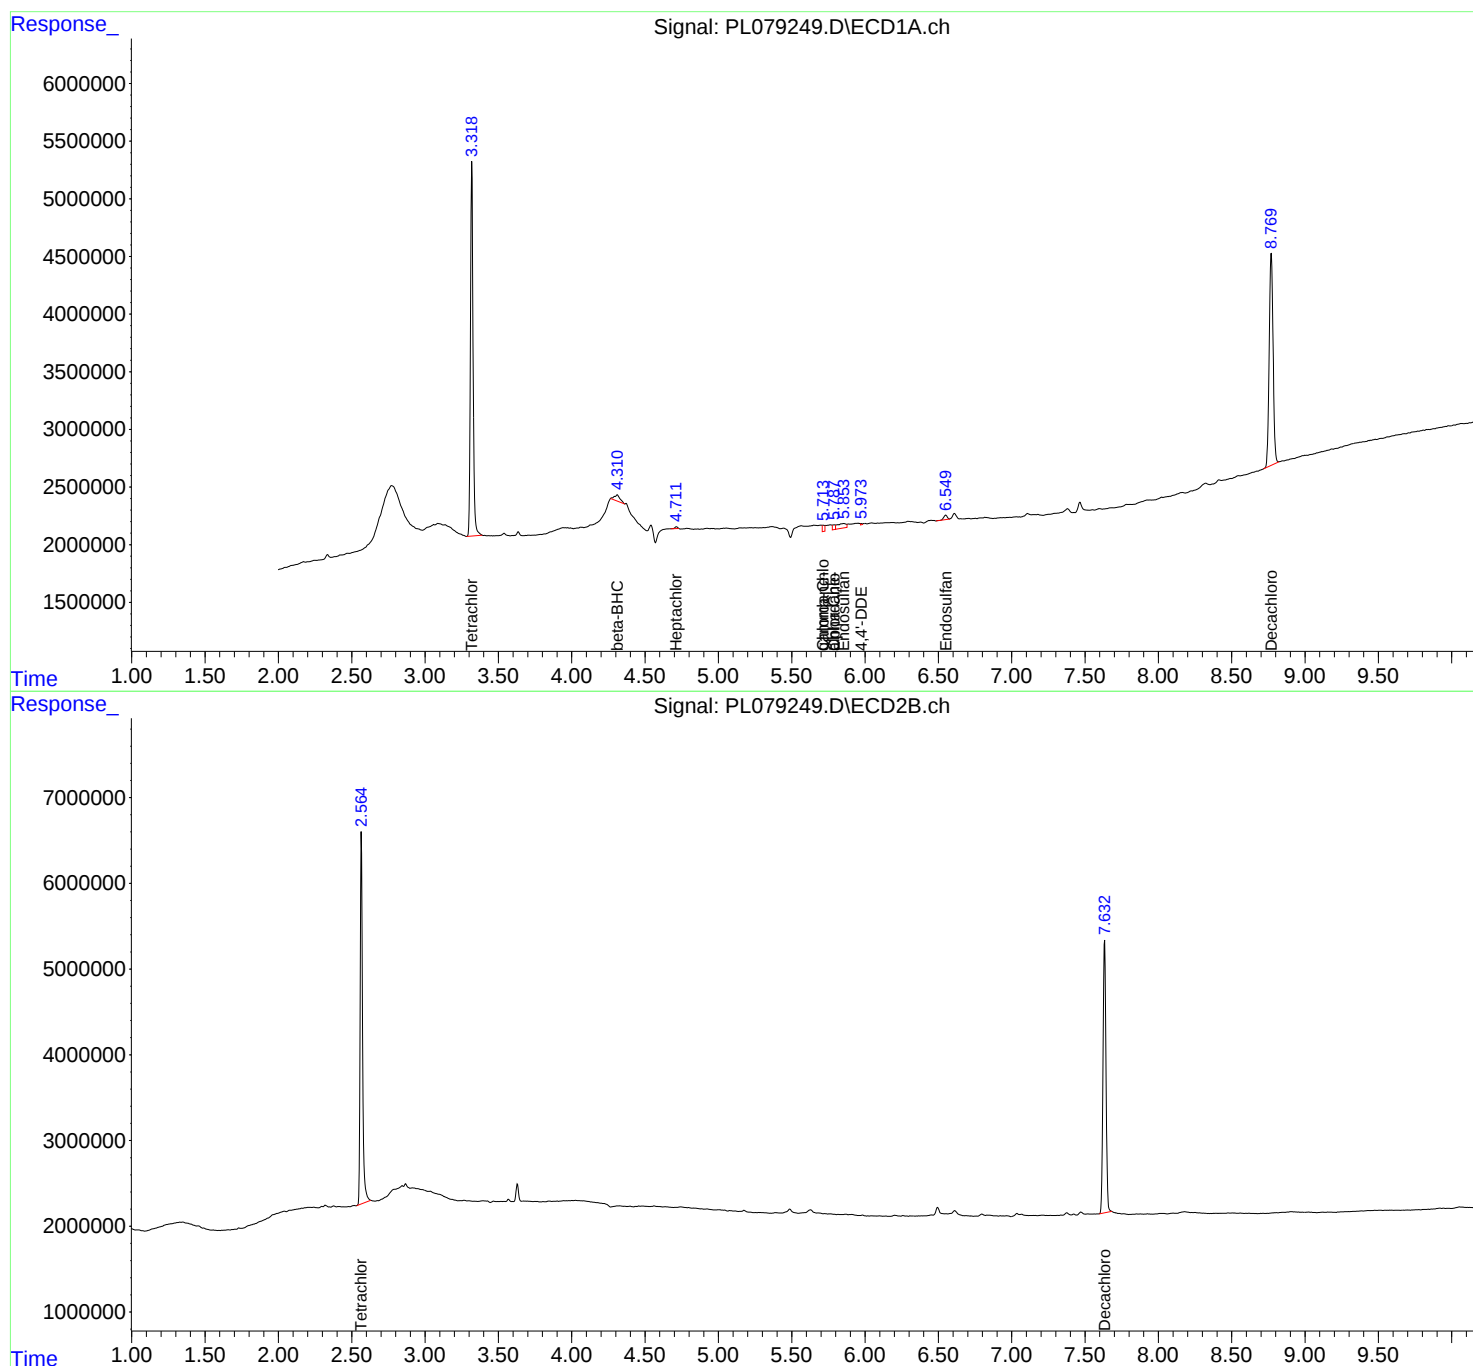


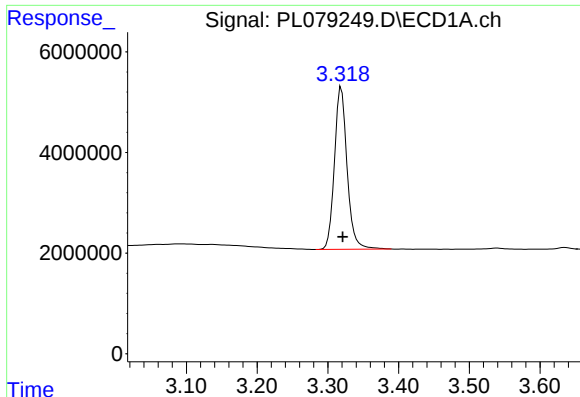

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 40100773
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

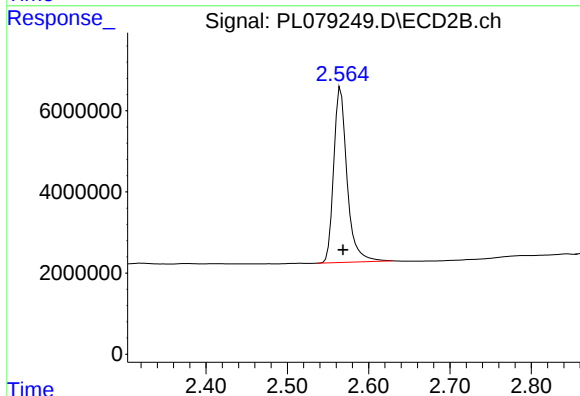


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 49470062
Conc: 19.42 ng/ml

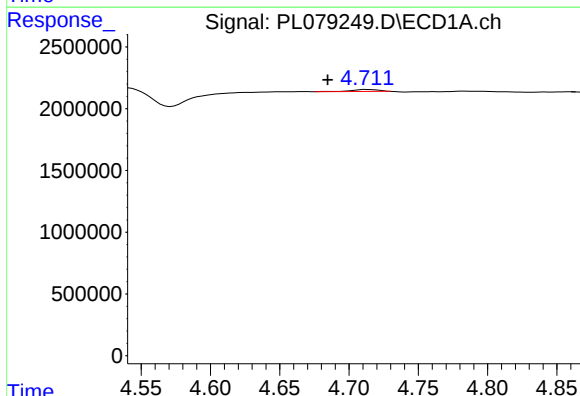


#4 Heptachlor

R.T.: 4.713 min
Delta R.T.: 0.028 min
Response: 209980
Conc: 0.07 ng/ml

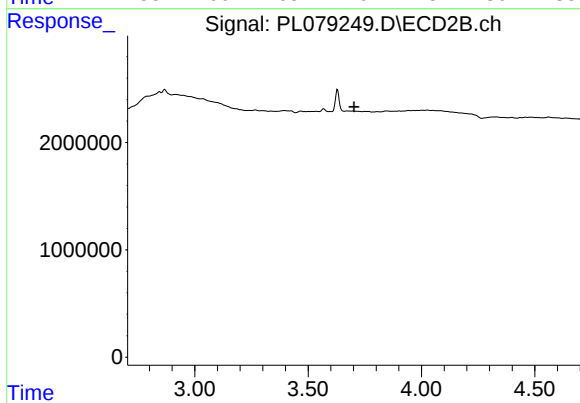

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.702 min
Response: 0
Conc: N.D.

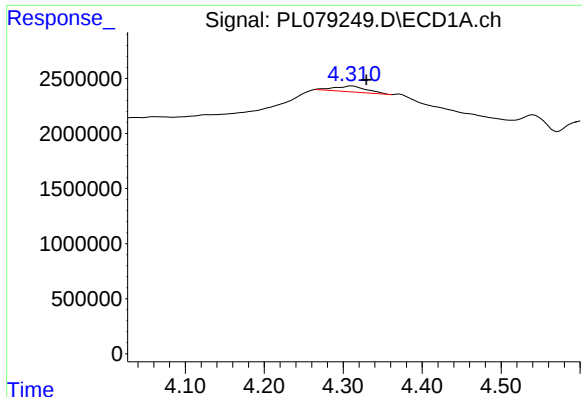

#6 beta-BHC


R.T.: 4.311 min
Delta R.T.: -0.019 min
Response: 1408956
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

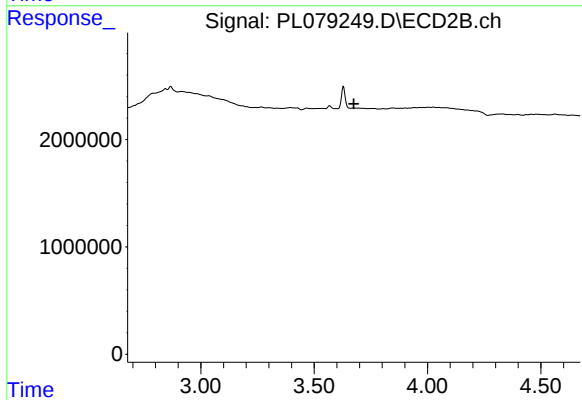


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.675 min
Response: 0
Conc: N.D.

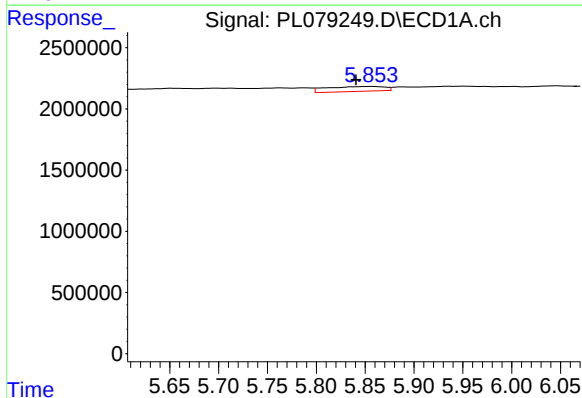


#9 Endosulfan I

R.T.: 5.856 min
Delta R.T.: 0.015 min
Response: 1657937
Conc: 0.69 ng/ml

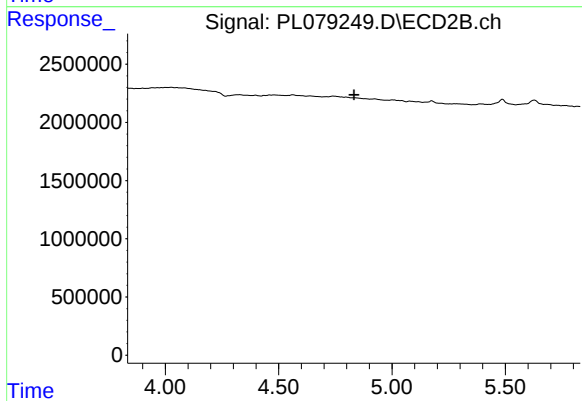

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

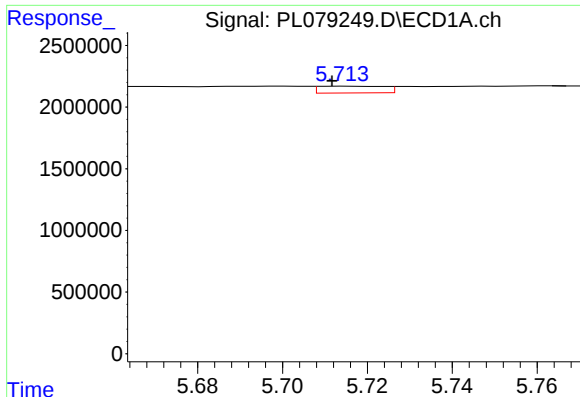

#10 gamma-Chlordane


R.T.: 5.715 min
Delta R.T.: 0.003 min
Response: 593383
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

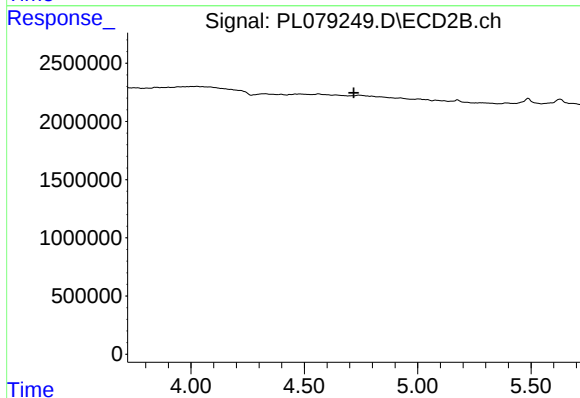


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

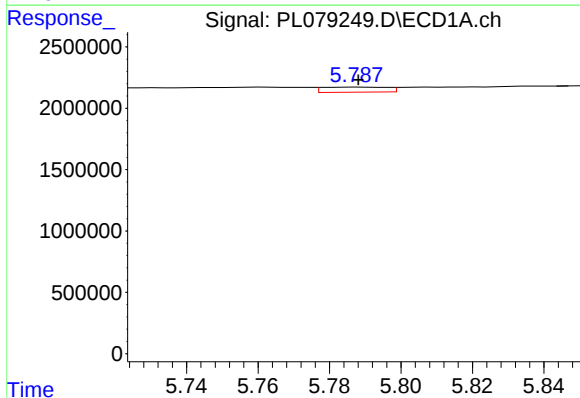


#11 alpha-Chlordane

R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 527768
Conc: 0.21 ng/ml

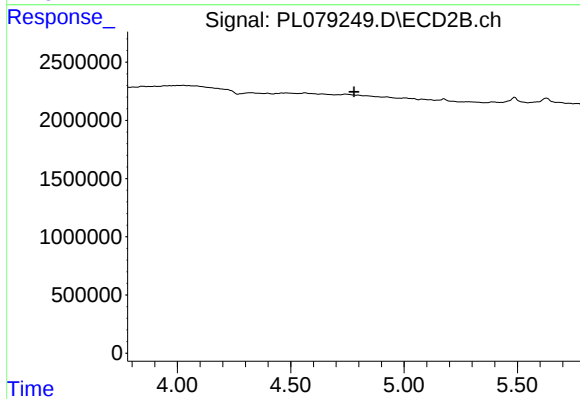

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

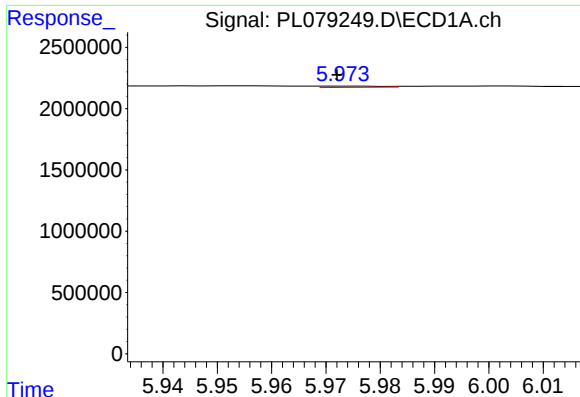

#12 4,4'-DDE


R.T.: 5.974 min
Delta R.T.: 0.002 min
Response: 79933
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

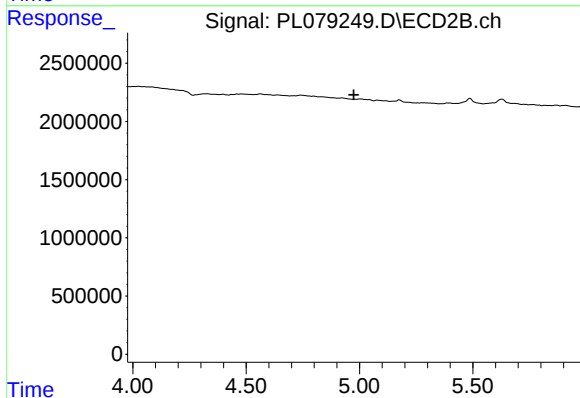


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

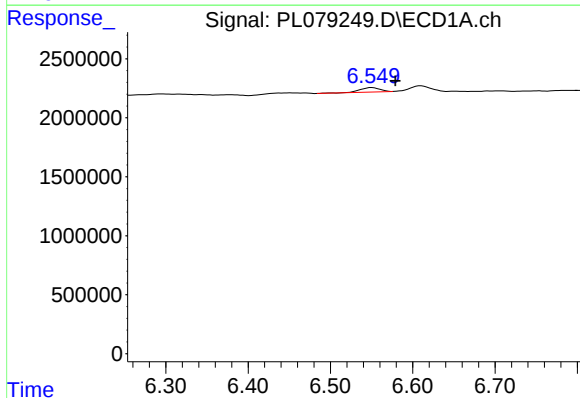


#15 Endosulfan II

R.T.: 6.550 min
Delta R.T.: -0.029 min
Response: 642933
Conc: 0.29 ng/ml

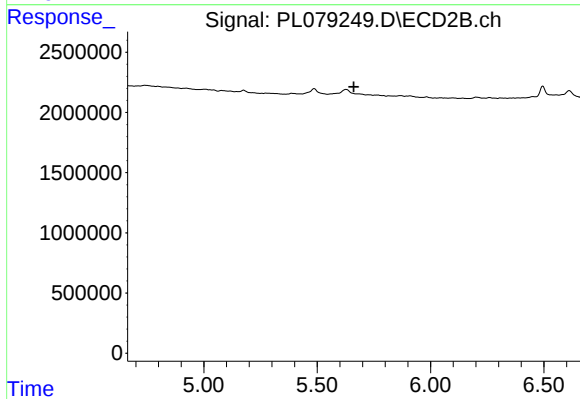

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.661 min
Response: 0
Conc: N.D.

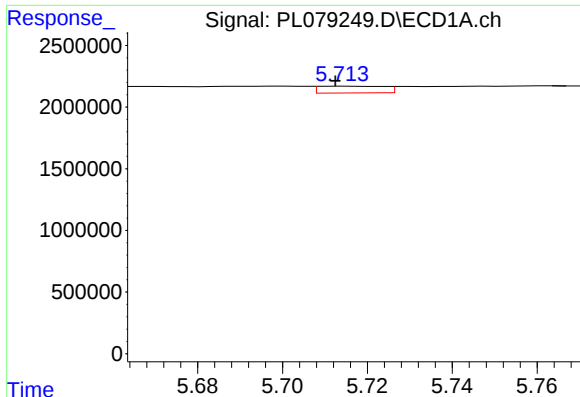

#25 Chlordane-3


R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 593383
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

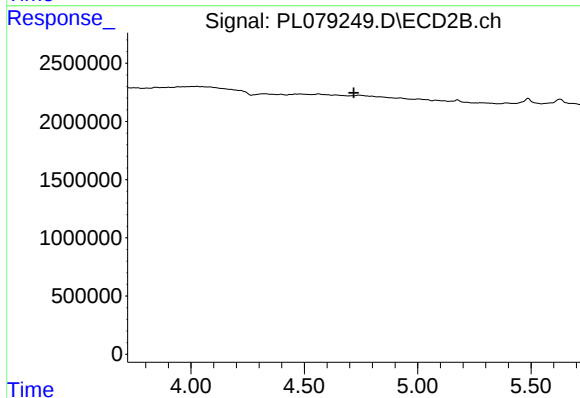


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

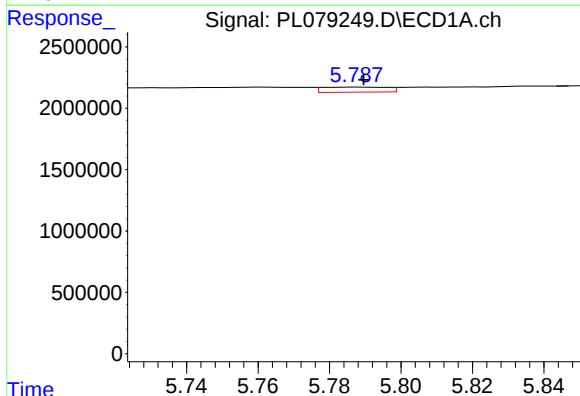


#26 Chlordane-4

R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 527768
Conc: 1.12 ng/ml

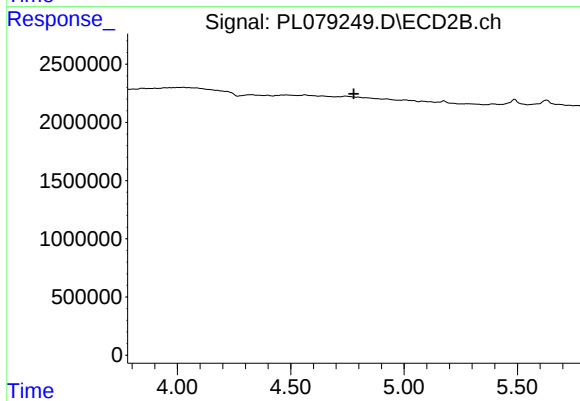

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 4.778 min
Response: 0
Conc: N.D.

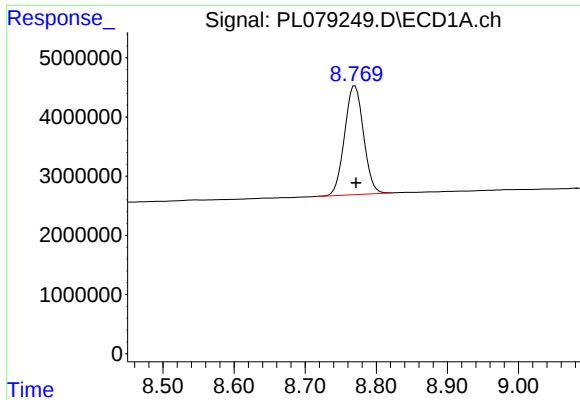

#28 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.002 min
Response: 34036709
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

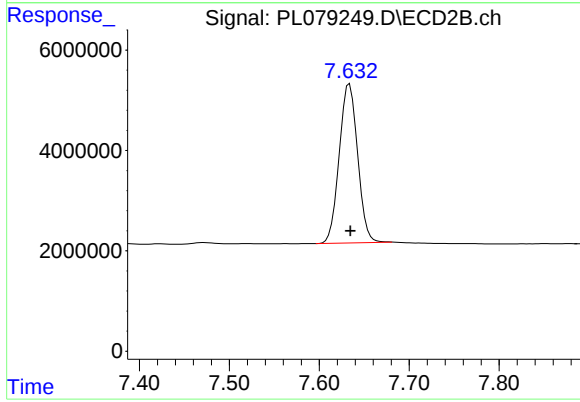

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: -0.001 min
Response: 45142453
Conc: 21.76 ng/ml