

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
 Data File : PL079281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2022 03:18
 Operator : AR\AJ
 Sample : N5698-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 06:08:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.567	38303291	29867237	18.394	11.727 #
28)	SA Decachlor...	8.769	7.633	17913115	22252297	10.709	10.727
Target Compounds							
2)	A alpha-BHC	0.000	3.060	0	7239629	N.D.	1.790 #
5)	MB Aldrin	0.000	3.977	0	67616920	N.D.	19.358 #
7)	B delta-BHC	4.589f	0.000	45830290	0	20.238	N.D. #
9)	A Endosulfan I	5.864f	0.000	88670900	0	36.923	N.D. #
15)	B Endosulfa...	6.606f	0.000	166853	0	0.074	N.D. #
16)	A 4,4'-DDD	6.504	0.000	3932823	0	2.239	N.D. #
19)	B Endosulfa...	6.925f	0.000	581707	0	0.289	N.D. #
21)	B Endrin ke...	7.431	0.000	272559	0	0.131	N.D. #
24)	Chlordane-2	0.000	4.068f	0	2388798	N.D.	22.495 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
Data File : PL079281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2022 03:18
Operator : AR\AJ
Sample : N5698-03
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 06:08:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

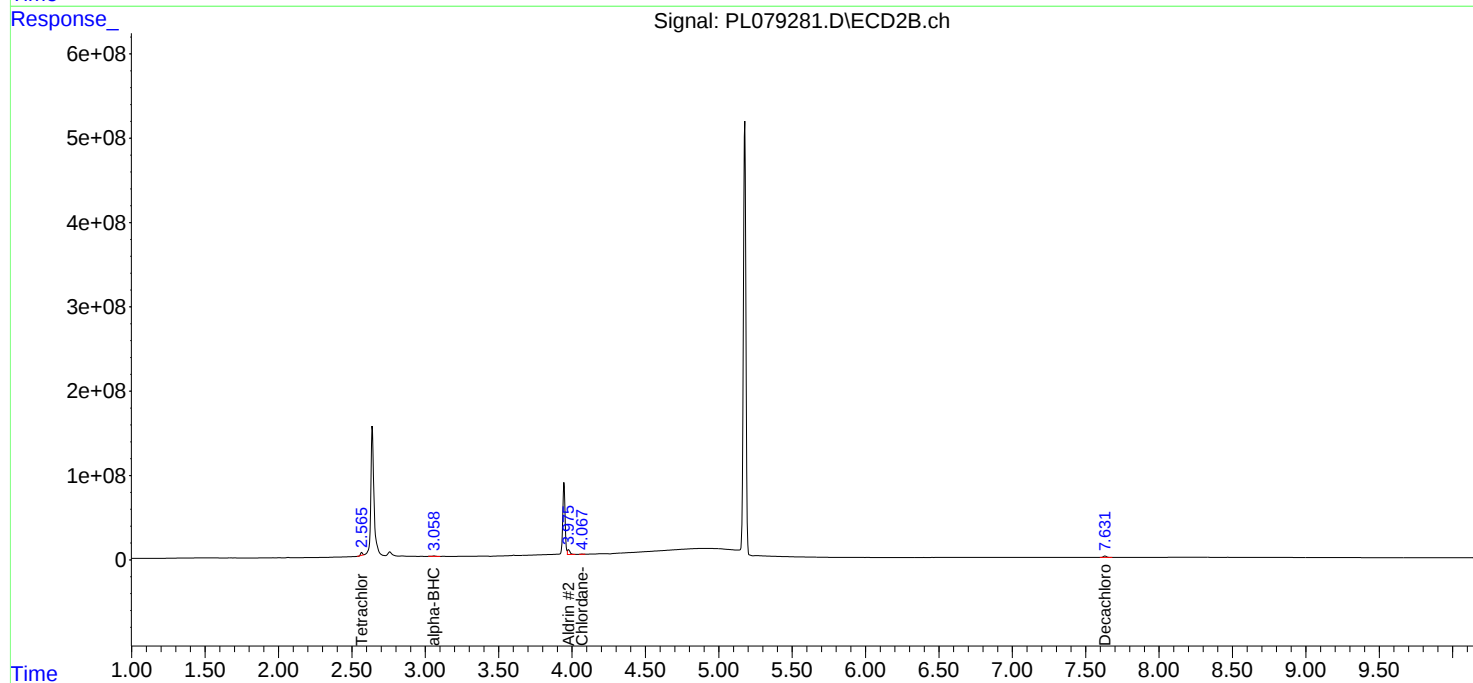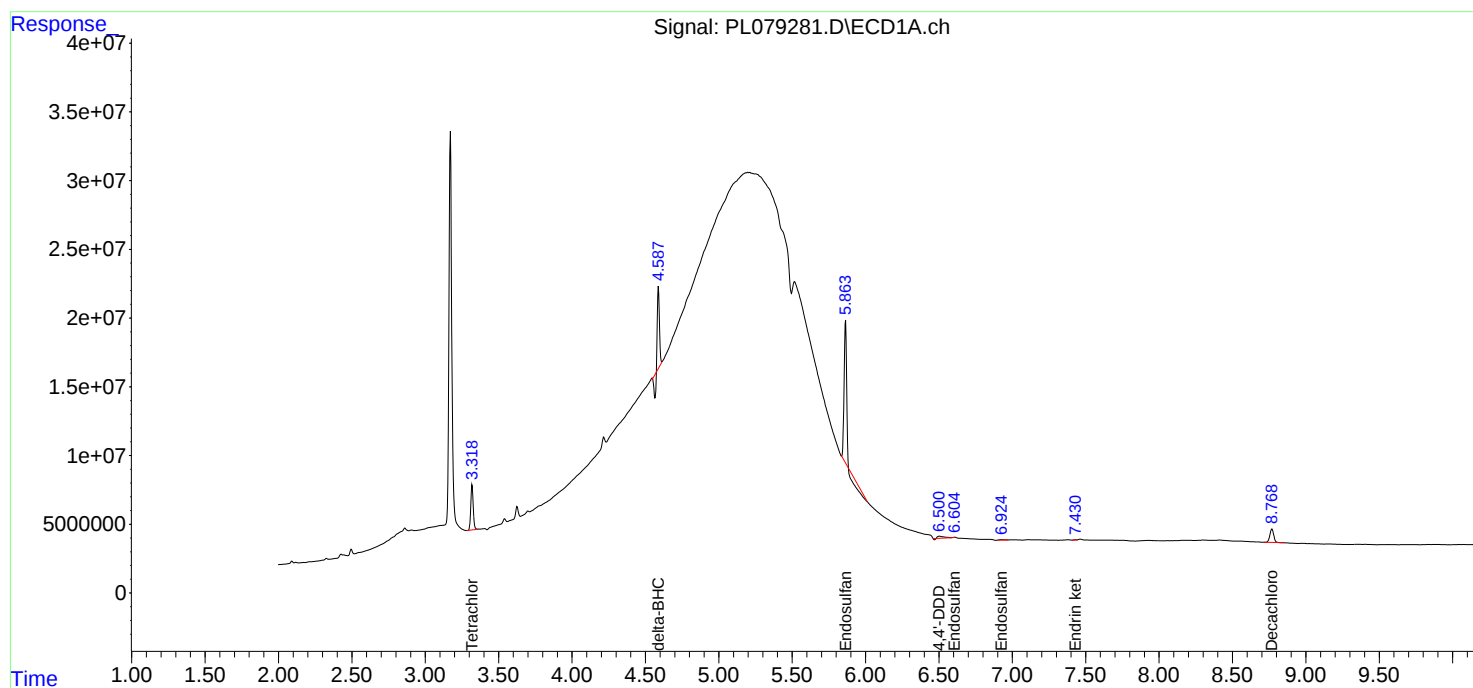


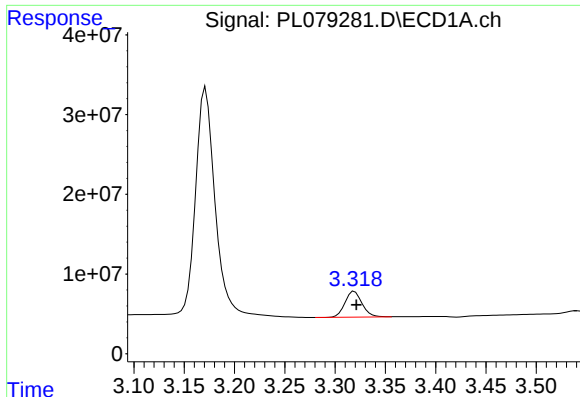

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 38303291
Conc: 18.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

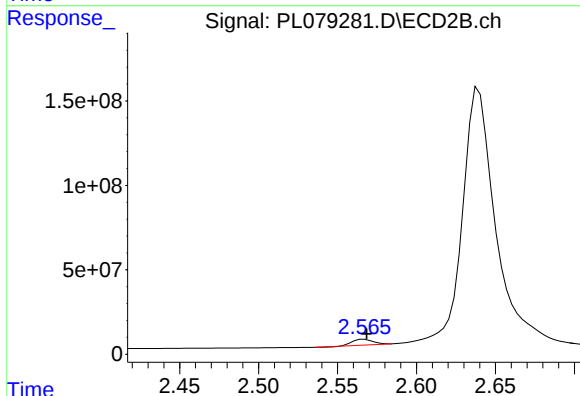


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: -0.002 min
Response: 29867237
Conc: 11.73 ng/ml

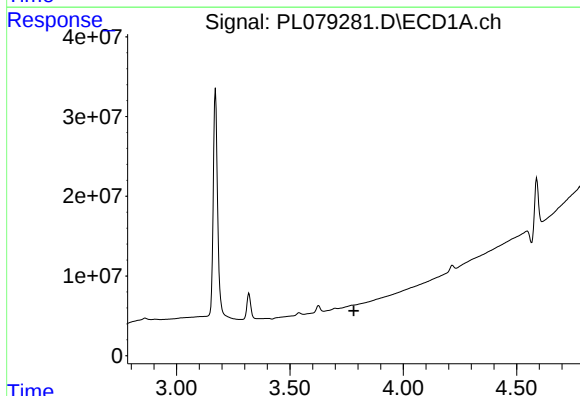


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.781 min
Response: 0
Conc: N.D.

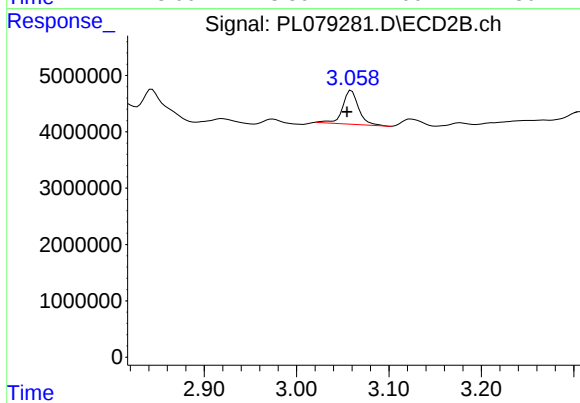

#2 alpha-BHC


R.T.: 3.060 min
Delta R.T.: 0.005 min
Response: 7239629
Conc: 1.79 ng/ml

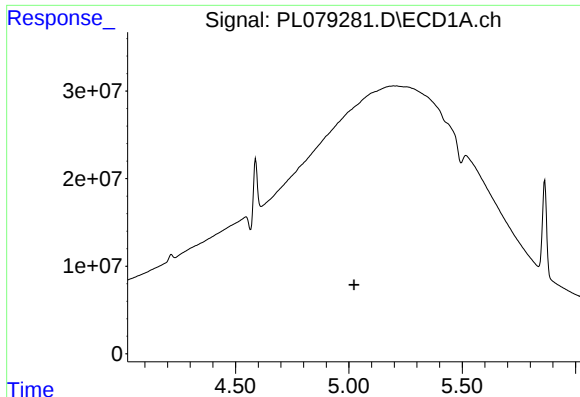

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

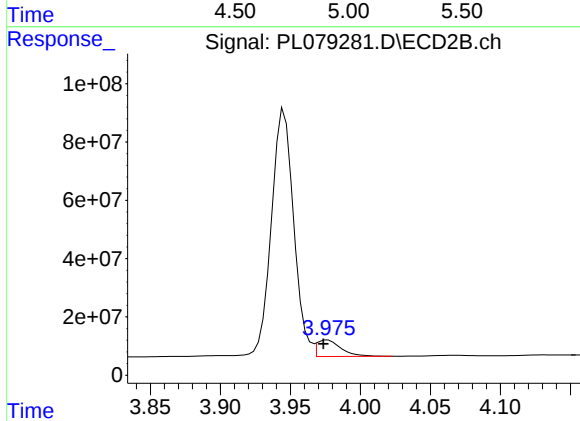


#5 Aldrin

R.T.: 3.977 min
Delta R.T.: 0.003 min
Response: 67616920
Conc: 19.36 ng/ml

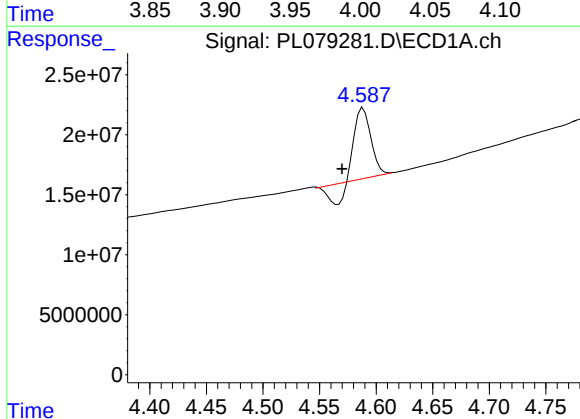


#7 delta-BHC

R.T.: 4.589 min
Delta R.T.: 0.019 min
Response: 45830290
Conc: 20.24 ng/ml

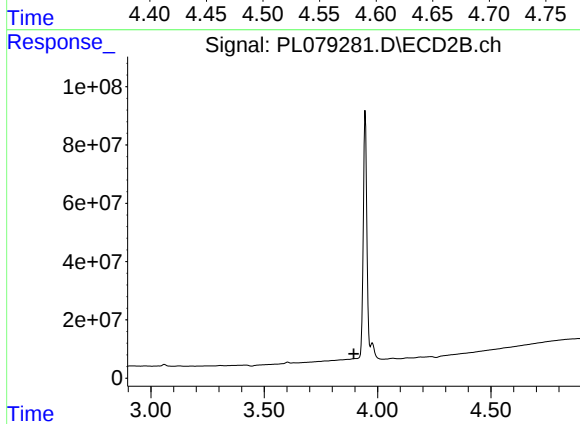

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 3.895 min
Response: 0
Conc: N.D.

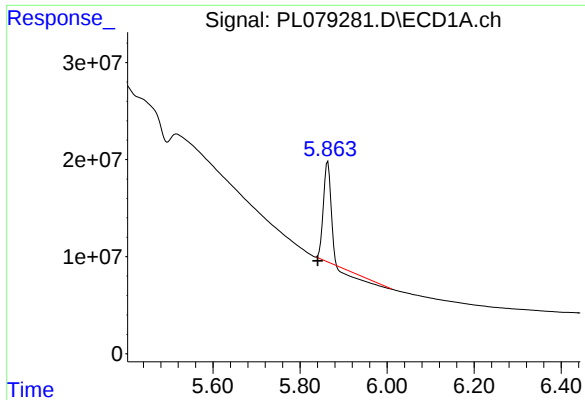

#9 Endosulfan I


R.T.: 5.864 min
Delta R.T.: 0.023 min
Response: 88670900
Conc: 36.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

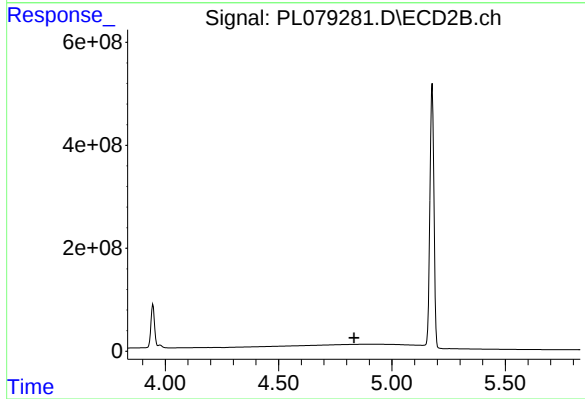


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

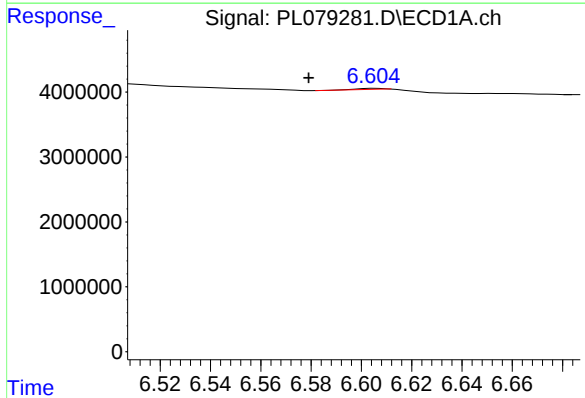


#15 Endosulfan II

R.T.: 6.606 min
Delta R.T.: 0.027 min
Response: 166853
Conc: 0.07 ng/ml

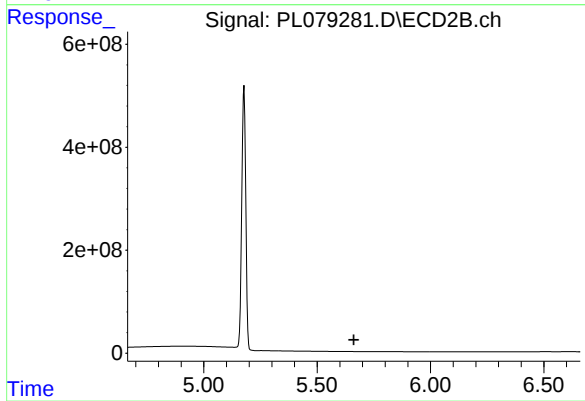

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.661 min
Response: 0
Conc: N.D.

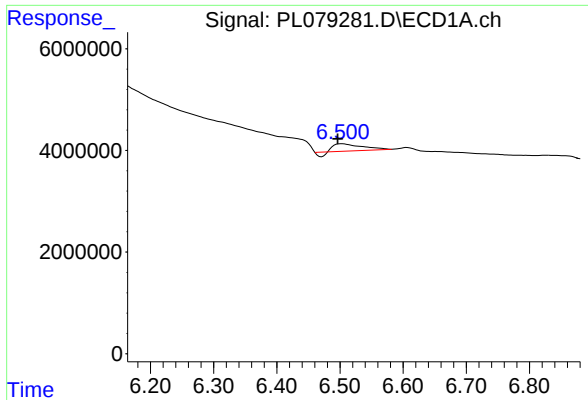

#16 4,4'-DDD


R.T.: 6.504 min
Delta R.T.: 0.007 min
Response: 3932823
Conc: 2.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

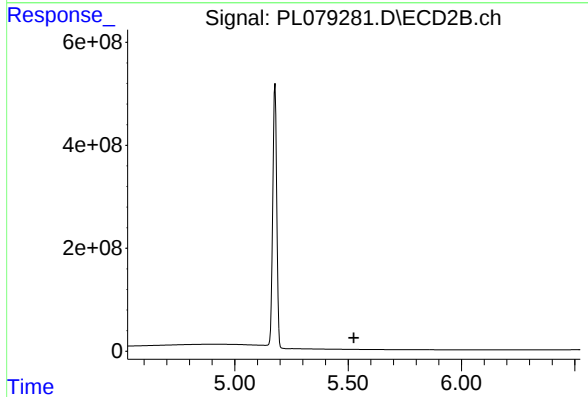


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.526 min
Response: 0
Conc: N.D.

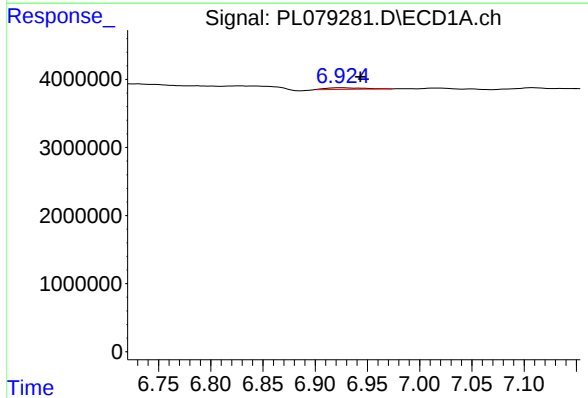


#19 Endosulfan Sulfate

R.T.: 6.925 min
Delta R.T.: -0.018 min
Response: 581707
Conc: 0.29 ng/ml

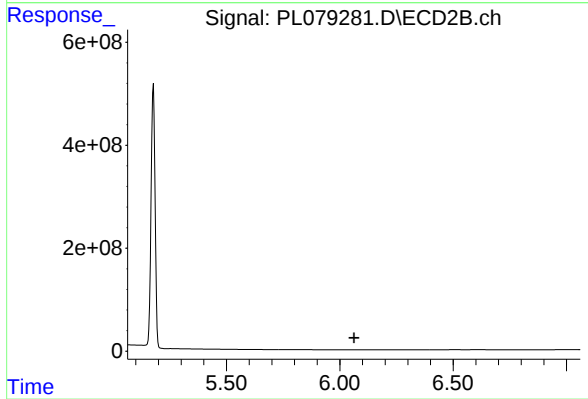

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.063 min
Response: 0
Conc: N.D.

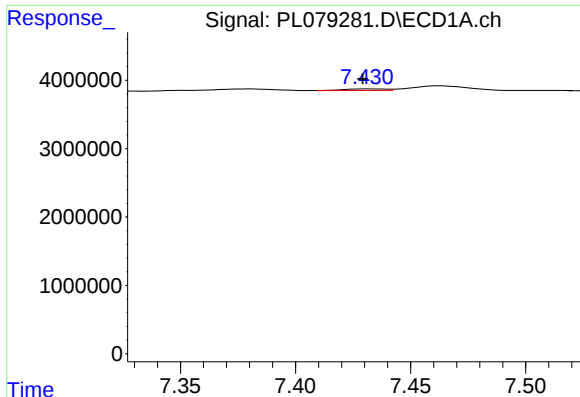

#21 Endrin ketone


R.T.: 7.431 min
Delta R.T.: 0.002 min
Response: 272559
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

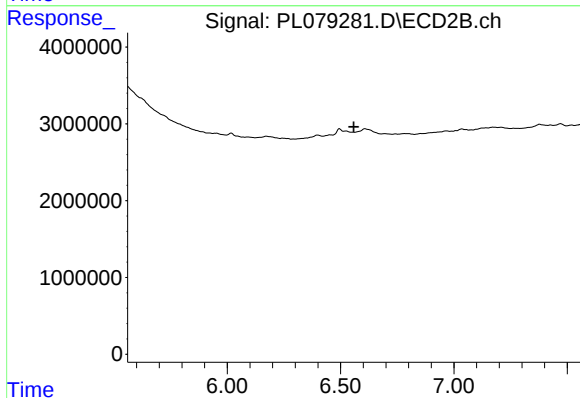


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.558 min
Response: 0
Conc: N.D.

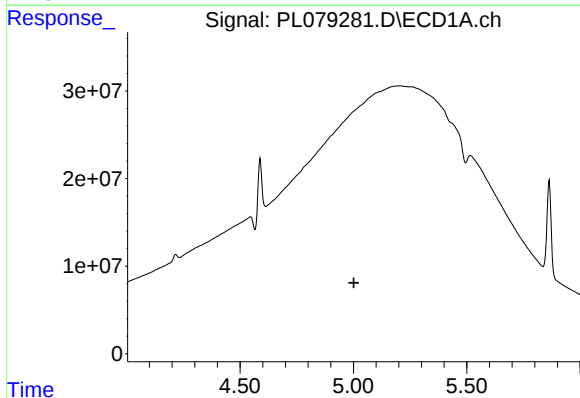


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.002 min
Response: 0
Conc: N.D.

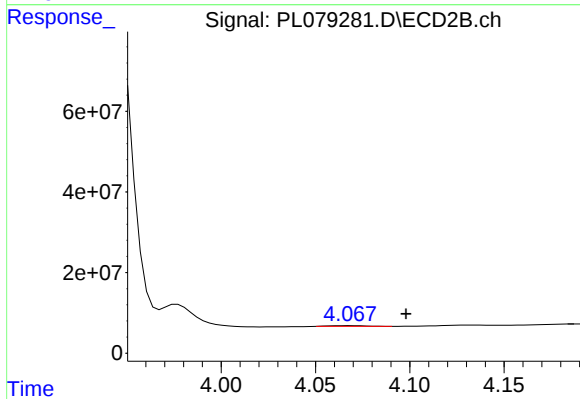

#24 Chlordane-2


R.T.: 4.068 min
Delta R.T.: -0.030 min
Response: 2388798
Conc: 22.49 ng/ml

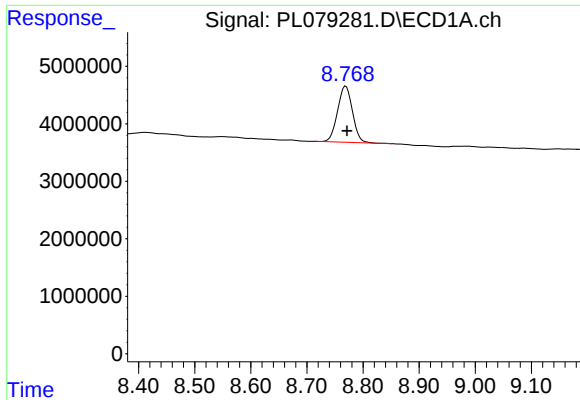

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.002 min
Response: 17913115
Conc: 10.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

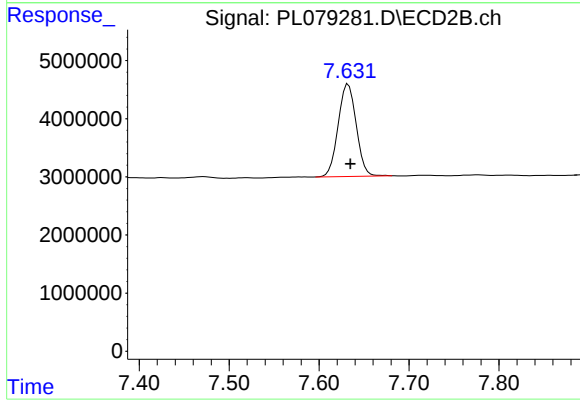

#28 Decachlorobiphenyl

R.T.: 7.633 min
Delta R.T.: -0.002 min
Response: 22252297
Conc: 10.73 ng/ml