

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
 Data File : PL079245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 17:21
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:25:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	2.565	99120226	145.3E6	47.599	57.059
28)	SA Decachlor...	8.774	7.636	77945265	100.1E6	46.597	48.231
Target Compounds							
23)	Chlordane-1	4.471	3.531	41379388	47549470	472.248	460.225
24)	Chlordane-2	5.004	4.097	46624319	48840149	458.064	459.915
25)	Chlordane-3	5.715	4.717	183.2E6	149.6E6	475.492	469.591
26)	Chlordane-4	5.792	4.777	224.7E6	159.7E6	474.845	465.415
27)	Chlordane-5	6.648	5.439	36738241	41625840	495.156	488.171



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
Data File : PL079245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 17:21
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:25:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

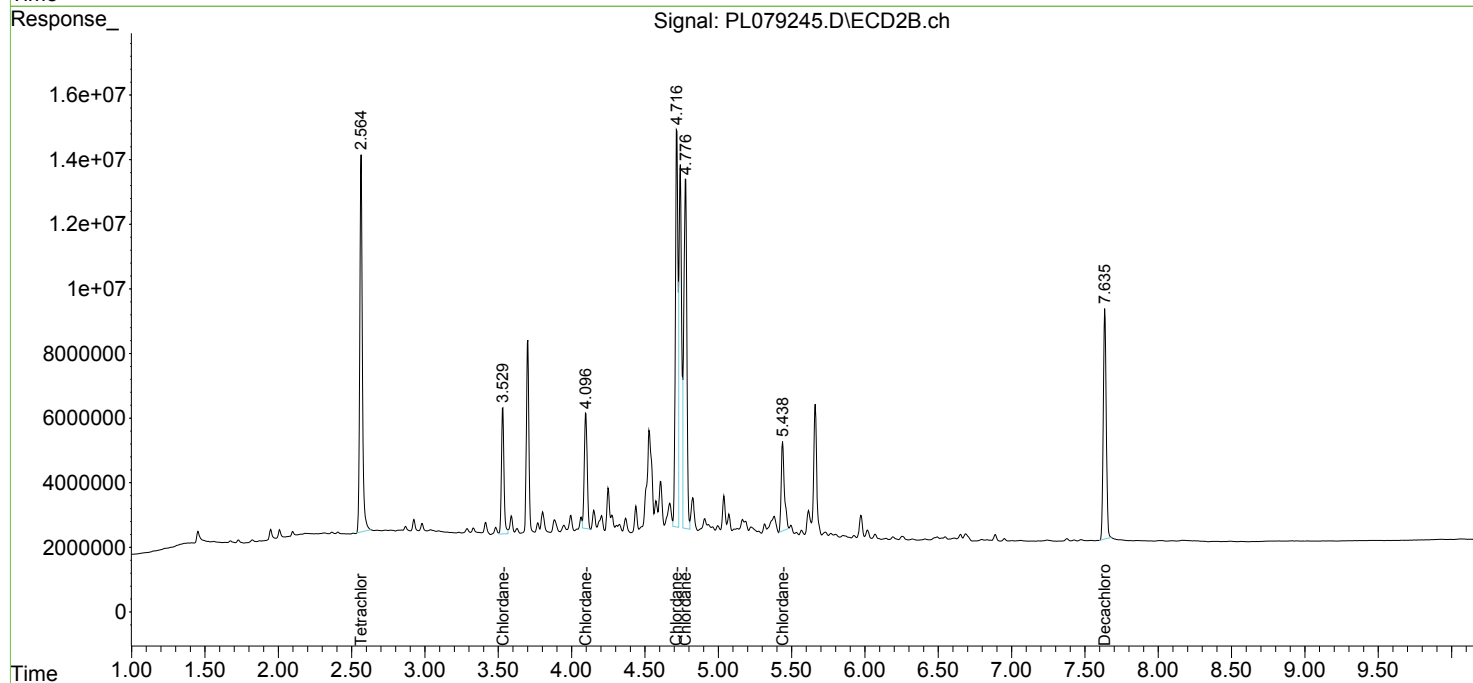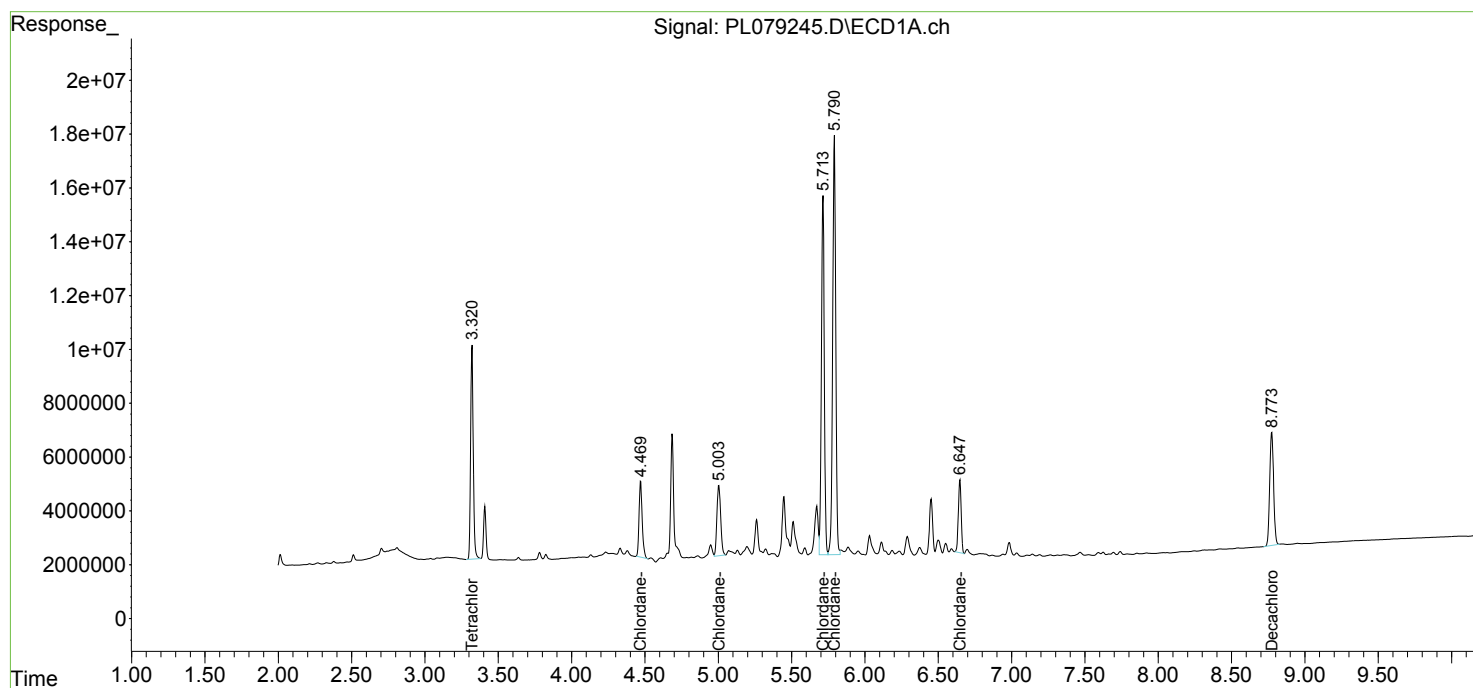


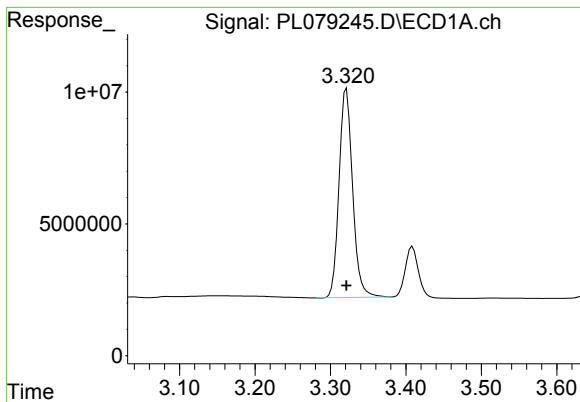

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 99120226
Conc: 47.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

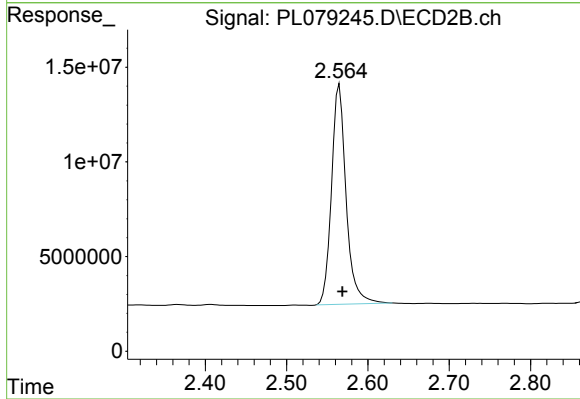


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: -0.004 min
Response: 145321019
Conc: 57.06 ng/ml

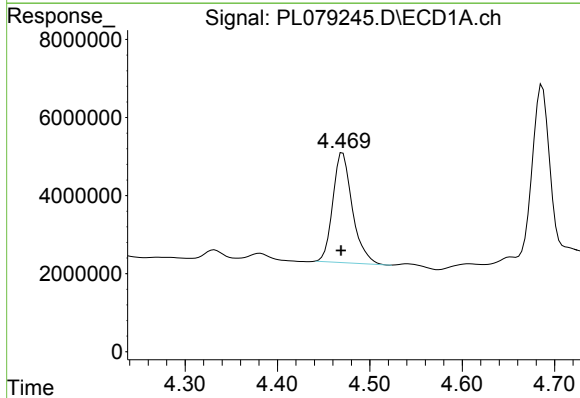


#23 Chlordane-1

R.T.: 4.471 min
Delta R.T.: 0.002 min
Response: 41379388
Conc: 472.25 ng/ml

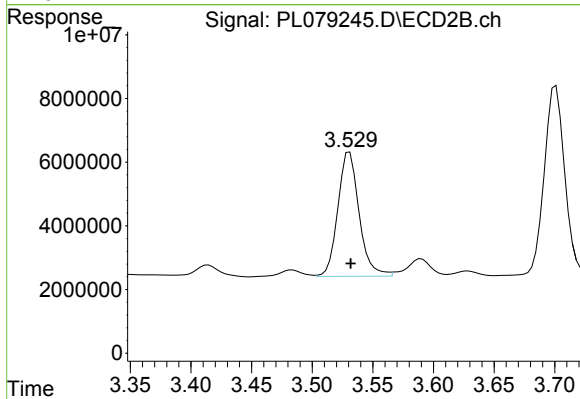

#23 Chlordane-1


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 47549470
Conc: 460.22 ng/ml

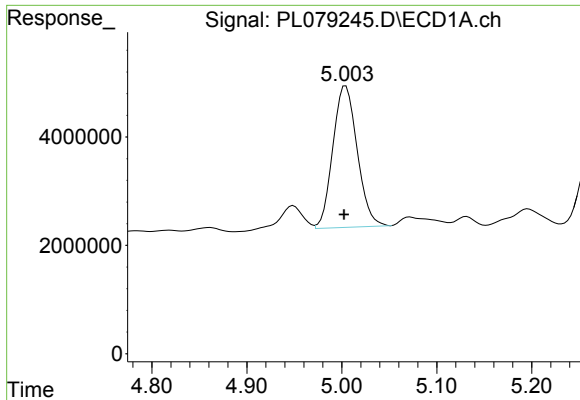

#24 Chlordane-2


R.T.: 5.004 min
Delta R.T.: 0.002 min
Response: 46624319
Conc: 458.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

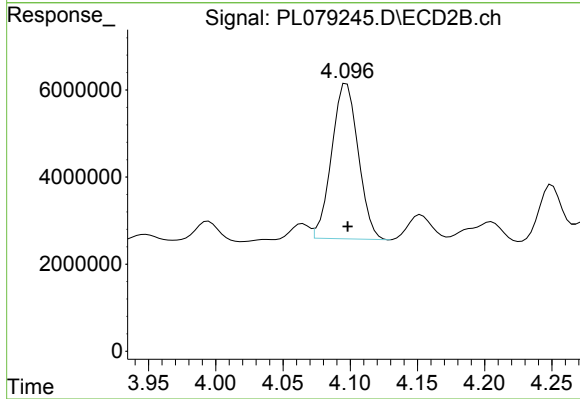


#24 Chlordane-2

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 48840149
Conc: 459.91 ng/ml

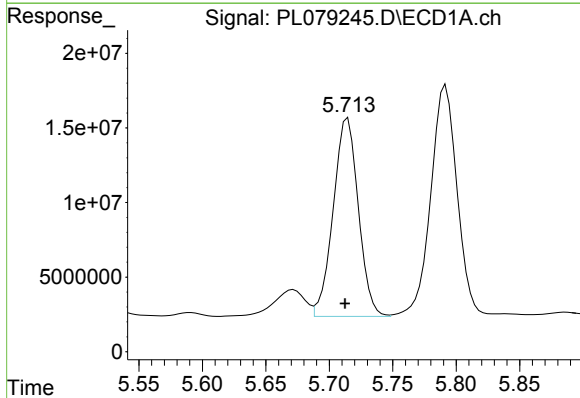


#25 Chlordane-3

R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 183160333
Conc: 475.49 ng/ml

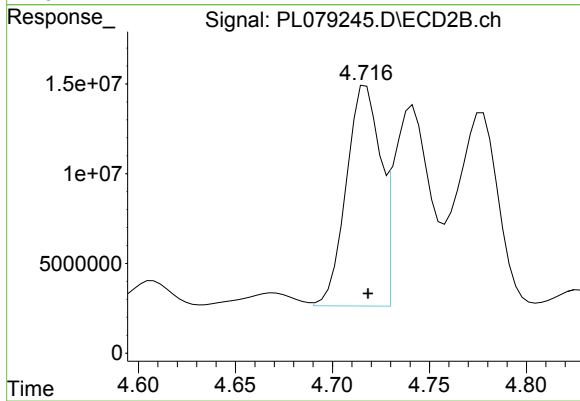

#25 Chlordane-3


R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 149618976
Conc: 469.59 ng/ml

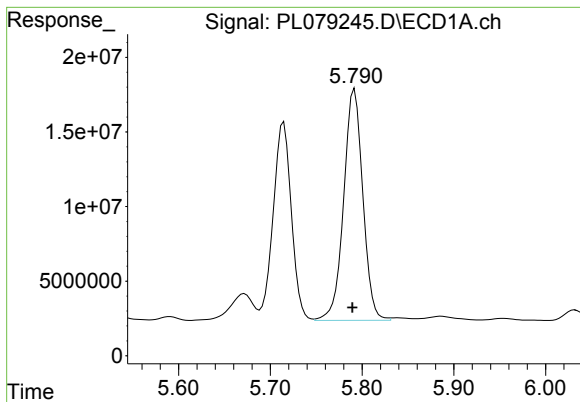

#26 Chlordane-4


R.T.: 5.792 min
Delta R.T.: 0.002 min
Response: 224678917
Conc: 474.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

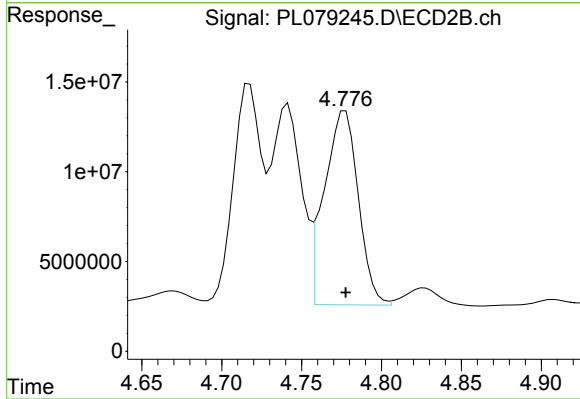


#26 Chlordane-4

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 159713267
Conc: 465.42 ng/ml

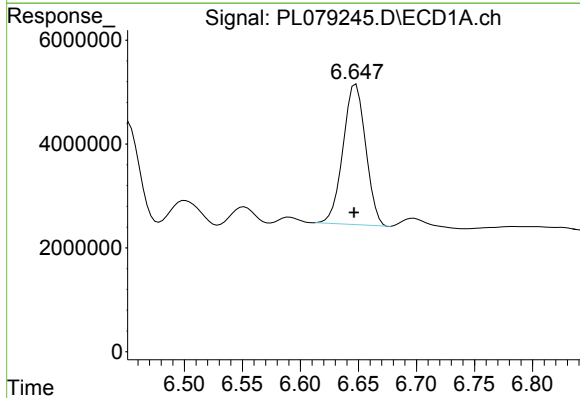


#27 Chlordane-5

R.T.: 6.648 min
Delta R.T.: 0.002 min
Response: 36738241
Conc: 495.16 ng/ml

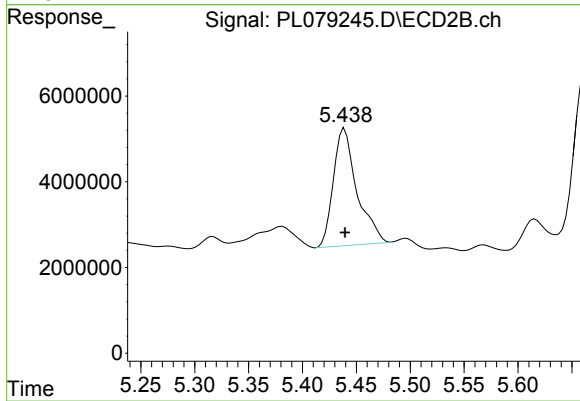

#27 Chlordane-5


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 41625840
Conc: 488.17 ng/ml

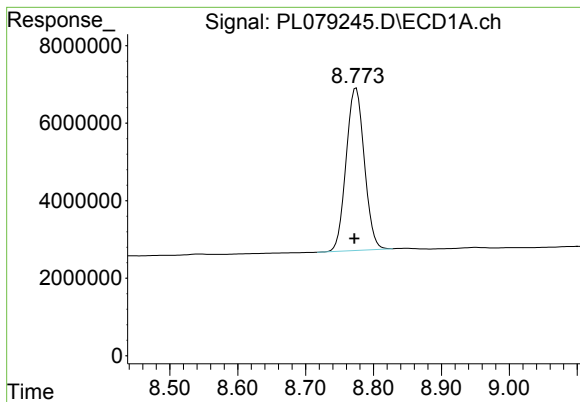

#28 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.003 min
Response: 77945265
Conc: 46.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

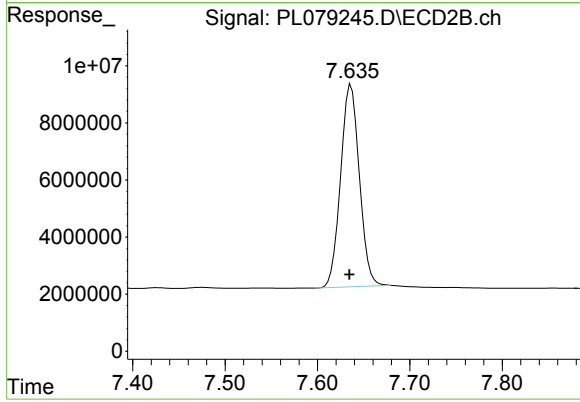

#28 Decachlorobiphenyl

R.T.: 7.636 min
Delta R.T.: 0.002 min
Response: 100052937
Conc: 48.23 ng/ml