

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
 Data File : PL079260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 21:32
 Operator : AR\AJ
 Sample : N5678-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 250FB-BP-BACKFILL-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:30:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 16 15:31:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.566	44831166	54999239	21.529	21.595
28)	SA Decachlor...	8.768	7.632	34395766	44148540	20.562	21.282

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111822\
Data File : PL079260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 21:32
Operator : AR\AJ
Sample : N5678-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
250FB-BP-BACKFILL-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:30:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111622.M
Quant Title : GC Extractables
QLast Update : Wed Nov 16 15:31:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

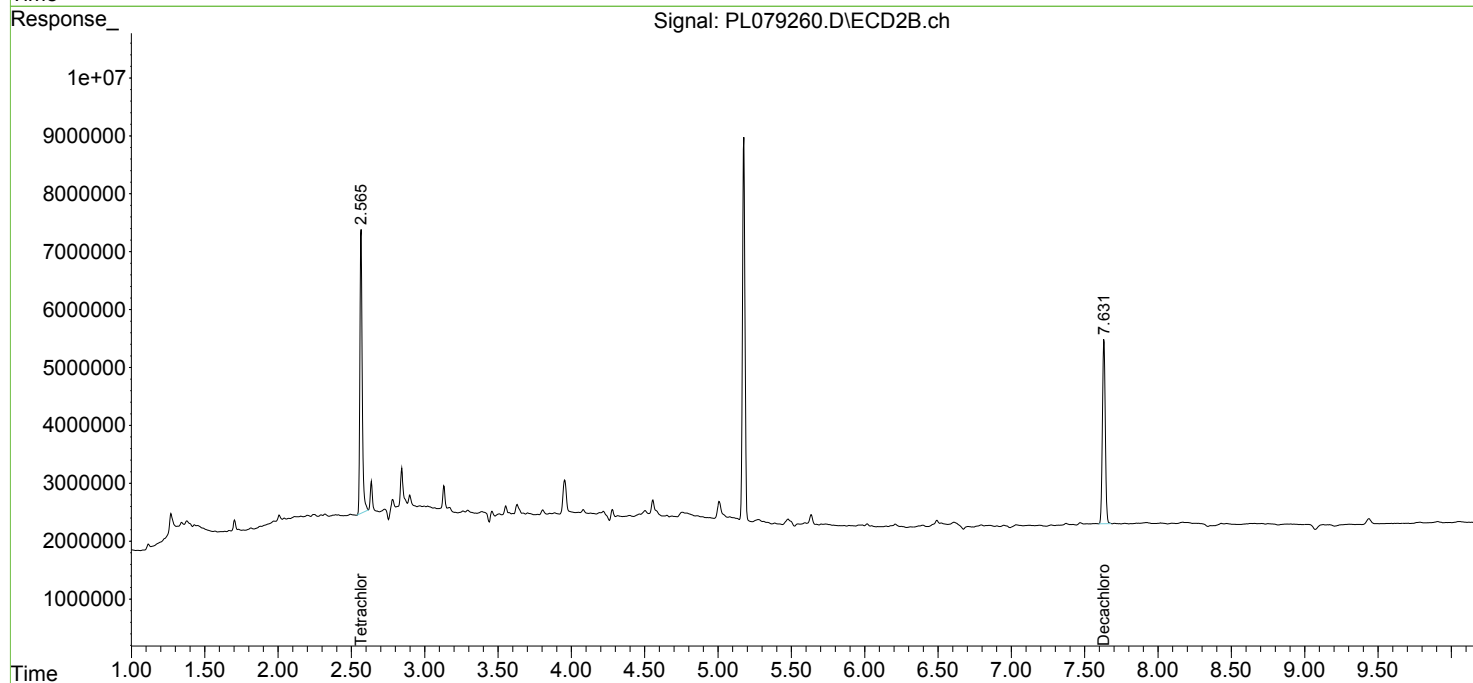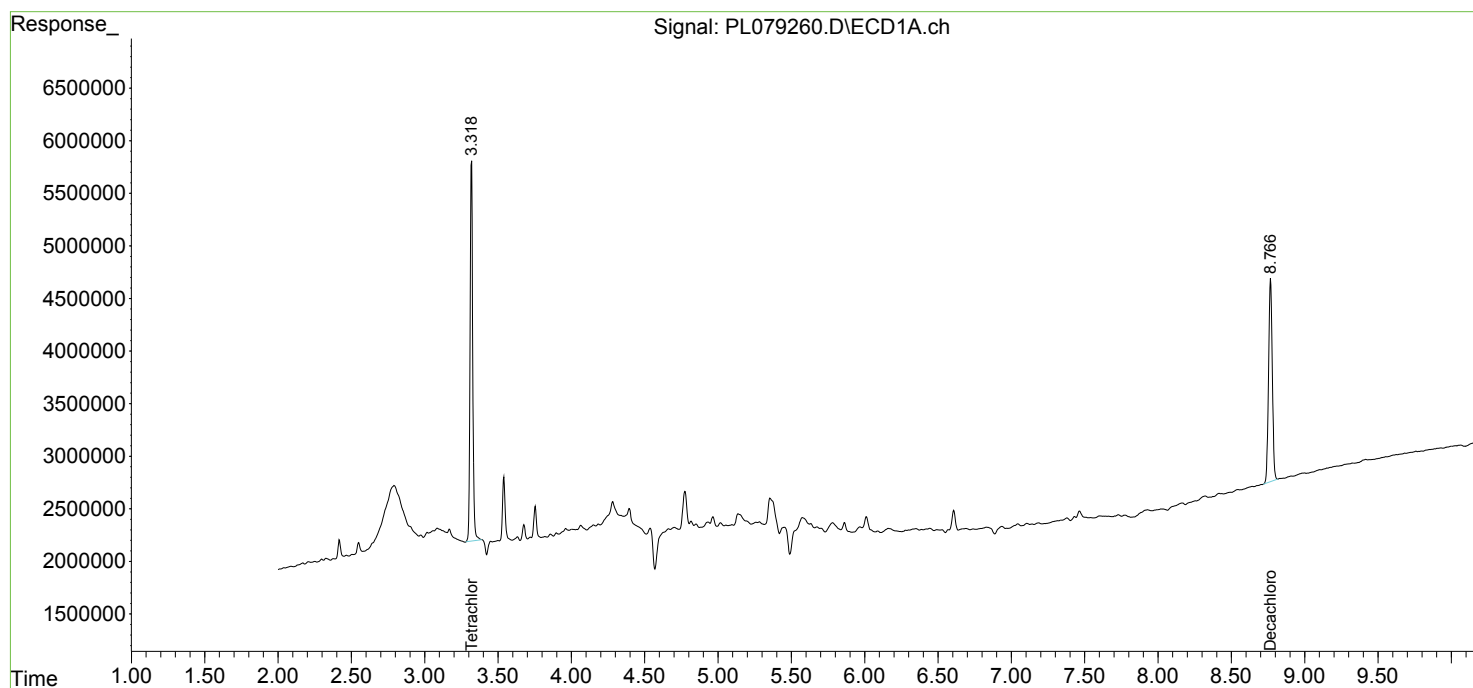


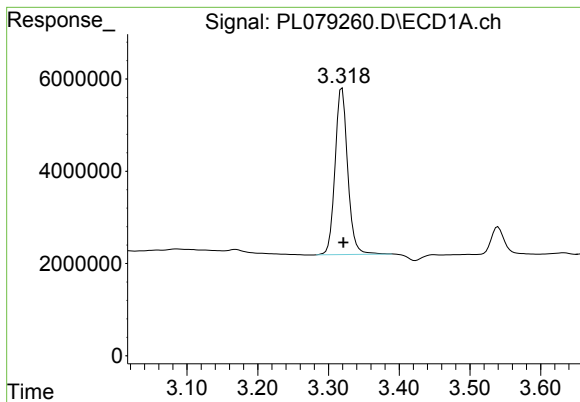

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 44831166
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
250FB-BP-BACKFILL-03

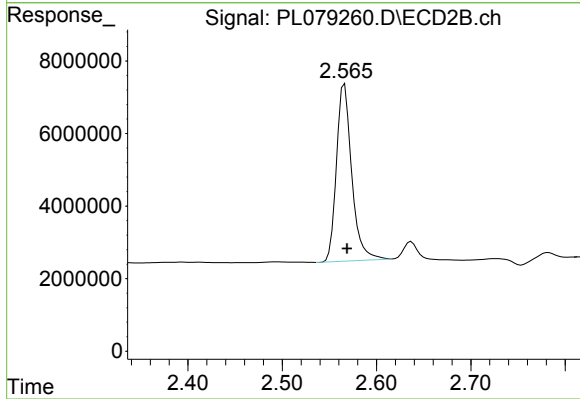


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: -0.003 min
Response: 54999239
Conc: 21.59 ng/ml

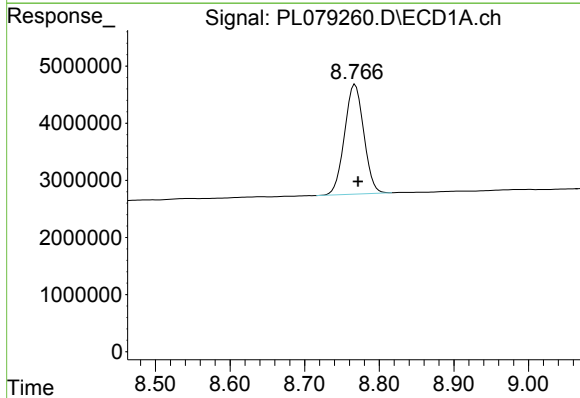

#28 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.004 min
Response: 34395766
Conc: 20.56 ng/ml

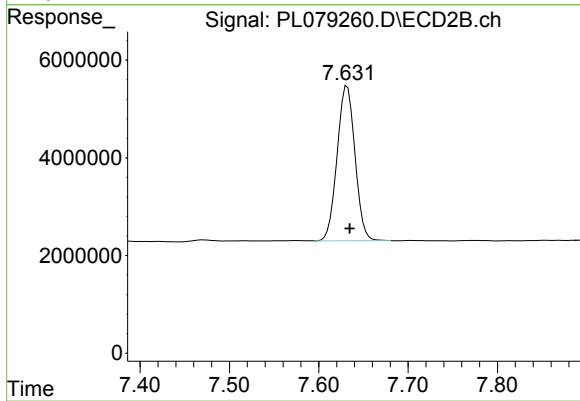

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: -0.003 min
Response: 44148540
Conc: 21.28 ng/ml