

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111824\
 Data File : PL093119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 15:04
 Operator : AR\AJ
 Sample : P4860-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PH2-BOT-005

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:29:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.778	55505777	59608074	22.653m	21.905
28) SA Decachlor...	9.055	7.915	38925323	56449072	20.226	20.683

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111824\
Data File : PL093119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 15:04
Operator : AR\AJ
Sample : P4860-10
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PH2-BOT-005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:29:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

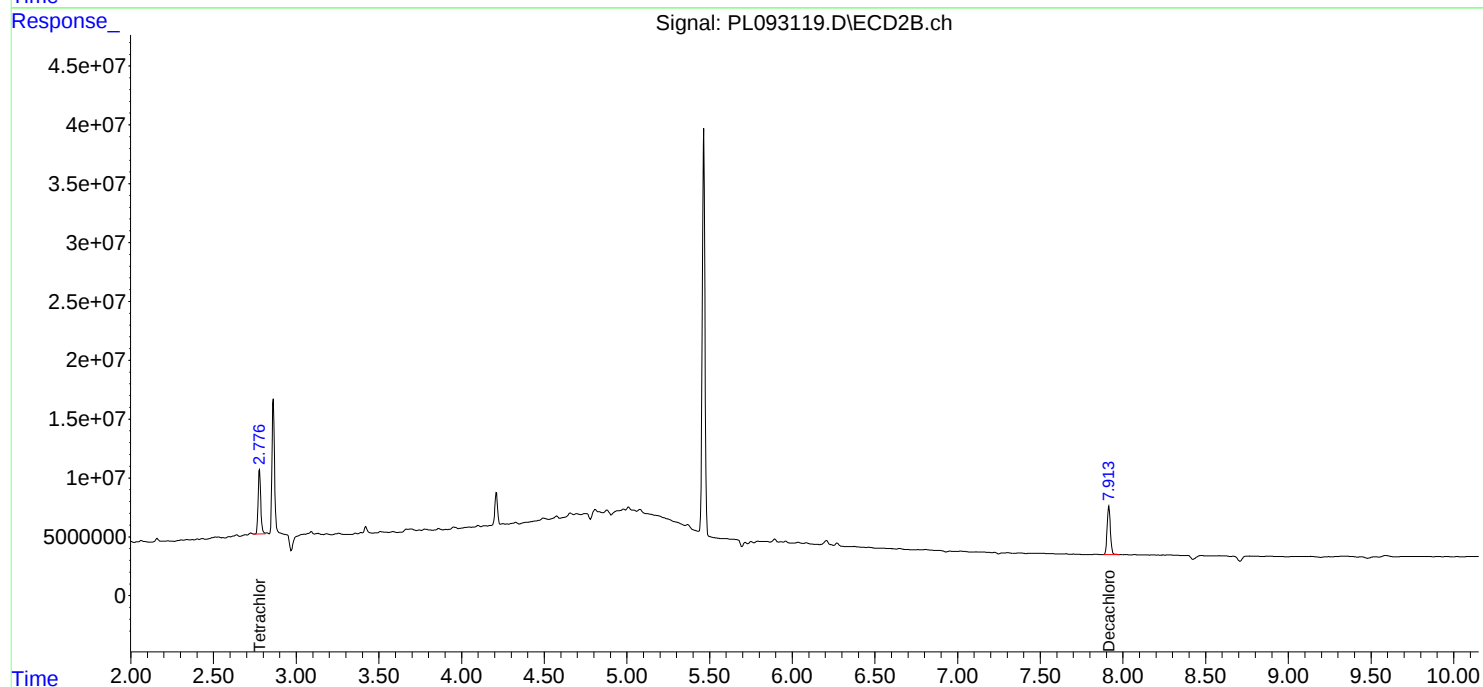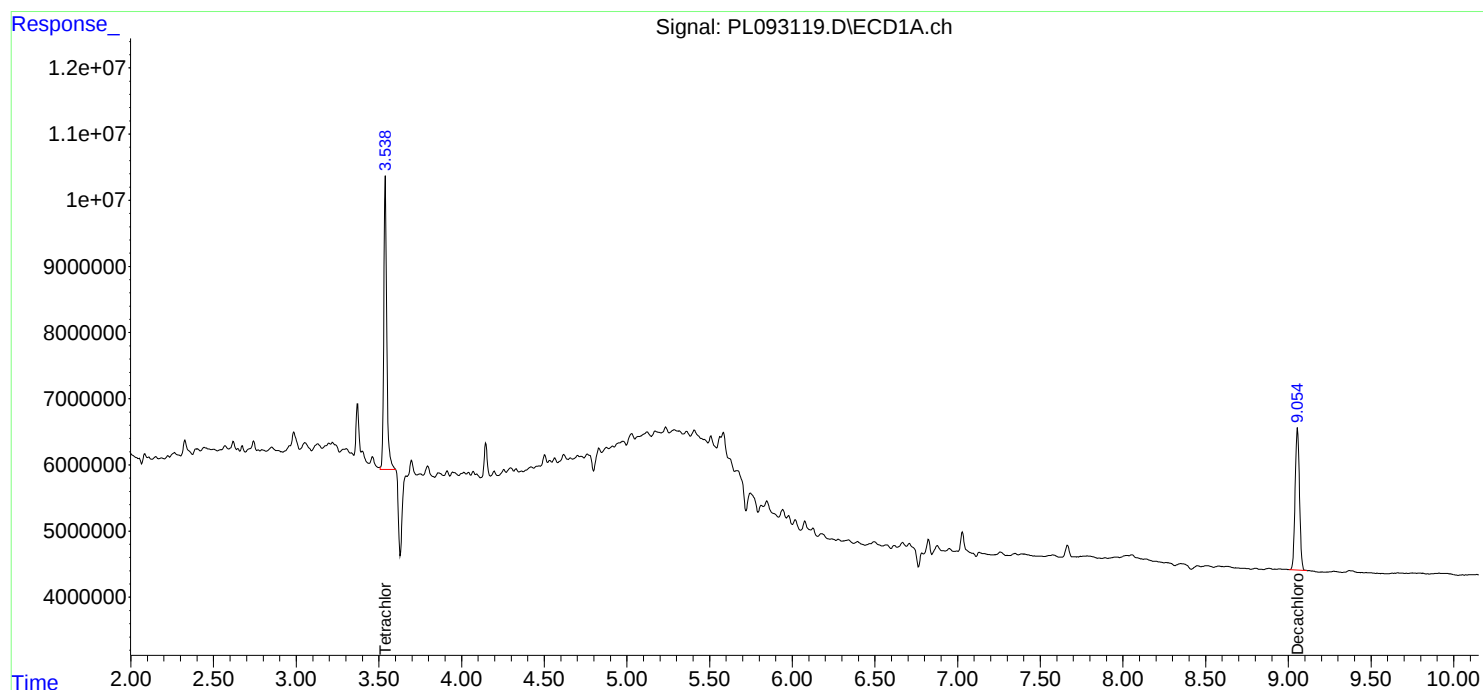

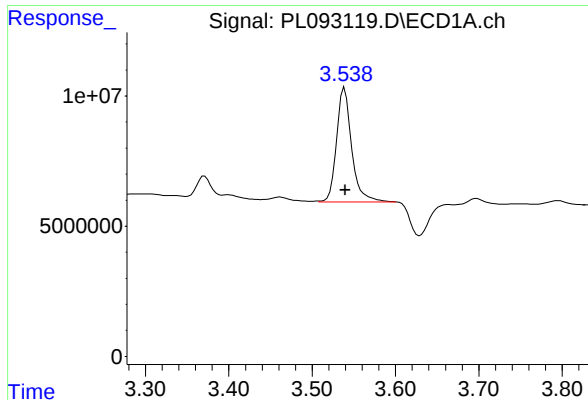


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: -0.002 min
Response: 55505777
Conc: 22.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PH2-BOT-005


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

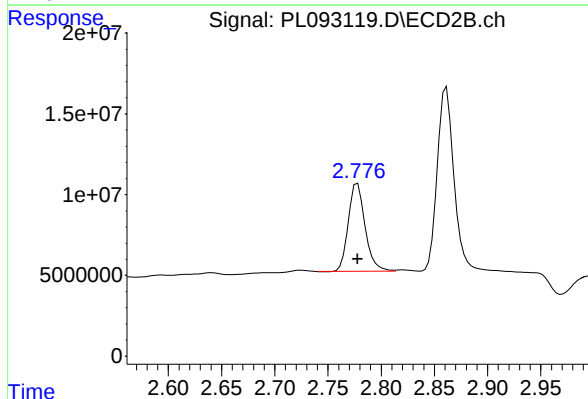


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 59608074
Conc: 21.91 ng/ml

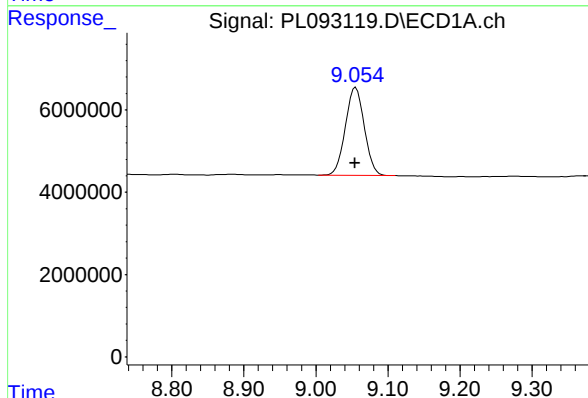

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.001 min
Response: 38925323
Conc: 20.23 ng/ml

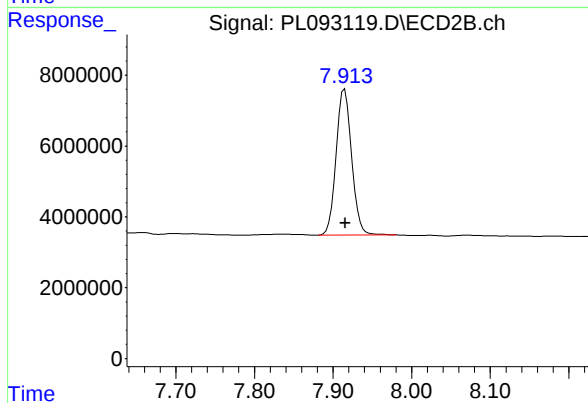

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.001 min
Response: 56449072
Conc: 20.68 ng/ml