

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
 Data File : PL042260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2018 15:25
 Operator : AJ\SJ
 Sample : I.BLK
 Misc : FOR MIREX
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:21:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.100	120.2E6	59488144	21.655	21.520
28)	SA Decachlor...	8.207	9.230	122.5E6	48704138	19.795	20.460
Target Compounds							
22)	Mirex	7.352	8.266f	625123	2632019	0.110	1.412 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
Data File : PL042260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2018 15:25
Operator : AJ\SJ
Sample : I.BLK
Misc : FOR MIREX
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:21:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

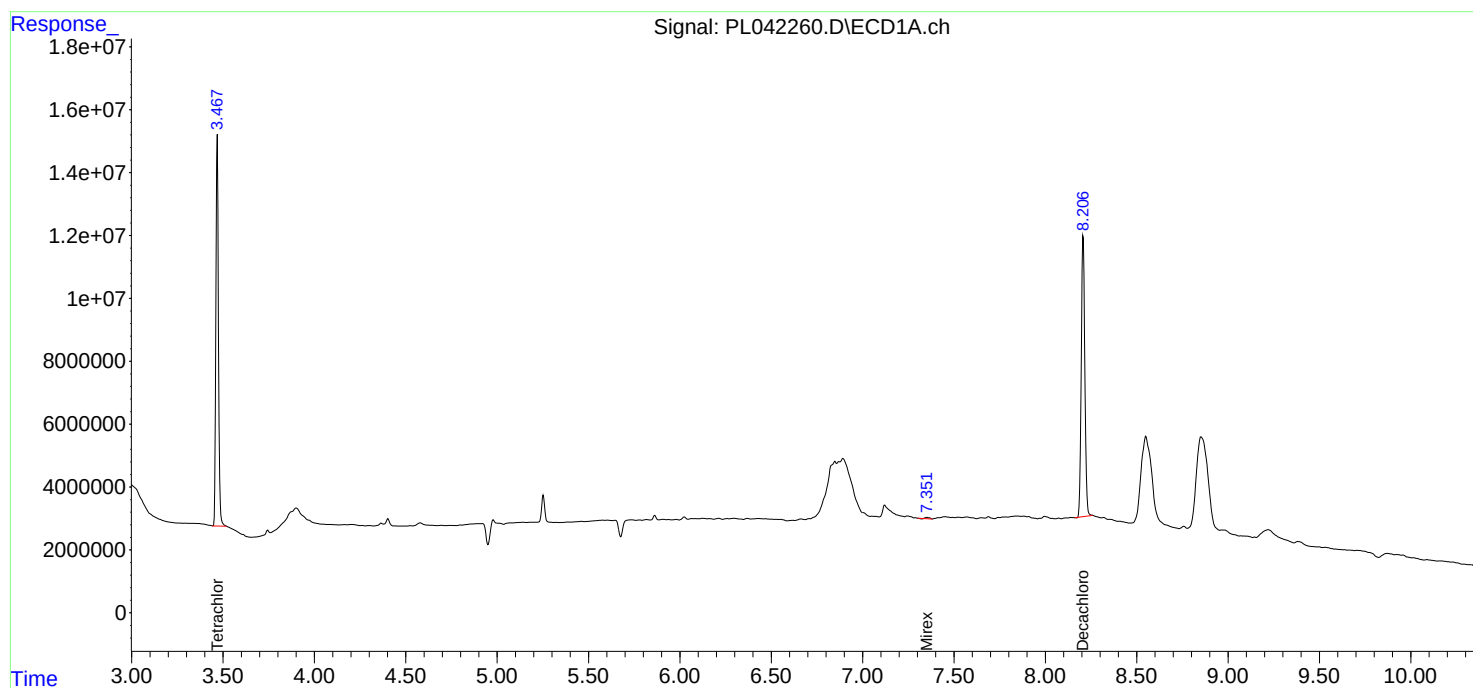


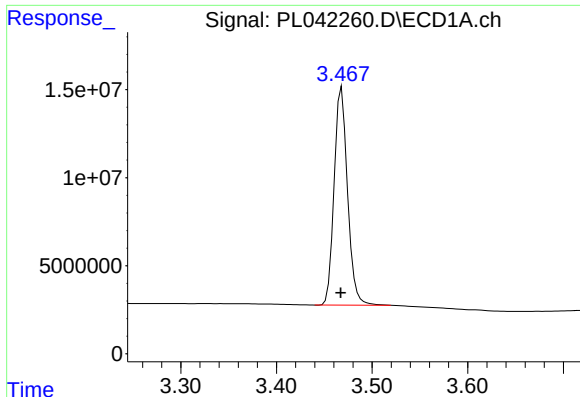

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.001 min
Response: 120193614
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

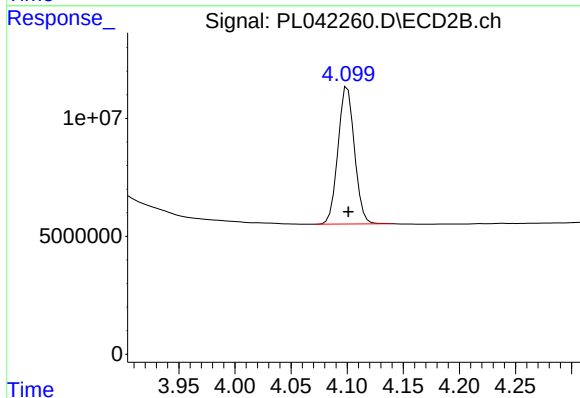


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 59488144
Conc: 21.52 ng/ml

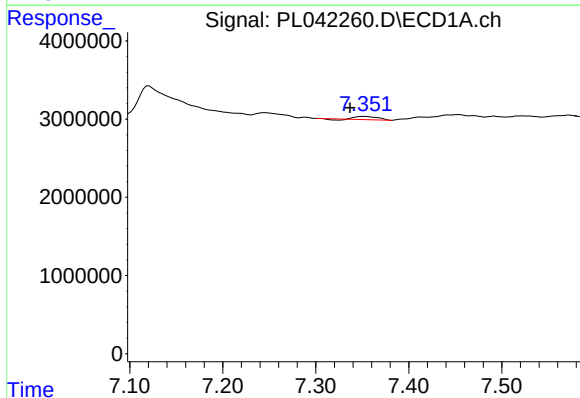


#22 Mirex

R.T.: 7.352 min
Delta R.T.: 0.015 min
Response: 625123
Conc: 0.11 ng/ml

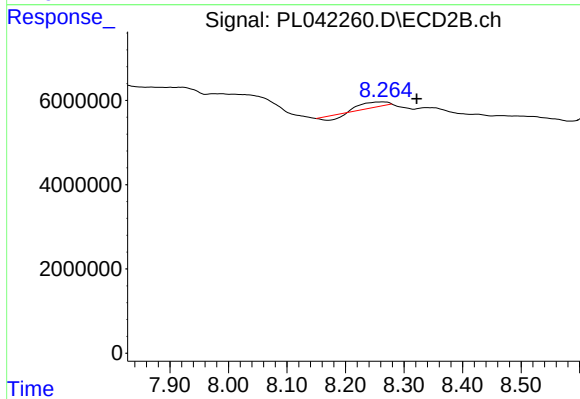

#22 Mirex

R.T.: 8.266 min
Delta R.T.: -0.056 min
Response: 2632019
Conc: 1.41 ng/ml

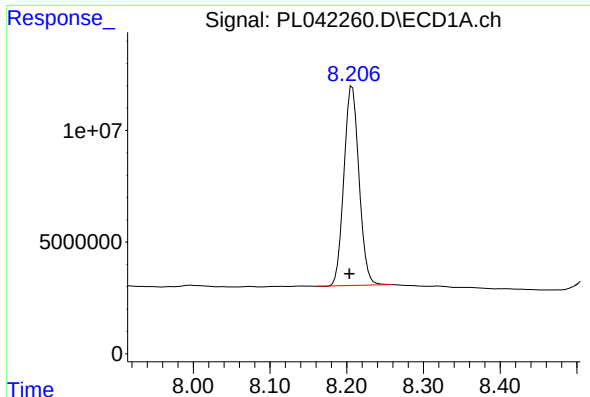

#28 Decachlorobiphenyl


R.T.: 8.207 min

Delta R.T.: 0.004 min

Response: 122499715

Conc: 19.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

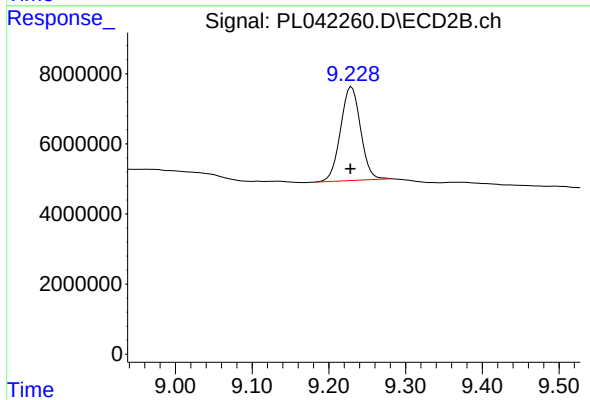

#28 Decachlorobiphenyl

R.T.: 9.230 min

Delta R.T.: 0.001 min

Response: 48704138

Conc: 20.46 ng/ml