

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111918\  
 Data File : PL042270.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Nov 2018 17:45  
 Operator : AJ\SJ  
 Sample : PSTDCCC050  
 Misc : FOR MIREX  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 19 08:22:50 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\Mirex-PL111718.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 15 11:21:10 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1  | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|---------|----------|--------|--------|
| -----                       |                 |       |       |         |          |        |        |
| System Monitoring Compounds |                 |       |       |         |          |        |        |
| 1)                          | SA Tetrachlo... | 3.467 | 4.101 | 299.9E6 | 152.9E6  | 54.029 | 55.327 |
| 28)                         | SA Decachlor... | 8.205 | 9.230 | 303.3E6 | 122.1E6  | 49.004 | 51.307 |
| Target Compounds            |                 |       |       |         |          |        |        |
| 22)                         | Mirex           | 7.339 | 8.323 | 286.0E6 | 99493049 | 50.168 | 53.372 |
| -----                       |                 |       |       |         |          |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL111918\  
Data File : PL042270.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Nov 2018 17:45  
Operator : AJ\SJ  
Sample : PSTDCCC050  
Misc : FOR MIREX  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 19 08:22:50 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\Mirex-PL111718.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 15 11:21:10 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

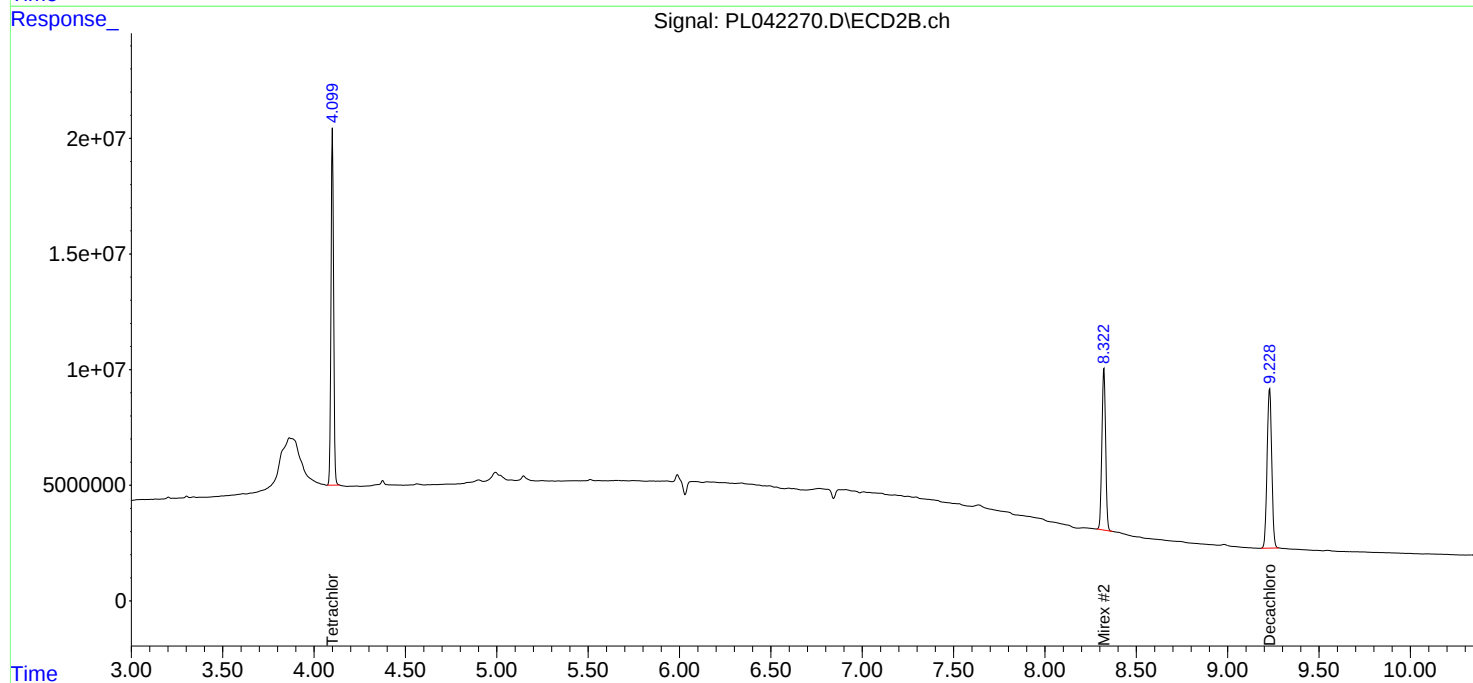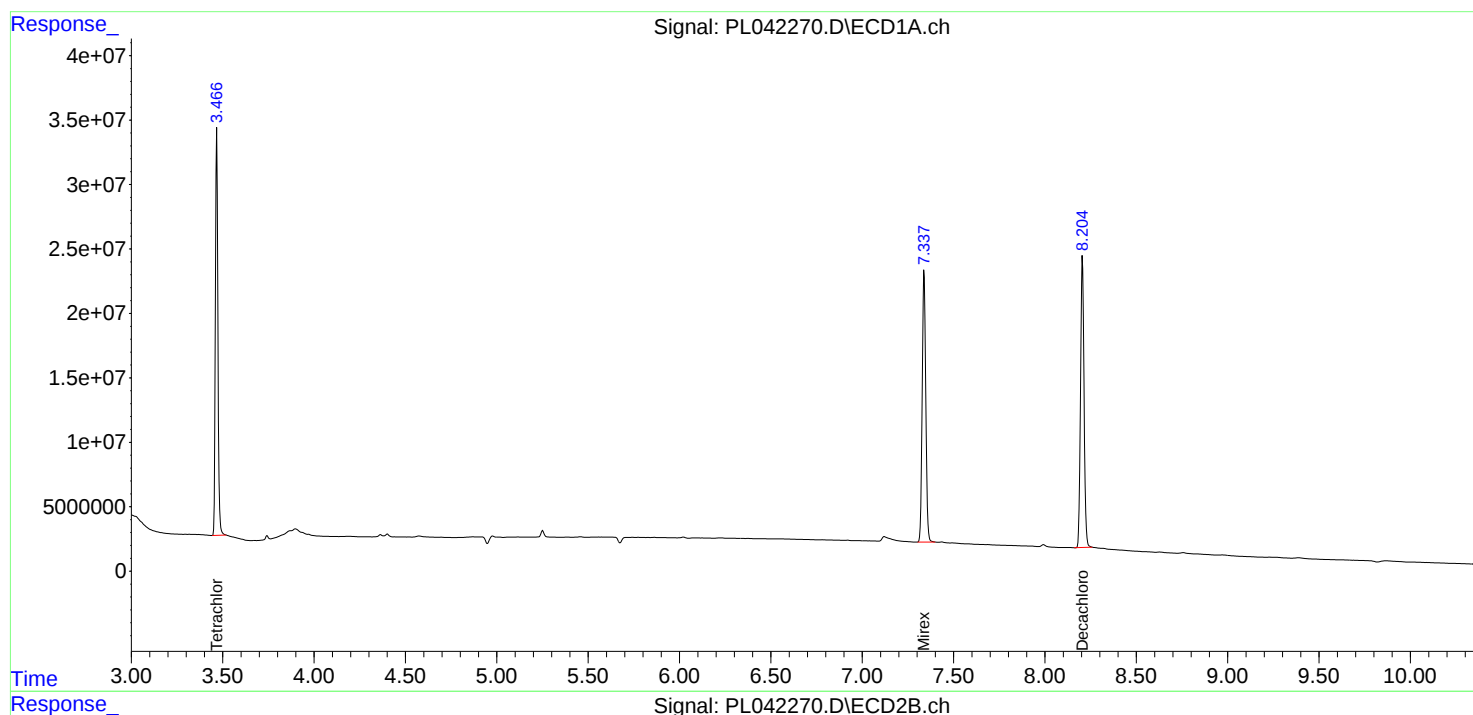


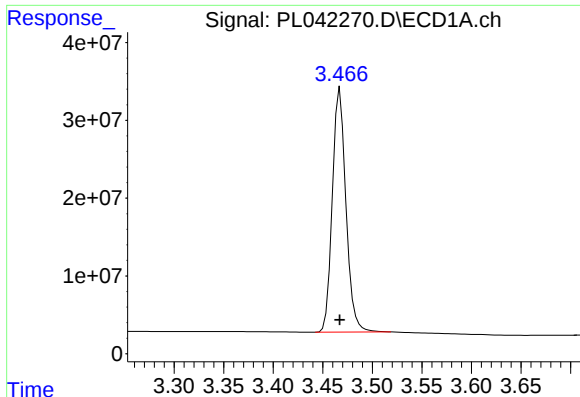

#1 Tetrachloro-m-xylene


R.T.: 3.467 min  
Delta R.T.: 0.000 min  
Response: 299883345  
Conc: 54.03 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

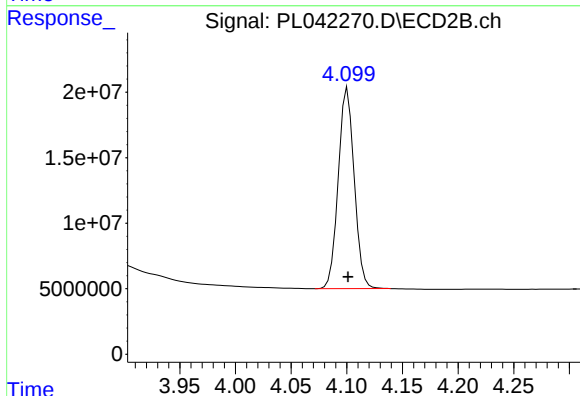


#1 Tetrachloro-m-xylene

R.T.: 4.101 min  
Delta R.T.: 0.000 min  
Response: 152945139  
Conc: 55.33 ng/ml

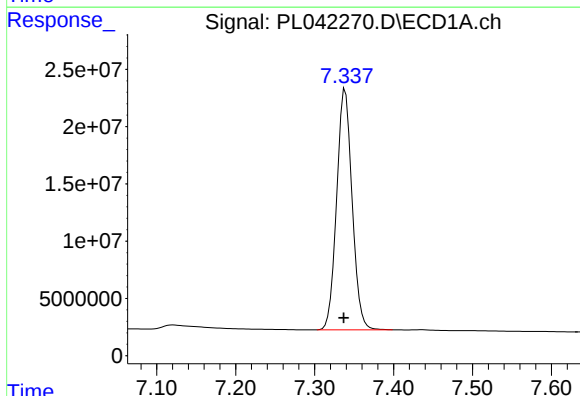


#22 Mirex

R.T.: 7.339 min  
Delta R.T.: 0.002 min  
Response: 285983896  
Conc: 50.17 ng/ml

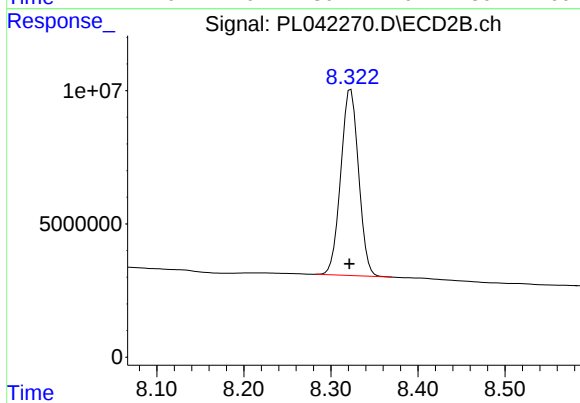

#22 Mirex

R.T.: 8.323 min  
Delta R.T.: 0.002 min  
Response: 99493049  
Conc: 53.37 ng/ml

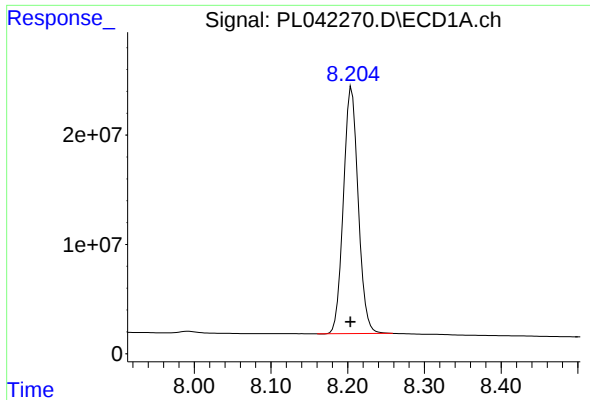

#28 Decachlorobiphenyl


R.T.: 8.205 min

Delta R.T.: 0.001 min

Response: 303256814

Conc: 49.00 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

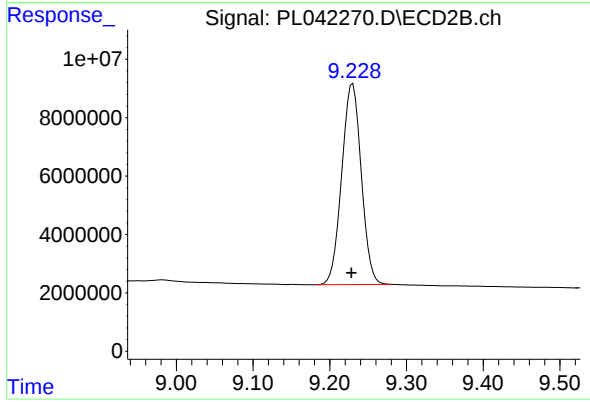

#28 Decachlorobiphenyl

R.T.: 9.230 min

Delta R.T.: 0.002 min

Response: 122131887

Conc: 51.31 ng/ml