

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
 Data File : PL042264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2018 16:21
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-06 (Sig #1); MIREX-MDL-S-04 (Sig #2)
 Misc : FOR MIREX
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MIREX-MDL-S-06

Manual Integrations
 APPROVED

Sohil
 11/19/2018 12:12:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:22:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 15 11:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	101.5E6	53186544	18.285	19.240
28)	SA Decachlor...	8.205	9.230	112.9E6	45445876	18.246	19.091
Target Compounds							
22)	Mirex	7.339	8.321	7654955	1698756	1.343	0.911m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111918\
Data File : PL042264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2018 16:21
Operator : AJ\SJ
Sample : MIREX-MDL-S-06 (Sig #1); MIREX-MDL-S-04 (Sig #2)
Misc : FOR MIREX
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-S-06


Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:22:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\Mirex-PL111718.M
Quant Title : GC Extractables
QLast Update : Thu Nov 15 11:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

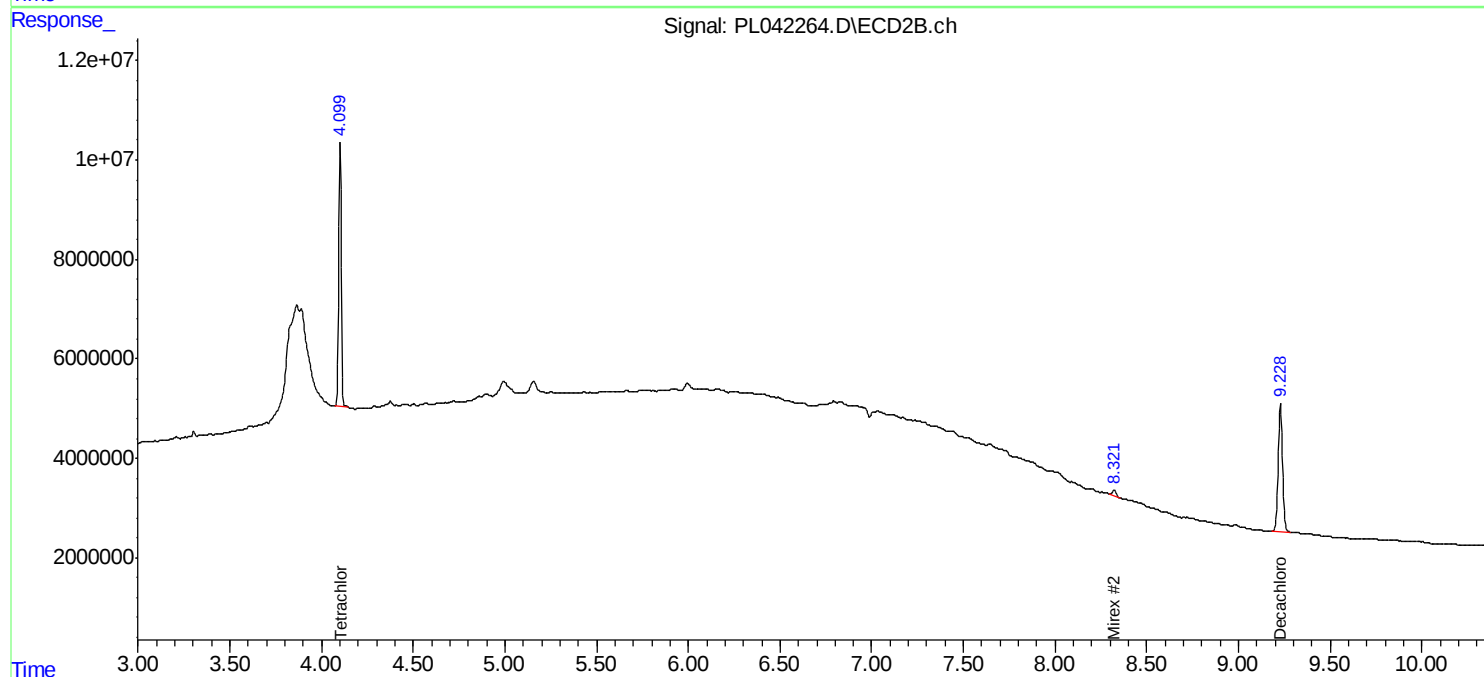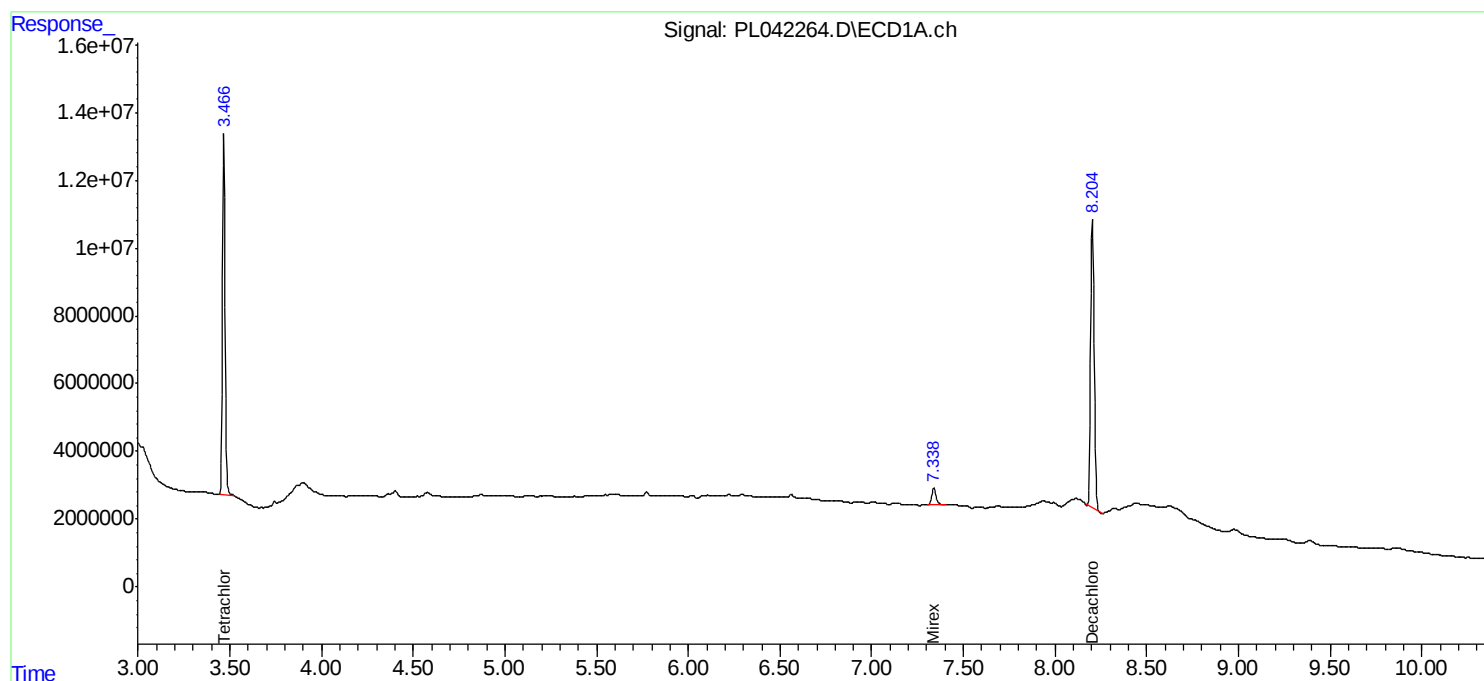

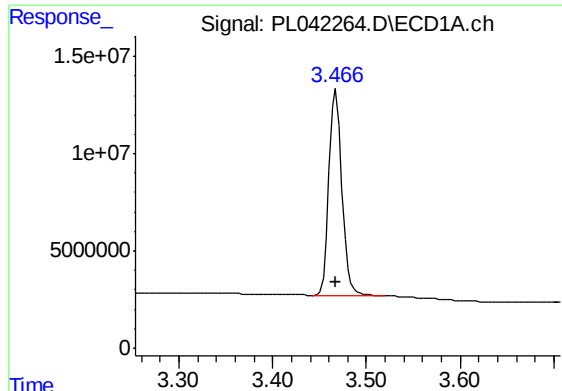


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 101490310
Conc: 18.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-S-06


Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:09 PM

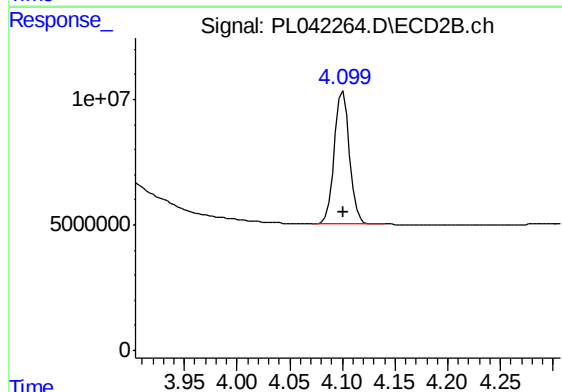


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 53186544
Conc: 19.24 ng/ml

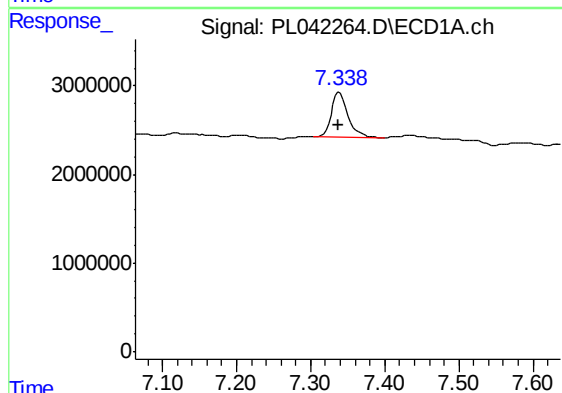


#22 Mirex

R.T.: 7.339 min
Delta R.T.: 0.002 min
Response: 7654955
Conc: 1.34 ng/ml

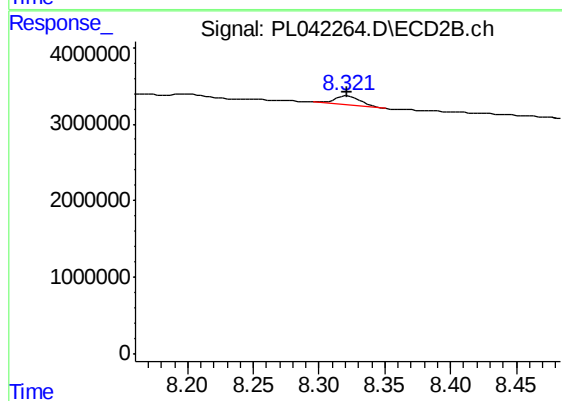

#22 Mirex

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 1698756
Conc: 0.91 ng/ml m

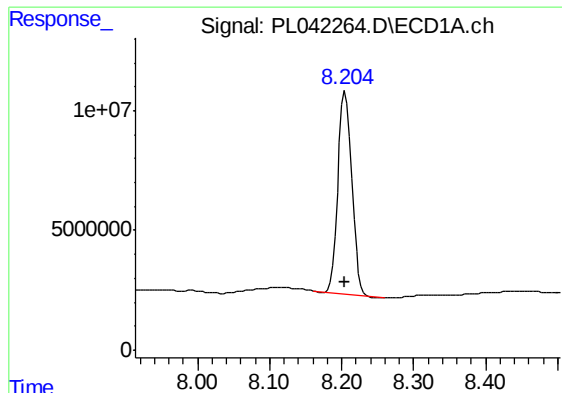


#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.001 min
Response: 112914112
Conc: 18.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
MIREX-MDL-S-06

Manual Integrations
APPROVED

Sohil
11/19/2018 12:12:09 PM

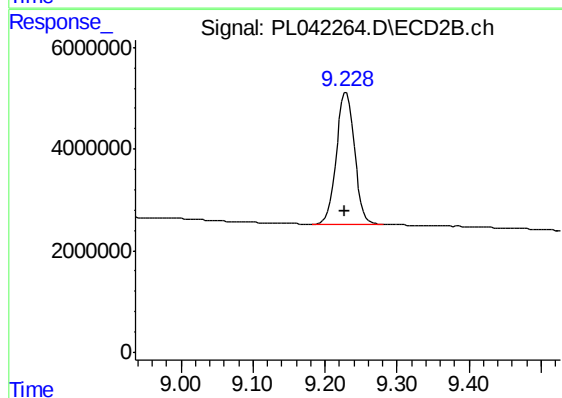

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.001 min
Response: 45445876
Conc: 19.09 ng/ml